

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
Data File : BP006281.D
Acq On : 22 Jul 2021 15:27
Operator : CG/JU
Sample : PB137815BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137815BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	385	392	403	rBV	5806620	8404461	49.97%	10.807%
2	6.975	652	661	669	rBV	5309370	8479403	50.42%	10.903%
3	7.799	790	801	808	rBV	1158259	1837859	10.93%	2.363%
4	8.952	989	997	1011	rBV	3211964	5290082	31.45%	6.802%
5	10.581	1265	1274	1284	rBV	1579256	2646038	15.73%	3.402%
6	13.051	1686	1694	1702	rBV	7973767	11670464	69.39%	15.007%
7	14.422	1918	1927	1934	rBV	2242704	3307992	19.67%	4.254%
8	15.916	2174	2181	2201	rVB	5139711	7250668	43.11%	9.323%
9	17.175	2388	2395	2402	rBV	2707161	3819971	22.71%	4.912%
10	19.751	2828	2833	2839	rBV	13160542	16818542	100.00%	21.626%
11	21.274	3087	3092	3097	rBV	3317817	4084141	24.28%	5.252%
12	23.627	3486	3492	3504	rVB2	2080606	4159755	24.73%	5.349%




Sum of corrected areas: 77769376

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
Data File : BP006281.D
Acq On : 22 Jul 2021 15:27
Operator : CG/JU
Sample : PB137815BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137815BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

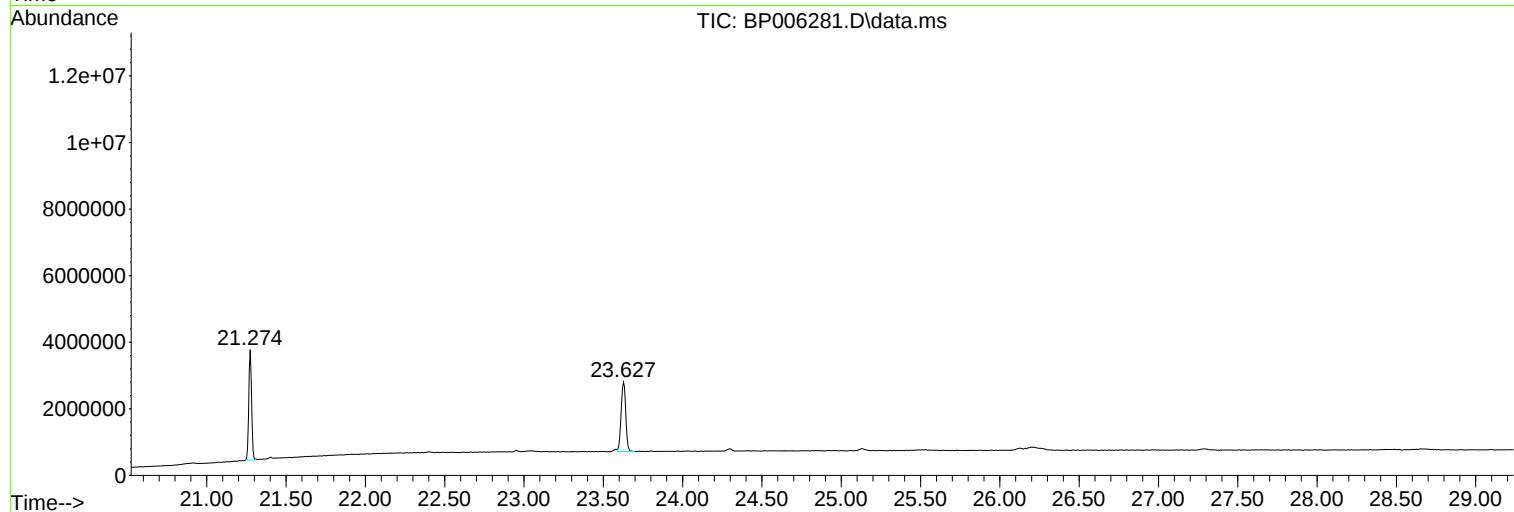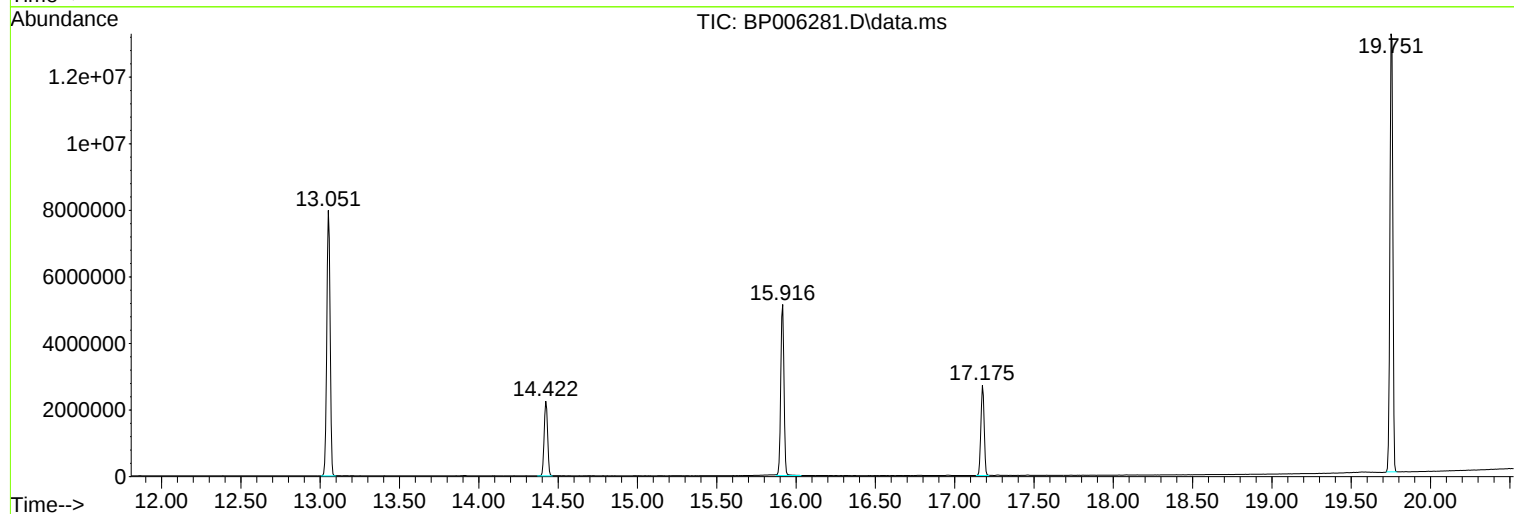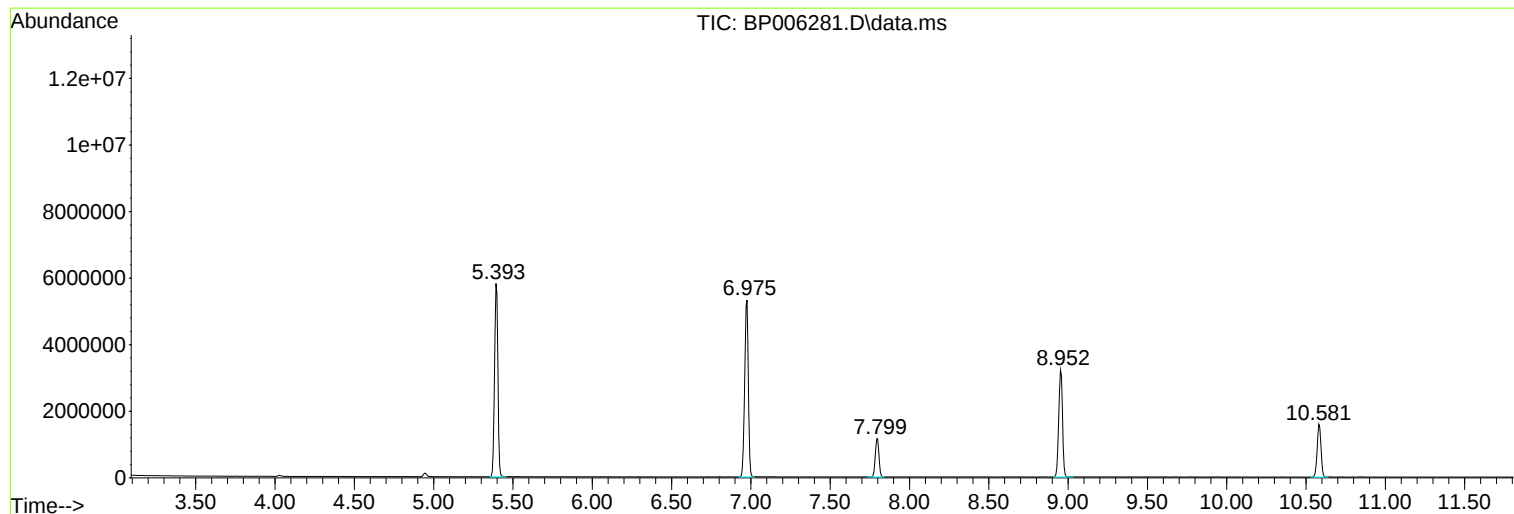

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
Data File : BP006281.D
Acq On : 22 Jul 2021 15:27
Operator : CG/JU
Sample : PB137815BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137815BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
Data File : BP006281.D
Acq On : 22 Jul 2021 15:27
Operator : CG/JU
Sample : PB137815BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137815BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------