
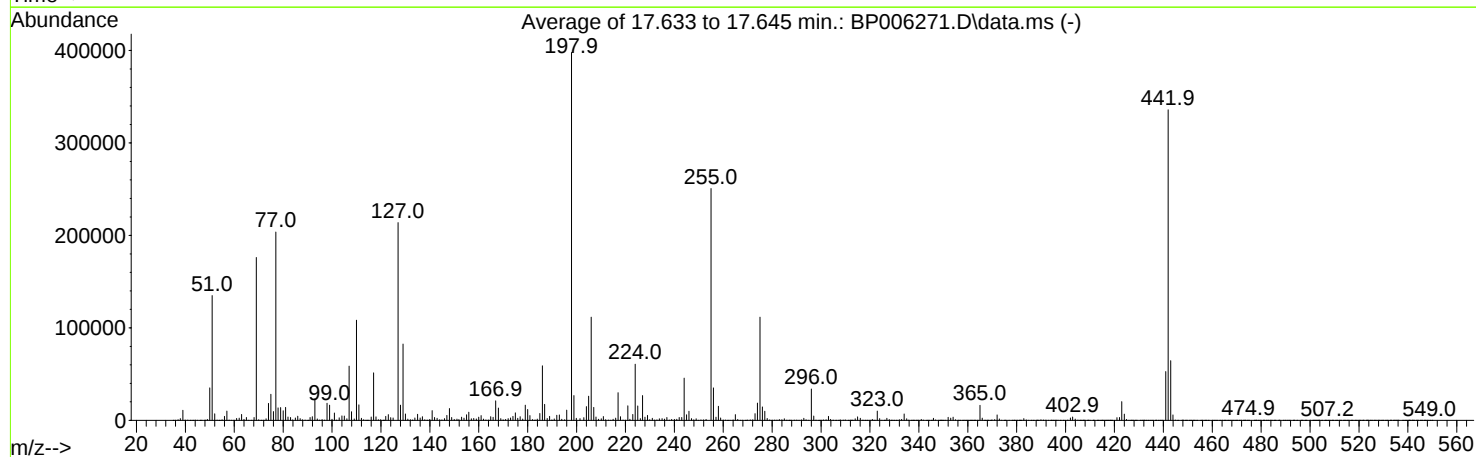


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
 Data File : BP006271.D
 Acq On : 22 Jul 2021 07:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 14:48:03 2021

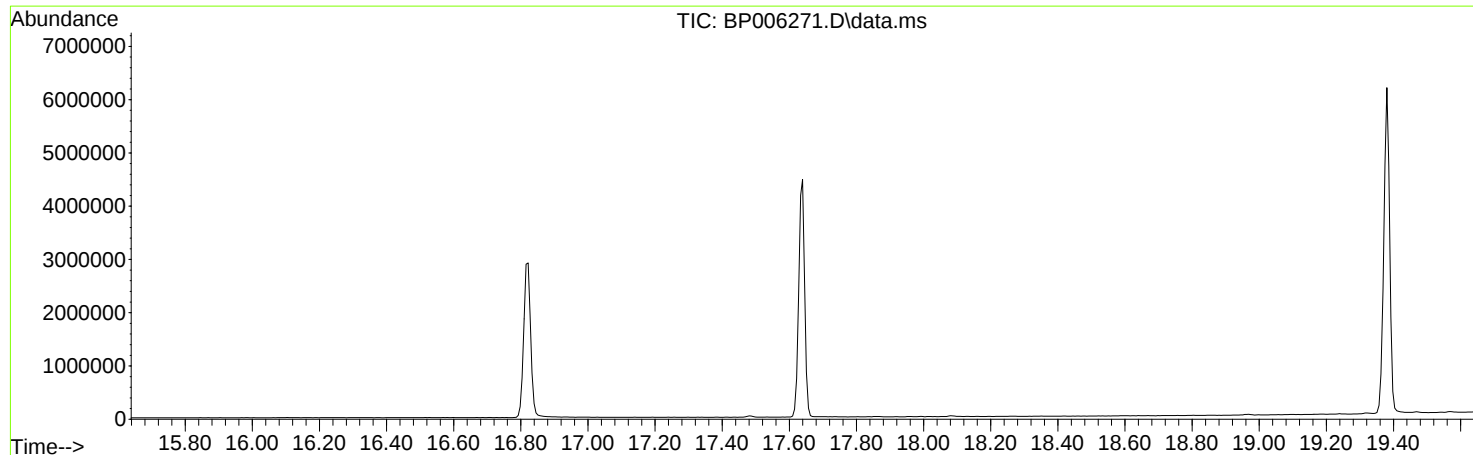

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	135046	PASS
68	69	0.00	2	1.8	3178	PASS
69	198	0.00	100	44.3	176219	PASS
70	69	0.00	2	0.4	752	PASS
127	198	10	80	53.8	213909	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	397803	PASS
199	198	5	9	6.7	26765	PASS
275	198	10	60	28.0	111581	PASS
365	198	1	100	4.1	16366	PASS
441	198	0.01	100	13.3	52757	PASS
442	442	100	100	100.0	335868	PASS
443	442	15	24	19.2	64544	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/22/2021	BNA_P	<u>BP006271.D</u>
Compound Name	Response	Retention Time
DDT	1420104	20.58
DDD	6229	20.15
DDE	2027	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8256	1428360	0.58

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
 Data File : BP006271.D
 Acq On : 22 Jul 2021 07:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 11:41:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:37:21 2021
 Response via : Initial Calibration

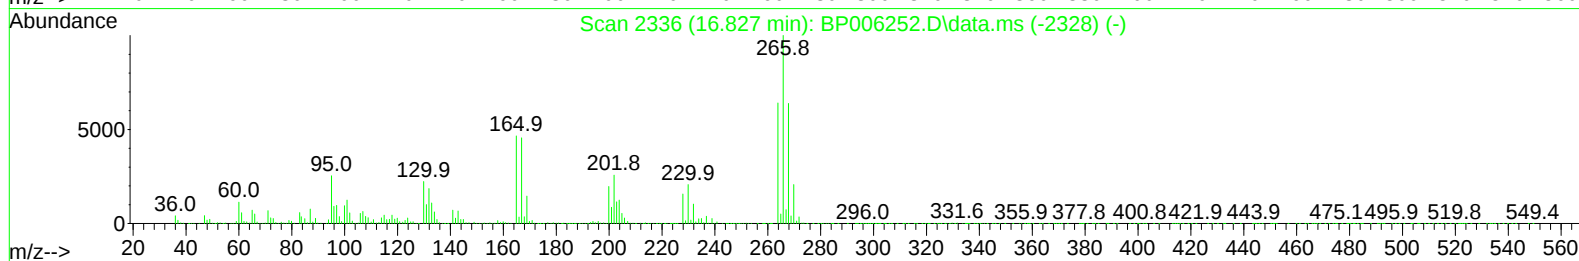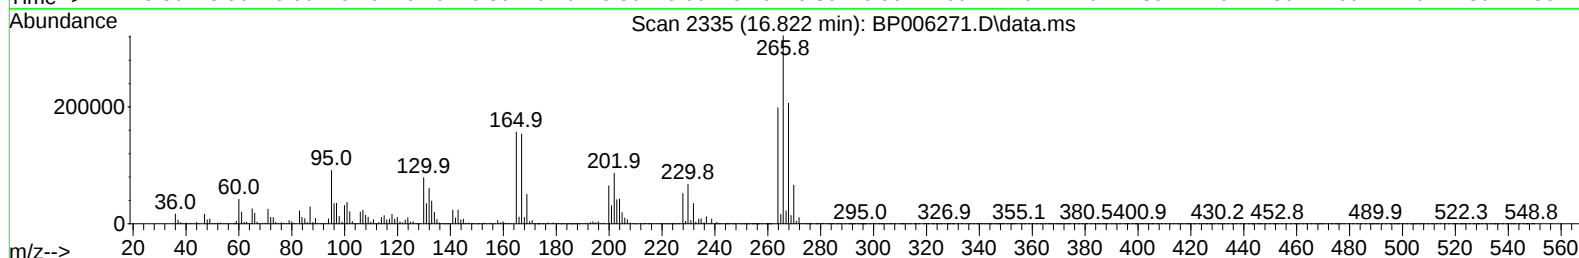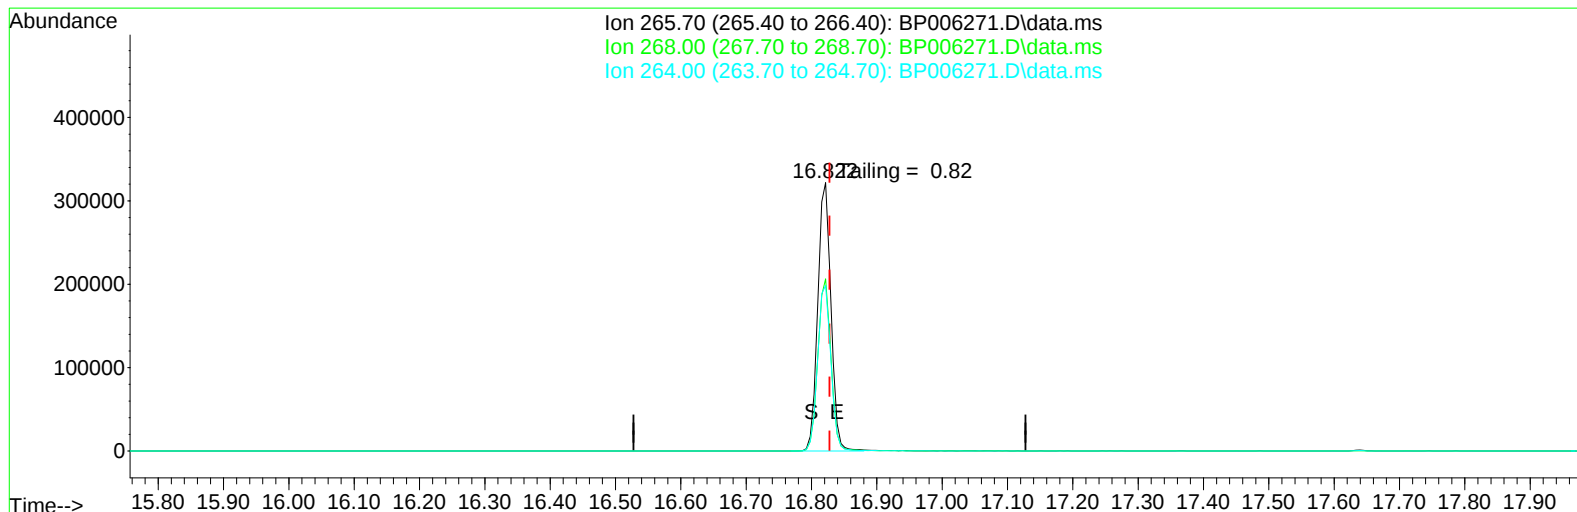

TIC: BP006271.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 1630634.72 ng




response 453646

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.17
264.00	62.90	61.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072221\
 Data File : BP006271.D
 Acq On : 22 Jul 2021 07:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 22 11:41:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 11:37:21 2021
 Response via : Initial Calibration

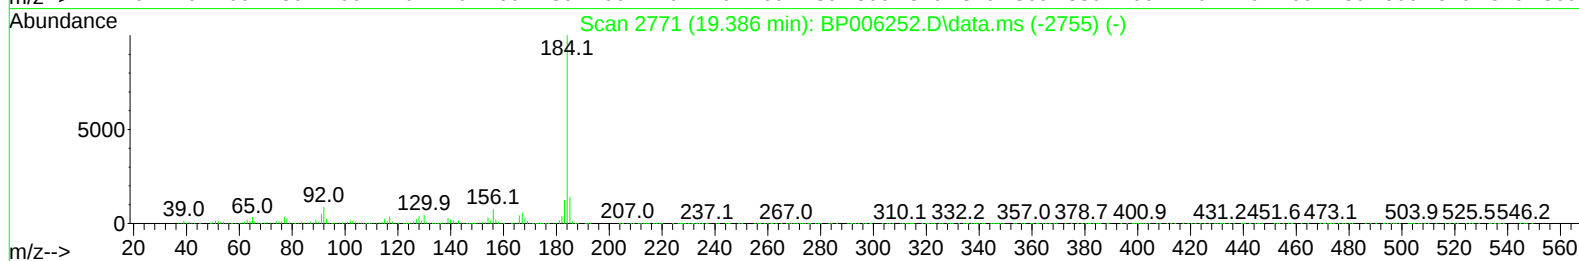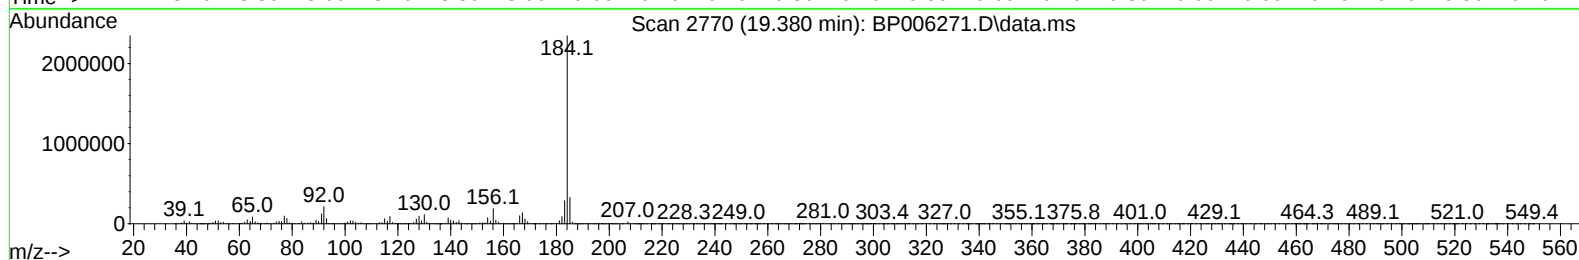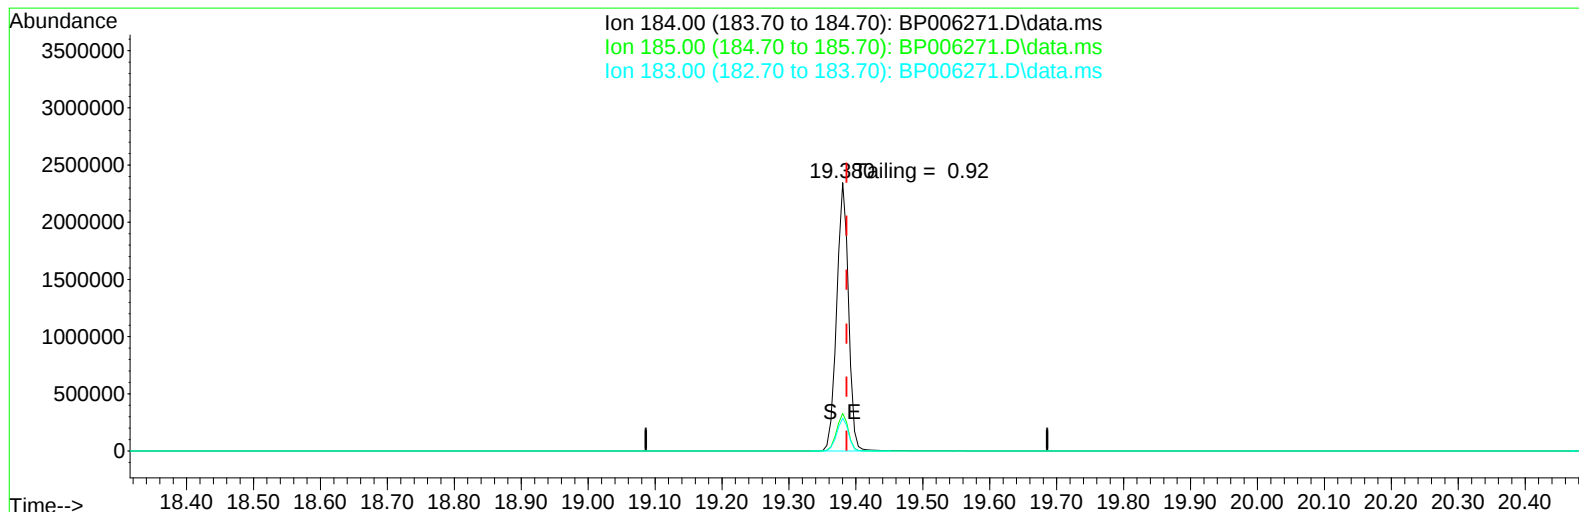

TIC: BP006271.D\data.ms

(77) Benzidine

19.380min (-0.006) 83501.51 ng

response 2875080

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.02
183.00	11.90	12.26
0.00	0.00	0.00