

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
 Data File : BP021088.D
 Acq On : 22 Jul 2024 14:47
 Operator : MA/JU
 Sample : P3238-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	649	657	660	rBV	703797	1141811	3.32%	0.268%
2	6.922	666	669	682	rVV	858621	1553755	4.52%	0.365%
3	7.234	714	722	724	rBV	698655	1174616	3.42%	0.276%
4	7.263	724	727	743	rVB	927525	1480600	4.31%	0.348%
5	7.681	791	798	806	rBV	761849	1295342	3.77%	0.305%
6	8.140	869	876	880	rBV	1176678	1793944	5.22%	0.422%
7	8.199	880	886	895	rVB2	549343	1343922	3.91%	0.316%
8	8.405	914	921	926	rBV	791301	1335515	3.89%	0.314%
9	8.475	926	933	936	rBV3	1502588	3271259	9.52%	0.769%
10	8.875	997	1001	1013	rVV	902039	1370966	3.99%	0.322%
11	9.381	1080	1087	1101	rBV	1224303	1995108	5.81%	0.469%
12	9.569	1116	1119	1126	rVV	685511	1258776	3.66%	0.296%
13	9.640	1126	1131	1145	rVB	1139936	1836770	5.35%	0.432%
14	9.863	1153	1169	1179	rBV	800049	1368260	3.98%	0.322%
15	10.434	1260	1266	1270	rVV	1136575	1850070	5.38%	0.435%
16	10.487	1270	1275	1286	rVV	1999878	3269153	9.52%	0.769%
17	10.616	1286	1297	1313	rVV2	480677	1550155	4.51%	0.364%
18	10.752	1313	1320	1329	rVB	1264796	1940623	5.65%	0.456%
19	11.434	1424	1436	1451	rBV	462901	1290354	3.76%	0.303%
20	11.763	1484	1492	1503	rBV	936909	2144561	6.24%	0.504%
21	12.099	1541	1549	1557	rBV	1866097	3351453	9.76%	0.788%
22	12.322	1580	1587	1597	rVB	2380757	3460903	10.07%	0.814%
23	12.469	1606	1612	1620	rVB	1286693	2407561	7.01%	0.566%
24	12.728	1648	1656	1662	rBV	1246245	2187774	6.37%	0.514%
25	12.822	1667	1672	1690	rVB	1259730	2234386	6.50%	0.525%
26	13.081	1709	1716	1719	rBV	1772705	2744136	7.99%	0.645%
27	13.116	1719	1722	1726	rVV	2088323	3123783	9.09%	0.734%
28	13.163	1726	1730	1738	rVB	1753245	2769153	8.06%	0.651%
29	13.393	1763	1769	1775	rBV	947182	1540341	4.48%	0.362%
30	13.716	1819	1824	1828	rVV	1387369	2043606	5.95%	0.481%
31	13.763	1828	1832	1838	rVV	1999095	2519325	7.33%	0.592%
32	13.893	1849	1854	1861	rVV	1239405	1769580	5.15%	0.416%
33	13.993	1861	1871	1873	rVV2	1469445	2519392	7.33%	0.592%
34	14.022	1873	1876	1888	rVB	1959935	3510508	10.22%	0.825%
35	14.240	1907	1913	1917	rBV	780045	1275695	3.71%	0.300%
36	14.298	1917	1923	1929	rVB	1467861	2497519	7.27%	0.587%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
 Data File : BP021088.D
 Acq On : 22 Jul 2024 14:47
 Operator : MA/JU
 Sample : P3238-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	14.369	1929	1935	1942	rVB	3092219	5298279	15.42%	1.246%
38	14.616	1966	1977	1986	rBV3	1833032	4920267	14.32%	1.157%
39	14.710	1986	1993	2001	rVV2	3596504	6334900	18.44%	1.490%
40	14.957	2025	2035	2051	rBV	1598853	2519773	7.33%	0.592%
41	15.140	2061	2066	2072	rVB	2047815	2800153	8.15%	0.658%
42	15.316	2088	2096	2100	rVV	2049348	3397285	9.89%	0.799%
43	15.375	2100	2106	2111	rVV2	4162330	8458171	24.62%	1.989%
44	15.428	2111	2115	2119	rVV	859786	1342259	3.91%	0.316%
45	15.492	2119	2126	2130	rVV2	961031	2026628	5.90%	0.477%
46	15.592	2137	2143	2147	rVV	2738889	3825906	11.14%	0.900%
47	16.281	2254	2260	2265	rBV	1828939	2658195	7.74%	0.625%
48	16.398	2269	2280	2285	rBV	2045904	3044028	8.86%	0.716%
49	16.569	2302	2309	2313	rVV	1474367	1906795	5.55%	0.448%
50	16.769	2337	2343	2351	rBV2	1439297	2751784	8.01%	0.647%
51	16.922	2364	2369	2381	rVV	1023948	1859209	5.41%	0.437%
52	17.110	2395	2401	2404	rBV	2026926	3021838	8.80%	0.711%
53	17.163	2404	2410	2415	rVV	17036136	28375838	82.59%	6.672%
54	17.222	2415	2420	2422	rVV	2390354	3816412	11.11%	0.897%
55	17.257	2422	2426	2433	rVV	6132731	9758673	28.40%	2.295%
56	17.545	2465	2475	2483	rBV	4285347	6985673	20.33%	1.643%
57	18.016	2546	2555	2558	rBV	2088786	3227405	9.39%	0.759%
58	18.063	2558	2563	2567	rVV	2853680	5067355	14.75%	1.191%
59	18.104	2567	2570	2574	rVV	2551453	3285065	9.56%	0.772%
60	18.151	2574	2578	2584	rVB	755159	1132721	3.30%	0.266%
61	18.222	2584	2590	2594	rBV2	2778153	5186851	15.10%	1.220%
62	18.263	2594	2597	2603	rVB	1205931	1925396	5.60%	0.453%
63	18.539	2639	2644	2650	rVB	1364333	2093698	6.09%	0.492%
64	18.604	2650	2655	2661	rBV	1788916	2602910	7.58%	0.612%
65	18.975	2713	2718	2723	rBV	745983	1444082	4.20%	0.340%
66	19.139	2739	2746	2751	rBV2	969894	1784467	5.19%	0.420%
67	19.263	2759	2767	2773	rVB	21110851	34356015	100.00%	8.078%
68	19.604	2820	2825	2827	rBV2	6386801	9437286	27.47%	2.219%
69	19.639	2827	2831	2838	rVV	14777899	23843004	69.40%	5.606%
70	19.704	2838	2842	2848	rVB2	915287	1643416	4.78%	0.386%
71	19.828	2858	2863	2868	rBV	1199044	1786060	5.20%	0.420%
72	19.898	2871	2875	2880	rVV	742721	1136473	3.31%	0.267%
73	19.969	2881	2887	2897	rVV3	1468936	3506540	10.21%	0.824%
74	20.157	2915	2919	2923	rVB2	2959874	4234031	12.32%	0.996%
75	20.257	2932	2936	2940	rBV2	2552001	3420995	9.96%	0.804%
76	20.316	2940	2946	2950	rBV3	1769877	3191930	9.29%	0.751%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
 Data File : BP021088.D
 Acq On : 22 Jul 2024 14:47
 Operator : MA/JU
 Sample : P3238-02MS
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MS

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

77	20.516	2976	2980	2984	rVV	1039767	1410648	4.11%	0.332%
78	20.575	2986	2990	2994	rVB	2968285	3235535	9.42%	0.761%
79	20.951	3050	3054	3061	rVB	1696712	2509448	7.30%	0.590%
80	21.127	3080	3084	3088	rBV	1972259	3206112	9.33%	0.754%
81	21.169	3088	3091	3095	rVV	1732452	2861909	8.33%	0.673%
82	21.216	3095	3099	3107	rVV3	1572640	4180479	12.17%	0.983%
83	21.298	3109	3113	3120	rVB	1396212	2393055	6.97%	0.563%
84	21.457	3136	3140	3146	rBV2	3630282	5117750	14.90%	1.203%
85	21.557	3149	3157	3163	rVV2	10722970	27235353	79.27%	6.404%
86	21.622	3163	3168	3179	rVB	12516185	19887396	57.89%	4.676%
87	21.769	3188	3193	3198	rBV	1390111	2572235	7.49%	0.605%
88	22.316	3282	3286	3292	rVB	1051900	1709643	4.98%	0.402%
89	22.392	3295	3299	3302	rVV	1058660	1654032	4.81%	0.389%
90	22.421	3302	3304	3310	rVB3	690624	1236747	3.60%	0.291%
91	22.598	3330	3334	3338	rBV4	862494	1530885	4.46%	0.360%
92	22.704	3347	3352	3361	rVV	2076441	4234608	12.33%	0.996%
93	22.792	3362	3367	3373	rVB	1906410	3355517	9.77%	0.789%
94	23.839	3537	3545	3546	rBV	6628886	10781248	31.38%	2.535%
95	23.904	3552	3556	3562	rVB	4961213	10230900	29.78%	2.406%
96	24.580	3666	3671	3677	rBV	1049640	2656035	7.73%	0.625%
97	24.645	3680	3682	3688	rVV2	1054644	2399639	6.98%	0.564%
98	24.727	3689	3696	3706	rVB	3922077	10627698	30.93%	2.499%
99	24.880	3716	3722	3727	rVB2	908110	1973846	5.75%	0.464%
100	28.686	4358	4369	4370	rBV2	1979203	4664658	13.58%	1.097%




Sum of corrected areas: 425293817

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
Data File : BP021088.D
Acq On : 22 Jul 2024 14:47
Operator : MA/JU
Sample : P3238-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE6MS

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

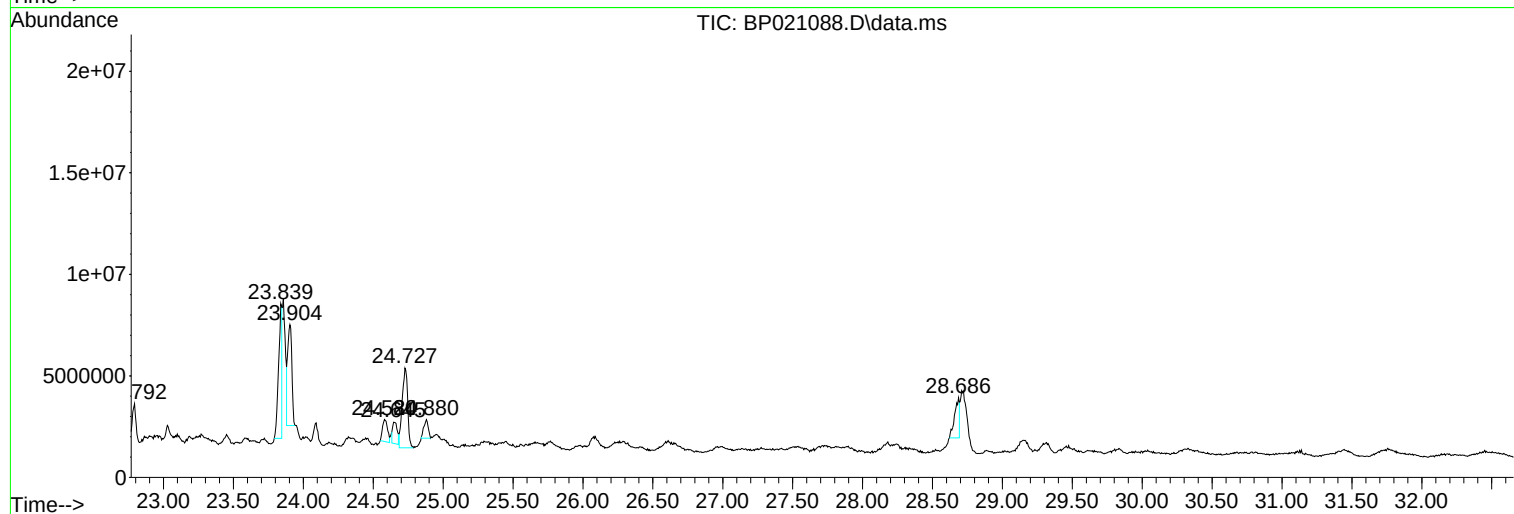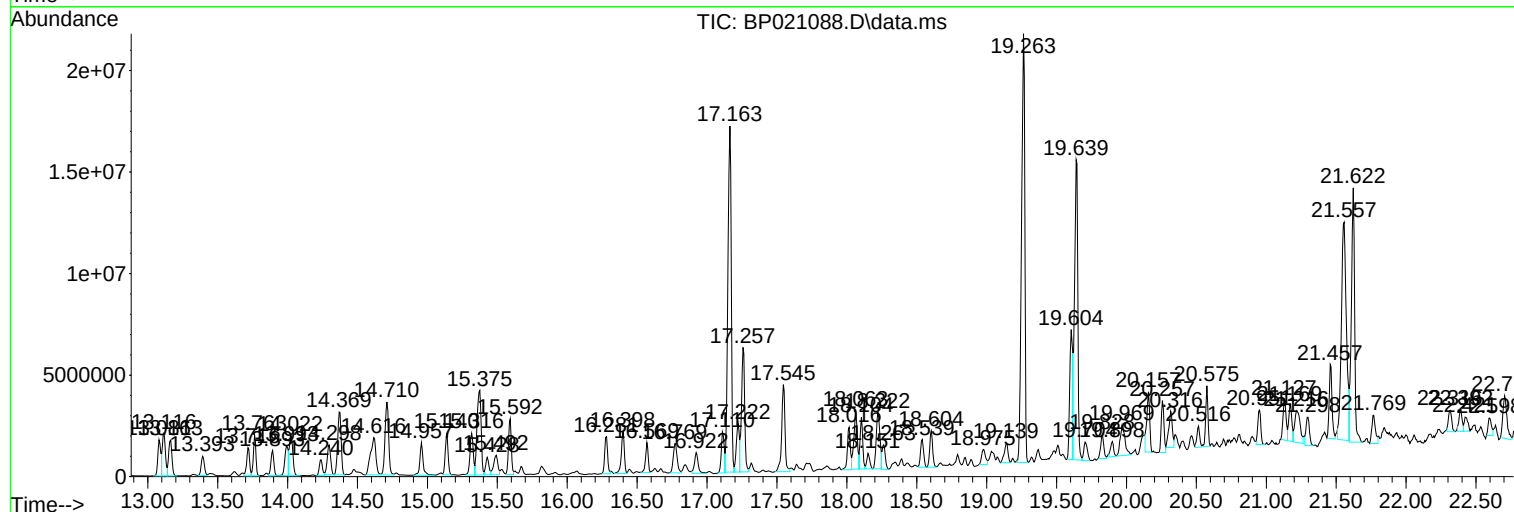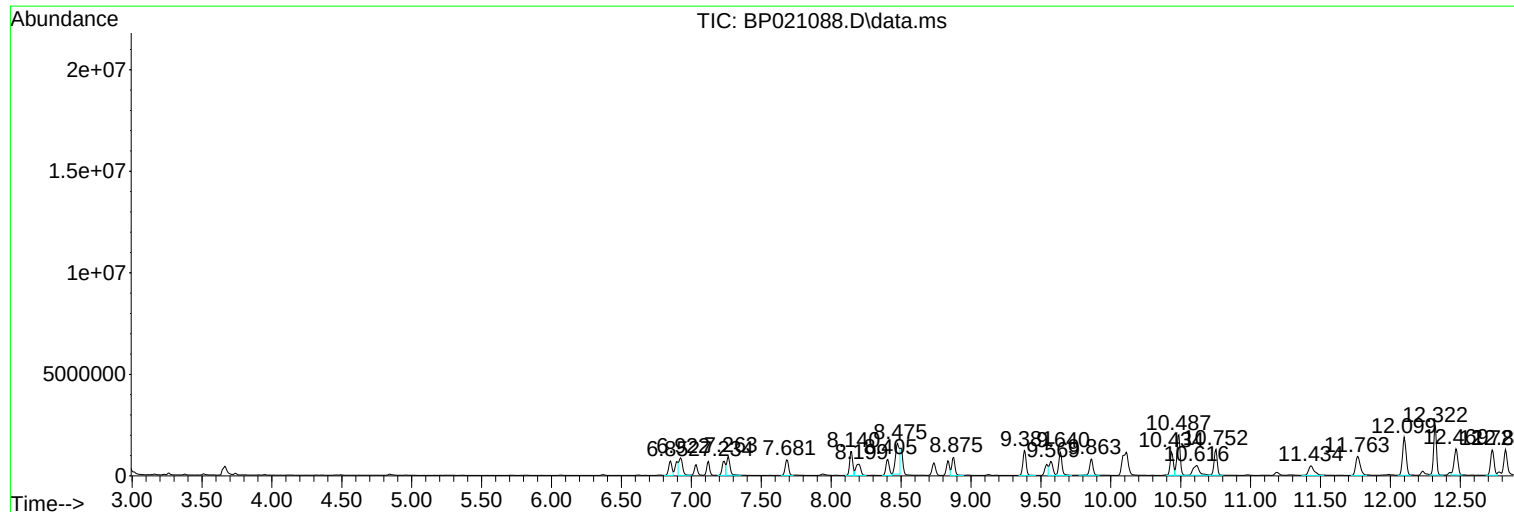

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
Data File : BP021088.D
Acq On : 22 Jul 2024 14:47
Operator : MA/JU
Sample : P3238-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE6MS

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072224\
Data File : BP021088.D
Acq On : 22 Jul 2024 14:47
Operator : MA/JU
Sample : P3238-02MS
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BE6MS

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc