

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
 Data File : BP025213.D
 Acq On : 22 Jul 2025 13:55
 Operator : CG/JU
 Sample : Q2639-11
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-43-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.661	288	293	304	rVB	834190	1229426	5.07%	0.532%
2	5.108	362	369	387	rBV	8985872	14315849	59.02%	6.201%
3	6.643	622	630	643	rBV	9329908	14793382	60.99%	6.407%
4	7.431	757	764	776	rBV	3128743	4754112	19.60%	2.059%
5	8.561	946	956	964	rBV	6160742	10077920	41.55%	4.365%
6	10.178	1223	1231	1244	rVB	3915896	6438803	26.54%	2.789%
7	10.313	1244	1254	1262	rBV	410947	715640	2.95%	0.310%
8	11.507	1449	1457	1467	rBV	158070	378646	1.56%	0.164%
9	12.684	1649	1657	1663	rBV	14442099	21881935	90.21%	9.478%
10	13.484	1789	1793	1800	rBV	172894	266089	1.10%	0.115%
11	14.072	1887	1893	1902	rBV	5104920	8187155	33.75%	3.546%
12	14.937	2035	2040	2047	rBV2	147407	248565	1.02%	0.108%
13	15.478	2126	2132	2140	rVB	605117	1056082	4.35%	0.457%
14	15.601	2147	2153	2161	rBV	11364270	17334796	71.46%	7.508%
15	16.113	2234	2240	2248	rBV2	481006	902315	3.72%	0.391%
16	16.319	2271	2275	2282	rVB2	194074	291366	1.20%	0.126%
17	16.831	2358	2362	2365	rBV	497719	661063	2.73%	0.286%
18	16.884	2365	2371	2377	rVB2	5309976	8792822	36.25%	3.808%
19	16.990	2385	2389	2393	rBV	378531	571424	2.36%	0.247%
20	17.031	2393	2396	2402	rVB	442262	655615	2.70%	0.284%
21	17.590	2488	2491	2494	rBV2	244584	346063	1.43%	0.150%
22	17.784	2521	2524	2526	rBV2	202706	273201	1.13%	0.118%
23	17.813	2526	2529	2534	rVB2	362645	451672	1.86%	0.196%
24	17.872	2534	2539	2547	rBV	4812110	6751709	27.83%	2.924%
25	18.154	2583	2587	2590	rBV	959212	1223351	5.04%	0.530%
26	18.954	2718	2723	2727	rBV	593898	893785	3.68%	0.387%
27	19.036	2734	2737	2740	rBV	404800	492147	2.03%	0.213%
28	19.089	2743	2746	2748	rBV3	387423	526473	2.17%	0.228%
29	19.231	2766	2770	2776	rVB2	733583	1172835	4.84%	0.508%
30	19.413	2798	2801	2805	rBV	369947	431426	1.78%	0.187%
31	19.466	2806	2810	2815	rBV	630516	924681	3.81%	0.401%
32	19.666	2838	2844	2849	rBV	17808098	24256447	100.00%	10.506%
33	20.007	2899	2902	2905	rBV3	332059	405840	1.67%	0.176%
34	20.148	2923	2926	2930	rBV	400741	618809	2.55%	0.268%
35	20.348	2956	2960	2962	rBV	846884	1045154	4.31%	0.453%
36	20.519	2986	2989	2994	rVB	1388796	1515907	6.25%	0.657%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025213.D
Acq On : 22 Jul 2025 13:55
Operator : CG/JU
Sample : Q2639-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-43-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	20.966	3062	3065	3075	rVB7	2165306	4354348	17.95%	1.886%
38	21.060	3077	3081	3089	rVB2	2385952	3475691	14.33%	1.505%
39	21.325	3118	3126	3139	rVB	7566802	16945256	69.86%	7.339%
40	21.483	3149	3153	3156	rBV	1605710	1818557	7.50%	0.788%
41	22.242	3278	3282	3294	rVB2	2293820	4574669	18.86%	1.981%
42	23.730	3530	3535	3544	rBV	3763389	8037513	33.14%	3.481%
43	24.466	3653	3660	3668	rVB	4172281	9830432	40.53%	4.258%
44	25.471	3824	3831	3842	rBV2	2563228	7072713	29.16%	3.063%
45	25.836	3885	3893	3904	rVB	3571929	10536287	43.44%	4.564%
46	29.724	4544	4554	4560	rBV3	2540516	9353609	38.56%	4.051%


Sum of corrected areas: 230881580

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025213.D
Acq On : 22 Jul 2025 13:55
Operator : CG/JU
Sample : Q2639-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-43-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

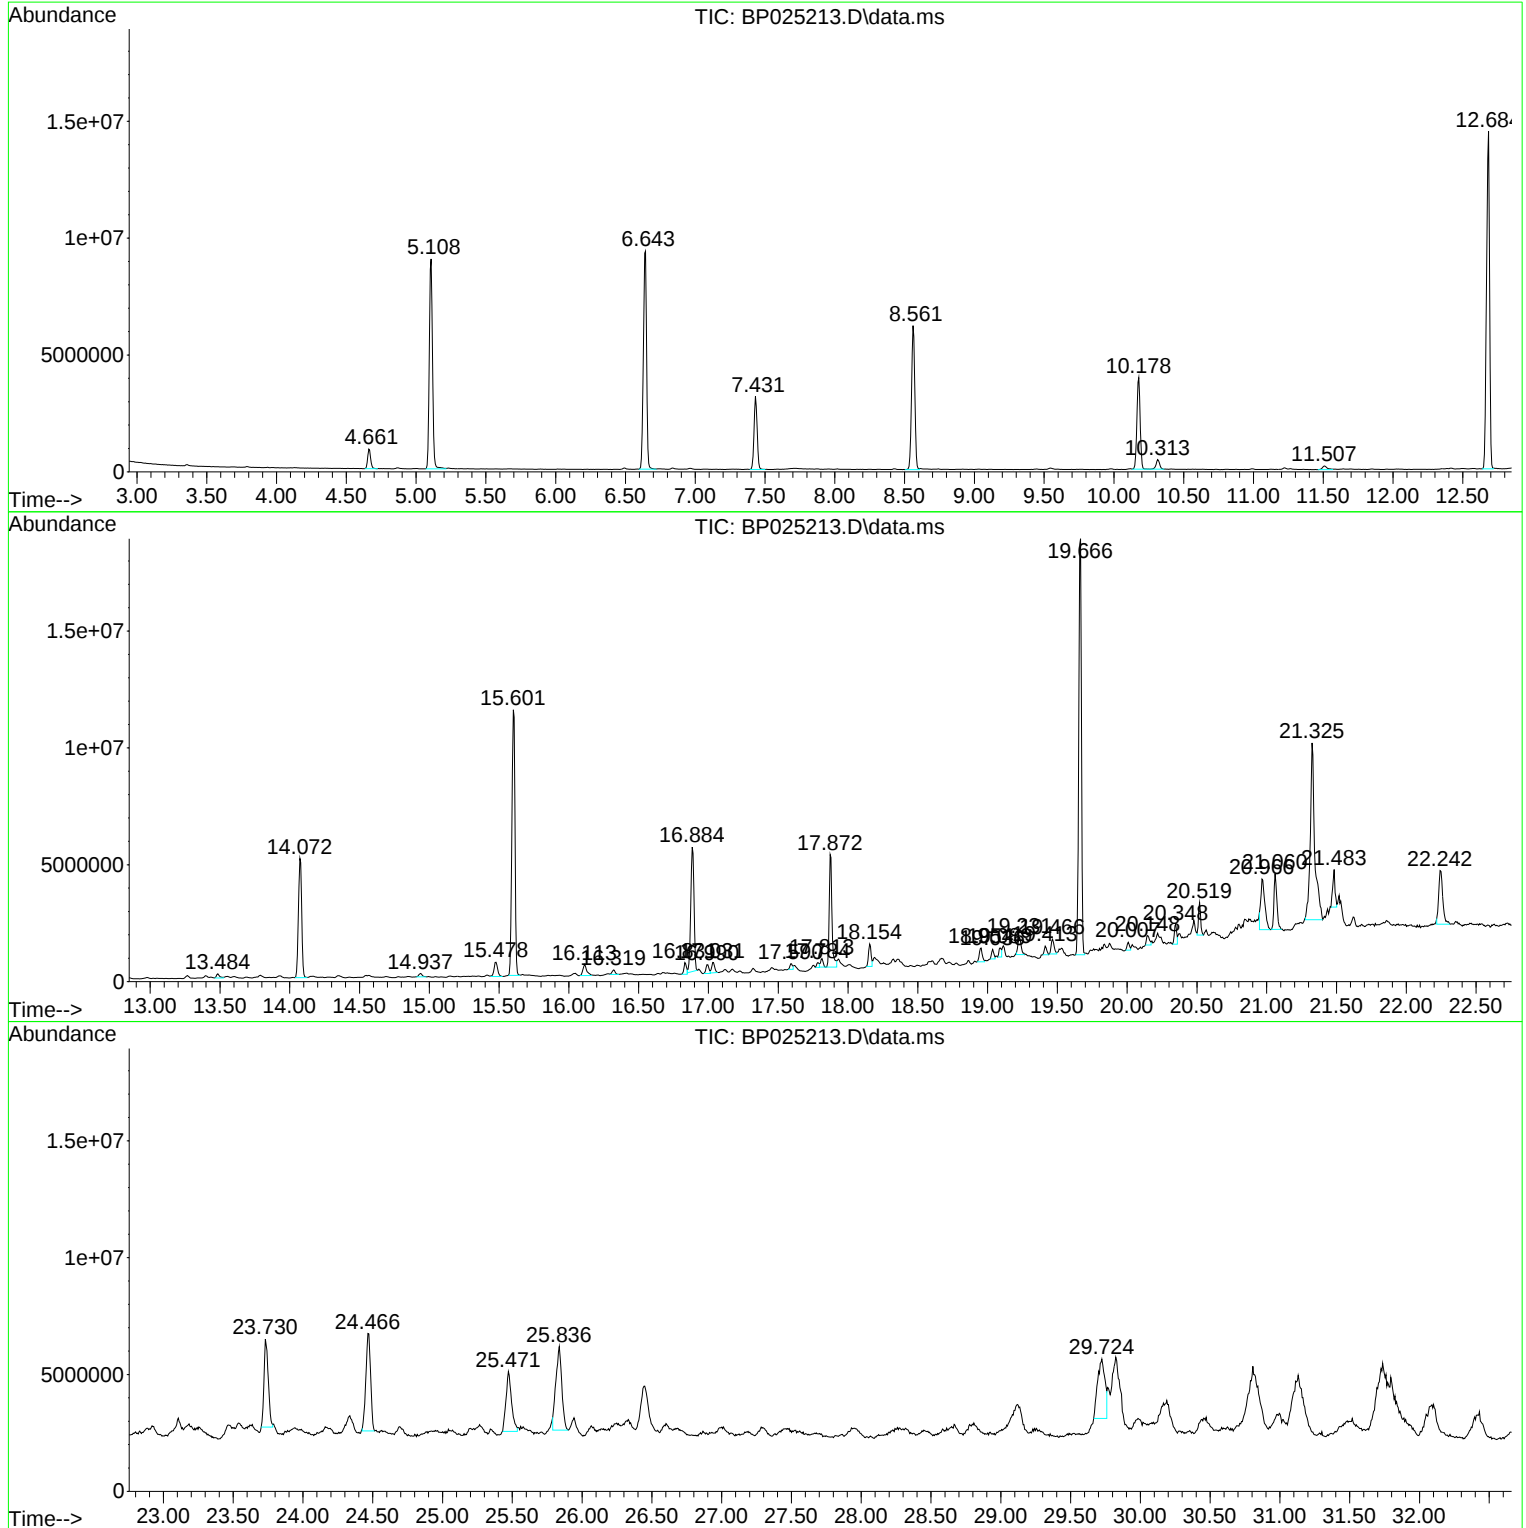

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025213.D
Acq On : 22 Jul 2025 13:55
Operator : CG/JU
Sample : Q2639-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-43-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072225\
Data File : BP025213.D
Acq On : 22 Jul 2025 13:55
Operator : CG/JU
Sample : Q2639-11
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-43-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------