

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
 Data File : BP006284.D
 Acq On : 23 Jul 2021 12:16
 Operator : CG/JU
 Sample : PB137674BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137674BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006284.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	385	392	405	rBV	6126744	8976313	49.69%	10.929%
2	6.975	652	661	670	rBV	5738818	9055823	50.13%	11.025%
3	7.793	792	800	810	rBV	1199186	1916860	10.61%	2.334%
4	8.952	987	997	1007	rBV	3475882	5573500	30.86%	6.786%
5	10.581	1267	1274	1283	rVB	1671000	2741549	15.18%	3.338%
6	13.052	1686	1694	1703	rBV	8388785	12054649	66.74%	14.676%
7	14.422	1920	1927	1934	rBV	2427322	3434047	19.01%	4.181%
8	15.916	2174	2181	2200	rVB	5244699	7581329	41.97%	9.230%
9	17.175	2387	2395	2407	rBV	2918295	4051721	22.43%	4.933%
10	19.751	2827	2833	2838	rBV	15613828	18063024	100.00%	21.992%
11	21.269	3086	3091	3097	rBV	3387041	4372311	24.21%	5.323%
12	23.627	3485	3492	3500	rVB2	2186751	4314807	23.89%	5.253%




Sum of corrected areas: 82135933

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006284.D
Acq On : 23 Jul 2021 12:16
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

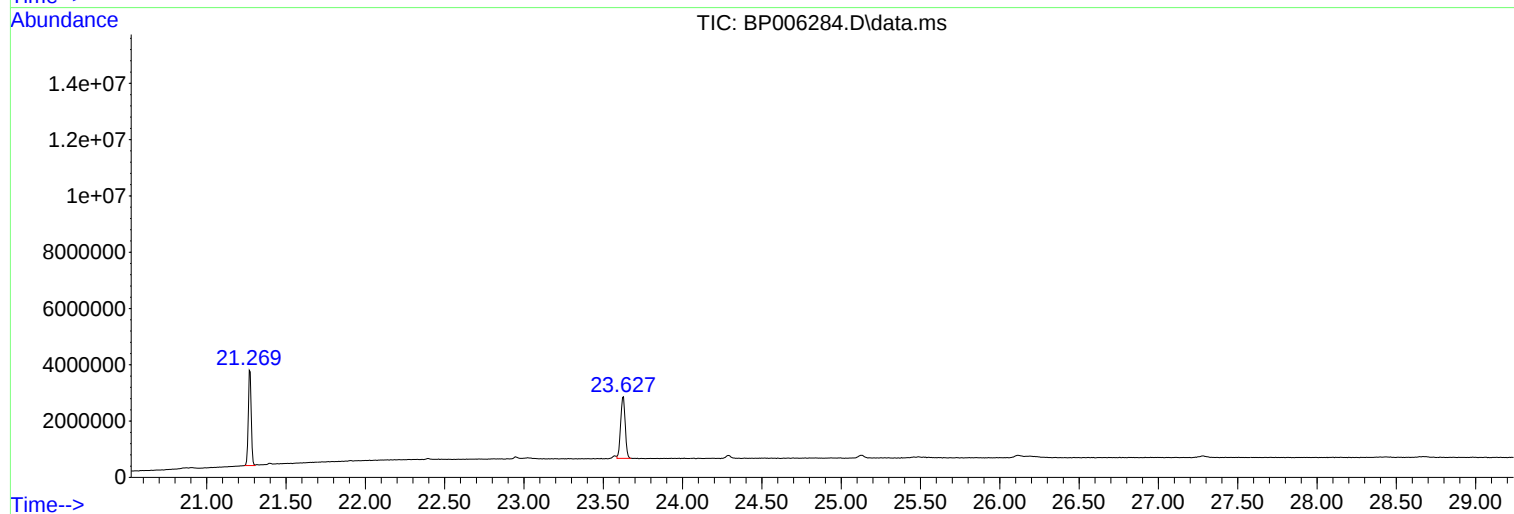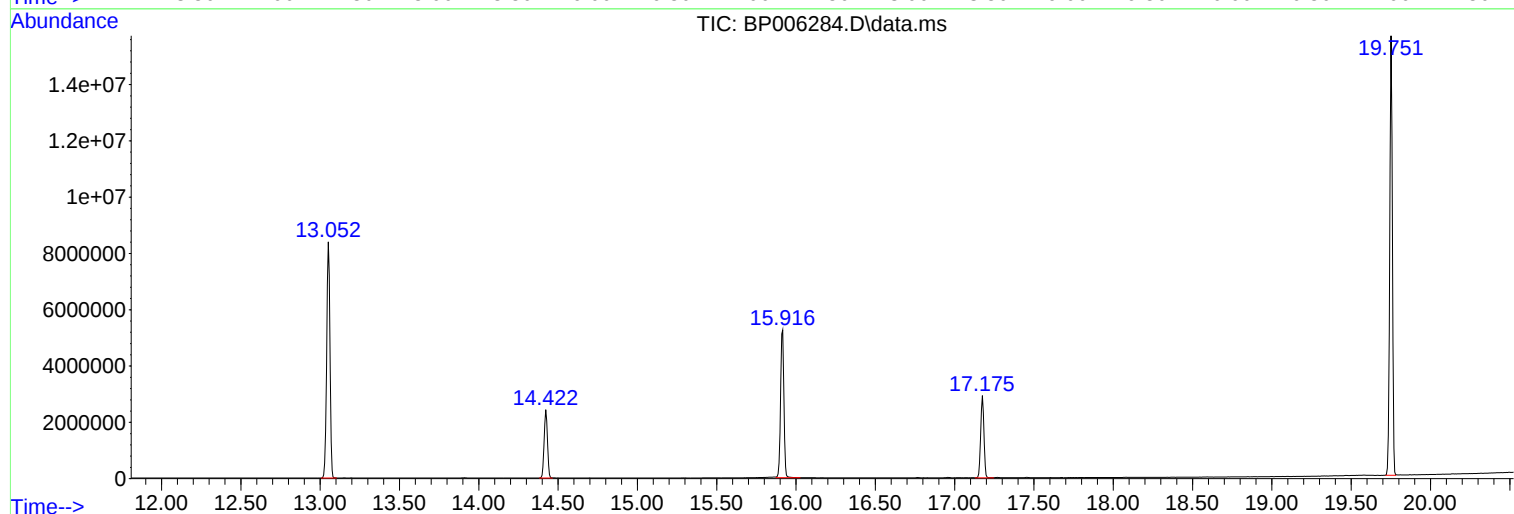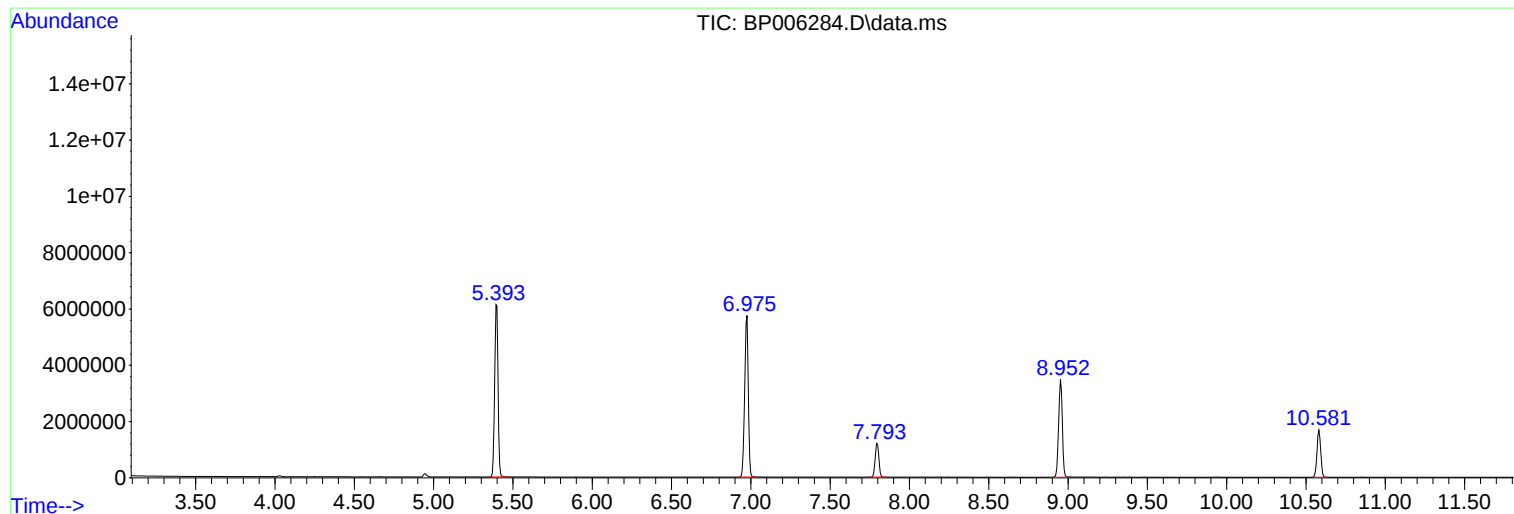

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006284.D
Acq On : 23 Jul 2021 12:16
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006284.D
Acq On : 23 Jul 2021 12:16
Operator : CG/JU
Sample : PB137674BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137674BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------