

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
 Data File : BP006286.D
 Acq On : 23 Jul 2021 13:29
 Operator : CG/JU
 Sample : PB137690BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137690BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006286.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	385	392	403	rBV	6066787	8697301	54.23%	11.359%
2	6.969	651	660	674	rBV	5655126	8864992	55.27%	11.578%
3	7.793	793	800	808	rVB	1200160	1847581	11.52%	2.413%
4	8.951	987	997	1006	rBV	3477354	5480294	34.17%	7.157%
5	10.581	1265	1274	1282	rBV	1657359	2684844	16.74%	3.506%
6	13.051	1686	1694	1707	rBV	8395991	11915957	74.29%	15.562%
7	14.422	1919	1927	1936	rBV	2317989	3369106	21.01%	4.400%
8	15.916	2174	2181	2201	rVB	4457290	6100210	38.03%	7.967%
9	17.175	2389	2395	2405	rVB	2734465	3820894	23.82%	4.990%
10	19.757	2828	2834	2839	rBV	13158131	16039036	100.00%	20.947%
11	21.274	3087	3092	3098	rBV	3236277	3886201	24.23%	5.075%
12	23.627	3486	3492	3501	rVB2	1968755	3864036	24.09%	5.046%




Sum of corrected areas: 76570452

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006286.D
Acq On : 23 Jul 2021 13:29
Operator : CG/JU
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

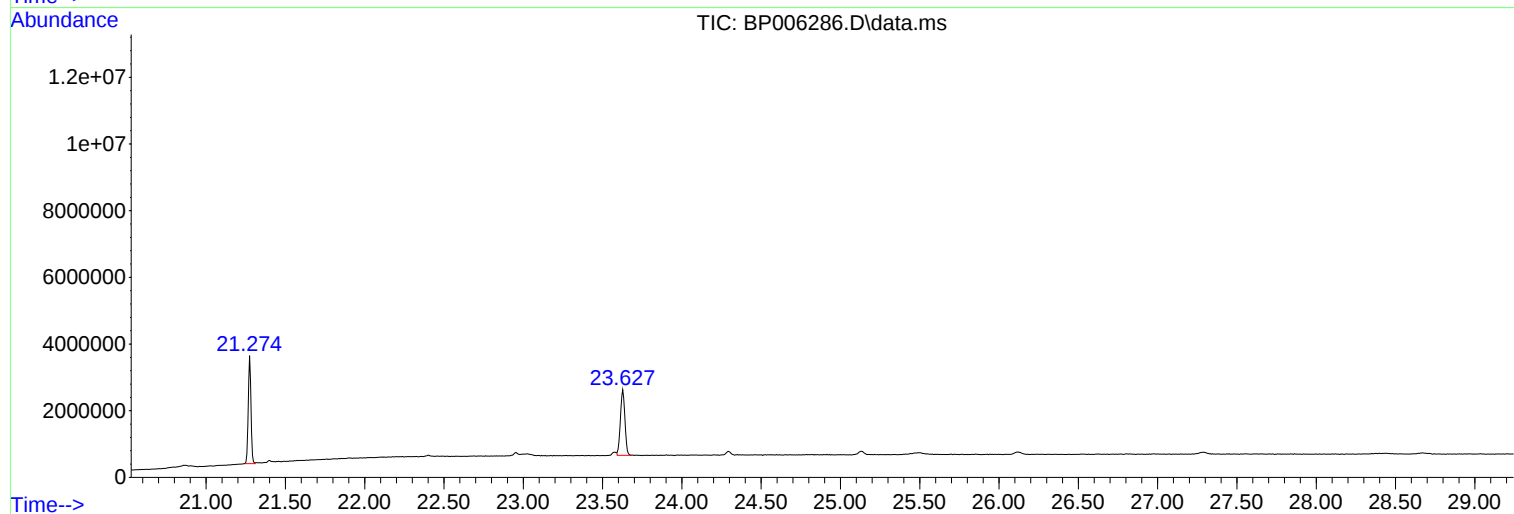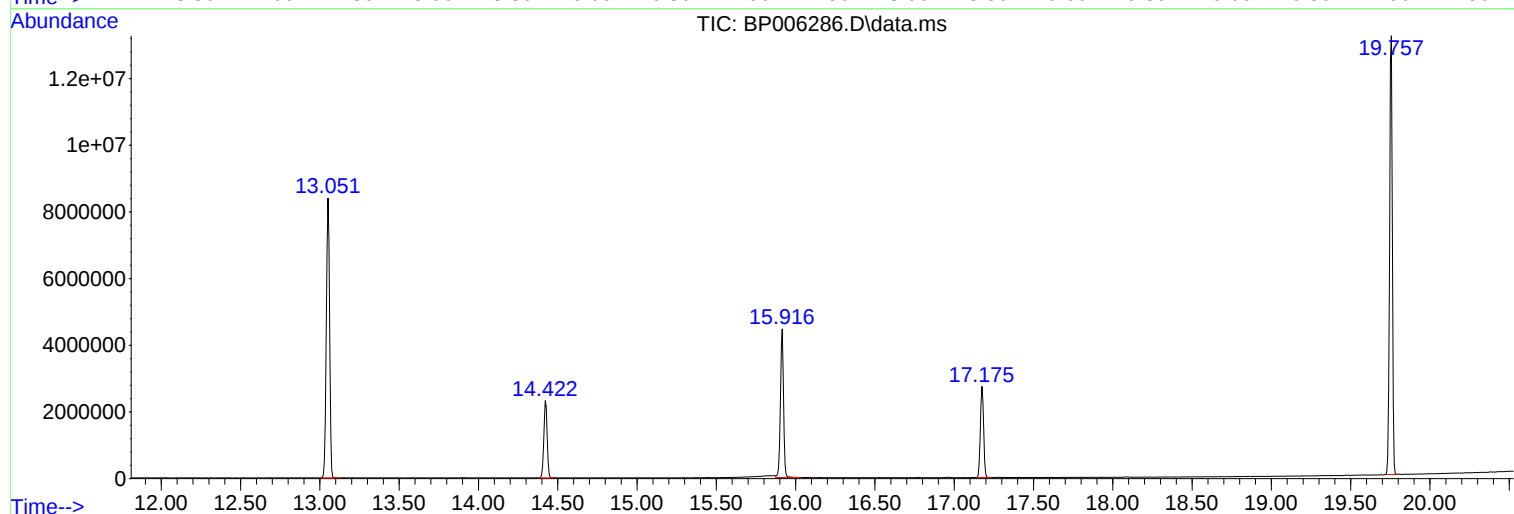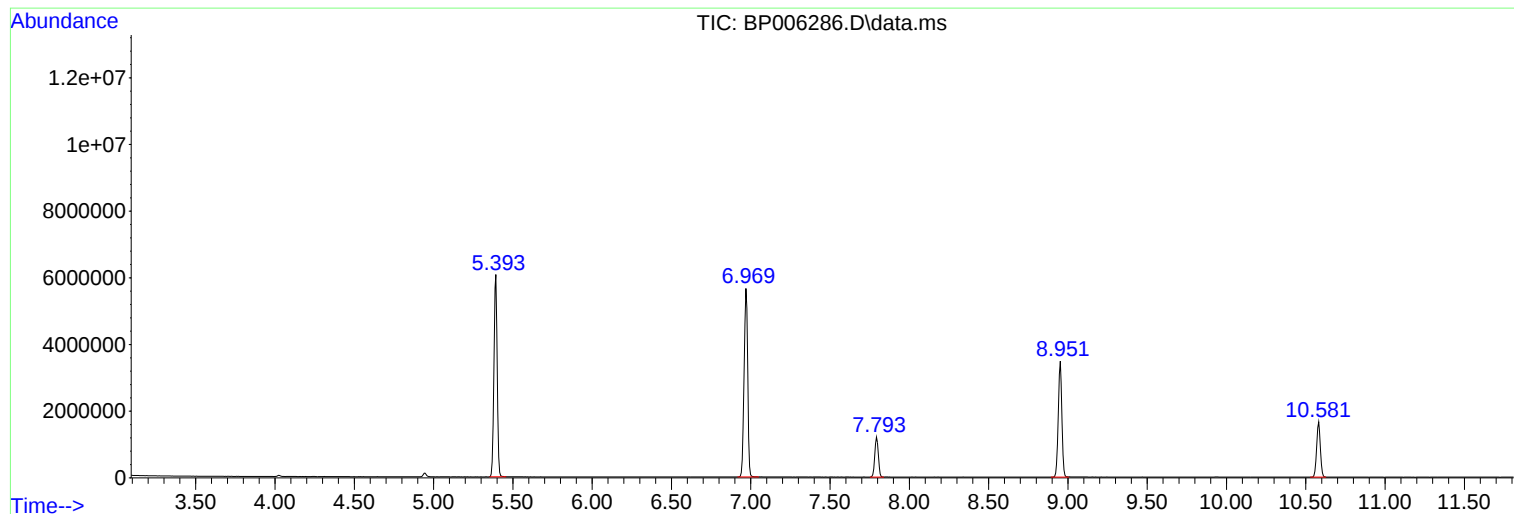

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006286.D
Acq On : 23 Jul 2021 13:29
Operator : CG/JU
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
Data File : BP006286.D
Acq On : 23 Jul 2021 13:29
Operator : CG/JU
Sample : PB137690BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137690BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------