
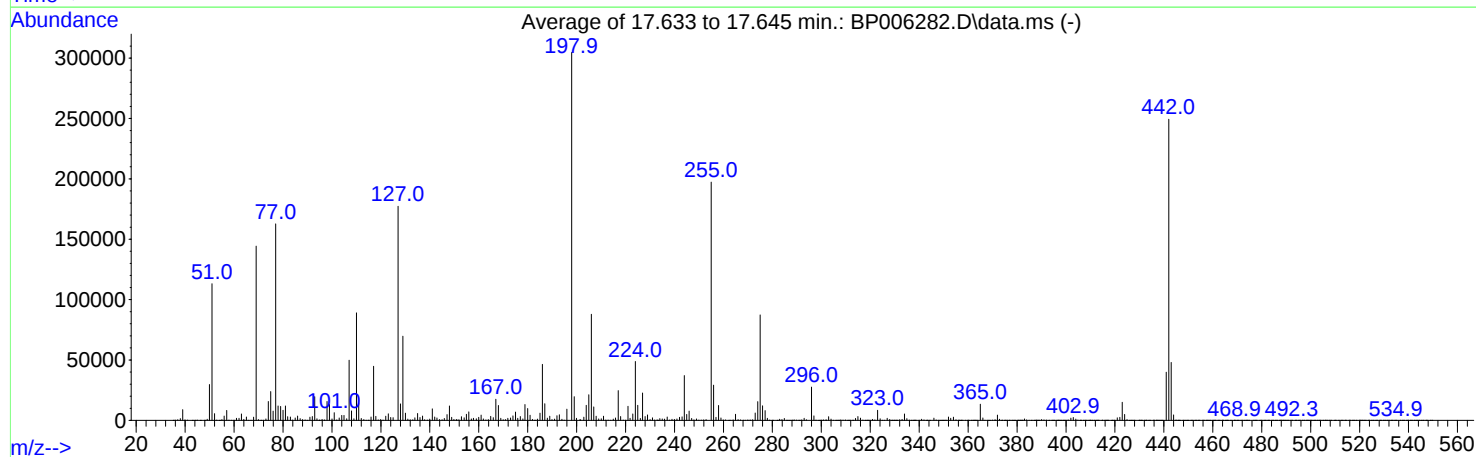


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
 Data File : BP006282.D
 Acq On : 23 Jul 2021 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 22 14:48:03 2021

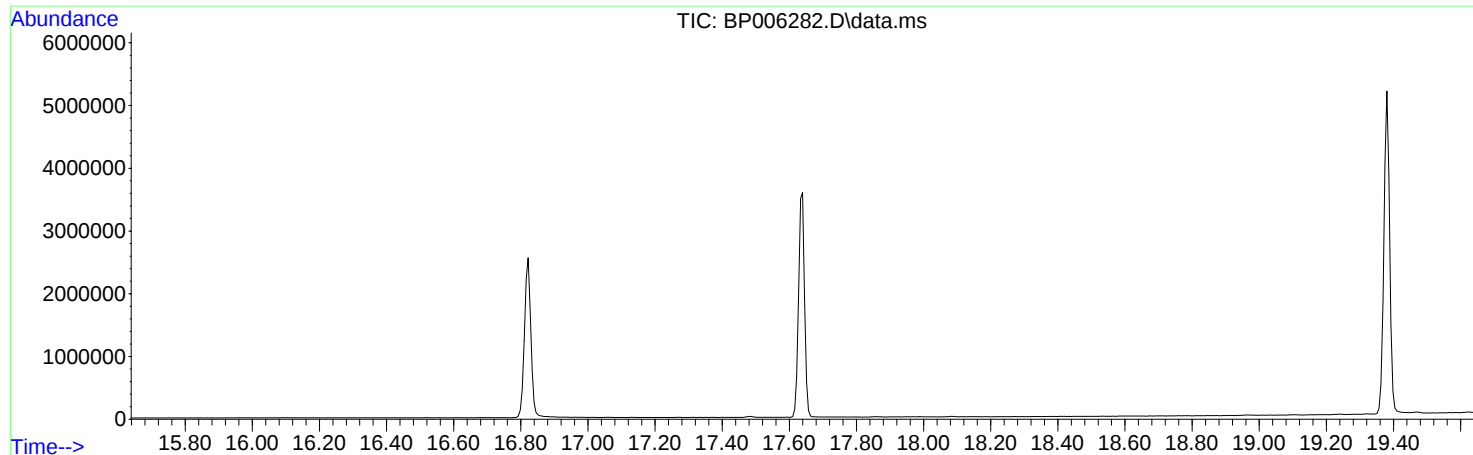




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	113186	PASS
68	69	0.00	2	1.8	2661	PASS
69	198	0.00	100	47.4	144263	PASS
70	69	0.00	2	0.5	704	PASS
127	198	10	80	58.2	177288	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	304640	PASS
199	198	5	9	6.4	19626	PASS
275	198	10	60	28.7	87363	PASS
365	198	1	100	4.4	13412	PASS
441	198	0.01	100	13.1	39831	PASS
442	442	100	100	100.0	249429	PASS
443	442	15	24	19.2	47960	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
 Data File : BP006282.D
 Acq On : 23 Jul 2021 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 23 12:30:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 14:48:03 2021
 Response via : Initial Calibration

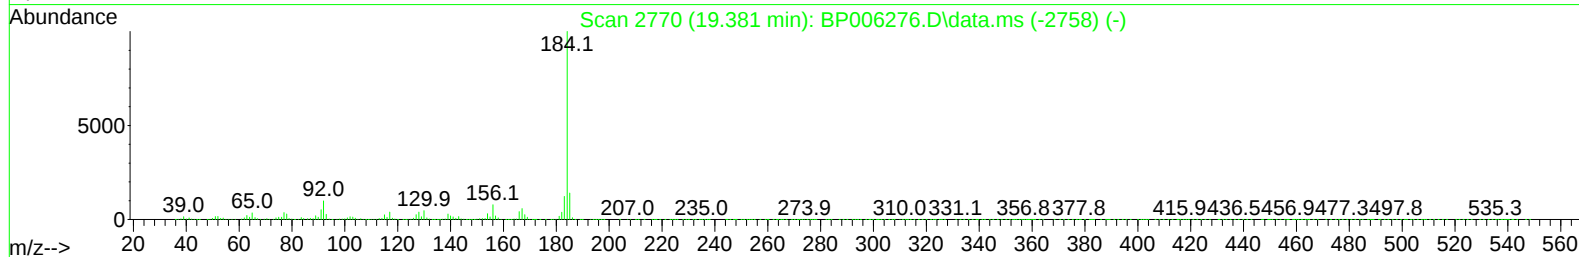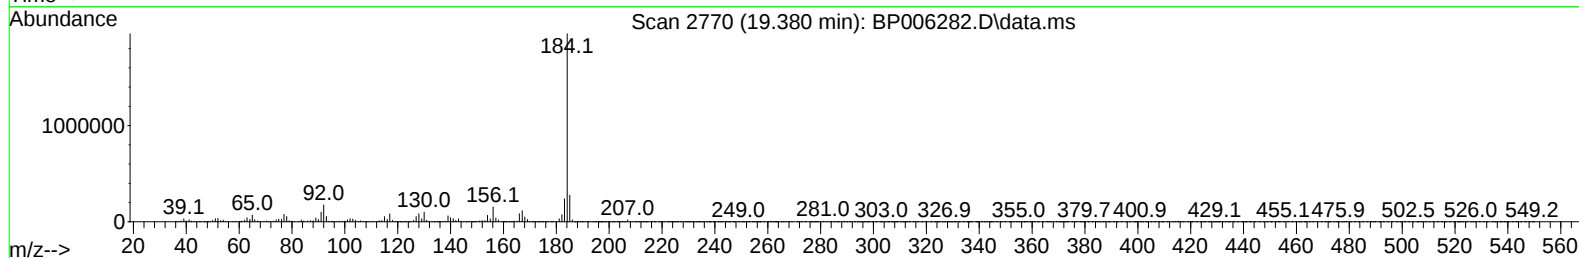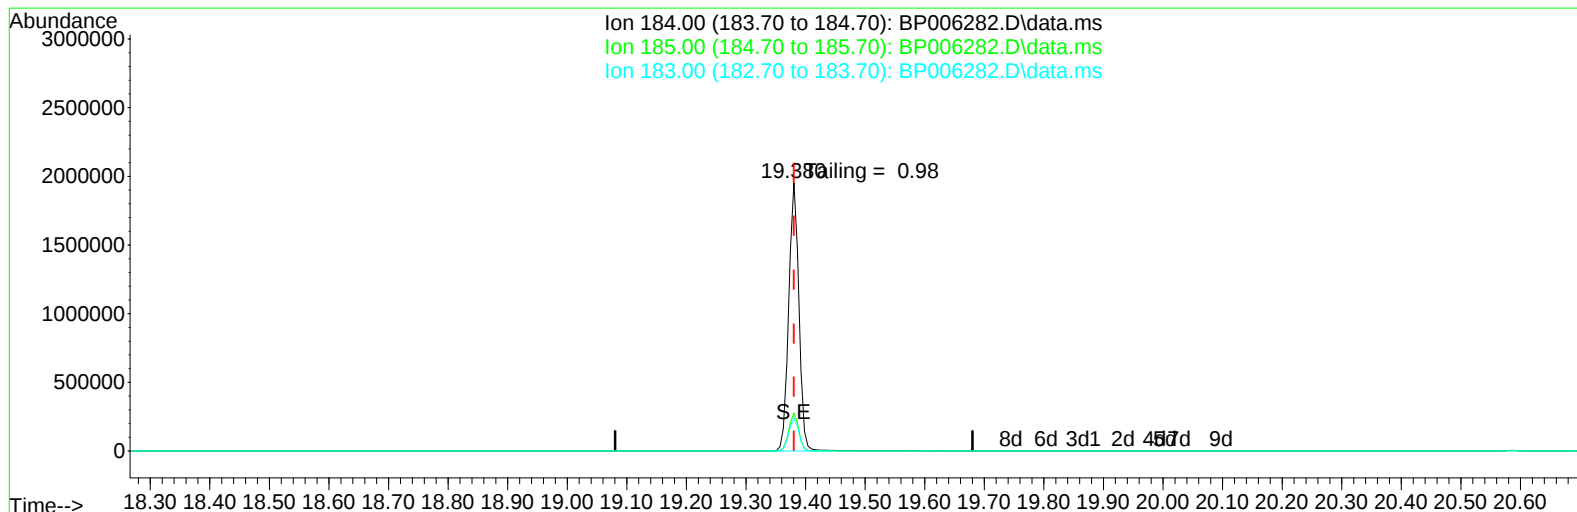

TIC: BP006282.D\data.ms

(77) Benzidine

19.380min (-0.000) 8035079.83 ng m




response 2306990

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.09
183.00	11.90	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072321\
 Data File : BP006282.D
 Acq On : 23 Jul 2021 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 23 12:30:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 22 14:48:03 2021
 Response via : Initial Calibration

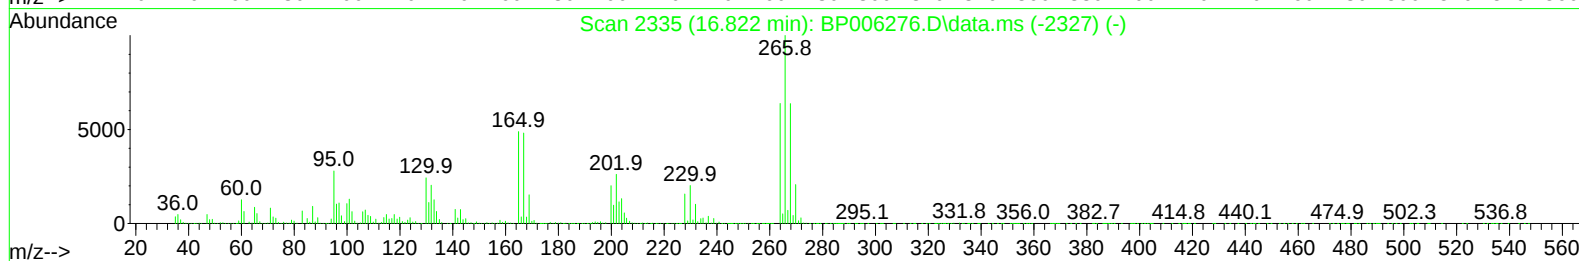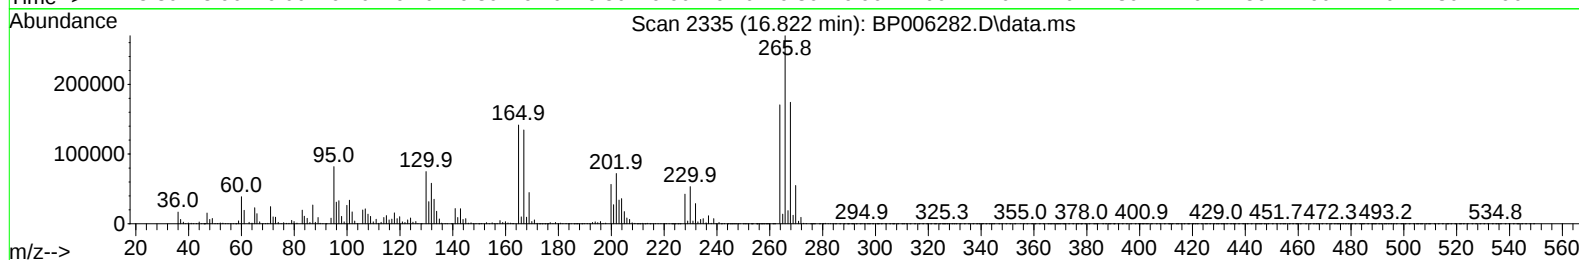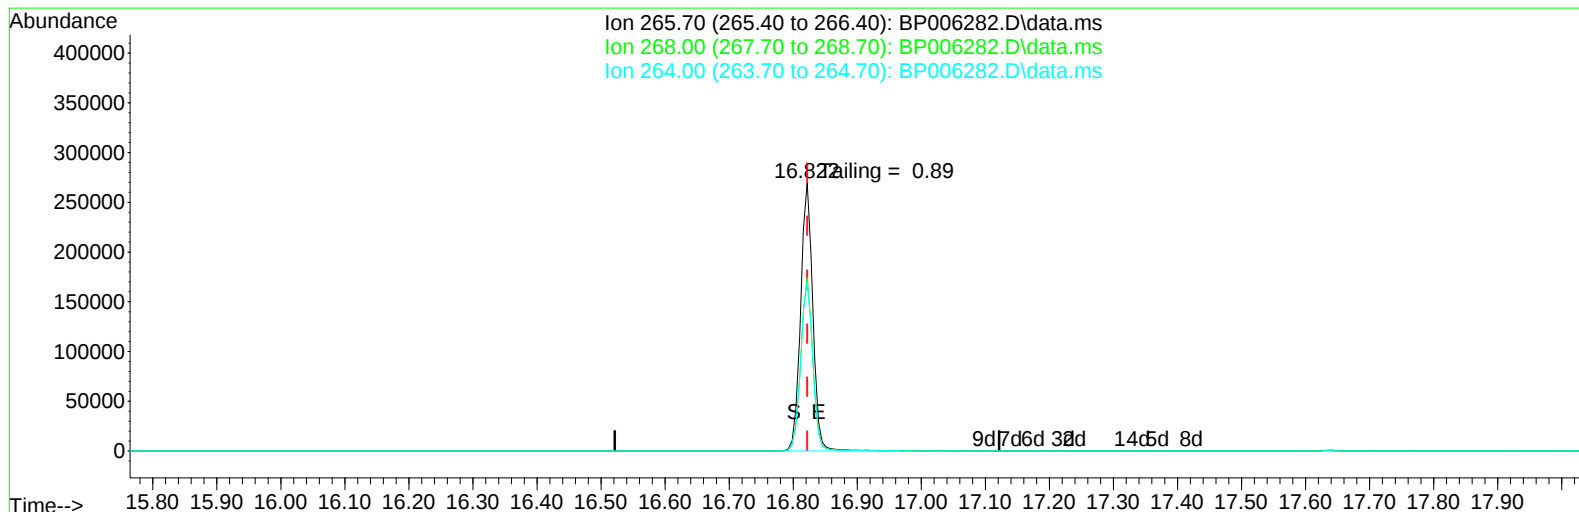

TIC: BP006282.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.000) 19742.50 ng m

response 358559

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	64.58
264.00	62.90	63.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/23/2021	BNA_P	BP006282.D
Compound Name	Response	Retention Time
DDT	1115249	20.58
DDD	6193	20.15
DDE	1439	19.65
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7632	1122881	0.68

Instrument :
BNA_P
ClientSampleId :
DFTPP