

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
 Data File : BP021108.D
 Acq On : 23 Jul 2024 21:32
 Operator : MA/JU
 Sample : P3238-03MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MSD

Quant Time: Jul 24 05:33:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 24 00:21:57 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
 Supervised By :mohammad ahmed 07/25/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.657	152	170019	20.000	ng/u1	0.00
20) Naphthalene-d8	10.434	136	687335	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.304	164	449553	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.133	188	952639	20.000	ng/u1	0.00
79) Chrysene-d12	21.574	240	885403	20.000	ng/u1	0.00
88) Perylene-d12	24.898	264	1148794	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	13194	3.531	ng/uL	0.00
4) Pyridine-d5	3.611	84	107722	9.959	ng/u1	0.00
7) Phenol-d5	6.875	99	324200	23.389	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.010	67	182192	21.689	ng/u1	0.00
11) 2-Chlorophenol-d4	7.216	132	265702	23.265	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	253850	22.050	ng/u1	0.00
21) Nitrobenzene-d5	8.816	128	131409	24.615	ng/u1	0.00
24) 2-Nitrophenol-d4	9.534	143	152875	25.019	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.081	165	290708	26.311	ng/u1	0.00
31) 4-Chloroaniline-d4	10.587	131	179007	12.229	ng/u1	0.00
46) Dimethylphthalate-d6	13.704	166	820494	25.107	ng/u1	-0.01
49) Acenaphthylene-d8	13.992	160	928648	25.307	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.592	143	167774m	36.083	ng/u1	0.00
60) Fluorene-d10	15.322	176	721717	26.919	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.492	200	95933	16.644	ng/u1	0.01
73) Anthracene-d10	17.233	188	1127045	26.637	ng/u1	0.01
81) Pyrene-d10	19.610	212	1144025	20.900	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.680	264	992933	17.525	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.222	88	38890	9.464	ng/uL	96
5) Pyridine	3.628	79	172009	15.418	ng/u1	96
6) Benzaldehyde	6.828	77	201059	28.772	ng/u1	97
8) Phenol	6.905	94	416351	29.684	ng/u1	97
10) Bis(2-Chloroethyl)ether	7.105	93	297359	25.663	ng/u1	98
12) 2-Chlorophenol	7.240	128	329896	28.821	ng/u1	99
13) 2-Methylphenol	8.122	108	311270	28.695	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.175	45	414230	24.745	ng/u1	95
16) Acetophenone	8.487	105	497828	28.018	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.463	70	235033	25.245	ng/u1	98
18) 4-Methylphenol	8.457	108	341961	29.426	ng/u1	100
19) Hexachloroethane	8.710	117	98886	19.225	ng/u1	98
22) Nitrobenzene	8.863	77	361219	28.245	ng/u1	97
23) Isophorone	9.381	82	676160	26.595	ng/u1	100
25) 2-Nitrophenol	9.563	139	190924	29.959	ng/u1	99
26) 2,4-Dimethylphenol	9.640	107	332116	26.428	ng/u1	98
27) Bis(2-Chloroethoxy)met...	9.852	93	404025	26.144	ng/u1	99
29) 2,4-Dichlorophenol	10.104	162	335565	30.817	ng/u1	99
30) Naphthalene	10.481	128	1301334	35.994	ng/u1	99
32) 4-Chloroaniline	10.616	127	218995	15.668	ng/u1	99
33) Hexachlorobutadiene	10.746	225	227893	27.912	ng/u1	99
34) Caprolactam	11.428	113	107831	32.146	ng/u1	94
35) 4-Chloro-3-methylphenol	11.763	107	374531	31.643	ng/u1	99
36) 2-Methylnaphthalene	12.093	142	817576	32.943	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
 Data File : BP021108.D
 Acq On : 23 Jul 2024 21:32
 Operator : MA/JU
 Sample : P3238-03MSD
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MSD


Quant Time: Jul 24 05:33:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 24 00:21:57 2024
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
 Supervised By :mohammad ahmed 07/25/2024


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.316	142	812134	31.818	ng/ul	100
39) 1,2,4,5-Tetrachloroben...	12.469	216	432674	29.636	ng/ul	96
40) Hexachlorocyclopentadiene	12.428	237	35079	4.593	ng/ul	98
41) 2,4,6-Trichlorophenol	12.722	196	283362	30.716	ng/ul	98
42) 2,4,5-Trichlorophenol	12.822	196	305071	31.255	ng/ul	99
43) 1,1'-Biphenyl	13.116	154	991620	30.183	ng/ul	99
44) 2-Chloronaphthalene	13.163	162	771379	29.411	ng/ul	99
45) 2-Nitroaniline	13.393	65	233441	32.185	ng/ul	96
47) Dimethylphthalate	13.757	163	953099	28.743	ng/ul	99
48) 2,6-Dinitrotoluene	13.898	165	207999	31.375	ng/ul	98
50) Acenaphthylene	14.022	152	1310887	31.552	ng/ul	100
51) 3-Nitroaniline	14.245	138	170663	29.583	ng/ul	95
52) Acenaphthene	14.369	153	1211294	43.926	ng/ul	99
53) 2,4-Dinitrophenol	14.487	184	68073	19.553	ng/ul	97
55) 4-Nitrophenol	14.610	109	143270	37.879	ng/ul	94
56) Dibenzofuran	14.710	168	1559744	41.304	ng/ul	98
57) 2,4-Dinitrotoluene	14.704	165	306584	33.688	ng/ul#	82
58) 2,3,4,6-Tetrachlorophenol	14.963	232	255967	30.625	ng/ul	97
59) Diethylphthalate	15.145	149	970643	29.290	ng/ul	100
61) Fluorene	15.375	166	1438569	46.684	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.369	204	479350	28.667	ng/ul	96
63) 4-Nitroaniline	15.428	138	197566	41.354	ng/ul	98
66) 4,6-Dinitro-2-methylph...	15.510	198	125354	20.508	ng/ul#	94
67) N-Nitrosodiphenylamine	15.604	169	828651	29.871	ng/ul	99
68) 4-Bromophenyl-phenylether	16.292	248	324887	29.096	ng/ul	97
69) Hexachlorobenzene	16.410	284	298932	23.349	ng/ul	97
70) Atrazine	16.586	200	234744	23.218	ng/ul	98
71) Pentachlorophenol	16.792	266	180375	25.940	ng/ul	99
72) Phenanthrene	17.181	178	9809280	198.492	ng/ul	97
74) Anthracene	17.269	178	3482001	69.113	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.087	216	409174	26.835	ng/ul	99
76) Pentachlorobenzene	14.628	250	403977	26.663	ng/ul	99
77) Carbazole	17.563	167	2148891	52.177	ng/ul	99
78) Di-n-butylphthalate	18.122	149	1709475	30.085	ng/ul	100
80) Fluoranthene	19.275	202	12843107	194.281	ng/ul	99
82) Pyrene	19.651	202	9110856	135.440	ng/ul	97
83) Butylbenzylphthalate	20.580	149	802548	28.635	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.480	252	242871	12.004	ng/ul	99
85) Benzo(a)anthracene	21.557	228	7333619	118.240	ng/ul	97
86) Bis(2-ethylhexyl)phtha...	21.463	149	1342907	33.295	ng/ul	99
87) Chrysene	21.627	228	6773367	117.527	ng/ul	97
89) Di-n-octyl phthalate	22.716	149	2064517	27.204	ng/ul	100
90) Benzo(b)fluoranthene	23.868	252	8637858	123.903	ng/ul	98
91) Benzo(k)fluoranthene	23.927	252	4442037	63.847	ng/ul	97
93) Benzo(a)pyrene	24.751	252	3502056	53.159	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	28.703	276	4181070m	49.252	ng/ul	
95) Dibenzo(a,h)anthracene	28.756	278	2898524	41.232	ng/ul	97
96) Benzo(g,h,i)perylene	29.862	276	527993m	7.637	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 9.464 ng/uL
RT: 3.222 min Scan# 40
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion: 88 Resp: 38890
Ion Ratio Lower Upper
88 100
43 30.4 25.4 38.0
58 69.7 59.2 88.8


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#5
Pyridine
Concen: 15.418 ng/uL
RT: 3.628 min Scan# 109
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion: 79 Resp: 172009
Ion Ratio Lower Upper
79 100
52 77.9 64.9 97.3
51 35.7 30.5 45.7





#6
Benzaldehyde
Concen: 28.772 ng/ul
RT: 6.828 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion: 77 Resp: 201059
Ion Ratio Lower Upper
77 100
105 102.0 79.3 118.9
106 95.6 74.6 112.0


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#8
Phenol
Concen: 29.684 ng/ul
RT: 6.905 min Scan# 666
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion: 94 Resp: 416351
Ion Ratio Lower Upper
94 100
65 27.8 23.4 35.0
66 39.9 33.9 50.9

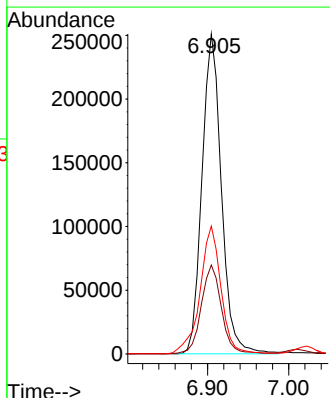



#10
Bis(2-Chloroethyl)ether
Concen: 25.663 ng/ul
RT: 7.105 min Scan# 700
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion: 93 Resp: 297359
Ion Ratio Lower Upper
93 100
63 75.8 61.5 92.3
95 32.6 25.1 37.7


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#12
2-Chlorophenol
Concen: 28.821 ng/ul
RT: 7.240 min Scan# 723
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion:128 Resp: 329896
Ion Ratio Lower Upper
128 100
64 48.5 37.9 56.9
130 32.0 25.6 38.4







#13
2-Methylphenol
Concen: 28.695 ng/ul
RT: 8.122 min Scan# 81
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

Tgt Ion:108 Resp: 311270
Ion Ratio Lower Upper
108 100
107 91.2 73.8 110.8



Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#14
2,2'-oxybis(1-Chloropropane)
Concen: 24.745 ng/ul
RT: 8.175 min Scan# 882
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion: 45 Resp: 414230
Ion Ratio Lower Upper
45 100
77 15.9 10.9 16.3
79 11.5 8.1 12.1







#16
Acetophenone
Concen: 28.018 ng/ul
RT: 8.487 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

Tgt Ion: 105 Resp: 497828
Ion Ratio Lower Upper
105 100
77 77.8 61.8 92.8
51 26.6 21.5 32.3



Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

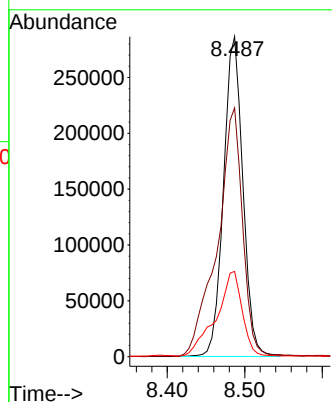




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#17
N-Nitroso-di-n-propylamine
Concen: 25.245 ng/ul
RT: 8.463 min Scan# 931
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion: 70 Resp: 235033
Ion Ratio Lower Upper
70 100
42 56.6 46.6 69.8
101 10.4 7.4 11.0
130 21.8 17.2 25.8

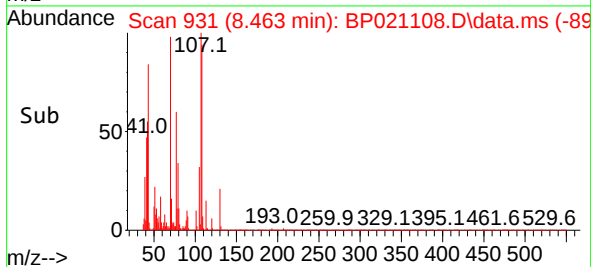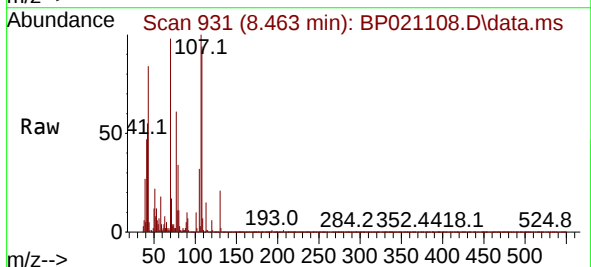



#18
4-Methylphenol
Concen: 29.426 ng/ul
RT: 8.457 min Scan# 918
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:108 Resp: 34196
Ion Ratio Lower Upper
108 100
107 109.5 87.8 131.8


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#19
Hexachloroethane
Concen: 19.225 ng/ul
RT: 8.710 min Scan# 973
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:117 Resp: 98886
Ion Ratio Lower Upper
117 100
201 112.4 88.2 132.2
199 69.1 55.8 83.6





#22
Nitrobenzene
Concen: 28.245 ng/ul
RT: 8.863 min Scan# 998
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion: 77 Resp: 361219
Ion Ratio Lower Upper
77 100
123 48.2 36.7 55.1
65 14.3 11.1 16.7


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#23
Isophorone
Concen: 26.595 ng/ul
RT: 9.381 min Scan# 1087
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion: 82 Resp: 676160
Ion Ratio Lower Upper
82 100
95 7.5 6.1 9.1
138 18.2 14.4 21.6





#25
2-Nitrophenol
Concen: 29.959 ng/ul
RT: 9.563 min Scan# 1118
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:139 Resp: 190924
Ion Ratio Lower Upper
139 100
65 52.4 42.9 64.3
109 33.1 26.2 39.4


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024




07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#26
2,4-Dimethylphenol
Concen: 26.428 ng/ul
RT: 9.640 min Scan# 1131
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Tgt Ion:107 Resp: 332116
Ion Ratio Lower Upper
107 100
121 48.1 39.6 59.4
122 81.6 66.3 99.5

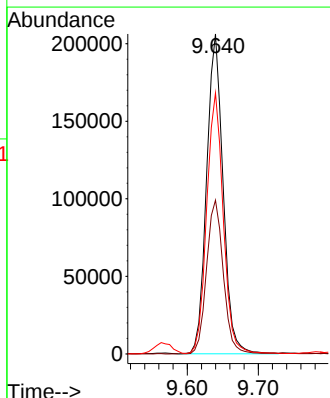





#27
Bis(2-Chloroethoxy)methane
Concen: 26.144 ng/ul
RT: 9.852 min Scan# 1167
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

Tgt Ion: 93 Resp: 404025
Ion Ratio Lower Upper
93 100
95 32.2 25.5 38.3
123 11.4 9.0 13.4



Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#29
2,4-Dichlorophenol
Concen: 30.817 ng/ul
RT: 10.104 min Scan# 1210
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:162 Resp: 335565
Ion Ratio Lower Upper
162 100
164 66.1 53.3 79.9
98 36.9 28.7 43.1





#30
Naphthalene
Concen: 35.994 ng/ul
RT: 10.481 min Scan# 1275
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:128 Resp: 1301334
Ion Ratio Lower Upper
128 100
129 11.0 8.6 13.0
127 13.1 10.8 16.2


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024




07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#32
4-Chloroaniline
Concen: 15.668 ng/ul
RT: 10.616 min Scan# 1297
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32




Tgt Ion:127 Resp: 218995
Ion Ratio Lower Upper
127 100
129 33.1 26.1 39.1

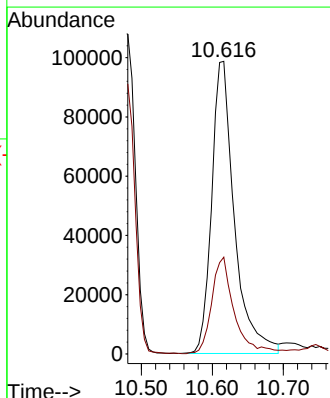

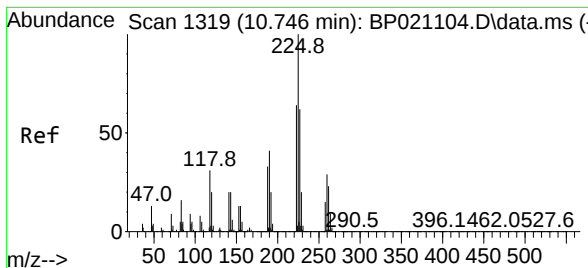

#33
Hexachlorobutadiene
Concen: 27.912 ng/ul
RT: 10.746 min Scan# 11
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

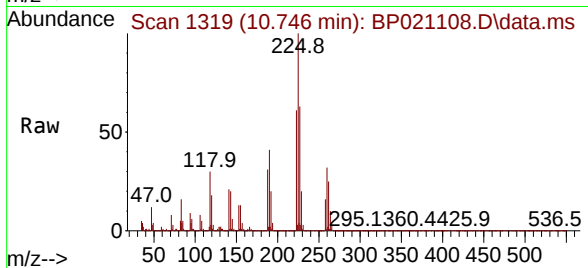

Tgt Ion:225 Resp: 22789
Ion Ratio Lower Upper
225 100
223 61.2 50.2 75.2
227 63.4 50.6 75.8


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

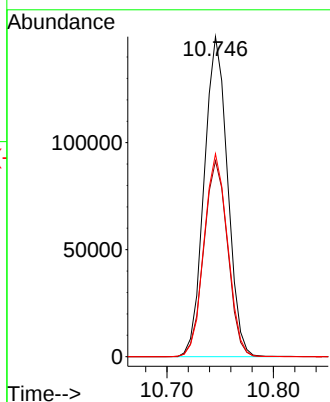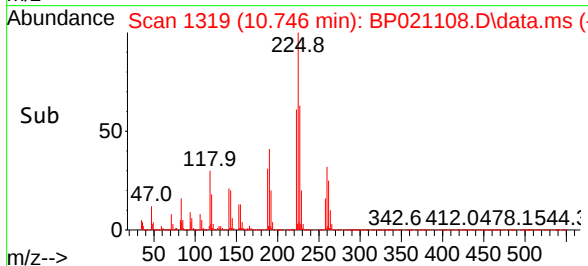




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024

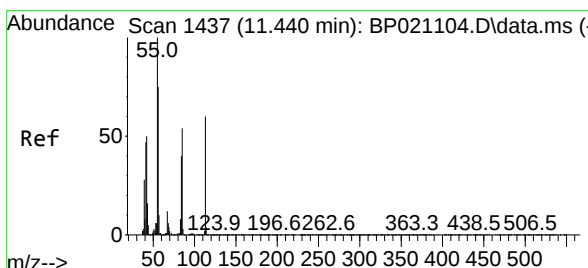

#34
Caprolactam
Concen: 32.146 ng/ul
RT: 11.428 min Scan# 1435
Delta R.T. -0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:113 Resp: 107831
Ion Ratio Lower Upper
113 100
55 165.2 140.2 210.4
56 125.7 105.5 158.3

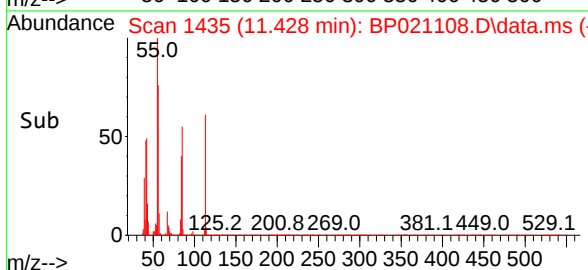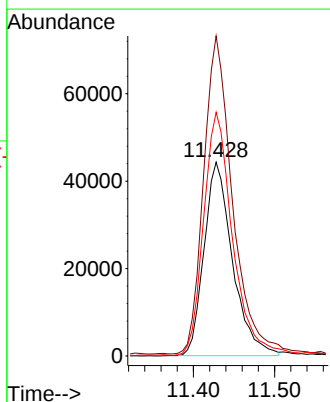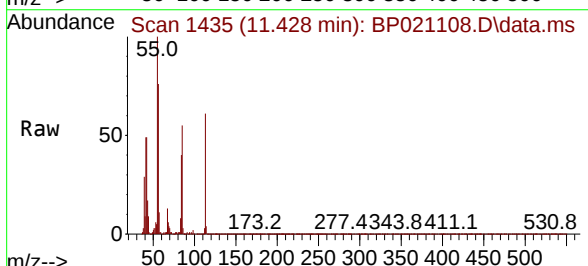



#35
4-Chloro-3-methylphenol
Concen: 31.643 ng/ul
RT: 11.763 min Scan# 1493
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:107 Resp: 37453
Ion Ratio Lower Upper
107 100
144 25.0 19.3 28.9
142 77.0 60.7 91.1


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#36
2-Methylnaphthalene
Concen: 32.943 ng/ul
RT: 12.093 min Scan# 1548
Delta R.T. -0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:142 Resp: 817576
Ion Ratio Lower Upper
142 100
141 90.2 72.6 108.8





#37
1-Methylnaphthalene
Concen: 31.818 ng/ul
RT: 12.316 min Scan# 1586
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:142 Resp: 812134
Ion Ratio Lower Upper
142 100
141 93.8 75.0 112.6
116 4.1 3.2 4.8


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#39
1,2,4,5-Tetrachlorobenzene
Concen: 29.636 ng/ul
RT: 12.469 min Scan# 1612
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:216 Resp: 432674
Ion Ratio Lower Upper
216 100
214 77.2 64.2 96.4
179 19.7 16.6 24.8
108 13.7 13.4 20.2





#40
Hexachlorocyclopentadiene
Concen: 4.593 ng/ul
RT: 12.428 min Scan# 1605
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:237 Resp: 35079
Ion Ratio Lower Upper
237 100
235 60.3 49.7 74.5
272 13.0 10.2 15.2


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#41
2,4,6-Trichlorophenol
Concen: 30.716 ng/ul
RT: 12.722 min Scan# 1655
Delta R.T. -0.018 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:196 Resp: 283362
Ion Ratio Lower Upper
196 100
198 94.9 76.6 115.0
200 30.6 26.0 39.0



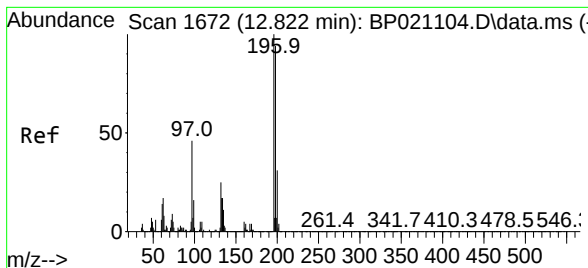

#42
2,4,5-Trichlorophenol
Concen: 31.255 ng/ul
RT: 12.822 min Scan# 1672
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

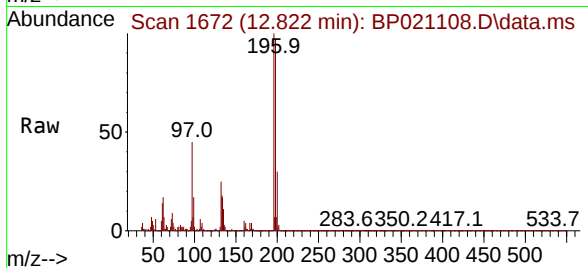

Tgt Ion:196 Resp: 30507
Ion Ratio Lower Upper
196 100
198 96.7 77.1 115.7
200 30.2 25.3 37.9


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

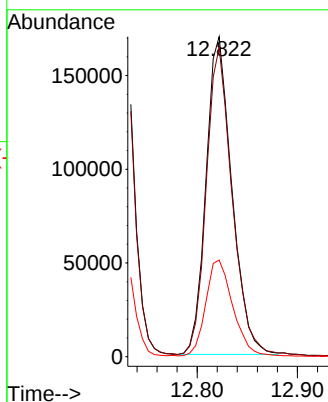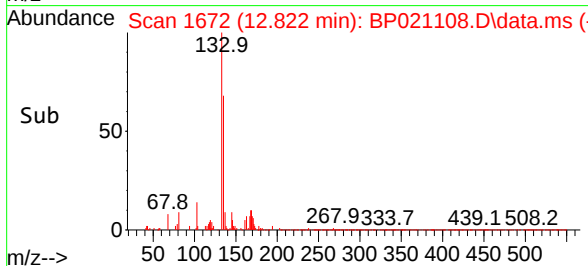


07/24/2024
Supervised By :mohammad
ahmed



07/25/2024

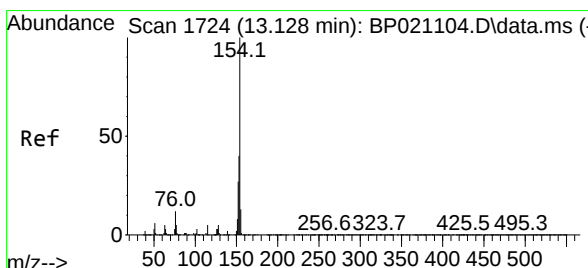


#43
1,1'-Biphenyl
Concen: 30.183 ng/ul
RT: 13.116 min Scan# 1722
Delta R.T. -0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

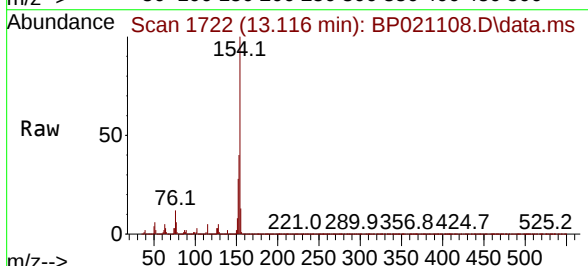


Tgt Ion:154 Resp: 991620
Ion Ratio Lower Upper
154 100
153 40.2 32.7 49.1
76 11.6 9.4 14.2

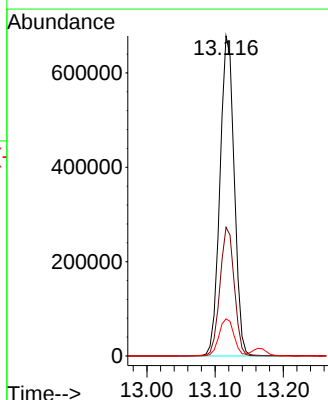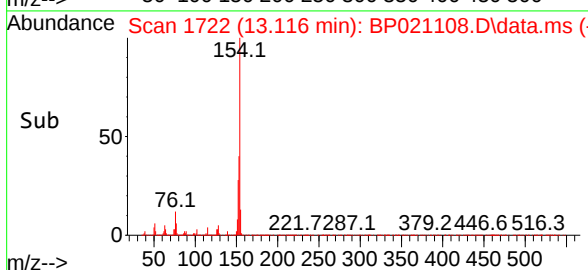



#44
2-Chloronaphthalene
Concen: 29.411 ng/ul
RT: 13.163 min Scan# 1731
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:162 Resp: 771379
Ion Ratio Lower Upper
162 100
164 32.6 26.3 39.5
127 38.9 31.8 47.8


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#45
2-Nitroaniline
Concen: 32.185 ng/ul
RT: 13.393 min Scan# 1769
Delta R.T. -0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion: 65 Resp: 233441
Ion Ratio Lower Upper
65 100
92 67.2 56.7 85.1
138 103.0 85.6 128.4





#47
Dimethylphthalate
Concen: 28.743 ng/ul
RT: 13.757 min Scan# 1831
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:163 Resp: 953099
Ion Ratio Lower Upper
163 100
194 4.3 3.4 5.0
164 10.4 8.1 12.1


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

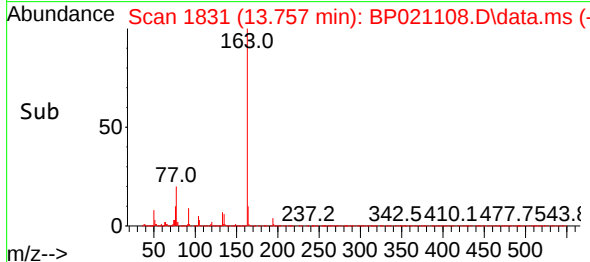


07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#48
2,6-Dinitrotoluene
Concen: 31.375 ng/ul
RT: 13.898 min Scan# 1855
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Tgt Ion:165 Resp: 207999
Ion Ratio Lower Upper
165 100
89 54.7 44.7 67.1
121 20.0 16.5 24.7

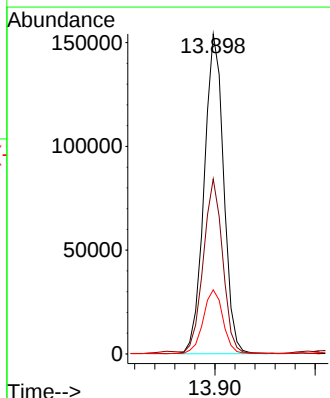



#50

Acenaphthylene

Concen: 31.552 ng/ul

RT: 14.022 min Scan# 1878

Delta R.T. -0.012 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD

Tgt Ion:152 Resp: 131088

Ion Ratio Lower Upper

152 100

151 20.3 16.2 24.2



153 13.1 10.3 15.5

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024



Supervised By :mohammad ahmed 07/25/2024



07/24/2024

Supervised By :mohammad
ahmed

07/25/2024



#51

3-Nitroaniline

Concen: 29.583 ng/ul

RT: 14.245 min Scan# 1914

Delta R.T. -0.000 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32




Tgt Ion:138 Resp: 170663


Ion Ratio Lower Upper

138 100

108 12.7 9.8 14.8

92 116.6 98.0 147.0

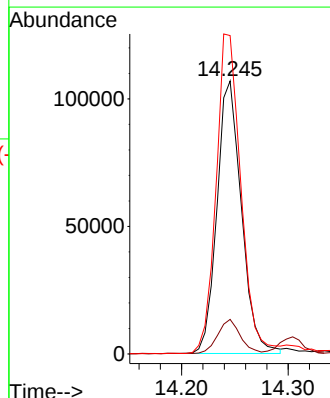



#52

Acenaphthene

Concen: 43.926 ng/ul

RT: 14.369 min Scan# 1936

Delta R.T. -0.006 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD

Tgt Ion:153 Resp: 1211294

Ion Ratio Lower Upper

153 100



152 47.3 37.8 56.6

154 87.6 71.8 107.6

Manual Integrations



APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

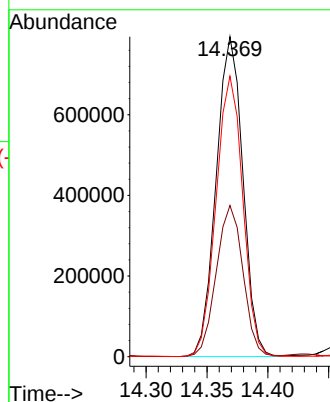

07/24/2024
Supervised By :mohammad
ahmed

07/25/2024



#53

2,4-Dinitrophenol

Concen: 19.553 ng/ul

RT: 14.487 min Scan# 1955

Delta R.T. 0.012 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32




Tgt Ion:184 Resp: 68073


Ion Ratio Lower Upper

184 100

63 59.0 50.3 75.5


154 66.9 53.0 79.6





#55
4-Nitrophenol
Concen: 37.879 ng/ul
RT: 14.610 min Scan# 1976
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:109 Resp: 143270
Ion Ratio Lower Upper
109 100
139 126.9 98.0 147.0
65 123.0 106.0 159.0


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

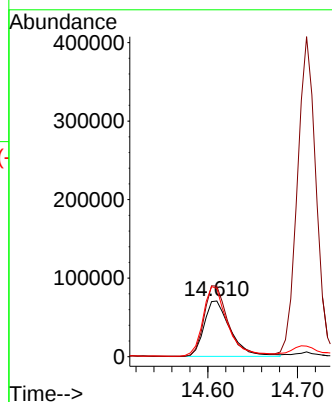




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#56
Dibenzofuran
Concen: 41.304 ng/ul
RT: 14.710 min Scan# 1993
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion:168 Resp: 1559744
Ion Ratio Lower Upper
168 100
139 37.4 31.1 46.7







#57
2,4-Dinitrotoluene
Concen: 33.688 ng/ul
RT: 14.704 min Scan# 1993
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

Tgt Ion:165 Resp: 306584
Ion Ratio Lower Upper
165 100
63 64.3 41.0 61.4
182 3.0 2.2 3.4



Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024

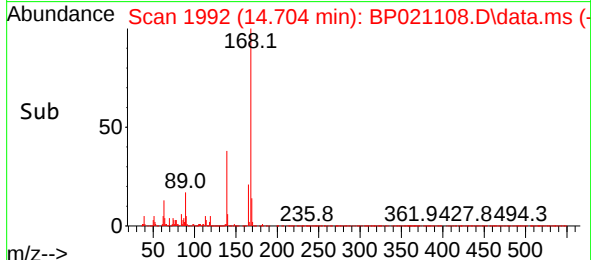

#58
2,3,4,6-Tetrachlorophenol
Concen: 30.625 ng/ul
RT: 14.963 min Scan# 2036
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion:232 Resp: 255967
Ion Ratio Lower Upper
232 100
131 40.4 34.4 51.6
130 2.3 2.0 3.0
166 29.3 24.4 36.6

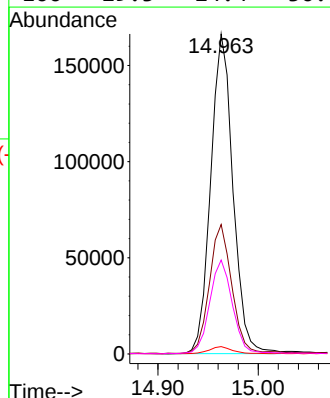



#59
Diethylphthalate
Concen: 29.290 ng/ul
RT: 15.145 min Scan# 2068
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :



A4BE6MSD

Tgt Ion:149 Resp: 97064
Ion Ratio Lower Upper
149 100
177 22.3 17.7 26.5
150 12.5 10.2 15.2

Manual Integrations



APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#61
Fluorene
Concen: 46.684 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:166 Resp: 1438569
Ion Ratio Lower Upper
166 100
165 98.0 78.1 117.1
167 13.6 10.9 16.3





#62
4-Chlorophenyl-phenylether
Concen: 28.667 ng/ul
RT: 15.369 min Scan# 2105
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:204 Resp: 479350
Ion Ratio Lower Upper
204 100
206 33.4 26.4 39.6
141 56.4 48.5 72.7


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

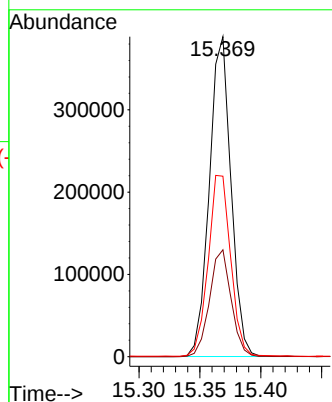


07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#63
4-Nitroaniline
Concen: 41.354 ng/ul
RT: 15.428 min Scan# 2115
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Tgt Ion:138 Resp: 197566
Ion Ratio Lower Upper
138 100
92 50.3 40.9 61.3
108 82.6 64.7 97.1







#66
4,6-Dinitro-2-methylphenol
Concen: 20.508 ng/ul
RT: 15.510 min Scan# 2129
Delta R.T. 0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

Tgt Ion:198 Resp: 125354
Ion Ratio Lower Upper
198 100
182 6.1 3.8 5.6
77 22.1 20.0 30.0



Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

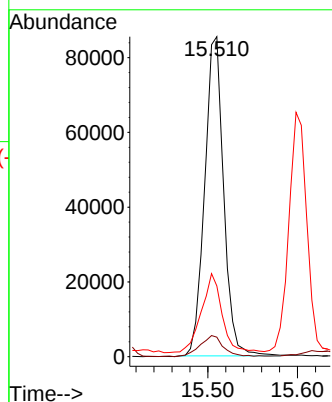




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#67
N-Nitrosodiphenylamine
Concen: 29.871 ng/ul
RT: 15.604 min Scan# 2145
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:169 Resp: 828651
Ion Ratio Lower Upper
169 100
168 66.8 53.4 80.2
167 36.5 28.4 42.6





#68
4-Bromophenyl-phenylether
Concen: 29.096 ng/ul
RT: 16.292 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:248 Resp: 32488
Ion Ratio Lower Upper
248 100
250 99.8 79.3 118.9
141 67.1 57.4 86.0


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024






07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#69
Hexachlorobenzene
Concen: 23.349 ng/ul
RT: 16.410 min Scan# 2282
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion:284 Resp: 298932
Ion Ratio Lower Upper
284 100
142 29.0 25.8 38.8
249 31.3 25.1 37.7





#70

Atrazine

Concen: 23.218 ng/ul

RT: 16.586 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :



A4BE6MSD

Tgt Ion:200	Resp: 234744
Ion Ratio	Lower Upper
200 100	
173 26.7	20.8 31.2
215 50.1	38.7 58.1

Manual Integrations



APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

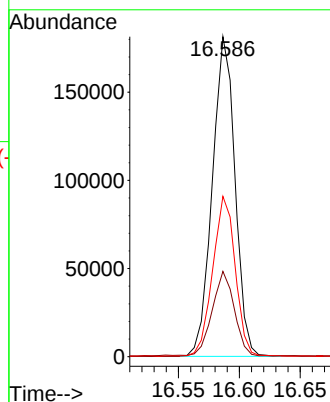

07/24/2024
Supervised By :mohammad
ahmed

07/25/2024



#71

Pentachlorophenol

Concen: 25.940 ng/ul




RT: 16.792 min Scan# 2347


Delta R.T. 0.012 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32


Tgt Ion:266	Resp: 180375
Ion Ratio	Lower Upper
266 100	
264 64.7	52.3 78.5
268 64.8	52.3 78.5





#72
Phenanthrene
Concen: 198.492 ng/u1
RT: 17.181 min Scan# 2411
Delta R.T. 0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:178 Resp: 9809280
Ion Ratio Lower Upper
178 100
179 16.1 12.2 18.4
176 20.1 15.0 22.4


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

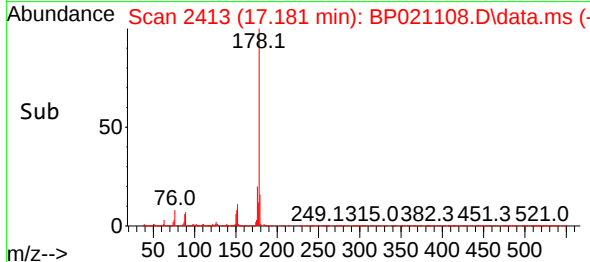




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#74
Anthracene
Concen: 69.113 ng/u1
RT: 17.269 min Scan# 2428
Delta R.T. 0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32


Tgt Ion:178 Resp: 3482001
Ion Ratio Lower Upper
178 100
179 15.5 12.5 18.7
176 18.5 14.8 22.2

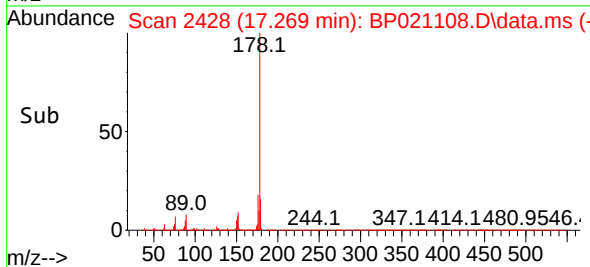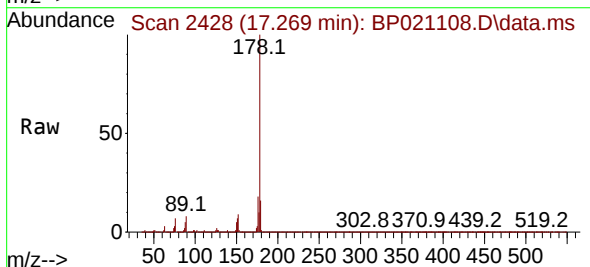



#75
1,2,3,4-Tetrachlorobenzene
Concen: 26.835 ng/uL
RT: 13.087 min Scan# 1717
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:216 Resp: 409174
Ion Ratio Lower Upper
216 100
214 78.4 63.2 94.8
218 48.3 38.2 57.4


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

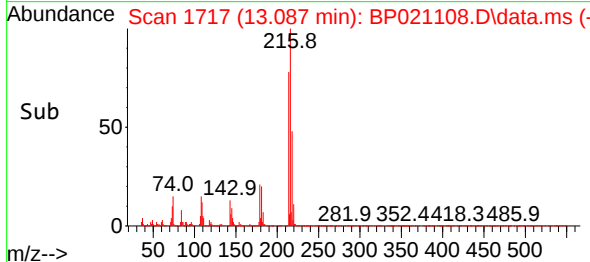




07/24/2024
Supervised By :mohammad
ahmed


07/25/2024



#76
Pentachlorobenzene
Concen: 26.663 ng/uL
RT: 14.628 min Scan# 1979
Delta R.T. -0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

Tgt Ion:250 Resp: 403977
Ion Ratio Lower Upper
250 100
248 64.2 50.8 76.2
252 63.5 51.6 77.4





#77

Carbazole

Concen: 52.177 ng/ul

RT: 17.563 min Scan# 2478

Delta R.T. -0.000 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD



Tgt Ion:167 Resp: 214889

Ion	Ratio	Lower	Upper
167	100		
166	21.8	17.3	25.9
139	13.0	10.2	15.2

Manual Integrations



APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024



07/24/2024
Supervised By :mohammad
ahmed

07/25/2024



#78

Di-n-butylphthalate

Concen: 30.085 ng/ul

RT: 18.122 min Scan# 2573




Delta R.T. 0.006 min


Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Tgt Ion:149 Resp: 1709475

Ion	Ratio	Lower	Upper
149	100		
150	9.2	7.4	11.0
104	5.0	3.9	5.9





#80

Fluoranthene

Concen: 194.281 ng/uI

RT: 19.275 min Scan# 21

Delta R.T. 0.012 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD

Tgt Ion:202 Resp:1284310

Ion Ratio Lower Upper

202 100

101 9.4 8.0 12.0



100 7.3 6.1 9.1

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024



Supervised By :mohammad ahmed 07/25/2024

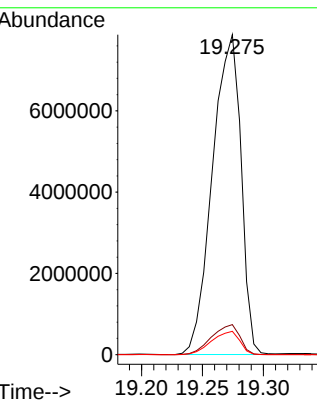

07/24/2024

Supervised By :mohammad
ahmed

07/25/2024



#82

Pyrene

Concen: 135.440 ng/uI

RT: 19.651 min Scan# 2833

Delta R.T. 0.012 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32




Tgt Ion:202 Resp: 9110856


Ion Ratio Lower Upper

202 100

101 10.5 9.4 14.2


100 8.8 7.8 11.6

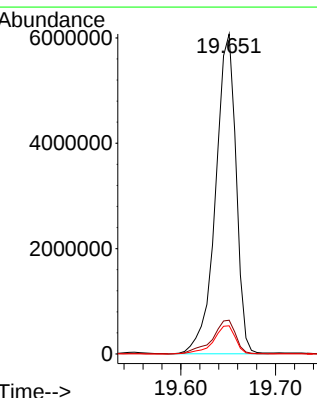



#83
Butylbenzylphthalate
Concen: 28.635 ng/ul
RT: 20.580 min Scan# 2991
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:149 Resp: 802548
Ion Ratio Lower Upper
149 100
91 65.3 54.1 81.1
206 23.0 17.0 25.6


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024




07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#84
3,3'-Dichlorobenzidine
Concen: 12.004 ng/ul
RT: 21.480 min Scan# 3144
Delta R.T. -0.000 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32




Tgt Ion:252 Resp: 242871
Ion Ratio Lower Upper
252 100
254 65.5 51.5 77.3
126 9.9 8.0 12.0

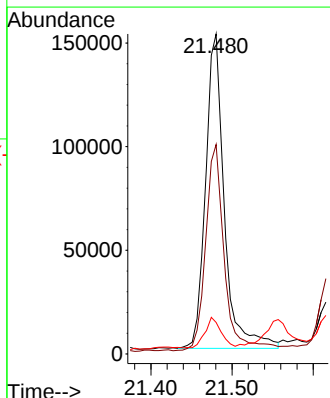

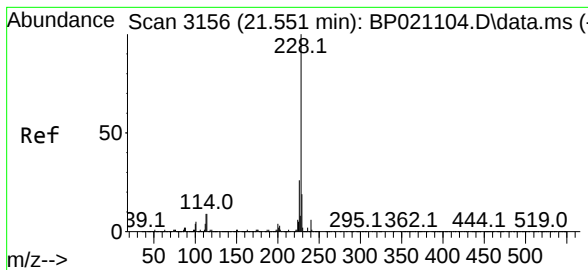

#85
 Benzo(a)anthracene
 Concen: 118.240 ng/ul
 RT: 21.557 min Scan# 3157
 Delta R.T. 0.006 min
 Lab File: BP021108.D
 Acq: 23 Jul 2024 21:32

Instrument :
 BNA_P
 ClientSampleId :
 A4BE6MSD


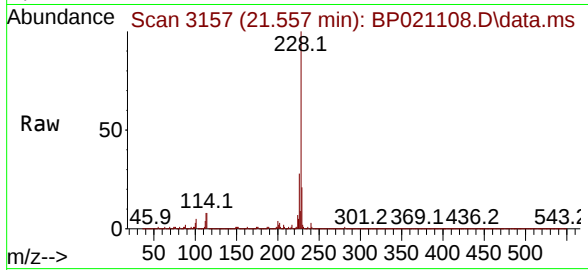


Tgt Ion: 228 Resp: 7333619

Ion	Ratio	Lower	Upper
228	100		
229	20.5	15.5	23.3
226	28.4	21.4	32.2


Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
 Supervised By :mohammad ahmed 07/25/2024

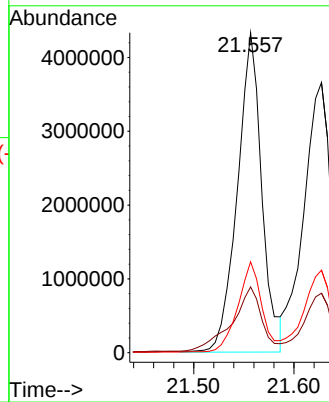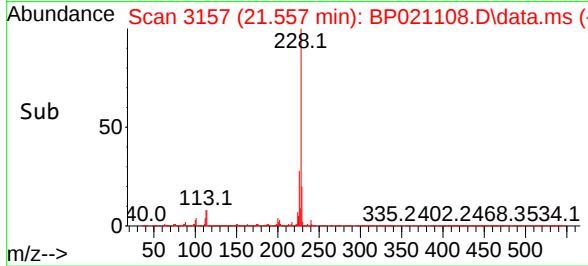

07/24/2024
 Supervised By :mohammad
 ahmed




07/25/2024

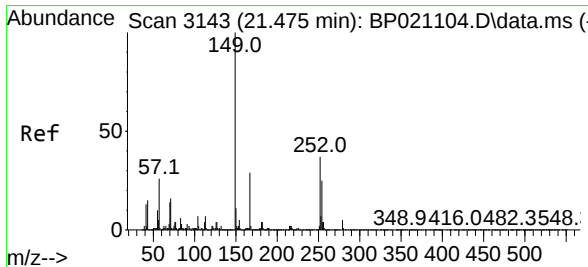


#86
 Bis(2-ethylhexyl)phthalate
 Concen: 33.295 ng/ul
 RT: 21.463 min Scan# 3141
 Delta R.T. -0.012 min
 Lab File: BP021108.D
 Acq: 23 Jul 2024 21:32

Tgt Ion: 149 Resp: 1342907

Ion	Ratio	Lower	Upper
149	100		
167	28.1	22.1	33.1
279	4.9	3.7	5.5

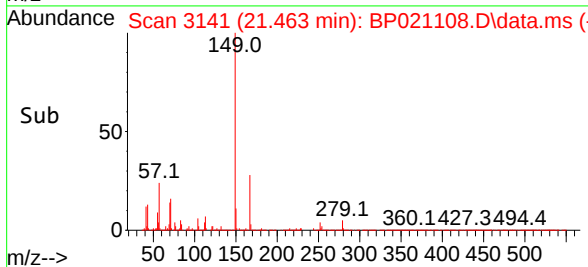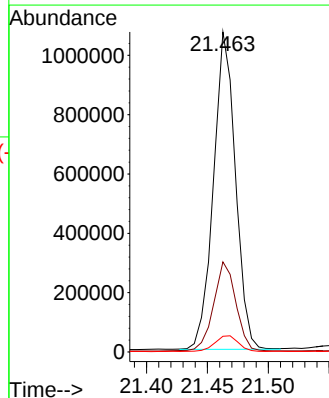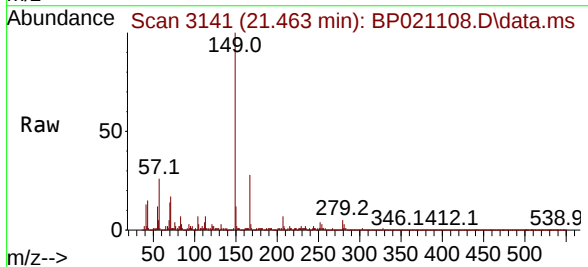



#87

Chrysene

Concen: 117.527 ng/ul

RT: 21.627 min Scan# 3168

Delta R.T. 0.006 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD

Tgt Ion:228 Resp: 677336

Ion Ratio Lower Upper

228 100



226 30.5 23.6 35.4

229 22.0 15.5 23.3

Manual Integrations



APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

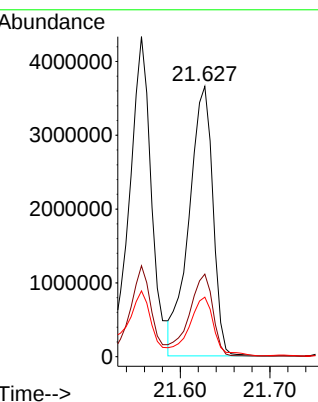

07/24/2024
Supervised By :mohammad
ahmed

07/25/2024



#89

Di-n-octyl phthalate

Concen: 27.204 ng/ul




RT: 22.716 min Scan# 3354


Delta R.T. -0.006 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32


Tgt Ion:149 Resp: 2064517

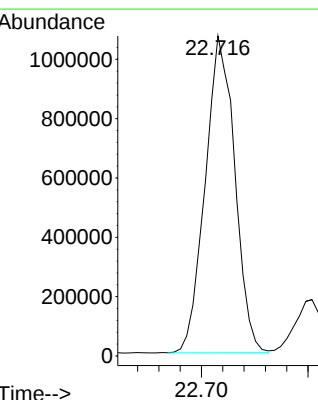



#90
Benzo(b)fluoranthene
Concen: 123.903 ng/ul
RT: 23.868 min Scan# 3550
Delta R.T. 0.012 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD



Tgt Ion:252 Resp: 863785
Ion Ratio Lower Upper
252 100
253 22.8 17.1 25.7
125 8.6 7.0 10.4


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024




07/24/2024
Supervised By :mohammad
ahmed



07/25/2024




#91
Benzo(k)fluoranthene
Concen: 63.847 ng/ul
RT: 23.927 min Scan# 3560
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32




Tgt Ion:252 Resp: 4442037
Ion Ratio Lower Upper
252 100
253 23.1 17.4 26.2
125 7.9 7.4 11.0

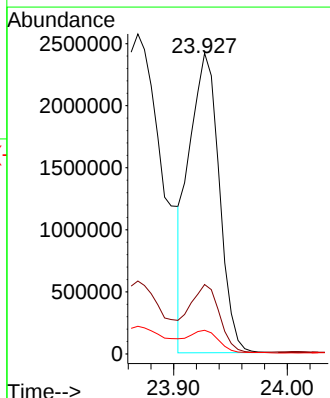

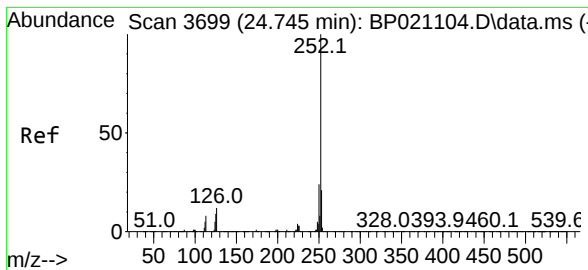

#93
Benzo(a)pyrene
Concen: 53.159 ng/ul
RT: 24.751 min Scan# 31
Delta R.T. 0.006 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32



Instrument :
BNA_P
ClientSampleId :
A4BE6MSD

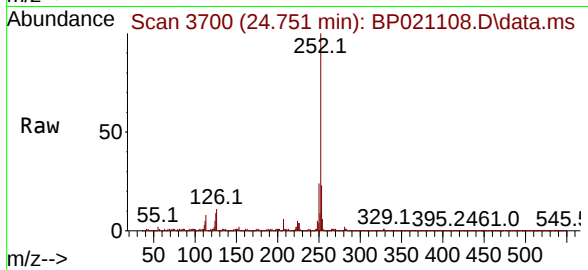

Tgt Ion: 252 Resp: 350205
Ion Ratio Lower Upper
252 100
253 22.9 17.4 26.0
125 9.2 7.7 11.5


Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024
Supervised By :mohammad ahmed 07/25/2024

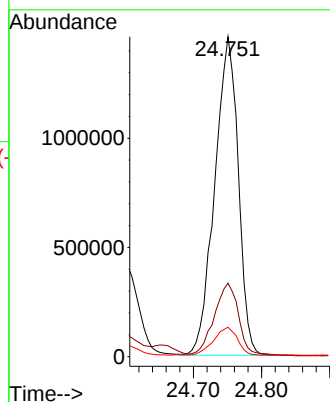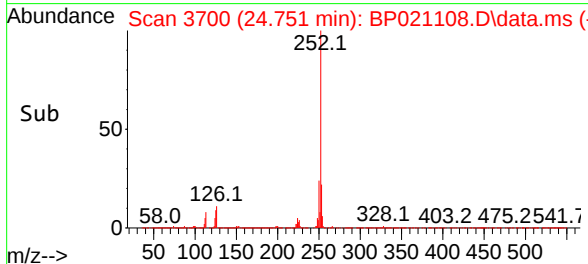


07/24/2024
Supervised By :mohammad
ahmed



07/25/2024

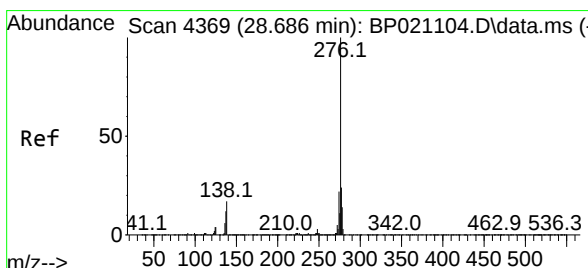


#94
Indeno(1,2,3-cd)pyrene
Concen: 49.252 ng/ul m
RT: 28.703 min Scan# 4372
Delta R.T. 0.018 min
Lab File: BP021108.D
Acq: 23 Jul 2024 21:32

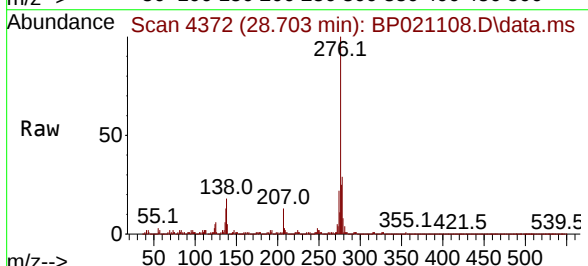

Tgt Ion: 276 Resp: 4181070
Ion Ratio Lower Upper
276 100
138 17.7 14.3 21.5
277 25.4 19.2 28.8

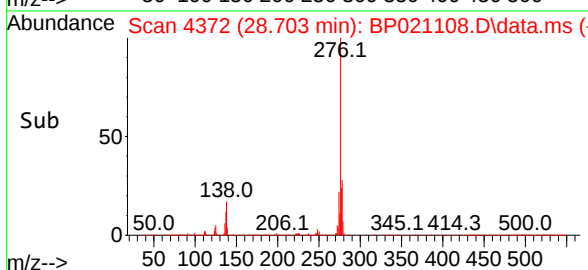



#95

Dibenzo(a,h)anthracene

Concen: 41.232 ng/ul

RT: 28.756 min Scan# 41

Delta R.T. -0.006 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Instrument :

BNA_P

ClientSampleId :

A4BE6MSD

Tgt Ion:278 Resp: 2898524

Ion Ratio Lower Upper

278 100

139 12.1 10.9 16.3



279 25.7 19.4 29.0

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 07/24/2024



Supervised By :mohammad ahmed 07/25/2024

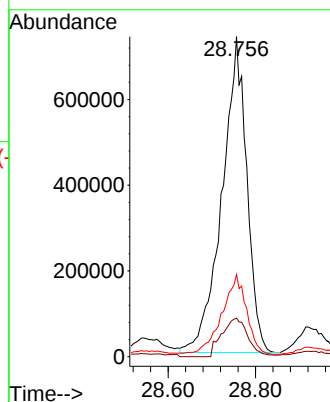

07/24/2024

Supervised By :mohammad
ahmed

07/25/2024



#96

Benzo(g,h,i)perylene

Concen: 7.637 ng/ul m

RT: 29.862 min Scan# 4569

Delta R.T. -0.018 min

Lab File: BP021108.D

Acq: 23 Jul 2024 21:32

Tgt Ion:276 Resp: 527993

Ion Ratio Lower Upper

276 100

138 18.3 15.3 22.9

277 25.0 18.2 27.2

