

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
 Data File : BP021096.D
 Acq On : 23 Jul 2024 12:56
 Operator : MA/JU
 Sample : PB161905BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK905

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021096.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	40	rVB	39077	53676	1.39%	0.152%
2	3.605	102	105	122	rBV	383640	654540	16.89%	1.855%
3	3.916	154	158	161	rVB2	8129	10975	0.28%	0.031%
4	6.769	638	643	648	rBV9	4404	7653	0.20%	0.022%
5	6.881	655	662	676	rBV	445990	863547	22.29%	2.448%
6	7.016	679	685	699	rVB	416626	661286	17.07%	1.874%
7	7.210	711	718	733	rBV	537705	899235	23.21%	2.549%
8	7.669	786	796	806	rBV	441136	766629	19.79%	2.173%
9	8.393	911	919	931	rBV	576071	1082672	27.95%	3.069%
10	8.828	985	993	1006	rBV	496505	862369	22.26%	2.444%
11	9.546	1105	1115	1126	rBV	428852	755095	19.49%	2.140%
12	10.087	1198	1207	1228	rBV	466505	1112170	28.71%	3.152%
13	10.298	1240	1243	1247	rVB6	3143	5540	0.14%	0.016%
14	10.440	1259	1267	1281	rBV	576828	1070546	27.63%	3.034%
15	10.604	1287	1295	1309	rBV	451303	934842	24.13%	2.650%
16	11.298	1410	1413	1417	rBV6	2692	4282	0.11%	0.012%
17	12.045	1534	1540	1549	rBV8	8309	21463	0.55%	0.061%
18	13.563	1793	1798	1802	rBV9	2152	4408	0.11%	0.012%
19	13.722	1816	1825	1836	rBV	1055083	1631907	42.12%	4.625%
20	13.998	1864	1872	1881	rBV	1323014	1993096	51.45%	5.649%
21	14.310	1915	1925	1936	rBV	970034	1479227	38.18%	4.193%
22	14.604	1967	1975	1991	rBV	235644	714669	18.45%	2.026%
23	14.722	1991	1995	2004	rVB	14519	44398	1.15%	0.126%
24	15.316	2090	2096	2112	rBV	1380523	2471480	63.79%	7.005%
25	15.481	2119	2124	2135	rBV	492451	777191	20.06%	2.203%
26	15.839	2183	2185	2189	rVB5	5397	6479	0.17%	0.018%
27	16.045	2217	2220	2224	rBV6	2795	5050	0.13%	0.014%
28	16.128	2228	2234	2239	rBV8	6234	11067	0.29%	0.031%
29	17.133	2398	2405	2415	rBV	1119459	1776390	45.85%	5.035%
30	17.233	2416	2422	2441	rVV	1855024	2746134	70.88%	7.783%
31	17.810	2518	2520	2525	rBV6	7310	9331	0.24%	0.026%
32	18.063	2559	2563	2571	rBV	70994	122267	3.16%	0.347%
33	19.163	2747	2750	2754	rBV3	29406	39721	1.03%	0.113%
34	19.622	2822	2828	2838	rBV2	2271692	3442689	88.86%	9.758%
35	21.586	3157	3162	3177	rVB2	1310347	2176319	56.17%	6.168%
36	24.710	3685	3693	3704	rVB2	1474337	3874183	100.00%	10.981%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
Data File : BP021096.D
Acq On : 23 Jul 2024 12:56
Operator : MA/JU
Sample : PB161905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK905

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	24.927	3724	3730	3743	rVB	776761	2189300	56.51%	6.205%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 35281826

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
Data File : BP021096.D
Acq On : 23 Jul 2024 12:56
Operator : MA/JU
Sample : PB161905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK905

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

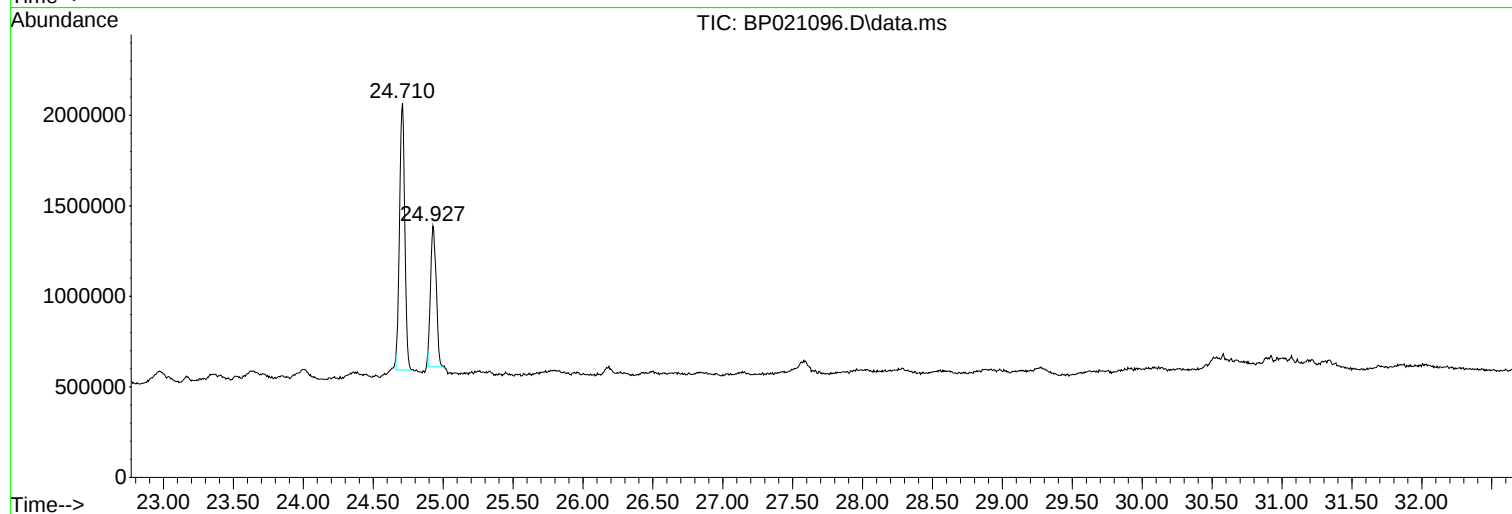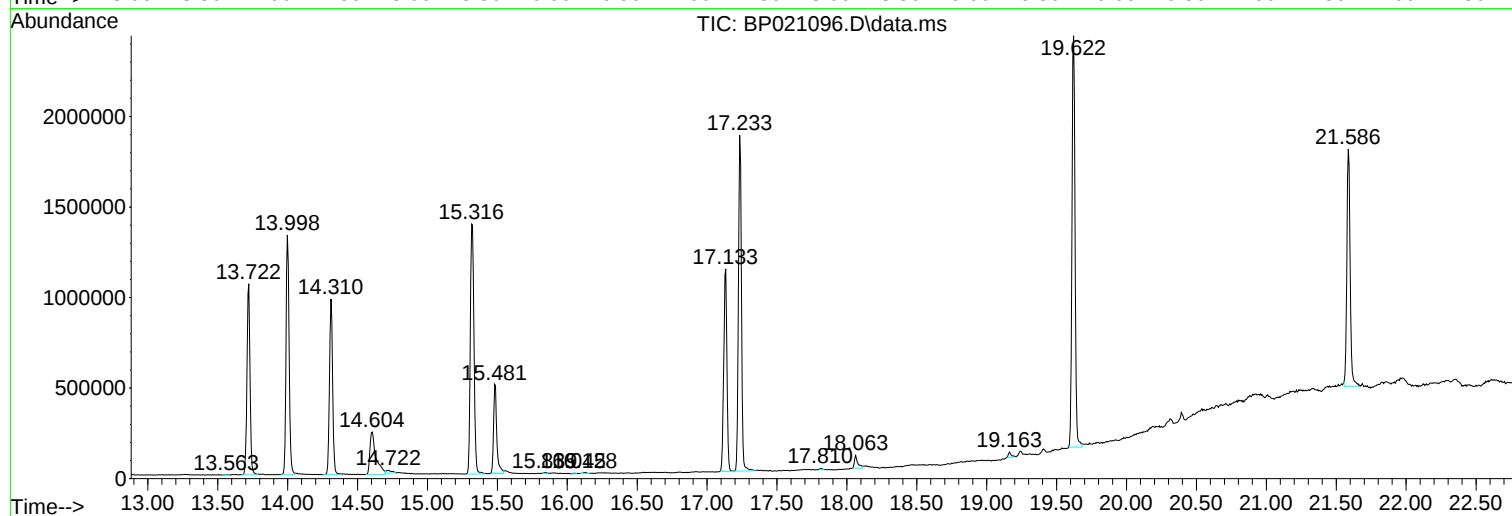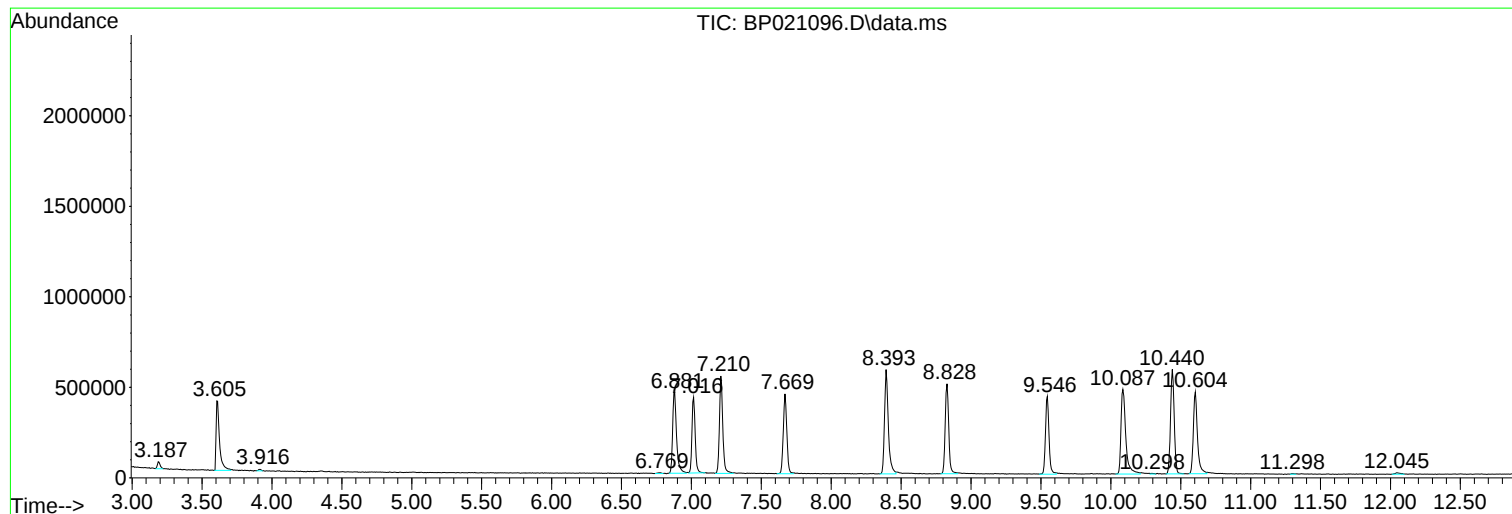

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
Data File : BP021096.D
Acq On : 23 Jul 2024 12:56
Operator : MA/JU
Sample : PB161905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK905

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072324\
Data File : BP021096.D
Acq On : 23 Jul 2024 12:56
Operator : MA/JU
Sample : PB161905BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK905

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------