
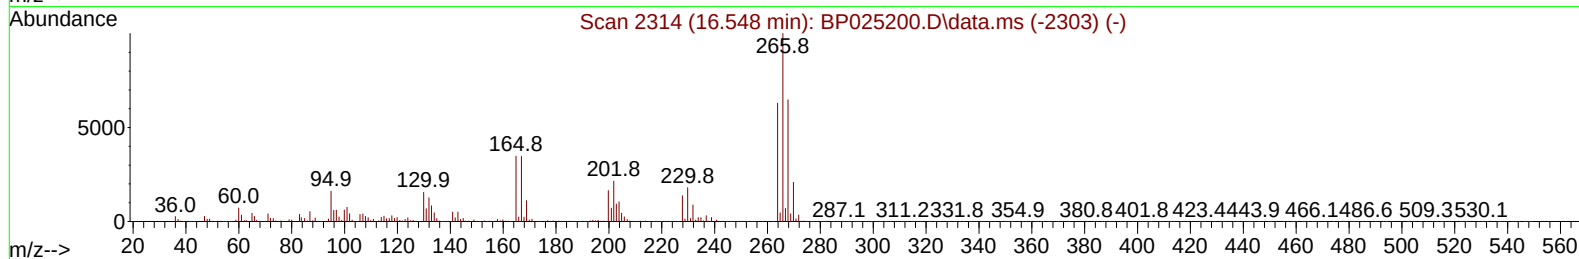
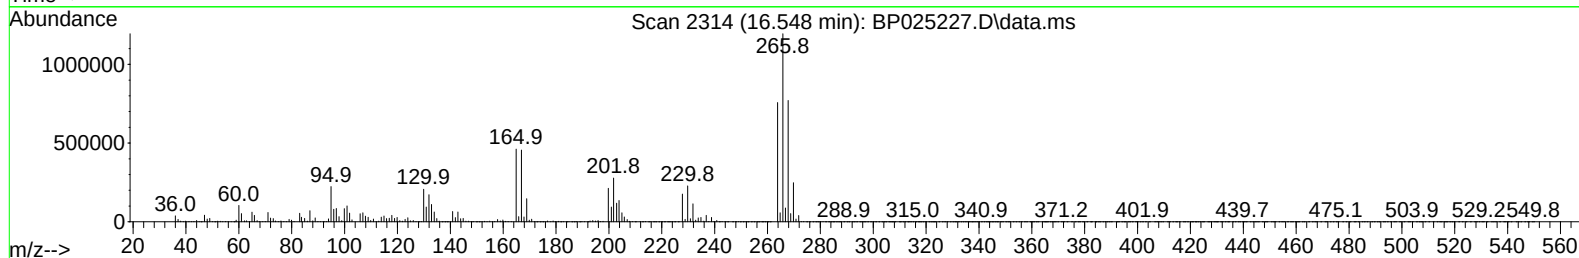


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025227.D
Acq On : 23 Jul 2025 16:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 17:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

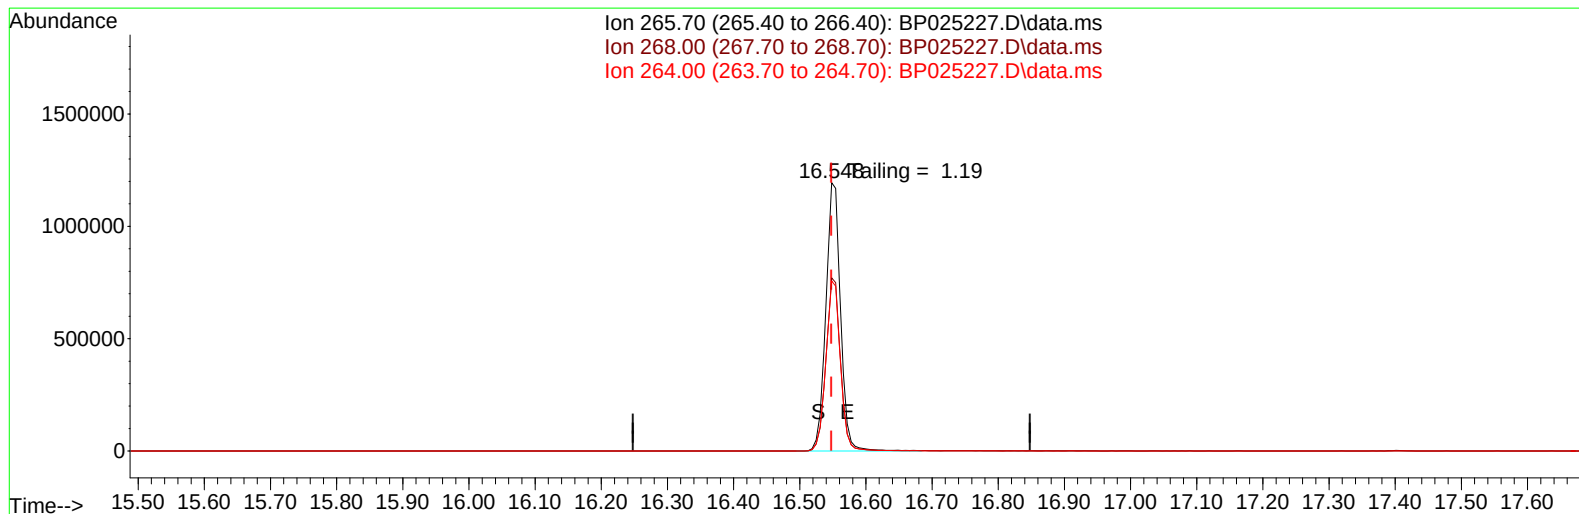

TIC: BP025227.D\data.ms

(70) Pentachlorophenol (C)




16.548min (+ 0.000) 694149.25 ng m

response 1844890

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	64.51
264.00	62.90	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025227.D
Acq On : 23 Jul 2025 16:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 23 17:14:32 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

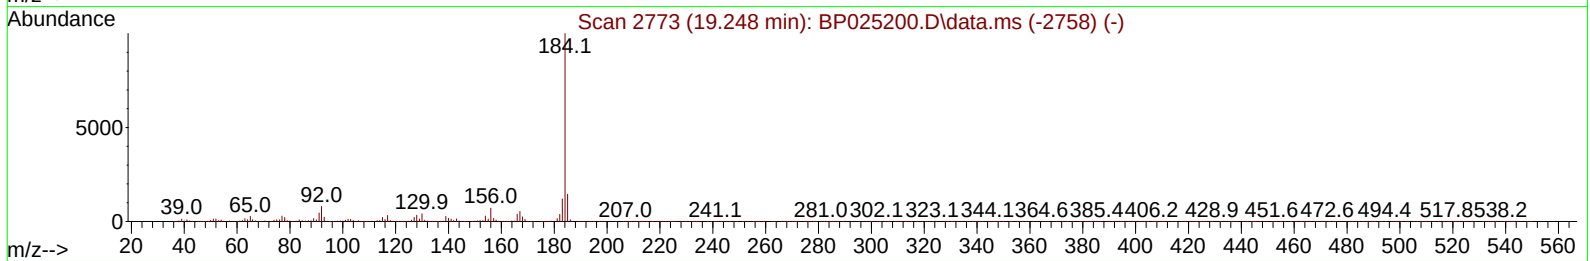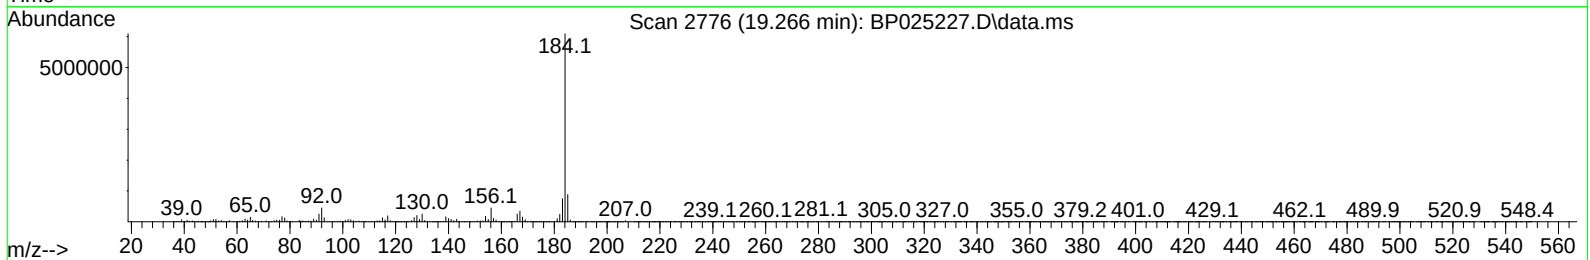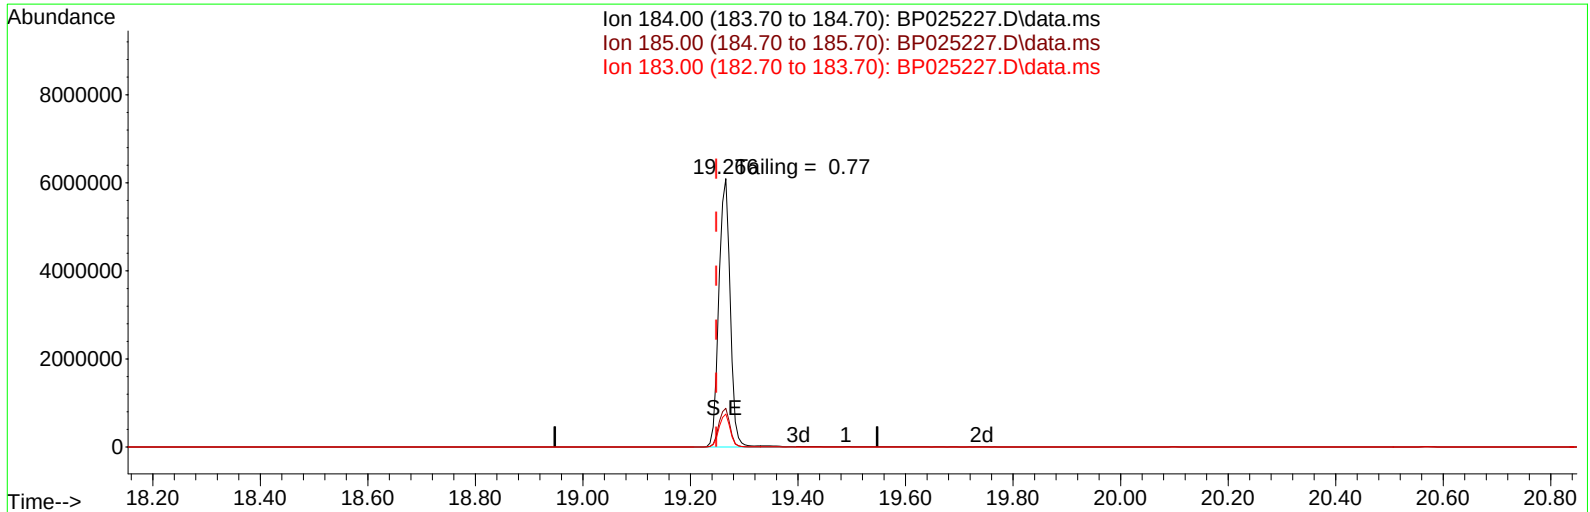

TIC: BP025227.D\data.ms

(77) Benzidine

19.266min (+ 0.018) 273382.31 ng m

response 9089196

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.46
183.00	12.00	12.30
0.00	0.00	0.00