

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
 Data File : BP025221.D
 Acq On : 23 Jul 2025 12:47
 Operator : CG/JU
 Sample : Q2638-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 OU4-TS-37-071725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP025221.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.655	286	292	299	rBV	452641	594122	1.87%	0.239%
2	5.102	361	368	384	rBV	4923132	6870575	21.61%	2.768%
3	6.637	621	629	642	rVB	5169217	7626381	23.99%	3.073%
4	7.437	757	765	773	rBV	2161519	3212233	10.10%	1.294%
5	8.560	949	956	968	rBV	3104041	5013700	15.77%	2.020%
6	10.184	1224	1232	1238	rBV	2784442	4803871	15.11%	1.935%
7	12.678	1650	1656	1670	rVB	9727400	12886274	40.53%	5.192%
8	13.784	1840	1844	1853	rVB	360321	532597	1.68%	0.215%
9	14.072	1887	1893	1901	rBV	4917961	6889427	21.67%	2.776%
10	14.554	1971	1975	1985	rVB3	209645	417301	1.31%	0.168%
11	15.484	2127	2133	2143	rVB	1077523	1734449	5.45%	0.699%
12	15.607	2147	2154	2160	rBV	6947585	11411873	35.89%	4.598%
13	15.748	2175	2178	2181	rBV	356584	479938	1.51%	0.193%
14	16.336	2274	2278	2290	rVB3	293987	535635	1.68%	0.216%
15	16.901	2368	2374	2379	rBV2	5507049	7916053	24.90%	3.189%
16	16.942	2379	2381	2387	rVB	508956	618657	1.95%	0.249%
17	17.036	2388	2397	2404	rBV2	328183	841131	2.65%	0.339%
18	17.807	2524	2528	2532	rBV2	224484	445154	1.40%	0.179%
19	17.883	2532	2541	2557	rVB	8254386	16680114	52.46%	6.720%
20	18.007	2558	2562	2566	rBV2	440338	721544	2.27%	0.291%
21	18.783	2690	2694	2699	rBV2	478111	704952	2.22%	0.284%
22	19.042	2734	2738	2745	rBV	1761947	2908410	9.15%	1.172%
23	19.236	2763	2771	2781	rBV2	3879633	6675966	21.00%	2.690%
24	19.425	2795	2803	2807	rBV	1897403	3044288	9.57%	1.227%
25	19.566	2820	2827	2837	rBV	6674397	14423048	45.36%	5.811%
26	19.666	2838	2844	2852	rVV2	18188530	31795816	100.00%	12.811%
27	19.742	2852	2857	2865	rVB	15525156	26617128	83.71%	10.724%
28	19.877	2876	2880	2887	rBV	1046780	2510581	7.90%	1.012%
29	20.060	2906	2911	2916	rBV2	1340811	2304298	7.25%	0.928%
30	20.272	2944	2947	2951	rVB	710486	778498	2.45%	0.314%
31	20.313	2951	2954	2959	rBV	445390	618180	1.94%	0.249%
32	20.519	2987	2989	2996	rVB3	455193	826746	2.60%	0.333%
33	21.001	3062	3071	3076	rBV2	2082466	5351429	16.83%	2.156%
34	21.066	3077	3082	3087	rVV	5024802	9350706	29.41%	3.767%
35	21.119	3087	3091	3098	rVB	8093255	11108479	34.94%	4.476%
36	21.201	3102	3105	3115	rVB2	864700	1384545	4.35%	0.558%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025221.D
Acq On : 23 Jul 2025 12:47
Operator : CG/JU
Sample : Q2638-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-37-071725

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	21.336	3120	3128	3133	rBV2	6375019	11924025	37.50%	4.804%
38	21.383	3133	3136	3141	rVB	1319395	1701800	5.35%	0.686%
39	22.254	3279	3284	3292	rVB2	1876303	3548662	11.16%	1.430%
40	23.765	3535	3541	3557	rVB2	2989341	7912756	24.89%	3.188%
41	24.471	3654	3661	3662	rBV	3199484	5524664	17.38%	2.226%
42	25.848	3889	3895	3906	rVB	2445036	6953131	21.87%	2.801%




Sum of corrected areas: 248199137

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025221.D
Acq On : 23 Jul 2025 12:47
Operator : CG/JU
Sample : Q2638-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-37-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

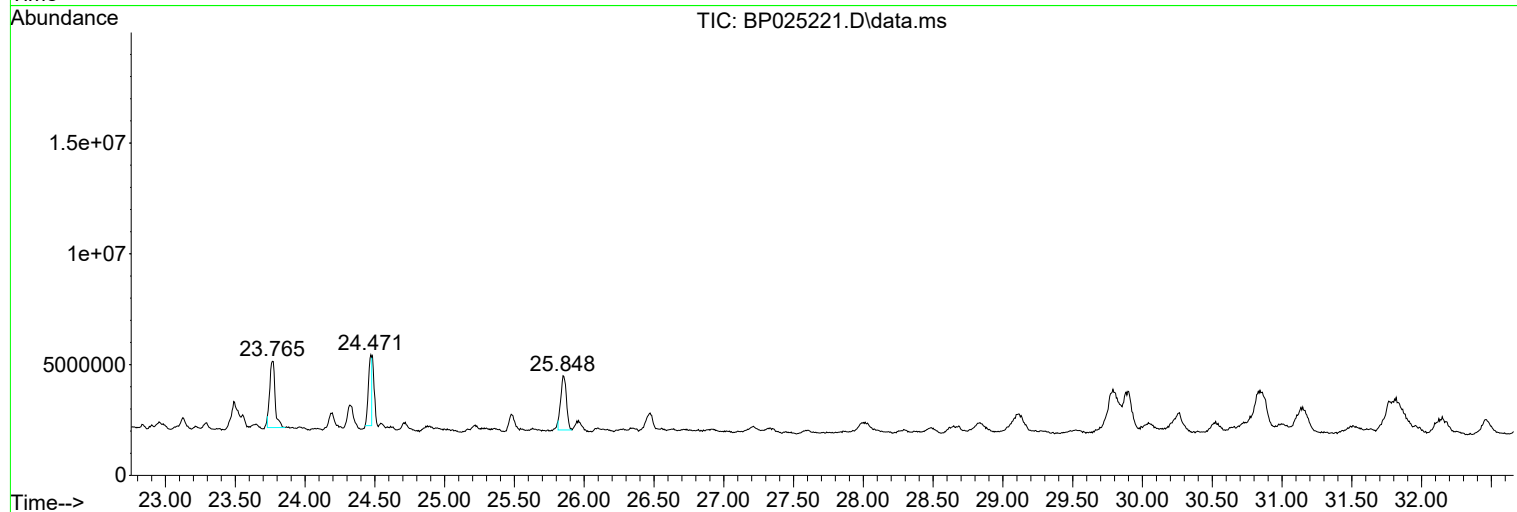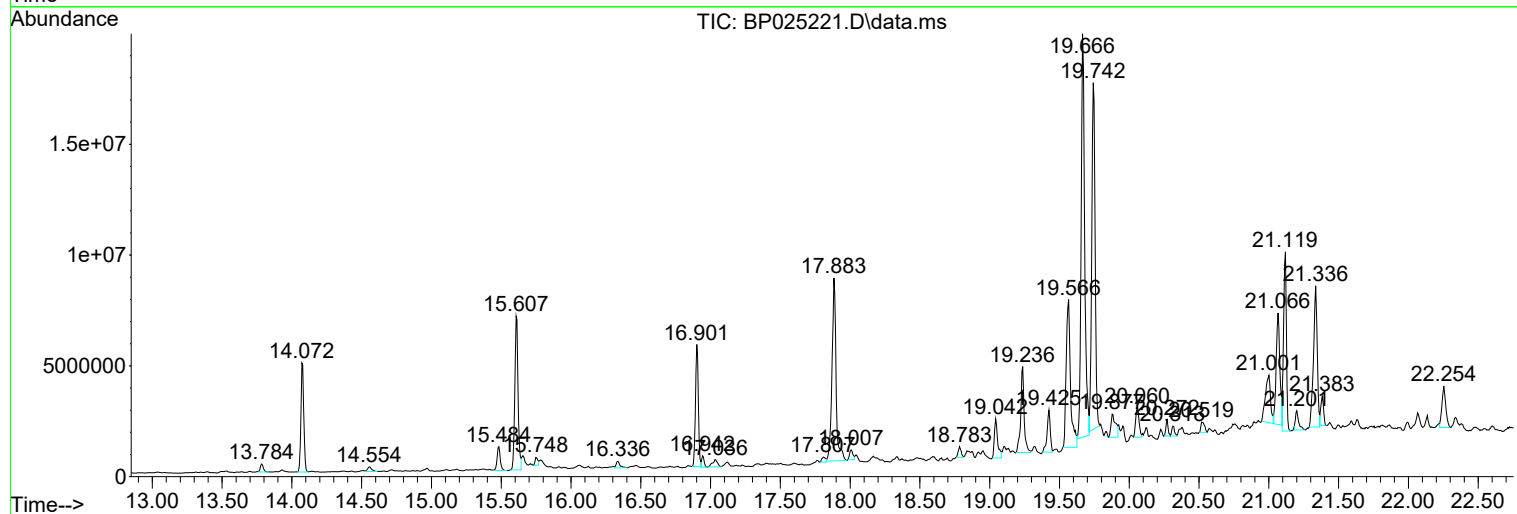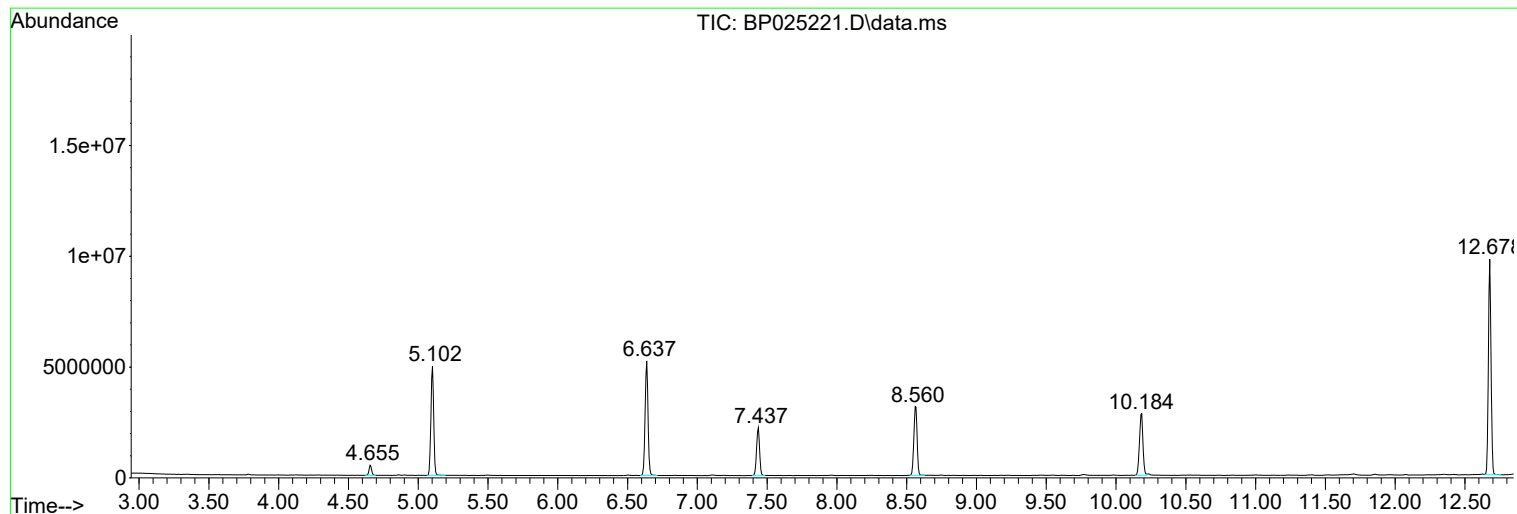

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025221.D
Acq On : 23 Jul 2025 12:47
Operator : CG/JU
Sample : Q2638-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-37-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072325\
Data File : BP025221.D
Acq On : 23 Jul 2025 12:47
Operator : CG/JU
Sample : Q2638-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
OU4-TS-37-071725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------