
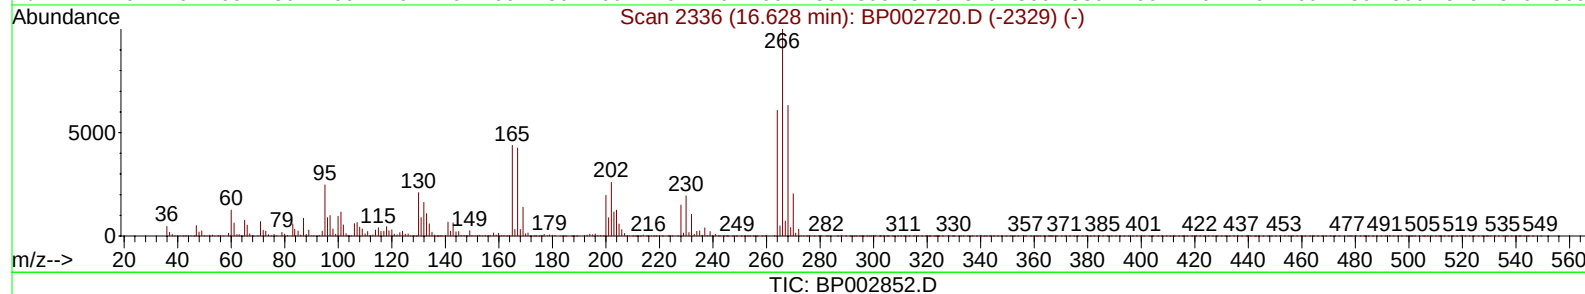
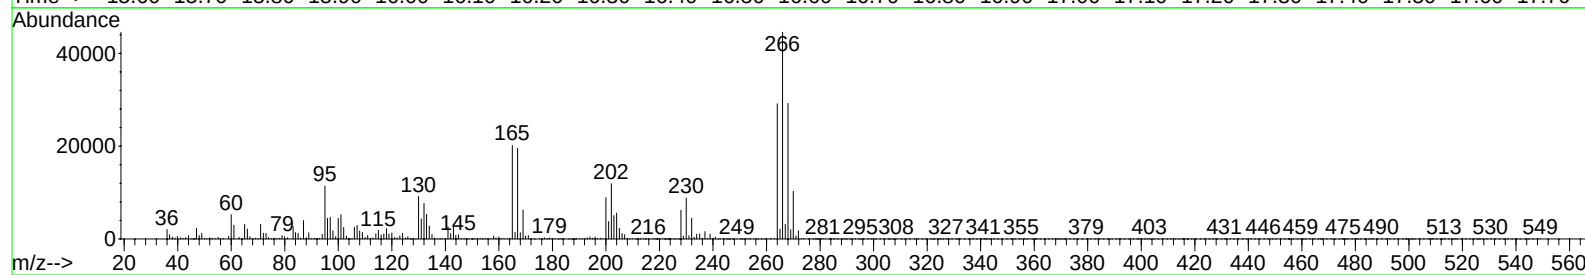


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072420\
Data File : BP002852.D
Acq On : 24 Jul 2020 13:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 15:50:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

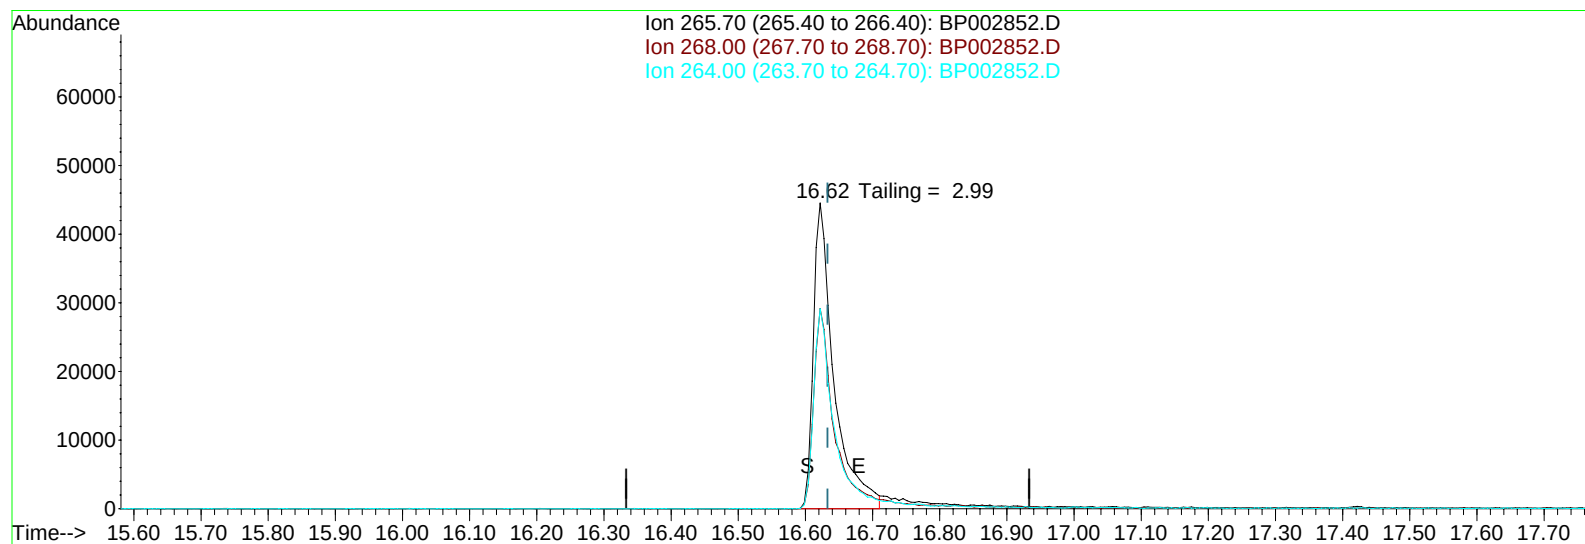

(70) Pentachlorophenol (C)




16.622min (-0.012) 1248213.62ng

response 99310

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	65.54
264.00	60.70	65.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072420\
 Data File : BP002852.D
 Acq On : 24 Jul 2020 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 15:50:31 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

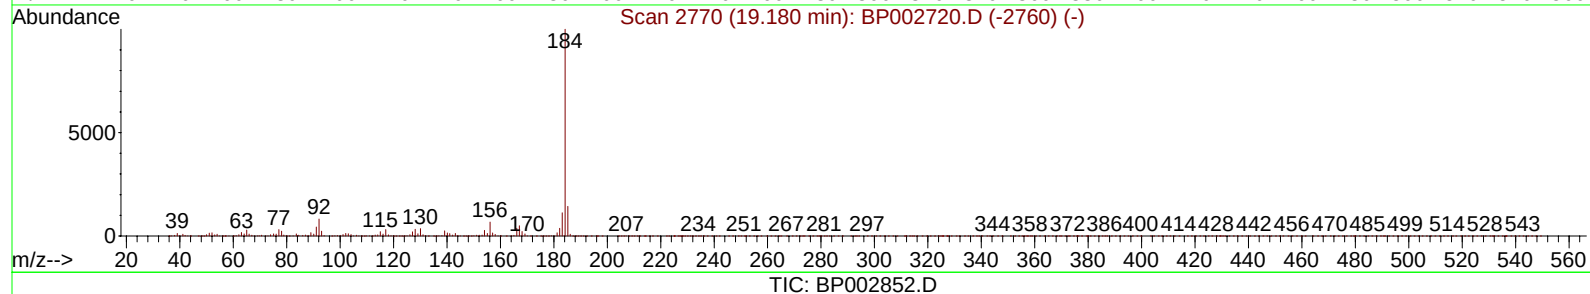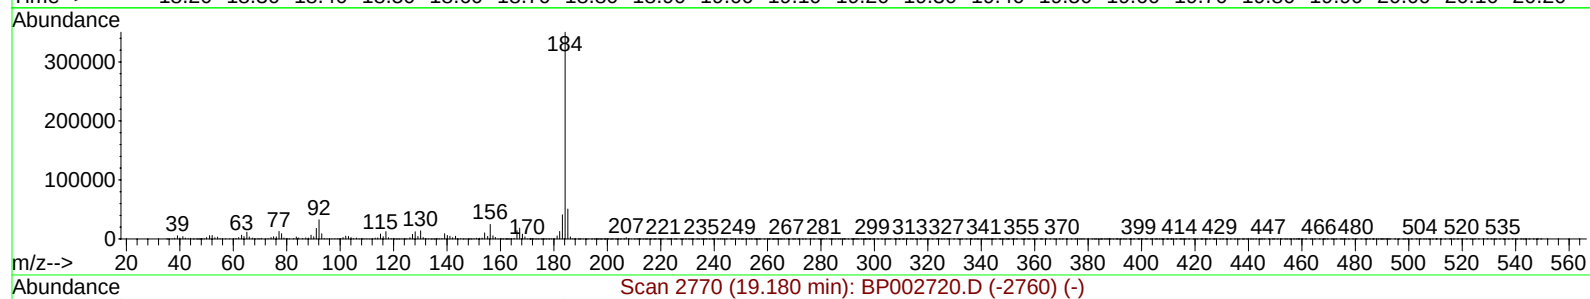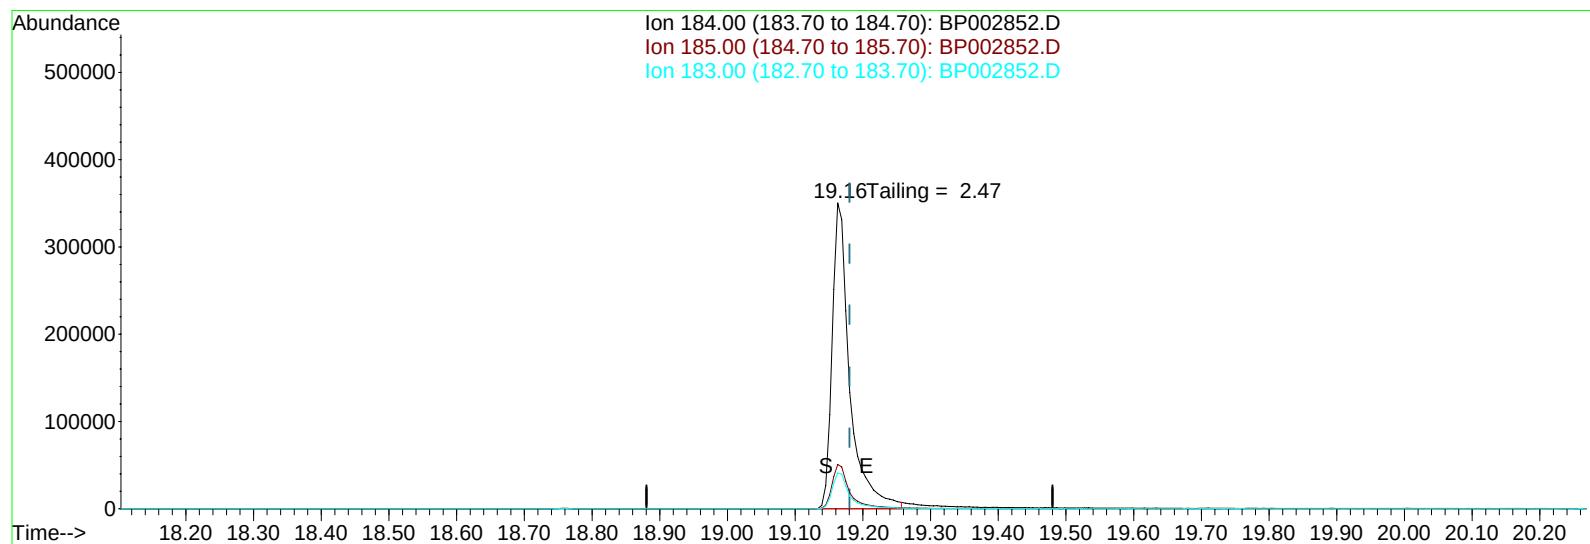

TIC: BP002852.D

(77) Benzidine

19.163min (-0.017) 1221479.57ng

response 635811

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.48
183.00	11.20	11.72
0.00	0.00	0.00