

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072420\
 Data File : BP002861.D
 Acq On : 24 Jul 2020 19:23
 Operator : CG/JU
 Sample : L3382-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CTR-005

Quant Time: Jul 25 00:15:36 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 24 15:50:46 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.53	152	58558	20.00	ng	0.00
21) Naphthalene-d8	10.31	136	222839	20.00	ng	0.00
39) Acenaphthene-d10	14.19	164	143860	20.00	ng	0.00
64) Phenanthrene-d10	16.95	188	352666	20.00	ng	0.00
76) Chrysene-d12	21.06	240	471973	20.00	ng	0.00
86) Perylene-d12	23.23	264	572353	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.16	112	469910	135.39	ng	0.00
7) Phenol-d6	6.74	99	543524	109.73	ng	0.00
23) Nitrobenzene-d5	8.68	82	420769	100.99	ng	0.00
42) 2,4,6-Tribromophenol	15.69	330	245367	163.40	ng	0.00
45) 2-Fluorobiphenyl	12.80	172	810973	87.21	ng	0.00
79) Terphenyl-d14	19.53	244	1688057	82.00	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072420\
Data File : BP002861.D
Acq On : 24 Jul 2020 19:23
Operator : CG/JU
Sample : L3382-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CTR-005

Quant Time: Jul 25 00:15:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 24 15:50:46 2020
Response via : Initial Calibration

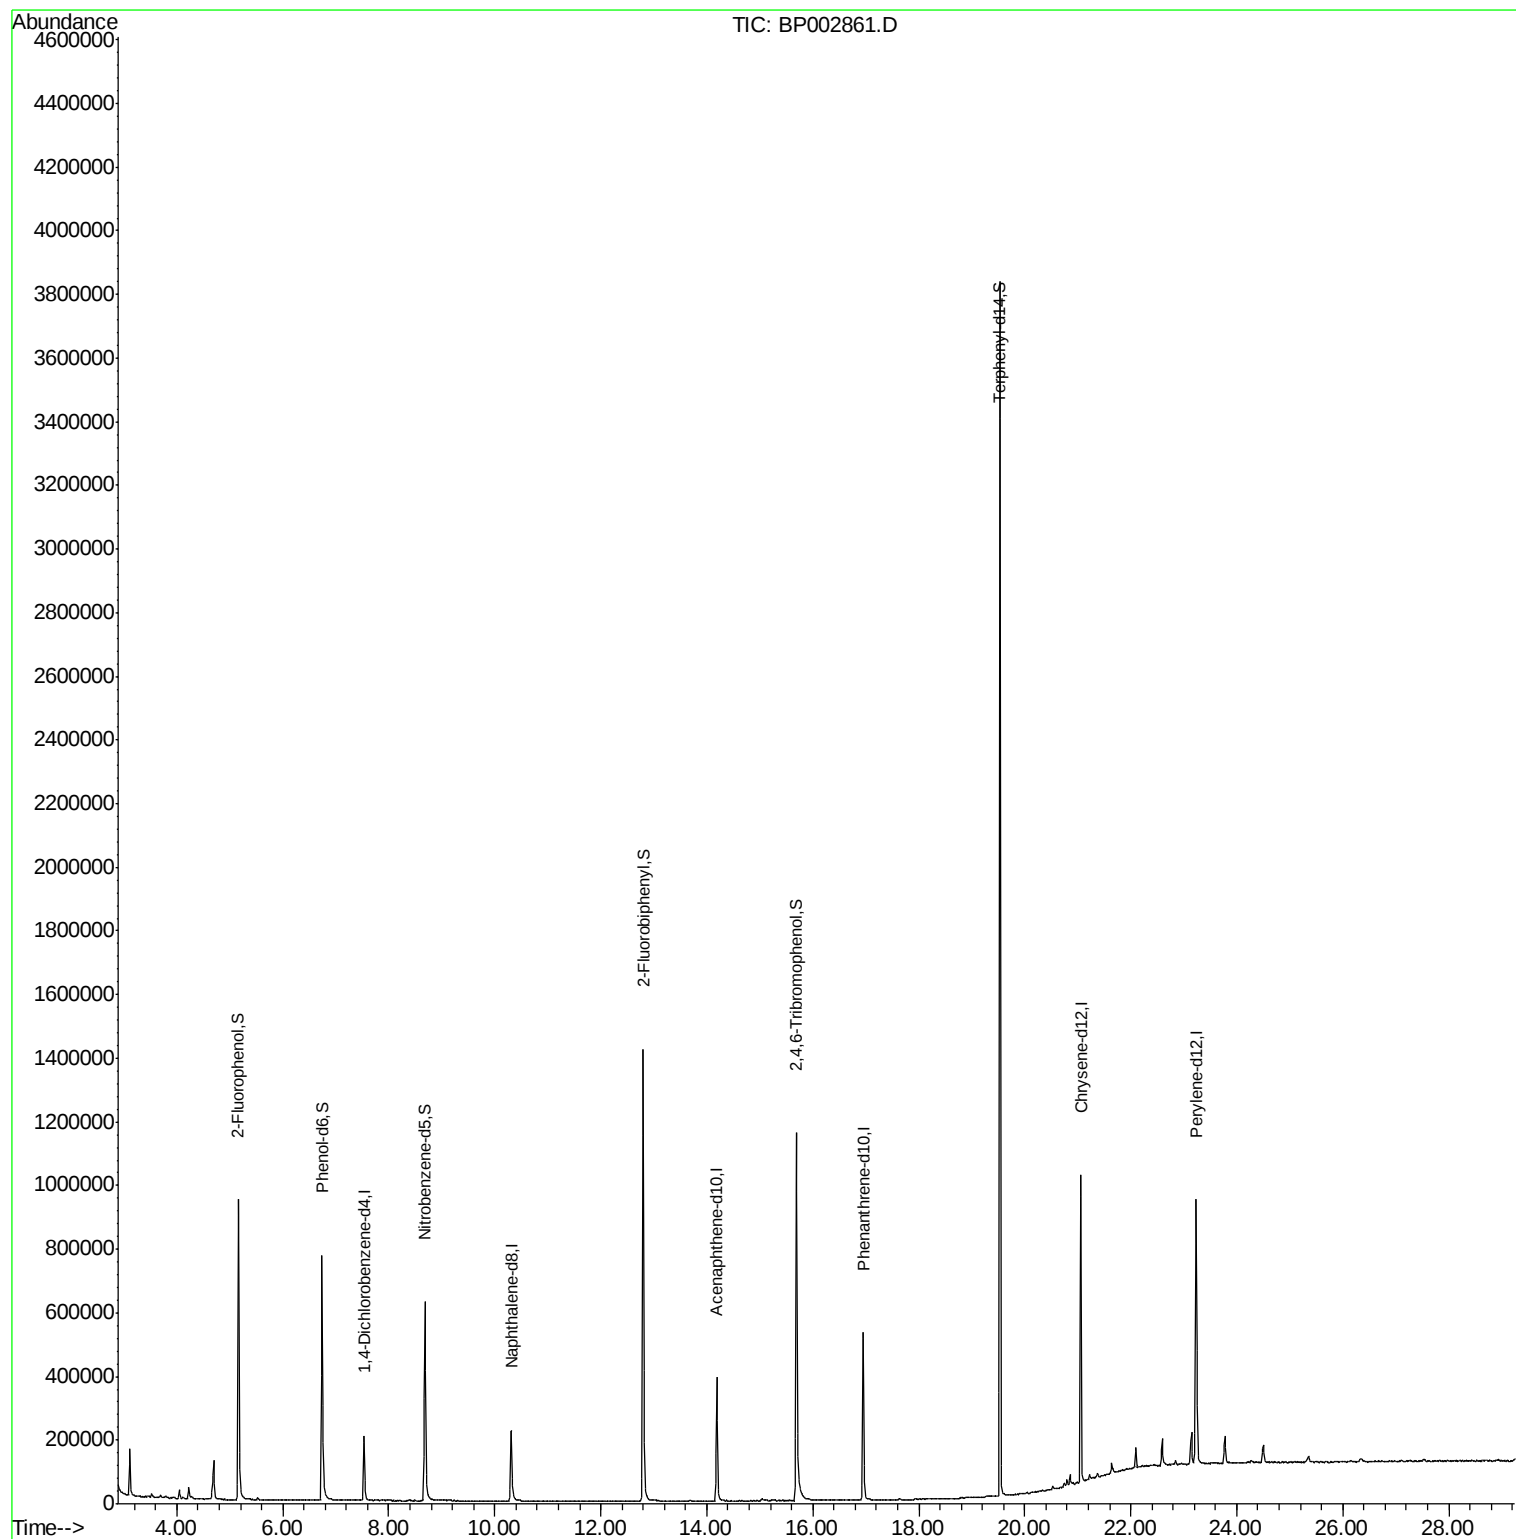







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.53 min Scan# 790
Delta R.T. -0.00 min
Lab File: BP002861.D
Acq: 24 Jul 2020 19:23

Instrument :
BNA_P
ClientSampleId :
CTR-005




Tot Ion	Ratio	Lower	Upper
152	100		
150	152.8	122.5	183.7
115	57.3	48.5	72.7

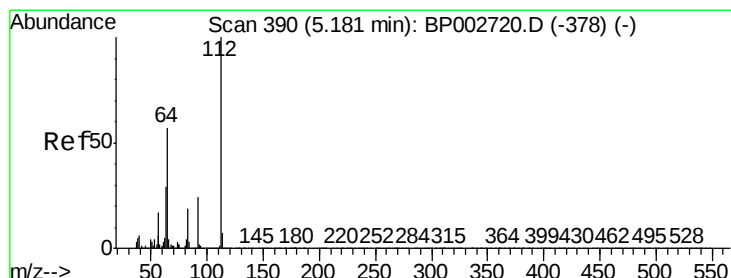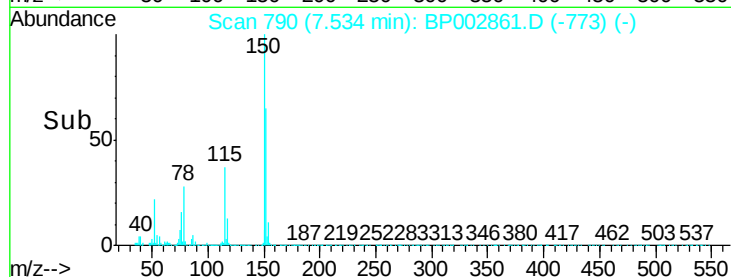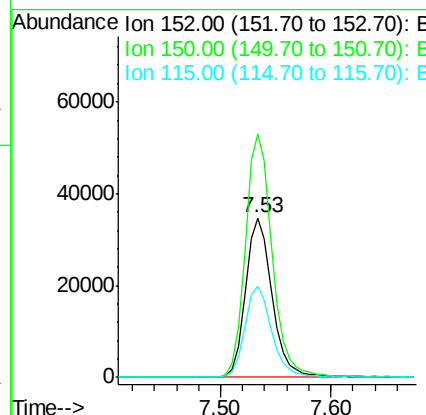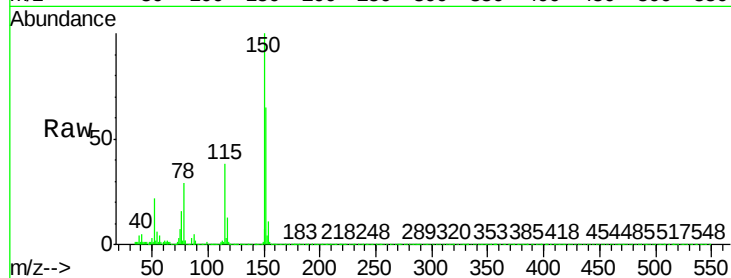


#5

2-Fluorophenol
Concen: 135.392 ng
RT: 5.16 min Scan# 387
Delta R.T. -0.00 min
Lab File: BP002861.D
Acq: 24 Jul 2020 19:23

Tgt Ion	Ratio	Lower	Upper
112	100		
64	58.5	48.1	72.1
63	31.1	24.9	37.3

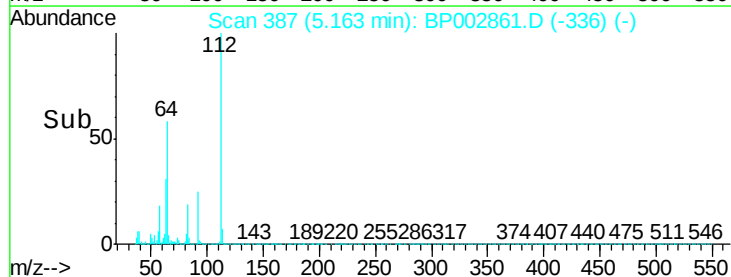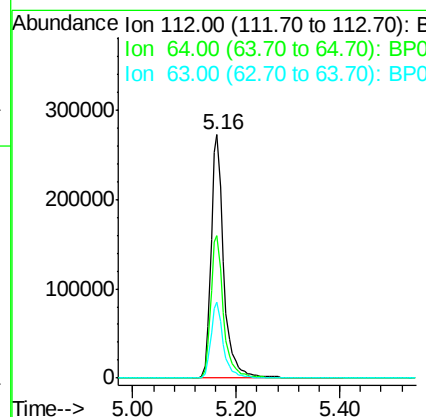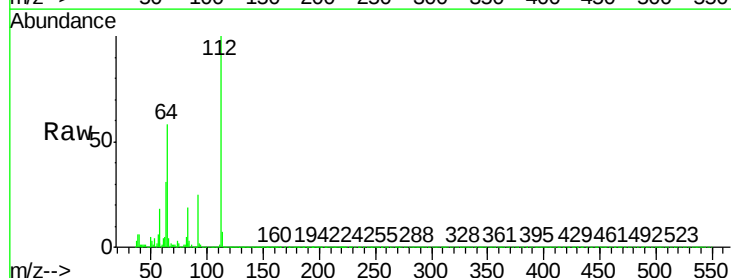

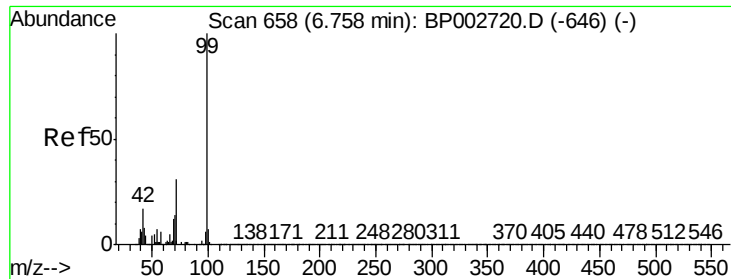

#7

Phenol-d6

Concen: 109.729 ng

RT: 6.74 min Scan# 655

Delta R.T. -0.00 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23

Instrument :

BNA_P

ClientSampleId :

CTR-005


Tot Ion: 99 Resp: 543524

Ion Ratio Lower Upper

99 100

42 17.8 14.2 21.4




71 32.7 26.1 39.1

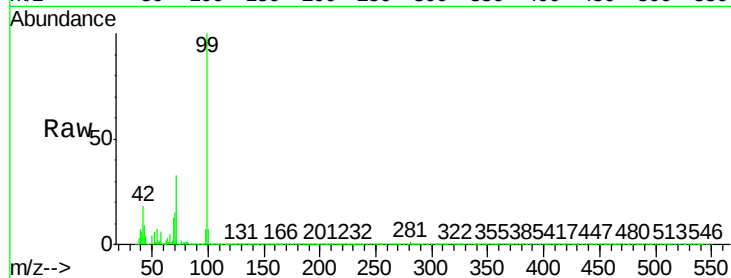

Abundance Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

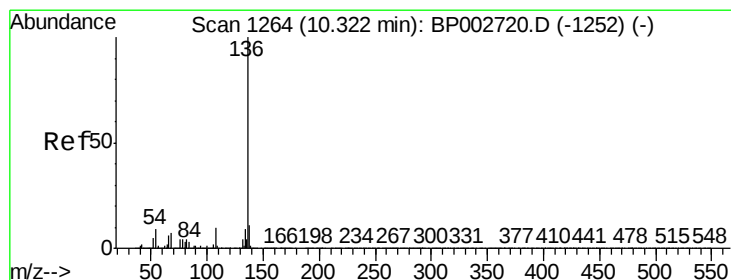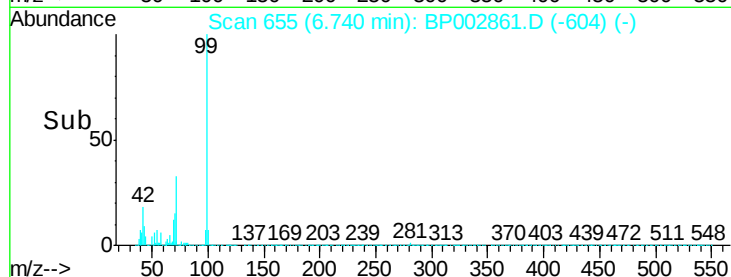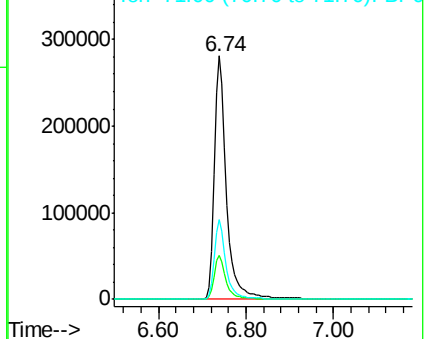

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.31 min Scan# 1262

Delta R.T. 0.01 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23

Tgt Ion: 136 Resp: 222839


Ion Ratio Lower Upper

136 100

137 10.7 8.8 13.2

54 8.7 7.3 10.9

68 7.0 5.7 8.5


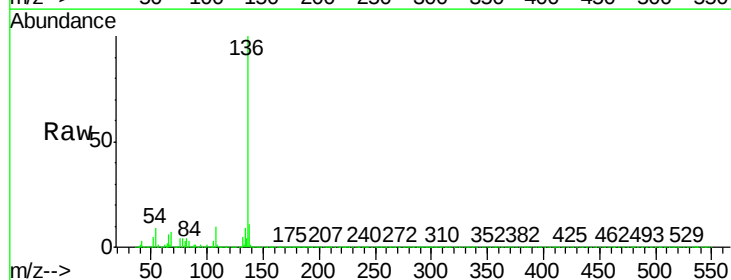



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0



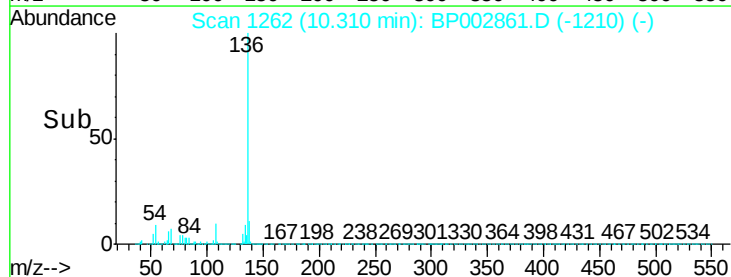
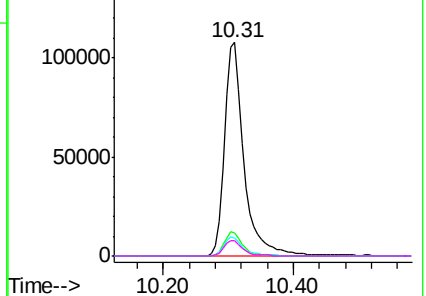


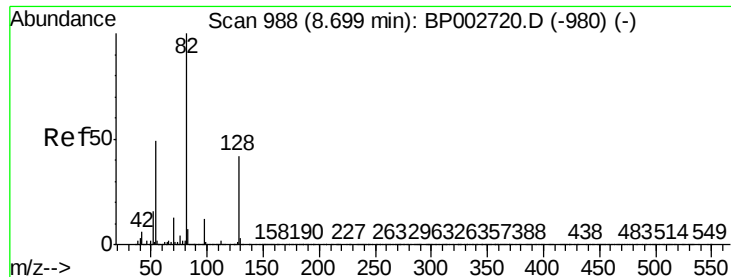

#23
 Nitrobenzene-d5
 Concen: 100.989 ng
 RT: 8.68 min Scan# 985
 Delta R.T. -0.00 min
 Lab File: BP002861.D
 Acq: 24 Jul 2020 19:23




Instrument :
 BNA_P
 ClientSampleId :
 CTR-005


Tot Ion	82	Resp	420769
Ion Ratio	Lower	Upper	
82	100		
128	40.0	32.6	49.0
54	48.8	38.9	58.3

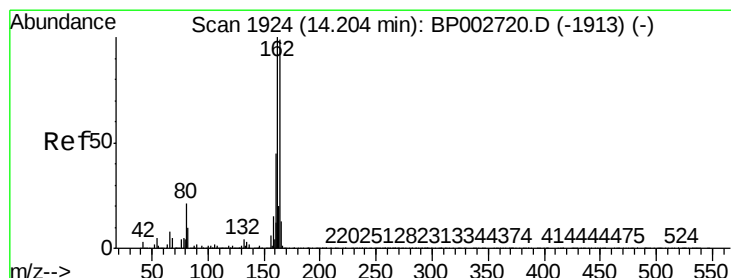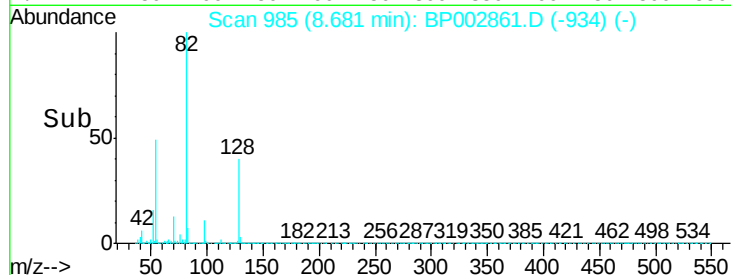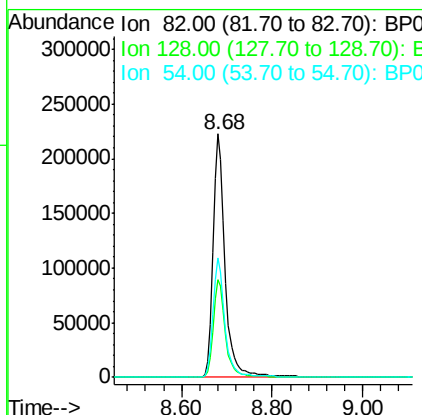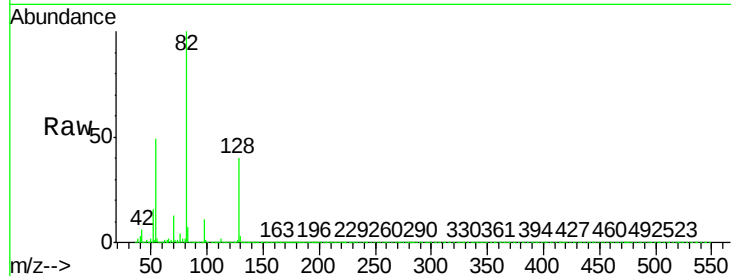

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.19 min Scan# 1921
 Delta R.T. -0.00 min
 Lab File: BP002861.D
 Acq: 24 Jul 2020 19:23

Tgt Ion	164	Resp	143860
Ion Ratio	Lower	Upper	
164	100		
162	100.6	78.4	117.6
160	47.3	36.1	54.1


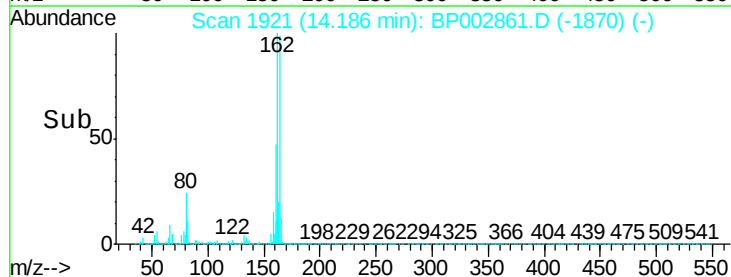
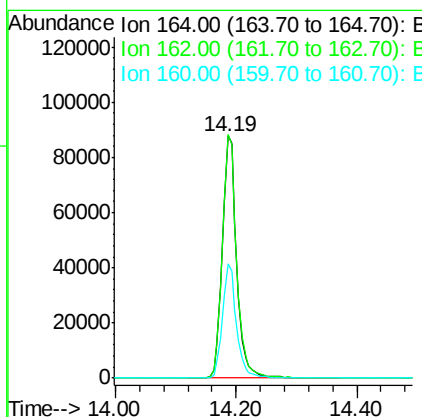
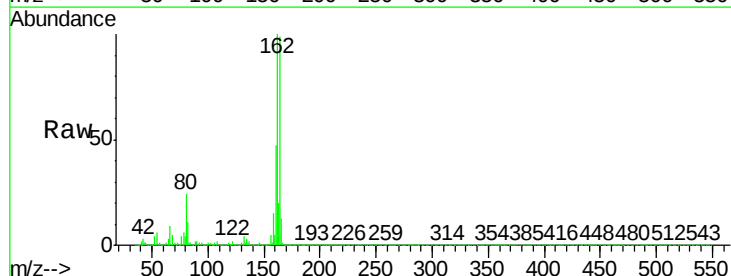


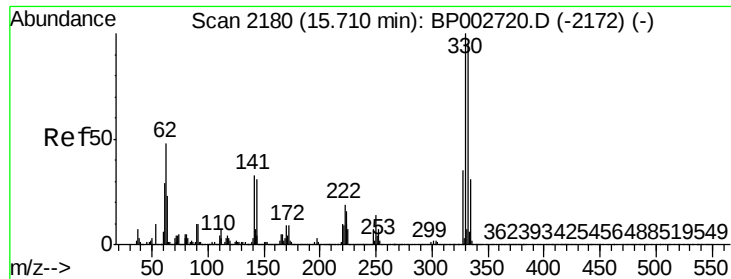

#42
 2,4,6-Tribromophenol
 Concen: 163.396 ng
 RT: 15.69 min Scan# 2177
 Delta R.T. -0.00 min
 Lab File: BP002861.D
 Acq: 24 Jul 2020 19:23




Instrument :
 BNA_P
 ClientSampleId :
 CTR-005


Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	77.6	116.4
141	36.8	29.0	43.6

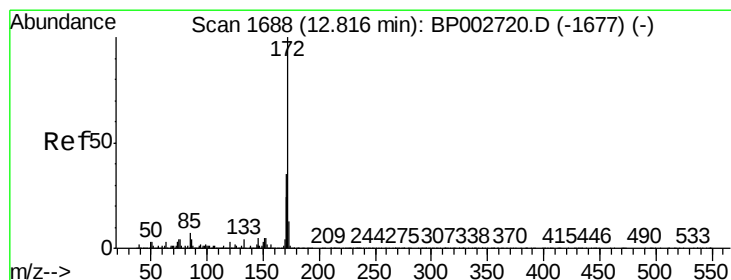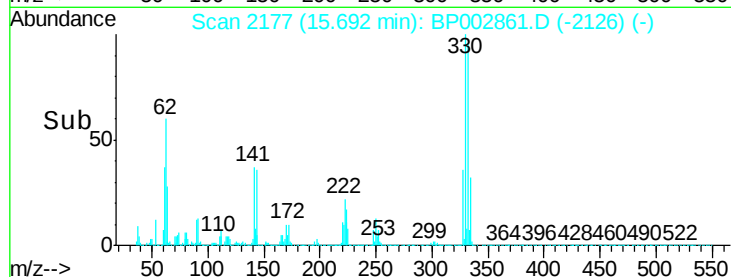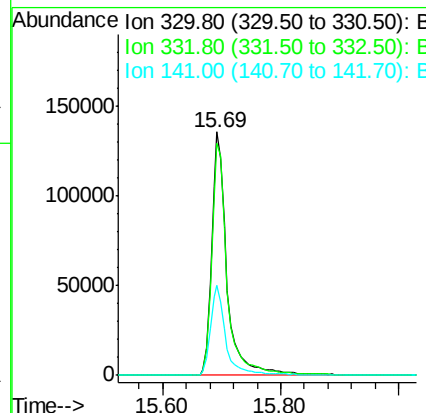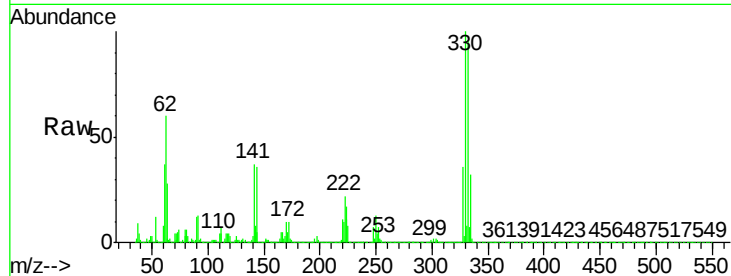

#45
 2-Fluorobiphenyl
 Concen: 87.207 ng
 RT: 12.80 min Scan# 1685
 Delta R.T. -0.00 min
 Lab File: BP002861.D
 Acq: 24 Jul 2020 19:23

Tgt Ion	Ratio	Lower	Upper
172	100		
171	33.8	27.0	40.4
170	24.1	19.4	29.2

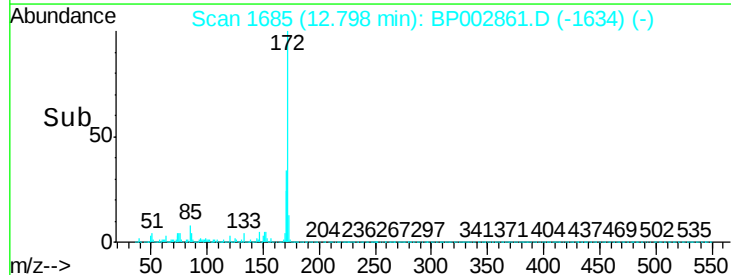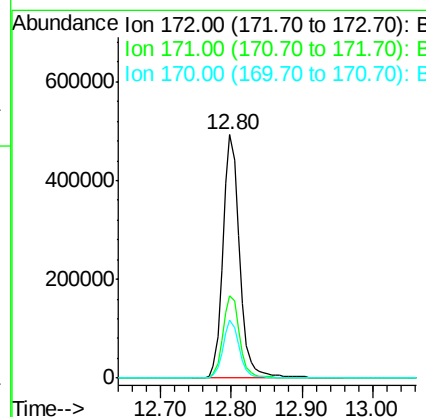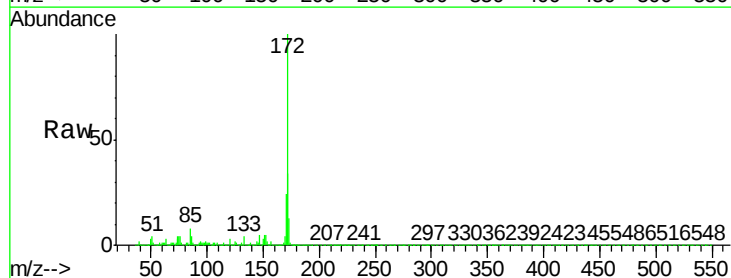

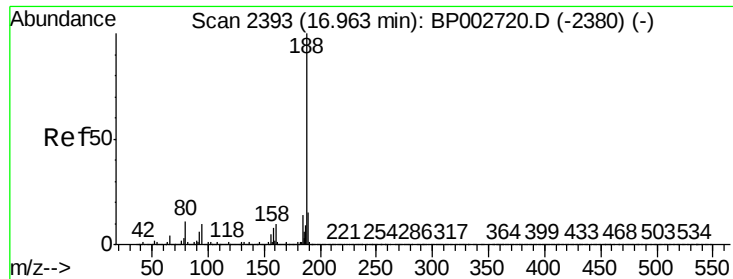

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.95 min Scan# 2391

Delta R.T. 0.01 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23

Instrument :

BNA_P

ClientSampled :

CTR-005


Tot Ion:188 Resp: 352666

Ion Ratio Lower Upper

188 100

94 10.4 8.5 12.7




80 10.7 9.0 13.4

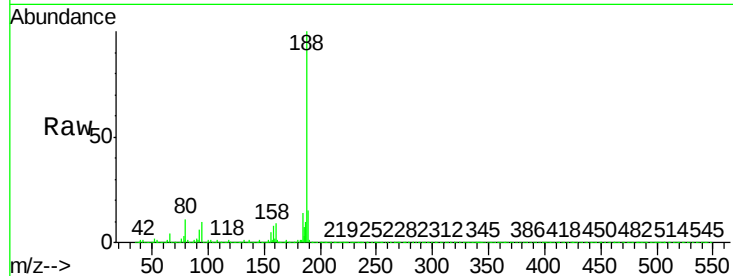

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0

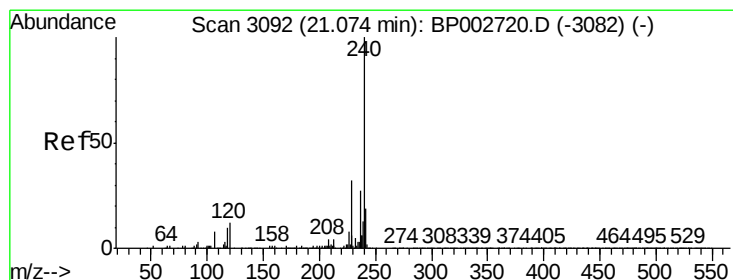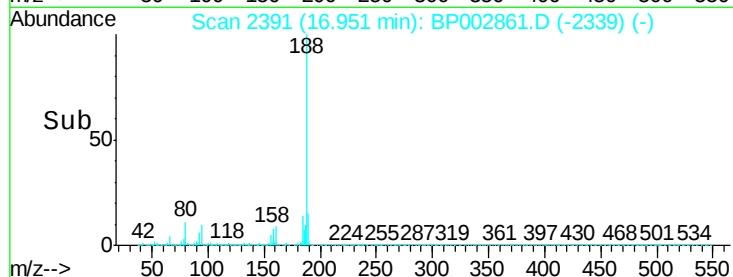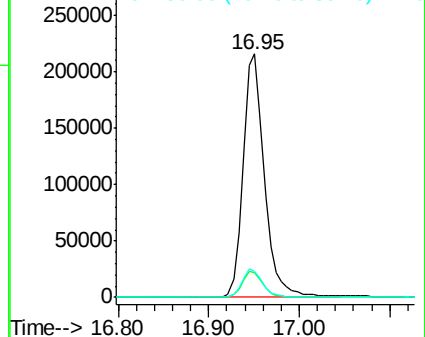

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.06 min Scan# 3089

Delta R.T. -0.00 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23


Tgt Ion:240 Resp: 471973

Ion Ratio Lower Upper

240 100

120 11.3 9.2 13.8



236 25.3 20.3 30.5

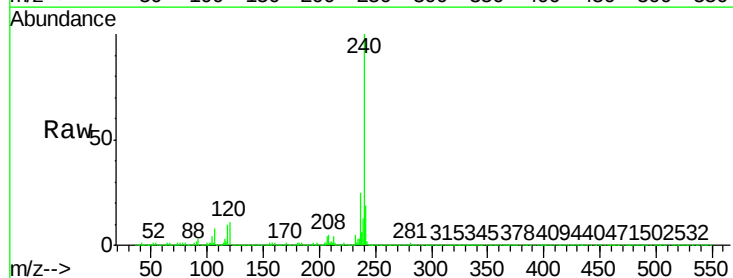


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

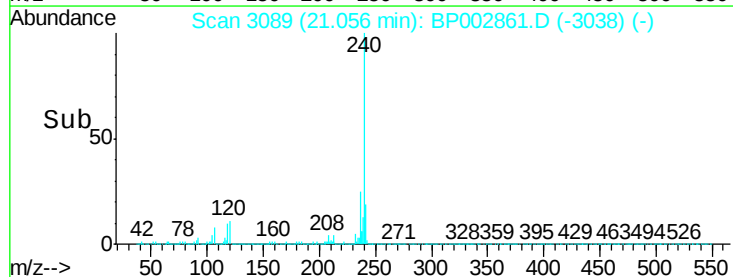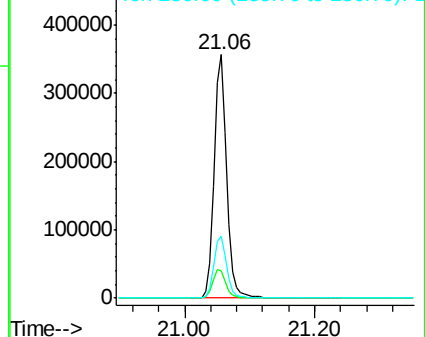

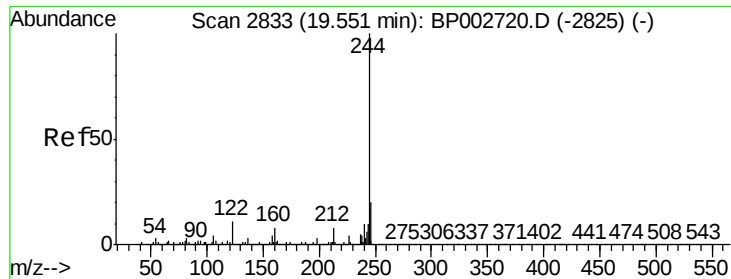

#79

Terphenyl-d14

Concen: 82.001 ng

RT: 19.53 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23

Instrument :


BNA_P

ClientSampleId :

CTR-005

Tot Ion:244 Resp: 1688057


Ion	Ratio	Lower	Upper
244	100		
212	8.1	5.8	8.8
122	11.3	7.9	11.9

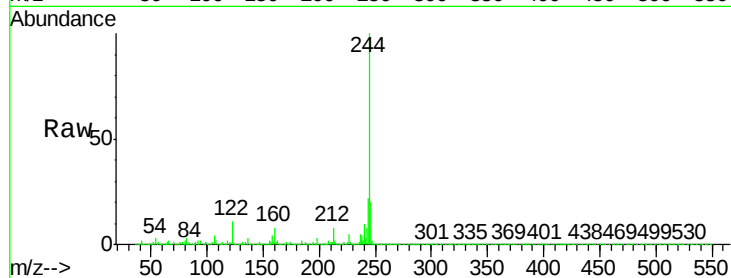

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E


Ion 122.00 (121.70 to 122.70): E

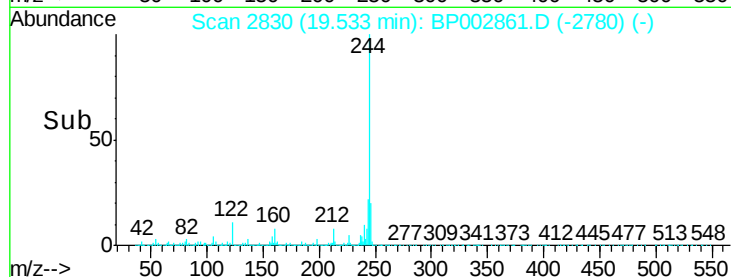

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

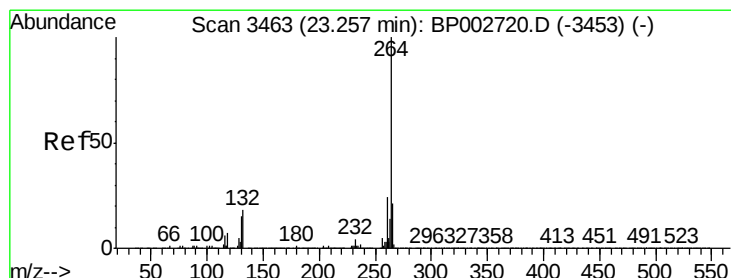

#86

Perylene-d12

Concen: 20.000 ng

RT: 23.23 min Scan# 3459


Delta R.T. -0.00 min

Lab File: BP002861.D

Acq: 24 Jul 2020 19:23

Tgt Ion:264 Resp: 572353


Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.6	29.4
265	20.8	16.7	25.1

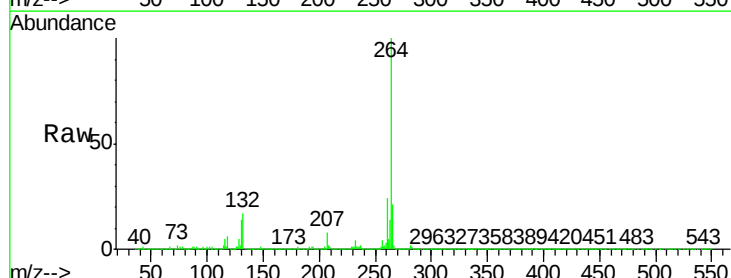

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

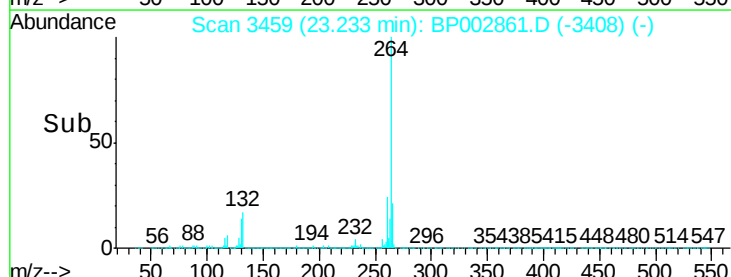

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E