


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072420\
 Data File : BP002852.D
 Acq On : 24 Jul 2020 13:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 24 15:50:46 2020

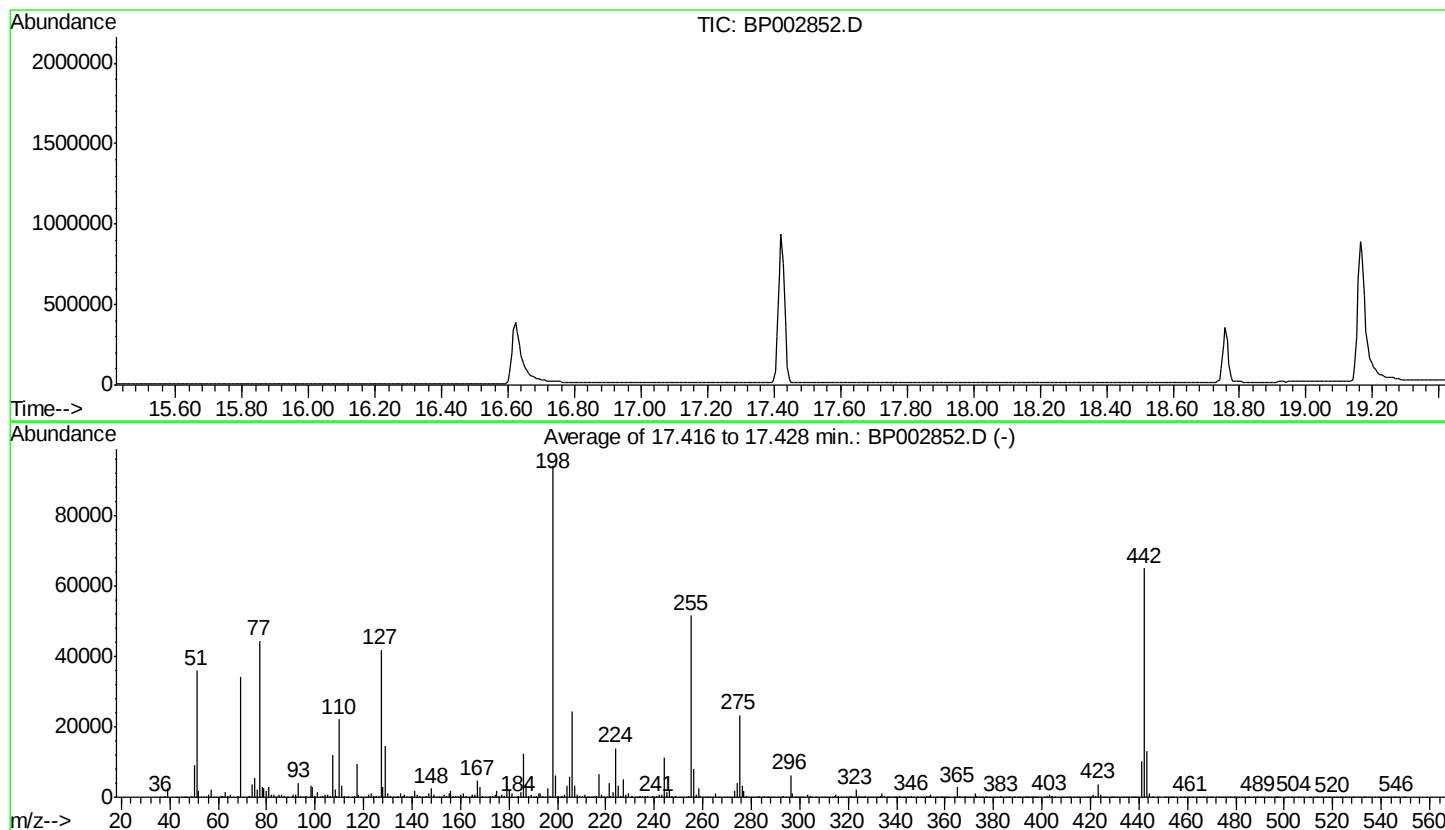

AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	35818	PASS
68	69	0.00	2	1.4	493	PASS
69	198	0.00	100	36.4	34273	PASS
70	69	0.00	2	0.6	192	PASS
127	198	10	80	44.4	41794	PASS
197	198	0.00	2	0.5	430	PASS
198	198	100	100	100.0	94091	PASS
199	198	5	9	6.7	6258	PASS
275	198	10	60	24.8	23304	PASS
365	198	1	100	2.9	2761	PASS
441	198	0.01	100	10.7	10074	PASS
442	198	50	100	69.1	65001	PASS
443	442	15	24	20.2	13143	PASS