

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072421\
 Data File : BP006293.D
 Acq On : 23 Jul 2021 18:43
 Operator : CG/JU
 Sample : SSTD01002
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602

Quant Time: Jul 24 02:44:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 02:41:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	257026	20.00	ng/ul	0.00
20) Naphthalene-d8	10.58	136	1138138	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.42	164	669856	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.17	188	1313586	20.00	ng/ul	0.00
79) Chrysene-d12	21.27	240	1226572	20.00	ng/ul	0.00
88) Perylene-d12	23.62	264	1247485	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	28583	4.40	ng/uL	0.00
4) Pyridine-d5	3.71	84	194553	12.26	ng/ul	0.00
7) Phenol-d5	6.96	99	231432	11.09	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.13	67	151213	13.74	ng/ul	0.00
11) 2-Chlorophenol-d4	7.33	132	181224	10.80	ng/ul	0.00
15) 4-Methylphenol-d8	8.50	113	181339	10.95	ng/ul	0.00
21) Nitrobenzene-d5	8.95	128	83232	9.57	ng/ul	0.00
24) 2-Nitrophenol-d4	9.66	143	75389	7.66	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.20	165	160246	8.47	ng/ul	0.00
31) 4-Chloroaniline-d4	10.72	131	263593	10.24	ng/ul	0.00
46) Dimethylphthalate-d6	13.84	166	494981	9.68	ng/ul	0.00
49) Acenaphthylene-d8	14.11	160	595885	9.97	ng/ul	0.00
54) 4-Nitrophenol-d4	14.62	143	83170	9.24	ng/ul	0.00
60) Fluorene-d10	15.42	176	419042	9.46	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.53	200	58357	6.36	ng/ul	0.00
73) Anthracene-d10	17.27	188	609837	9.87	ng/ul	0.00
81) Pyrene-d10	19.51	212	644128	10.57	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.46	264	640161	9.54	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.33	88	29605	4.394	ng/uL 96
5) Pyridine	3.73	79	210153	12.836	ng/ul 96
6) Benzaldehyde	6.94	77	116357	10.724	ng/ul 99
8) Phenol	6.99	94	242063	11.116	ng/ul 99
10) Bis(2-Chloroethyl)ether	7.23	93	195742	11.829	ng/ul 99
12) 2-Chlorophenol	7.36	128	184774	10.528	ng/ul 97
13) 2-Methylphenol	8.23	108	172563	10.407	ng/ul 98
14) 2,2'-oxybis(1-Chloropropan	8.33	45	220758	13.425	ng/ul 98
16) Acetophenone	8.62	105	294584	10.830	ng/ul 97
17) N-Nitroso-di-n-propylamine	8.60	70	156587	12.401	ng/ul 98
18) 4-Methylphenol	8.56	108	187212	10.603	ng/ul 98
19) Hexachloroethane	8.86	117	75674	9.972	ng/ul 98
22) Nitrobenzene	8.99	77	223251	10.055	ng/ul 99
23) Isophorone	9.52	82	392635	9.990	ng/ul 99
25) 2-Nitrophenol	9.70	139	85516	7.978	ng/ul 96
26) 2,4-Dimethylphenol	9.76	107	215648	9.600	ng/ul 99
27) Bis(2-Chloroethoxy)methane	10.00	93	260647	11.147	ng/ul 99
29) 2,4-Dichlorophenol	10.23	162	156730	8.420	ng/ul 99
30) Naphthalene	10.63	128	617810	9.852	ng/ul 100
32) 4-Chloroaniline	10.74	127	262728	10.094	ng/ul 100
33) Hexachlorobutadiene	10.92	225	98643	7.008	ng/ul 97
34) Caprolactam	11.52	113	46355	7.540	ng/ul 98

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072421\
 Data File : BP006293.D
 Acq On : 23 Jul 2021 18:43
 Operator : CG/JU
 Sample : SSTD01002
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602

Quant Time: Jul 24 02:44:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 02:41:40 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.86	107	185216	9.365	ng/ul	99
36) 2-Methylnaphthalene	12.24	142	419482	9.520	ng/ul	98
37) 1-Methylnaphthalene	12.46	142	420401	9.469	ng/ul	98
39) 1,2,4,5-Tetrachlorobenzene	12.60	216	183697	7.629	ng/ul	98
40) Hexachlorocyclopentadiene	12.59	237	105677	6.914	ng/ul	98
41) 2,4,6-Trichlorophenol	12.85	196	110640	7.411	ng/ul	98
42) 2,4,5-Trichlorophenol	12.92	196	122036	7.582	ng/ul	97
43) 1,1'-Biphenyl	13.26	154	524708	9.841	ng/ul	100
44) 2-Chloronaphthalene	13.29	162	395205	9.422	ng/ul	99
45) 2-Nitroaniline	13.50	65	105518	9.477	ng/ul	96
47) Dimethylphthalate	13.89	163	487255	9.255	ng/ul	100
48) 2,6-Dinitrotoluene	14.00	165	79974	7.499	ng/ul	90
50) Acenaphthylene	14.14	152	591475	9.649	ng/ul	99
51) 3-Nitroaniline	14.33	138	81500	8.227	ng/ul	98
52) Acenaphthene	14.48	153	437369	9.950	ng/ul	98
53) 2,4-Dinitrophenol	14.53	184	36572	5.231	ng/ul	99
55) 4-Nitrophenol	14.63	109	70782	8.351	ng/ul	97
56) Dibenzofuran	14.82	168	590296	9.324	ng/ul	99
57) 2,4-Dinitrotoluene	14.79	165	115132	7.638	ng/ul	99
58) 2,3,4,6-Tetrachlorophenol	15.05	232	92928	6.470	ng/ul	98
59) Diethylphthalate	15.26	149	501937	9.723	ng/ul	100
61) Fluorene	15.47	166	482944	9.229	ng/ul	100
62) 4-Chlorophenyl-phenylether	15.47	204	223880	7.888	ng/ul	99
63) 4-Nitroaniline	15.49	138	77966	8.011	ng/ul	98
66) 4,6-Dinitro-2-methylphenol	15.55	198	57355	6.217	ng/ul	100
67) N-Nitrosodiphenylamine	15.69	169	402969	10.216	ng/ul	99
68) 4-Bromophenyl-phenylether	16.37	248	105272	6.828	ng/ul	99
69) Hexachlorobenzene	16.47	284	144440	8.350	ng/ul	98
70) Atrazine	16.65	200	131326	8.198	ng/ul	98
71) Pentachlorophenol	16.82	266	74980	6.597	ng/ul	97
72) Phenanthrene	17.21	178	733162	9.828	ng/ul	99
74) Anthracene	17.30	178	744431	9.879	ng/ul	100
75) 1,2,3,4-Tetrachlorobenzene	13.22	216	182810	8.283	ng/ul	98
76) Pentachlorobenzene	14.73	250	178081	8.045	ng/ul	99
77) Carbazole	17.57	167	663667	10.031	ng/ul	100
78) Di-n-butylphthalate	18.15	149	772699	10.250	ng/ul	99
80) Fluoranthene	19.19	202	798432	10.434	ng/ul	99
82) Pyrene	19.54	202	841595	10.635	ng/ul	100
83) Butylbenzylphthalate	20.43	149	313116	10.998	ng/ul	99
84) 3,3'-Dichlorobenzidine	21.19	252	241047	8.552	ng/ul	100
85) Benzo(a)anthracene	21.25	228	789414	9.969	ng/ul	100
86) Bis(2-ethylhexyl)phthalate	21.20	149	499685	11.504	ng/ul	100
87) Chrysene	21.30	228	753608	9.703	ng/ul	100
89) Di-n-octyl phthalate	22.11	149	795739	9.945	ng/ul	100
90) Benzo(b)fluoranthene	22.90	252	823812	9.848	ng/ul	99
91) Benzo(k)fluoranthene	22.95	252	763923	9.207	ng/ul	99
93) Benzo(a)pyrene	23.51	252	706848	9.614	ng/ul	99
94) Indeno(1,2,3-cd)pyrene	26.04	276	896286	9.646	ng/ul	99
95) Dibenzo(a,h)anthracene	26.07	278	765830	9.856	ng/ul	98
96) Benzo(g,h,i)perylene	26.79	276	743151	9.518	ng/ul	97

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP072421\
Data File : BP006293.D
Acq On : 23 Jul 2021 18:43
Operator : CG/JU
Sample : SSTD01002
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Quant Time: Jul 24 02:44:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 02:41:40 2021
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072421\
Data File : BP006293.D
Acq On : 23 Jul 2021 18:43
Operator : CG/JU
Sample : SSTD01002
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampled :
SSTD010602

Quant Time: Jul 24 02:44:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 02:41:40 2021
Response via : Initial Calibration

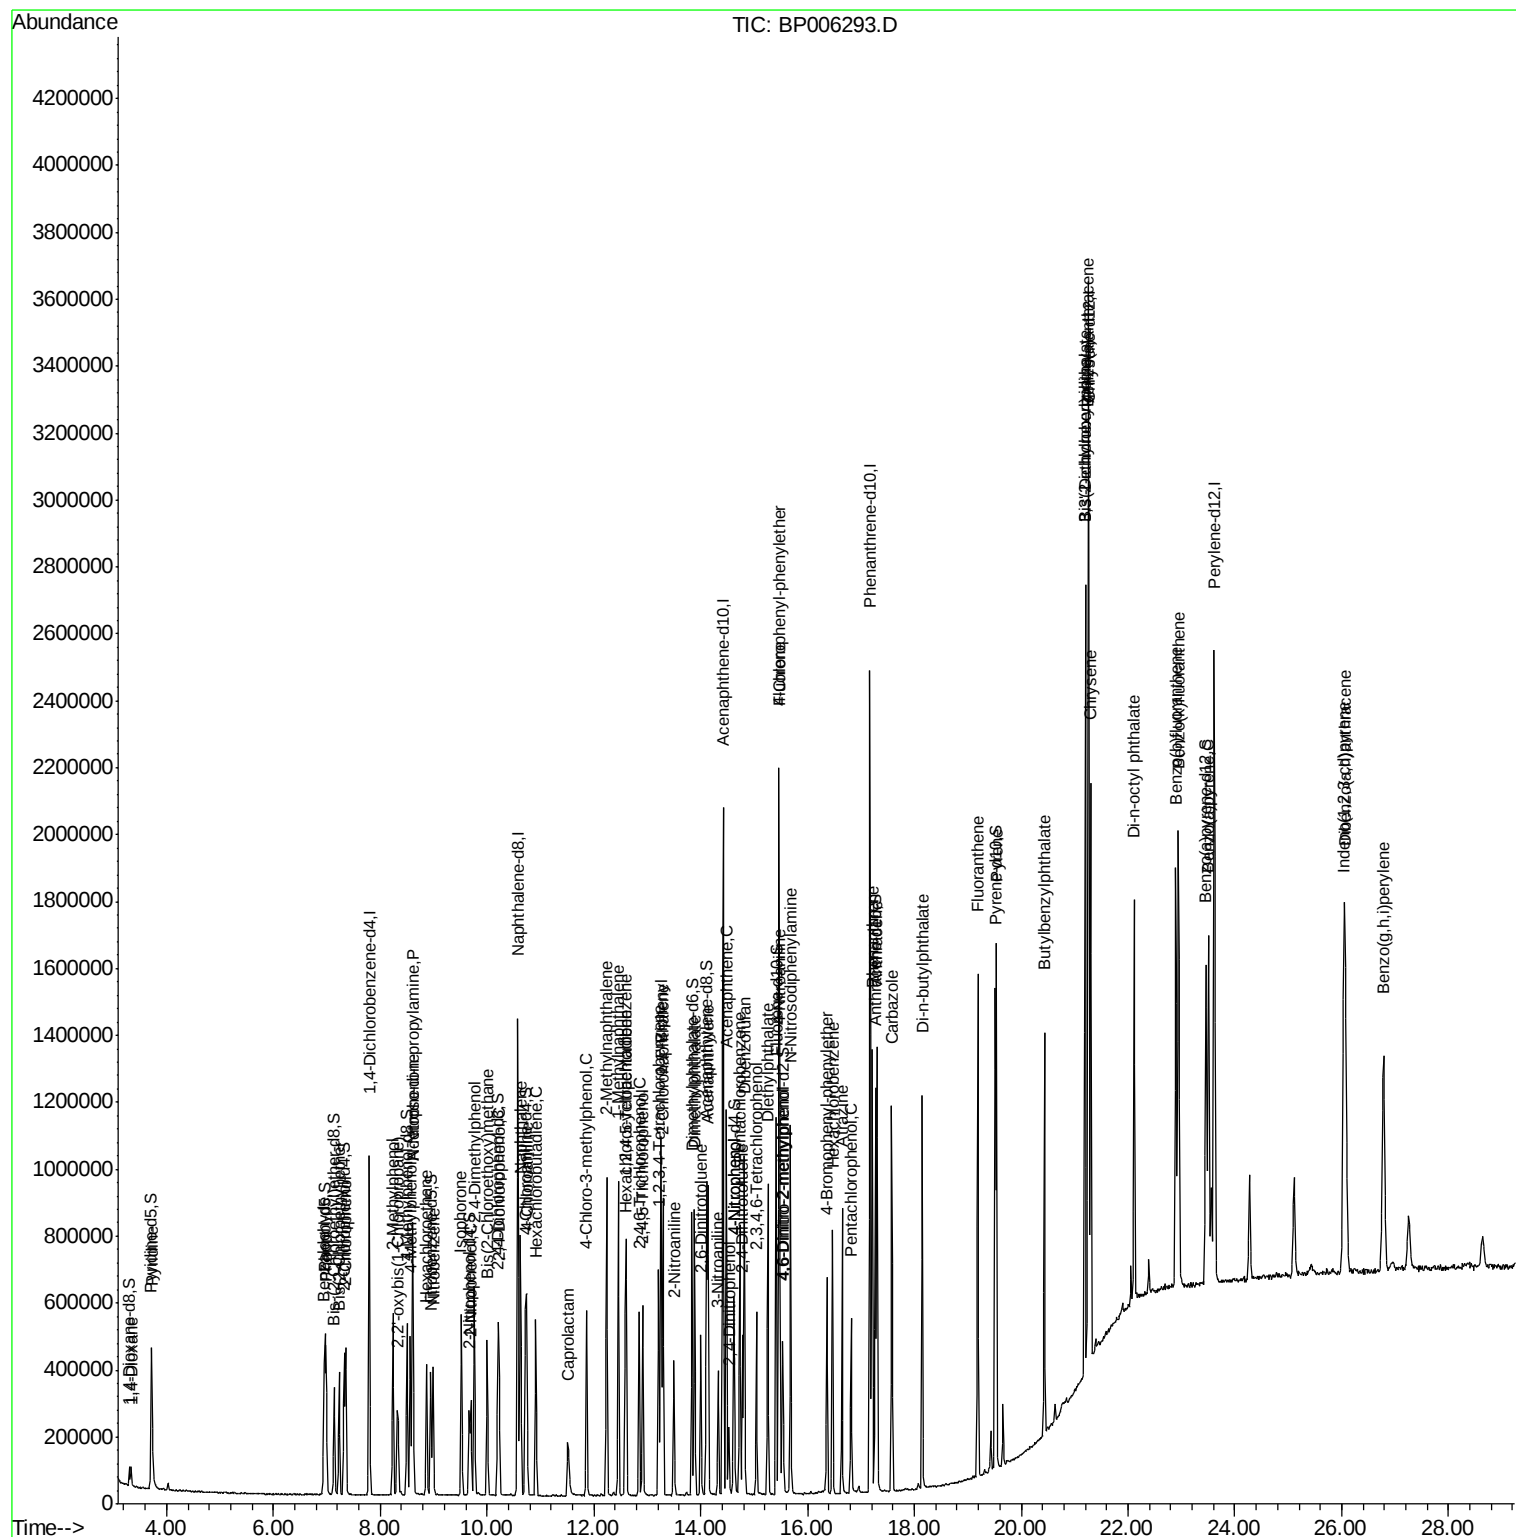

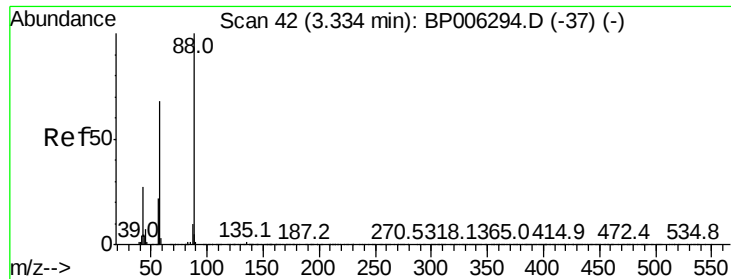

#2

1,4-Dioxane

Concen: 4.394 ng/uL

RT: 3.33 min Scan# 42

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion: 88 Resp: 29605

Ion	Ratio	Lower	Upper
88	100		
43	23.8	22.4	33.6
58	69.1	54.2	81.4

88 100

43 23.8 22.4 33.6

58 69.1 54.2 81.4






Abundance

Ion 88.00 (87.70 to 88.70): BP0

Ion 43.00 (42.70 to 43.70): BP0

Ion 58.00 (57.70 to 58.70): BP0

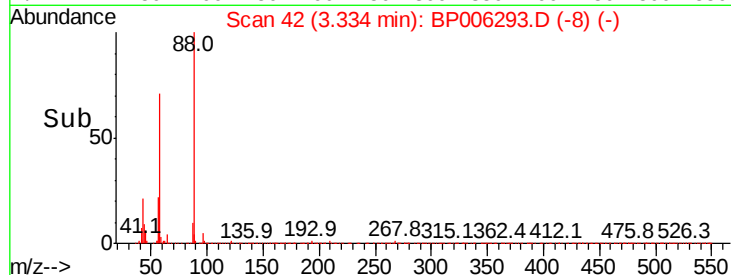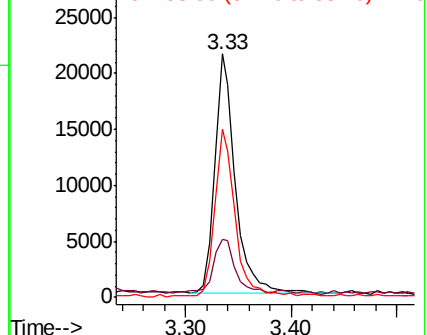

#5

Pyridine

Concen: 12.836 ng/uL

RT: 3.73 min Scan# 109

Delta R.T. 0.01 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion: 79 Resp: 210153

Ion	Ratio	Lower	Upper
79	100		
52	59.3	50.6	75.8
51	29.5	22.8	34.2

79 100

52 59.3 50.6 75.8

51 29.5 22.8 34.2






Abundance

Ion 79.00 (78.70 to 79.70): BP0

Ion 52.00 (51.70 to 52.70): BP0

Ion 51.00 (50.70 to 51.70): BP0

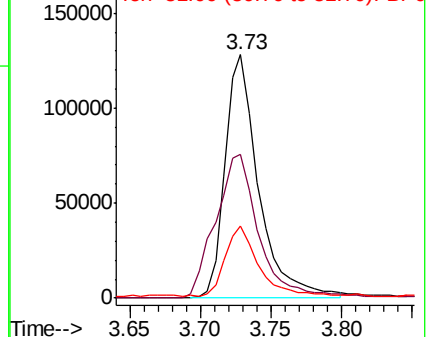

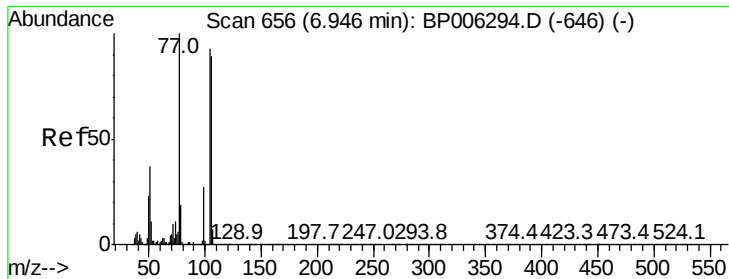

#6

Benzaldehyde

Concen: 10.724 ng/ul

RT: 6.94 min Scan# 655

Delta R.T. -0.01 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602





Tot Ion: 77 Resp: 116357

Ion Ratio Lower Upper

77 100

105 90.9 74.5 111.7

106 89.0 71.0 106.4

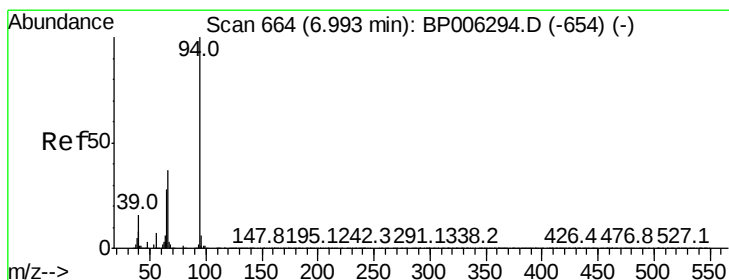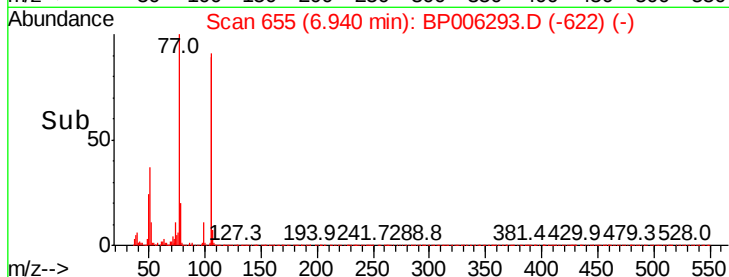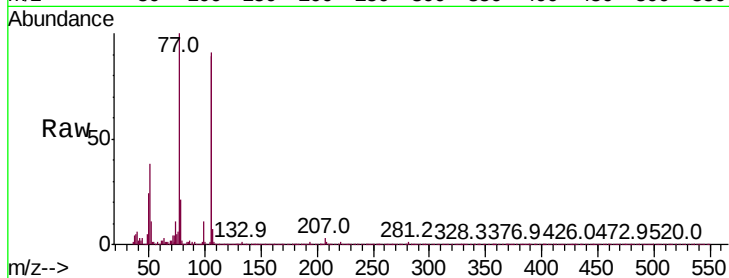

#8

Phenol

Concen: 11.116 ng/ul

RT: 6.99 min Scan# 664

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43




Tgt Ion: 94 Resp: 242063


Ion Ratio Lower Upper

94 100

65 27.2 22.6 33.8

66 36.5 29.5 44.3

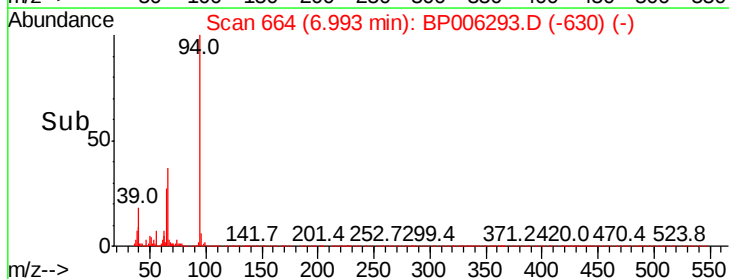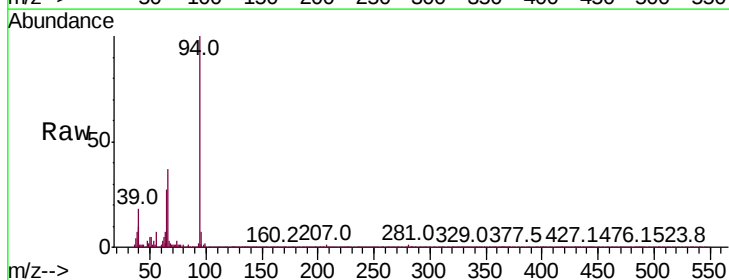



#10

Bis(2-Chloroethyl)ether

Concen: 11.829 ng/ul

RT: 7.23 min Scan# 704

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion: 93 Resp: 195742

Ion Ratio Lower Upper

93 100

63 74.6 60.3 90.5




95 32.5 25.8 38.8



Abundance Ion 93.00 (92.70 to 93.70): BP0

Ion 63.00 (62.70 to 63.70): BP0

Ion 95.00 (94.70 to 95.70): BP0

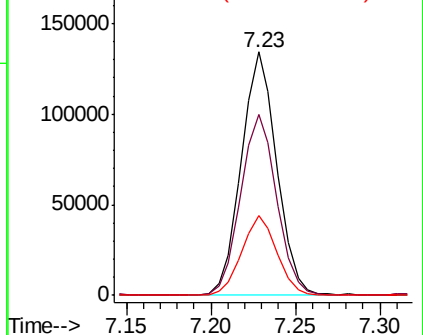

#12

2-Chlorophenol

Concen: 10.528 ng/ul

RT: 7.36 min Scan# 726

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion: 128 Resp: 184774

Ion Ratio Lower Upper

128 100

64 48.6 37.9 56.9



130 34.4 25.4 38.2




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 64.00 (63.70 to 64.70): BP0

Ion 130.00 (129.70 to 130.70): E




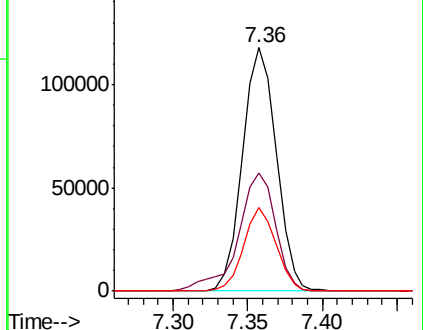




#13
2-Methylphenol
Concen: 10.407 ng/ul
RT: 8.23 min Scan# 875
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:108 Resp: 172563
Ion Ratio Lower Upper
108 100
107 88.8 72.9 109.3

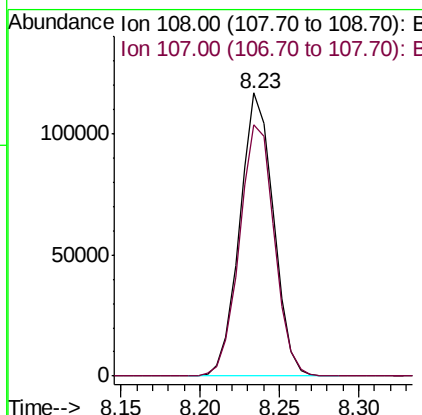

#14
2,2'-oxybis(1-Chloropropane)
Concen: 13.425 ng/ul
RT: 8.33 min Scan# 891
Delta R.T. 0.01 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion: 45 Resp: 220758
Ion Ratio Lower Upper
45 100
77 18.7 14.6 21.8
79 14.4 10.6 16.0


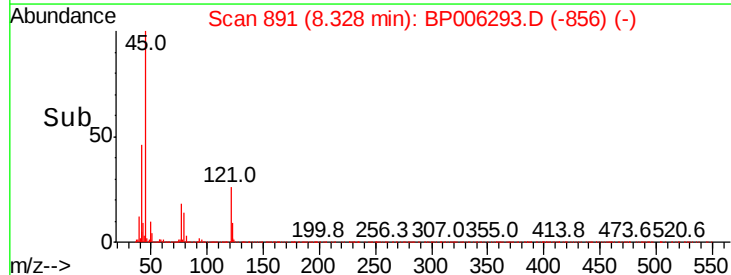
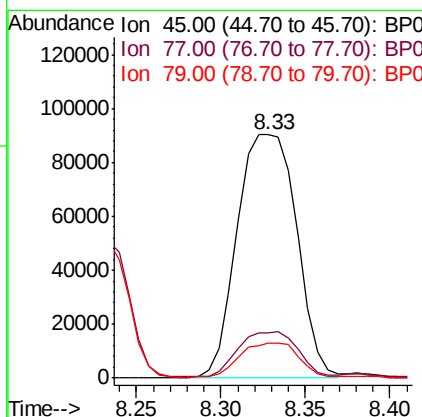



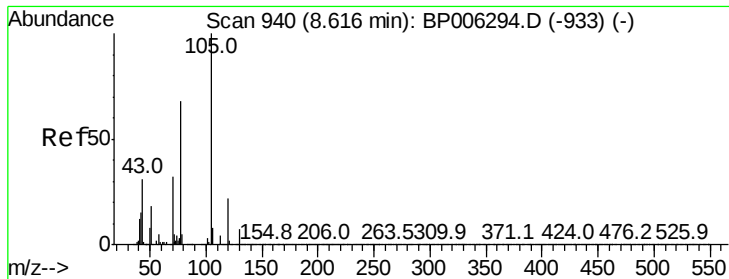

#16
Acetophenone
Concen: 10.830 ng/ul
RT: 8.62 min Scan# 940
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
105	100		
77	84.4	65.0	97.4
51	22.0	17.9	26.9

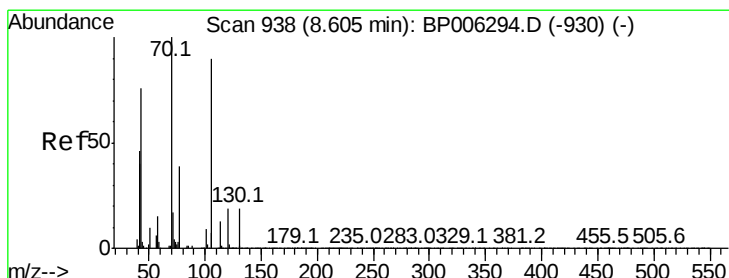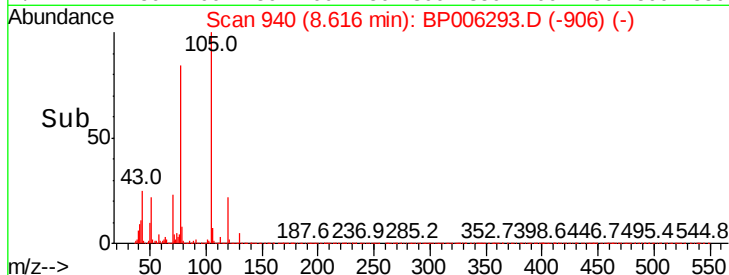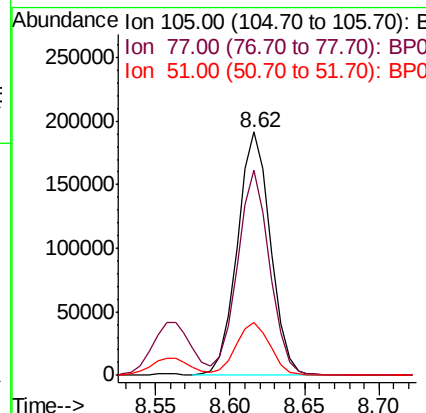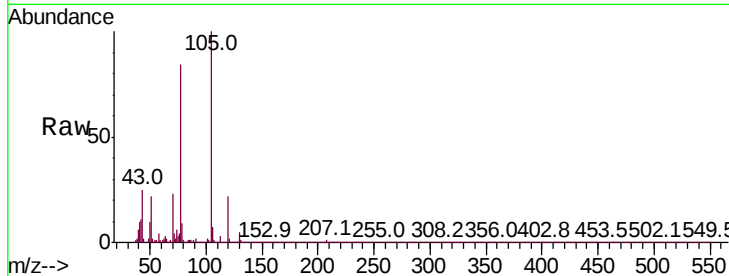

#17
N-Nitroso-di-n-propylamine
Concen: 12.401 ng/ul
RT: 8.60 min Scan# 938
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
70	100		
42	48.2	37.0	55.6
101	8.3	7.3	10.9
130	19.0	15.2	22.8

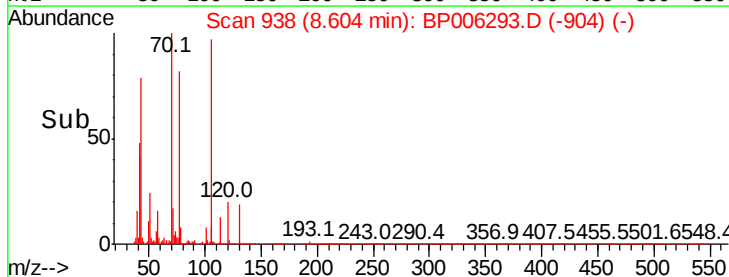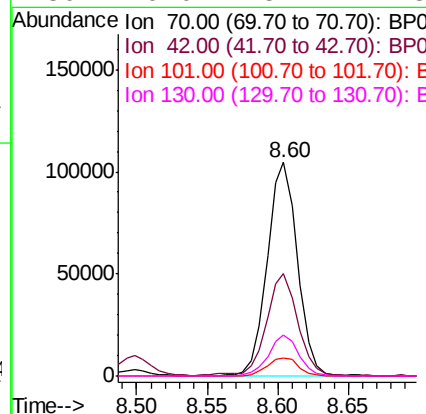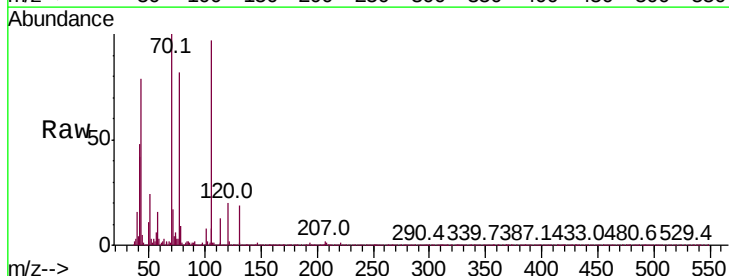

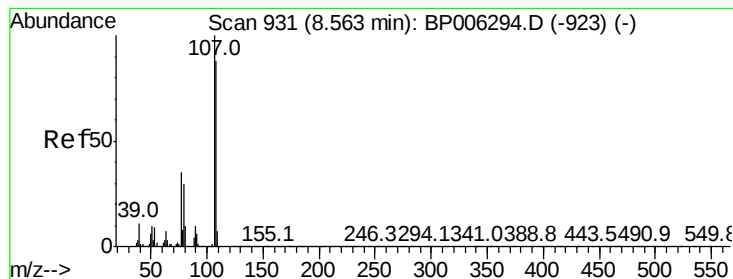

#18

4-Methylphenol

Concen: 10.603 ng/ul

RT: 8.56 min Scan# 931

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :





SSTD010602

Tot Ion:108 Resp: 187212

Ion Ratio Lower Upper

108 100

107 116.5 91.1 136.7

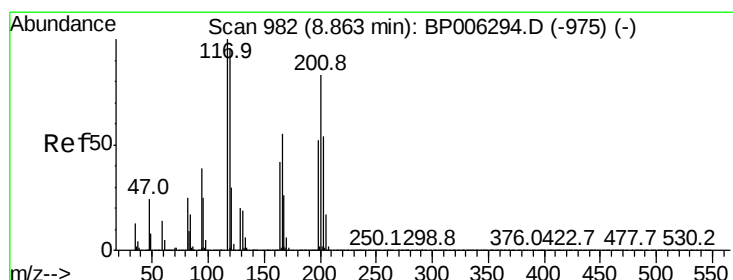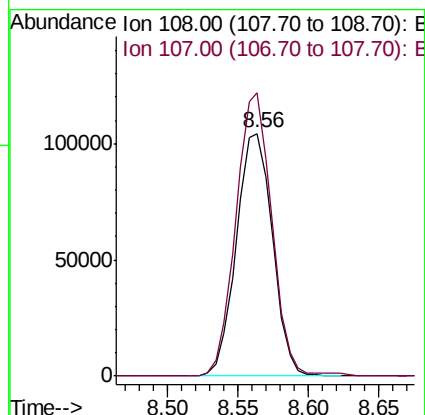

#19

Hexachloroethane

Concen: 9.972 ng/ul

RT: 8.86 min Scan# 982

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43




Tgt Ion:117 Resp: 75674


Ion Ratio Lower Upper

117 100

201 84.4 66.3 99.5

199 52.7 41.4 62.2


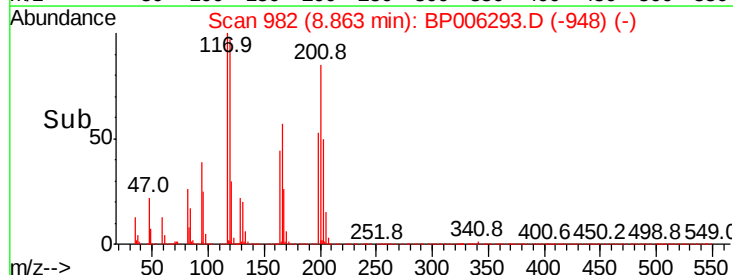
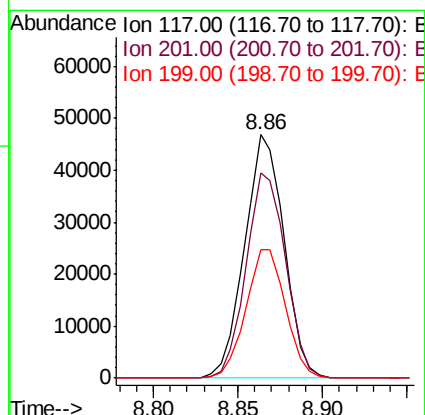





#22
Nitrobenzene
Concen: 10.055 ng/ul
RT: 8.99 min Scan# 1004
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
77	100		
123	40.8	33.3	49.9
65	13.1	10.4	15.6

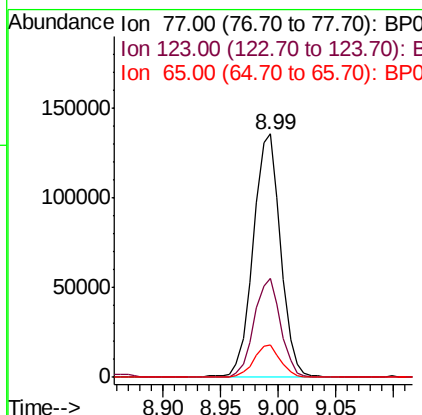

#23
Isophorone
Concen: 9.990 ng/ul
RT: 9.52 min Scan# 1094
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
82	100		
95	6.9	5.9	8.9
138	15.8	13.0	19.6

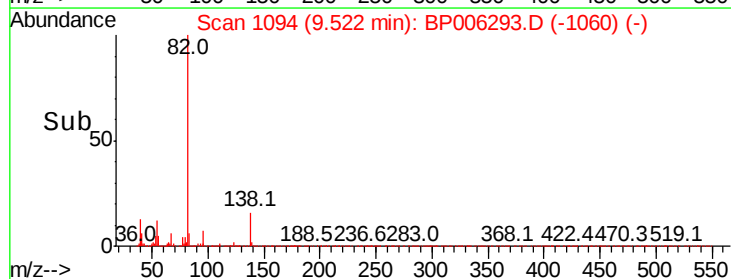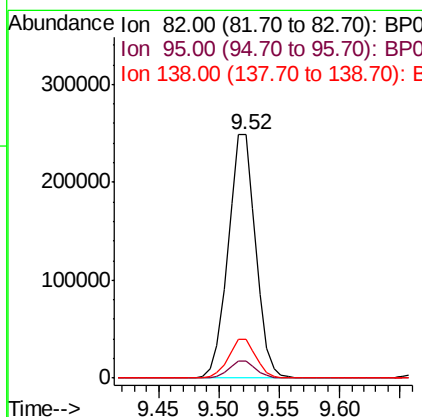



#25

2-Nitrophenol

Concen: 7.978 ng/ul

RT: 9.70 min Scan# 1124





Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion	Ratio	Lower	Upper
139	100		
65	53.2	44.8	67.2
109	34.2	25.6	38.4

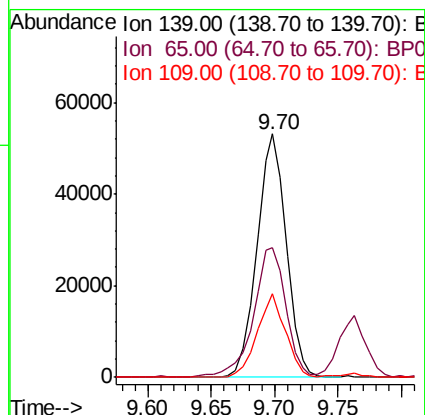

#26

2,4-Dimethylphenol

Concen: 9.600 ng/ul




RT: 9.76 min Scan# 1135


Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
107	100		
121	49.4	39.9	59.9
122	82.3	65.0	97.4

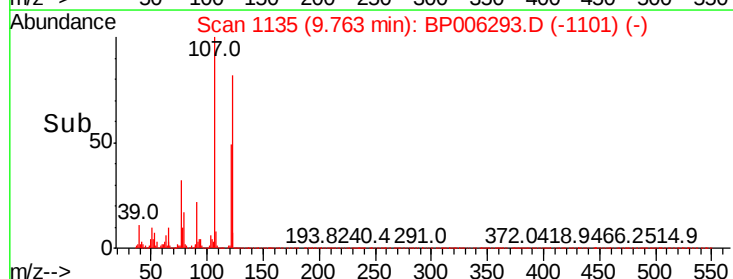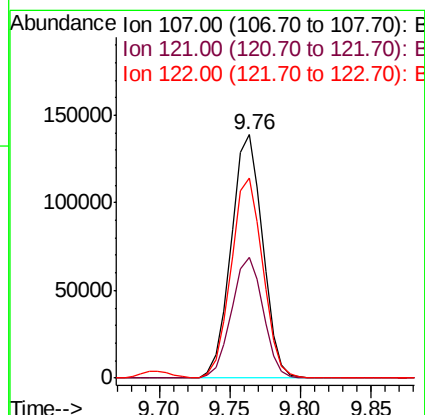

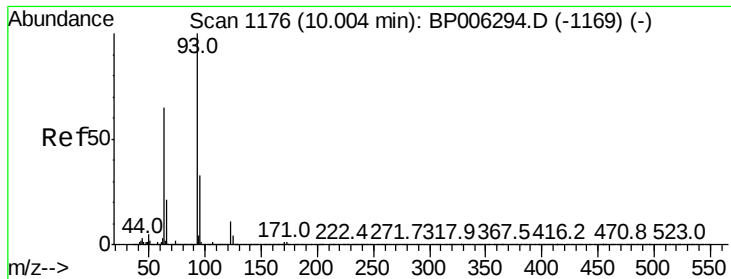

#27

Bis(2-Chloroethoxy)methane

Concen: 11.147 ng/ul

RT: 10.00 min Scan# 1176

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion: 93 Resp: 260647

Ion Ratio Lower Upper

93 100

95 31.8 26.1 39.1




123 10.8 8.7 13.1



Abundance Ion 93.00 (92.70 to 93.70): BPC

Ion 95.00 (94.70 to 95.70): BPC

Ion 123.00 (122.70 to 123.70): BPC

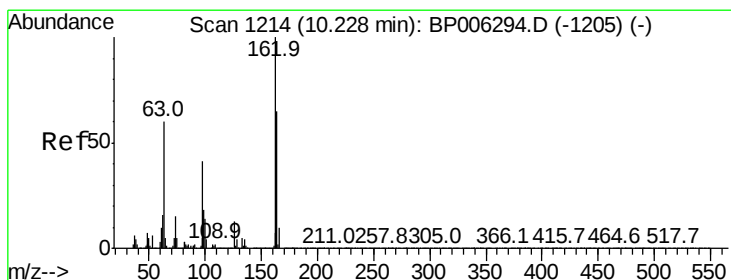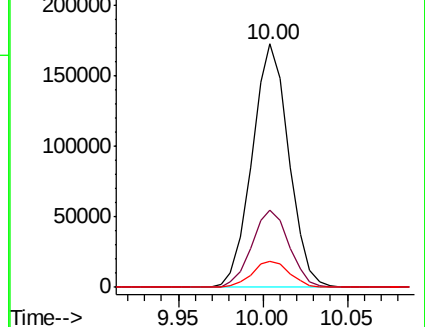

#29

2,4-Dichlorophenol

Concen: 8.420 ng/ul

RT: 10.23 min Scan# 1214

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion: 162 Resp: 156730

Ion Ratio Lower Upper

162 100

164 66.1 51.9 77.9



98 41.2 32.5 48.7




Abundance Ion 162.00 (161.70 to 162.70): E

Ion 164.00 (163.70 to 164.70): E

Ion 98.00 (97.70 to 98.70): BPC

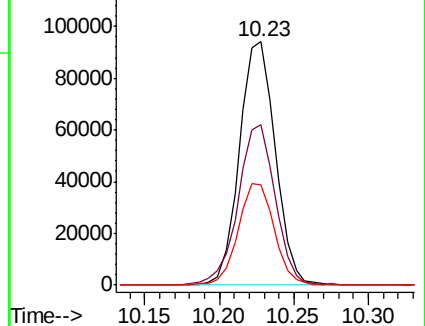

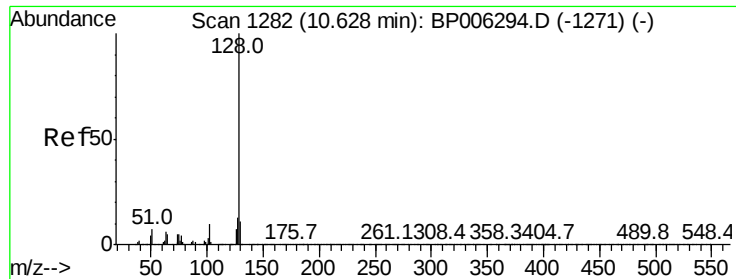

#30

Naphthalene

Concen: 9.852 ng/ul

RT: 10.63 min Scan# 1282

Delta R.T. -0.00 min





Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion:128 Resp: 617810

Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.8	13.2
127	13.3	10.7	16.1

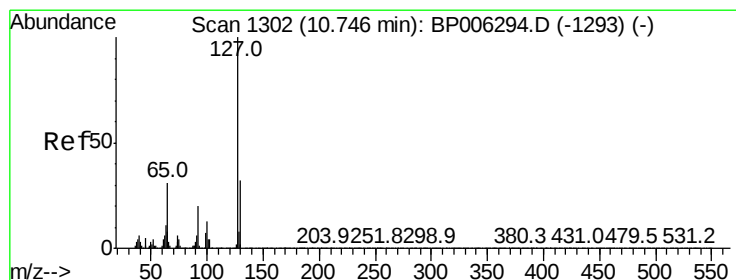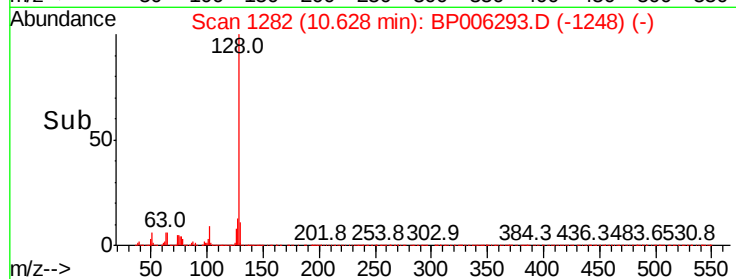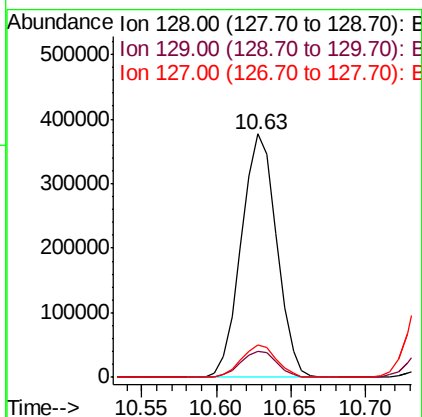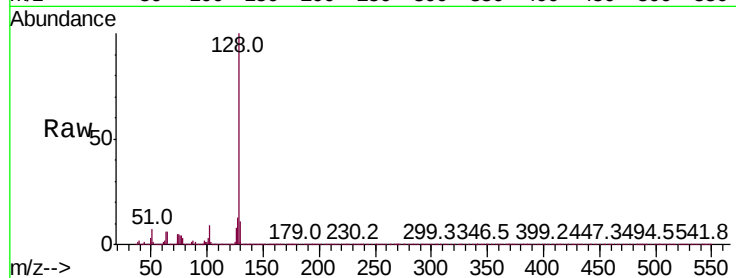

#32

4-Chloroaniline

Concen: 10.094 ng/ul

RT: 10.74 min Scan# 1301




Delta R.T. -0.01 min


Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion:127 Resp: 262728

Ion	Ratio	Lower	Upper
127	100		
129	32.2	25.7	38.5


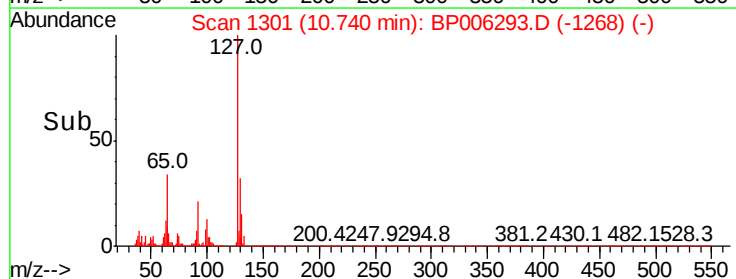
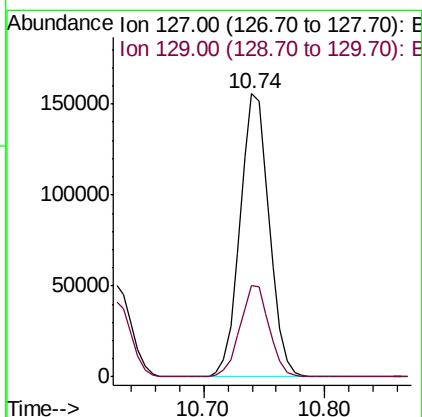
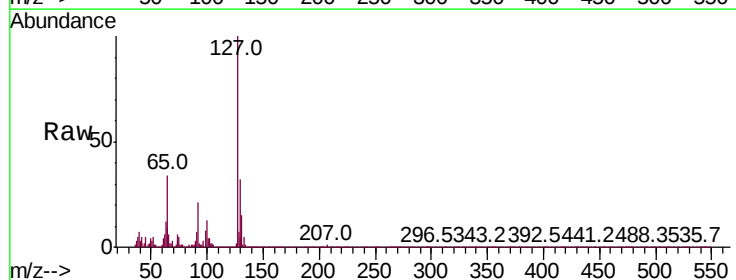




#33
Hexachlorobutadiene
Concen: 7.008 ng/ul
RT: 10.92 min Scan# 1331
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:225 Resp: 98643
Ion Ratio Lower Upper
225 100
223 61.1 50.3 75.5
227 62.4 51.8 77.6

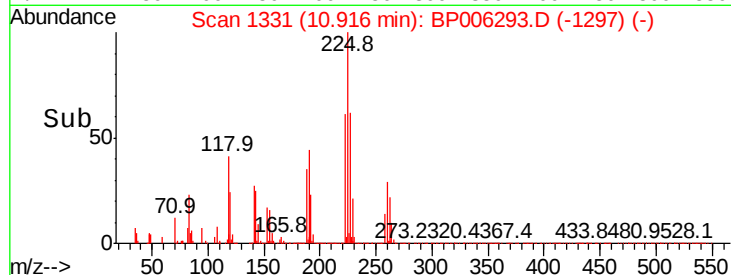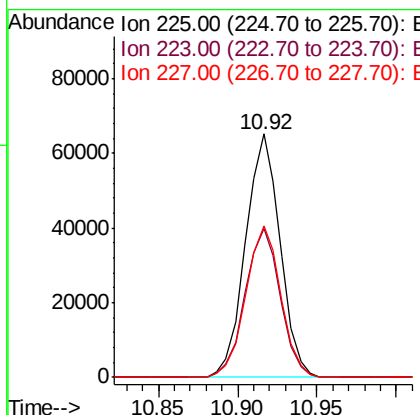

#34
Caprolactam
Concen: 7.540 ng/ul
RT: 11.52 min Scan# 1434
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion:113 Resp: 46355
Ion Ratio Lower Upper
113 100
55 140.8 112.2 168.2
56 107.3 89.2 133.8



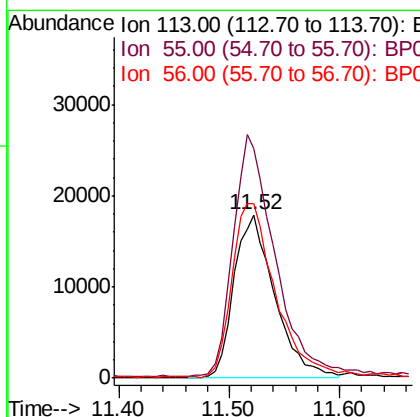





#35
4-Chloro-3-methylphenol
Concen: 9.365 ng/ul
RT: 11.86 min Scan# 1492
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
107	100		
144	24.1	18.3	27.5
142	74.1	58.5	87.7

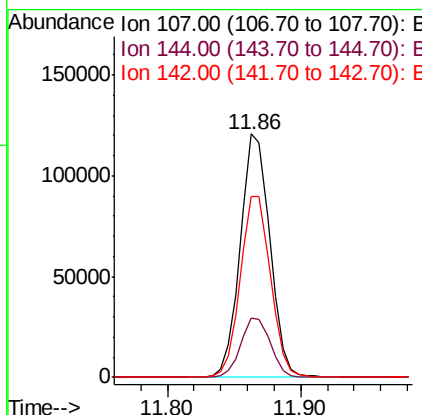

#36
2-Methylnaphthalene
Concen: 9.520 ng/ul
RT: 12.24 min Scan# 1556
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
142	100		
141	92.7	72.6	108.8

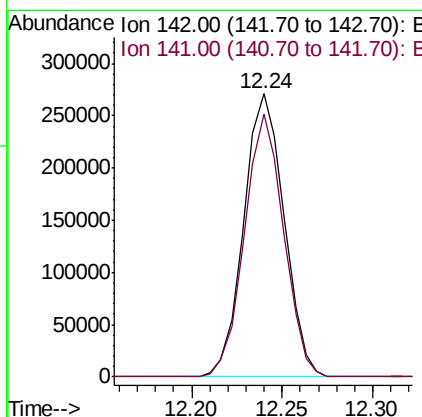

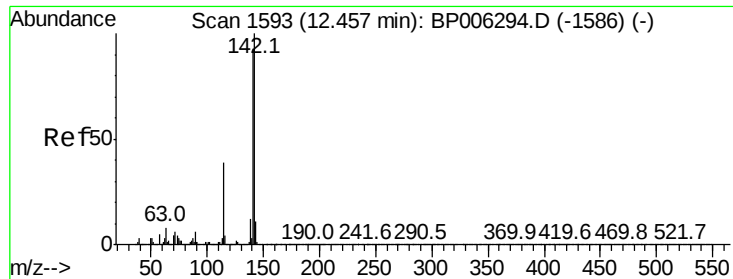

#37

1-Methylnaphthalene

Concen: 9.469 ng/ul

RT: 12.46 min Scan# 1593

Delta R.T. -0.00 min





Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion:142 Resp: 420401

Ion	Ratio	Lower	Upper
142	100		
141	94.8	74.5	111.7
116	4.3	3.5	5.3

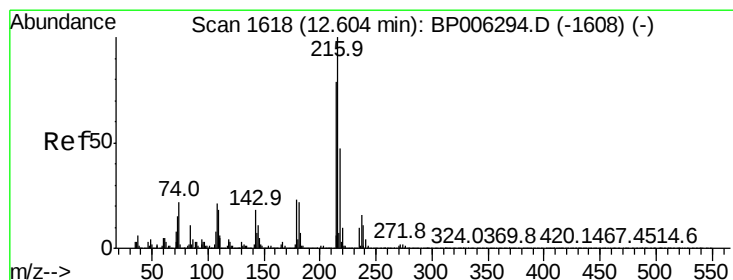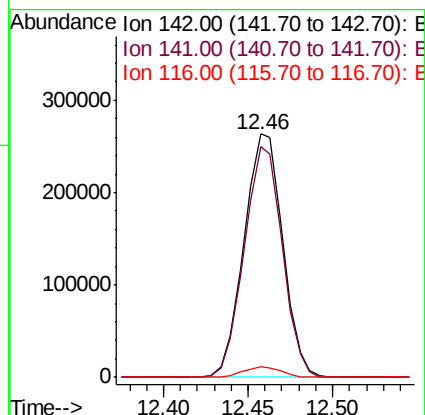

#39

1,2,4,5-Tetrachlorobenzene

Concen: 7.629 ng/ul

RT: 12.60 min Scan# 1618




Delta R.T. -0.00 min


Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion:216 Resp: 183697

Ion	Ratio	Lower	Upper
216	100		
214	77.6	63.5	95.3
179	24.3	18.7	28.1
108	23.4	16.9	25.3


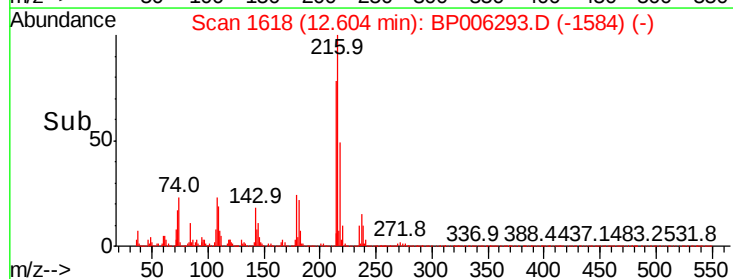

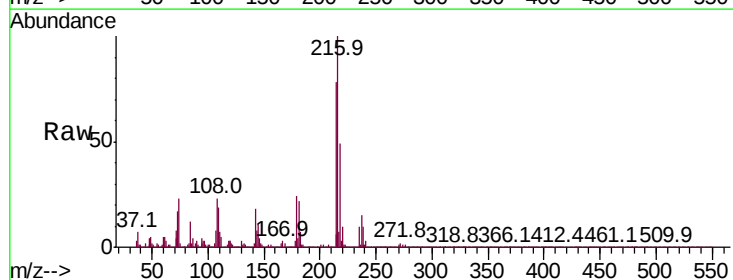




#40
Hexachlorocyclopentadiene
Concen: 6.914 ng/ul
RT: 12.59 min Scan# 1615
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
237	100		
235	60.7	49.4	74.2
272	12.3	9.2	13.8

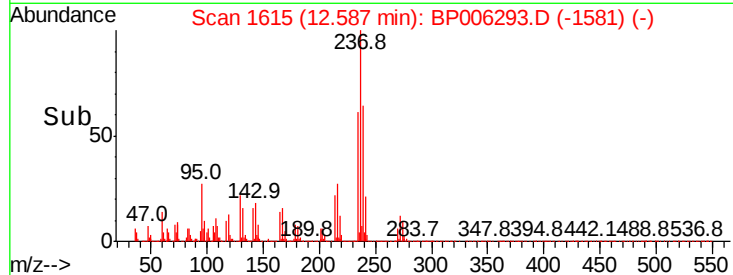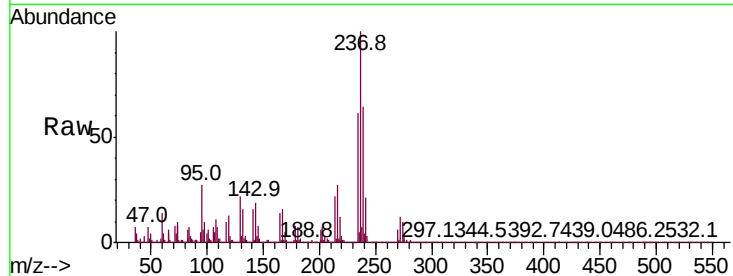

#41
2,4,6-Trichlorophenol
Concen: 7.411 ng/ul
RT: 12.85 min Scan# 1660
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
196	100		
198	96.2	75.6	113.4
200	31.7	24.2	36.2


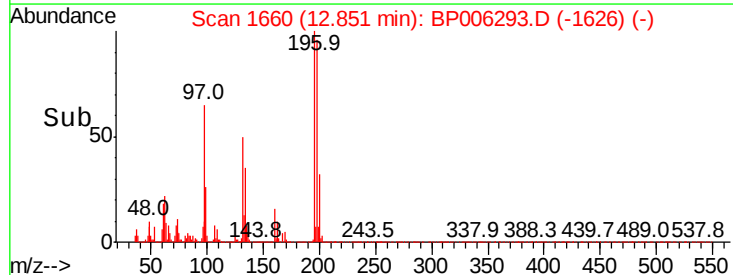






#42
 2,4,5-Trichlorophenol
 Concen: 7.582 ng/ul
 RT: 12.92 min Scan# 1671
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602


Tot Ion	Ratio	Lower	Upper
196	100		
198	98.5	76.1	114.1
200	31.1	24.2	36.4

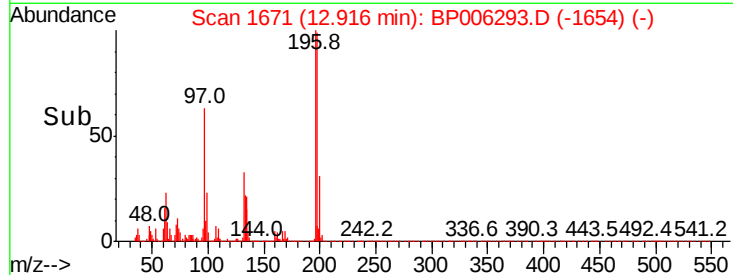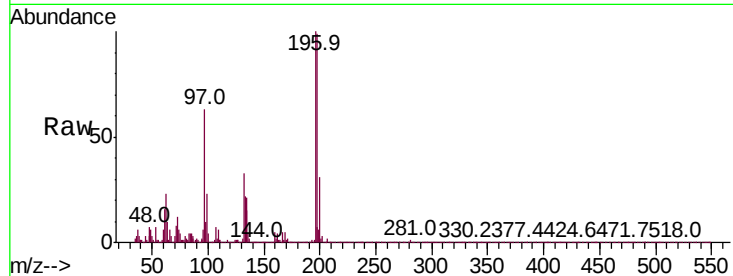

#43
 1,1'-Biphenyl
 Concen: 9.841 ng/ul
 RT: 13.26 min Scan# 1729
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
154	100		
153	41.2	33.0	49.4
76	14.7	12.3	18.5


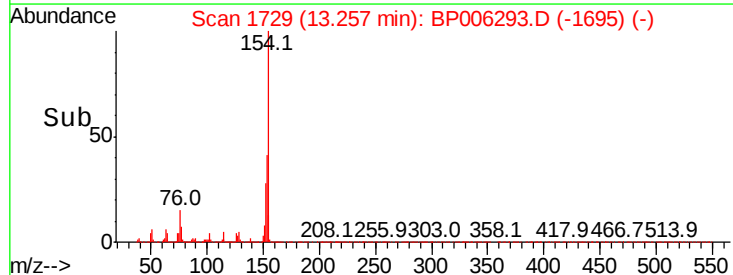




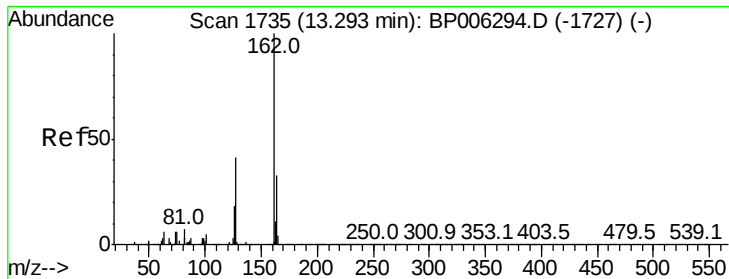

#44
2-Chloronaphthalene
Concen: 9.422 ng/ul
RT: 13.29 min Scan# 1735
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
162	100		
164	32.8	26.3	39.5
127	44.8	34.7	52.1

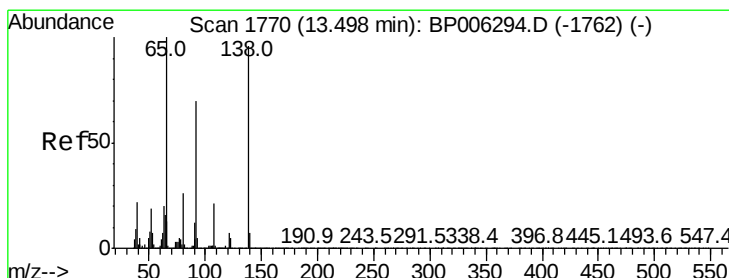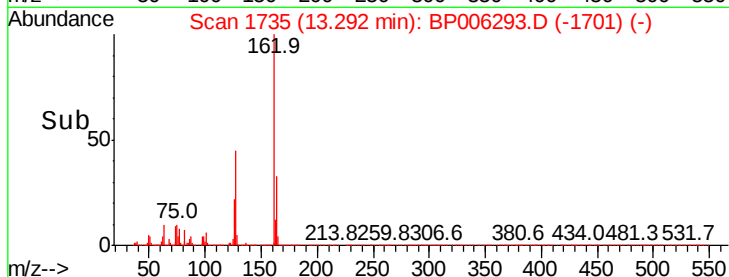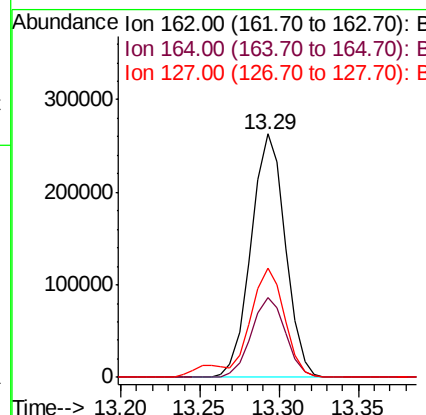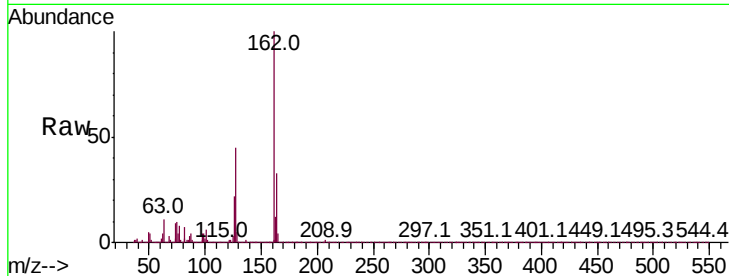

#45
2-Nitroaniline
Concen: 9.477 ng/ul
RT: 13.50 min Scan# 1770
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
65	100		
92	68.1	55.8	83.8
138	100.3	76.3	114.5


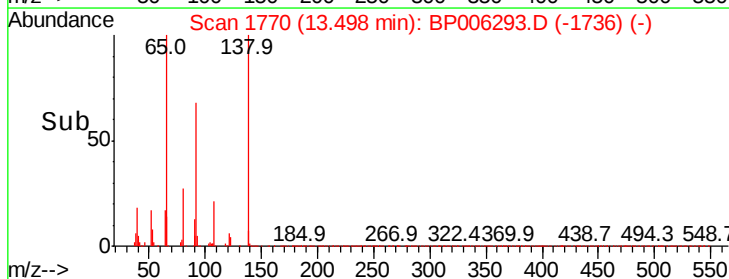
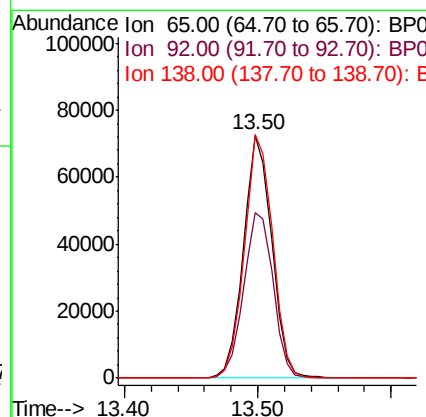
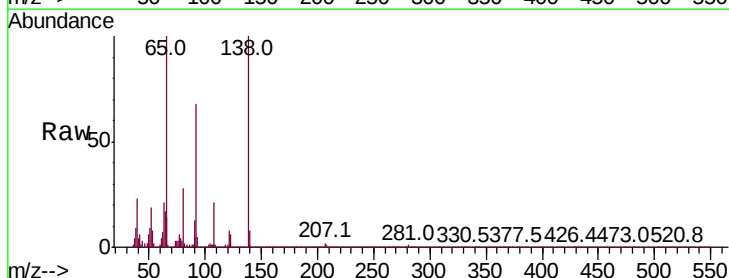


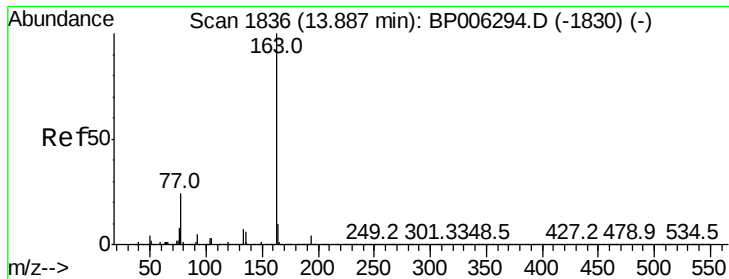

#47
Dimethylphthalate
Concen: 9.255 ng/ul
RT: 13.89 min Scan# 1836
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:163 Resp: 487255
Ion Ratio Lower Upper
163 100
194 3.8 3.0 4.6
164 10.1 8.2 12.4

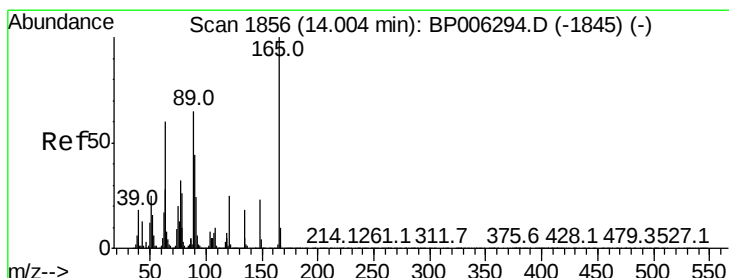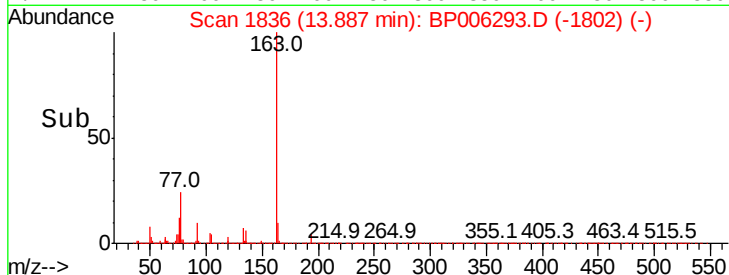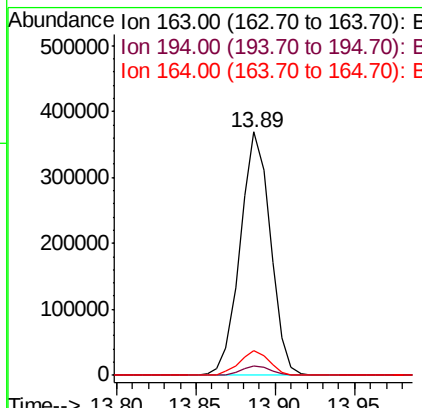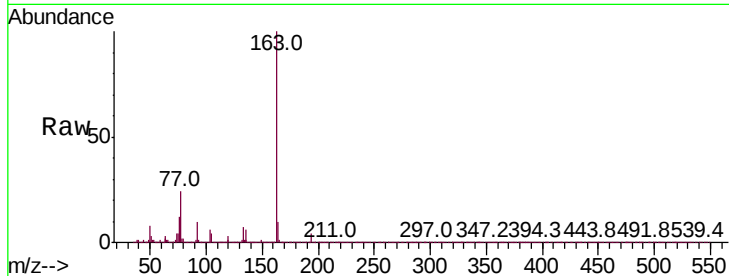

#48
2,6-Dinitrotoluene
Concen: 7.499 ng/ul
RT: 14.00 min Scan# 1855
Delta R.T. -0.01 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion:165 Resp: 79974
Ion Ratio Lower Upper
165 100
89 74.4 52.3 78.5
121 27.4 19.8 29.6

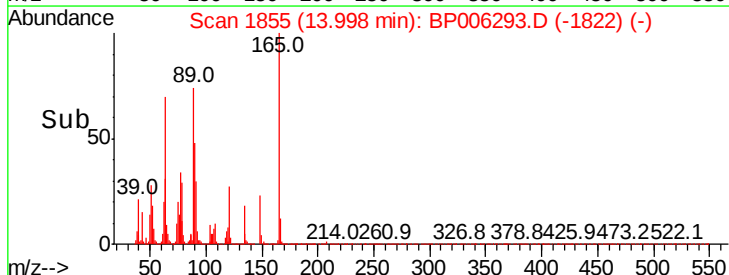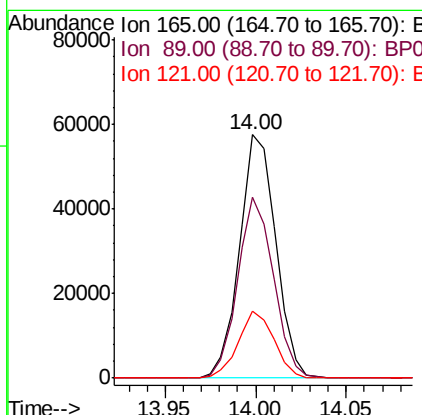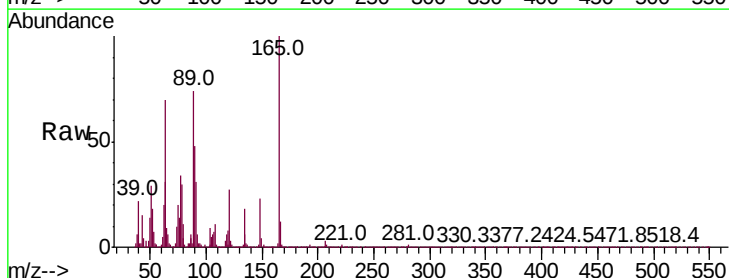

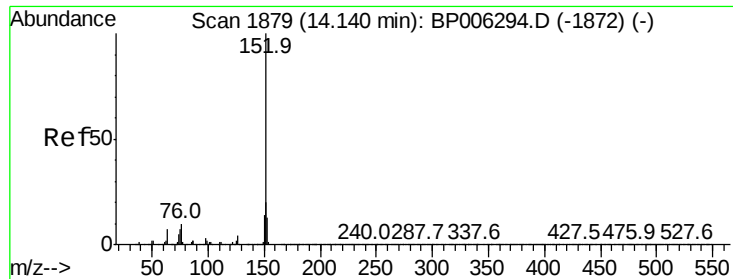

#50

Acenaphthylene

Concen: 9.649 ng/ul

RT: 14.14 min Scan# 1879

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:152 Resp: 591475

Ion Ratio Lower Upper

152 100

151 20.0 16.2 24.2




153 12.9 10.6 15.8

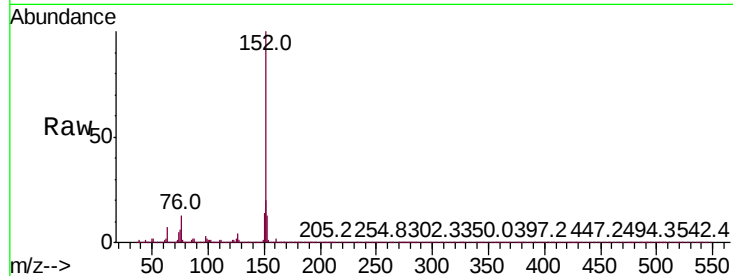

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

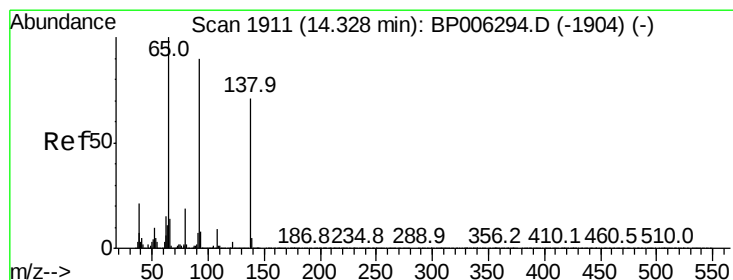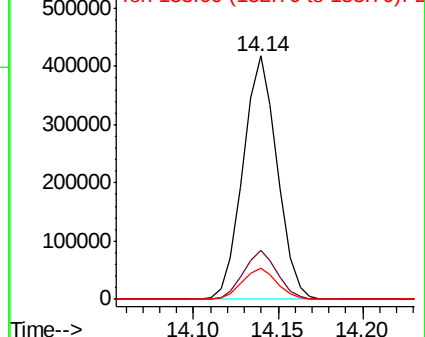

#51

3-Nitroaniline

Concen: 8.227 ng/ul

RT: 14.33 min Scan# 1911

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:138 Resp: 81500

Ion Ratio Lower Upper

138 100

108 14.2 9.8 14.6



92 124.8 101.0 151.6




Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BPO

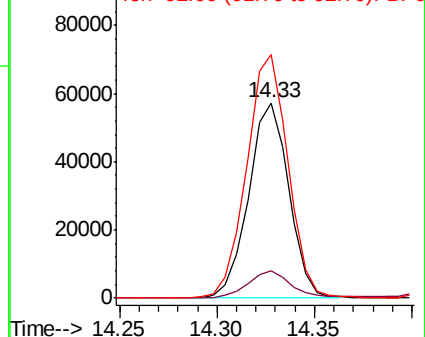



#52

Acenaphthene

Concen: 9.950 ng/ul

RT: 14.48 min Scan# 1937

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:153 Resp: 437369

Ion Ratio Lower Upper

153 100

152 47.4 38.0 57.0




154 89.0 69.0 103.6



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

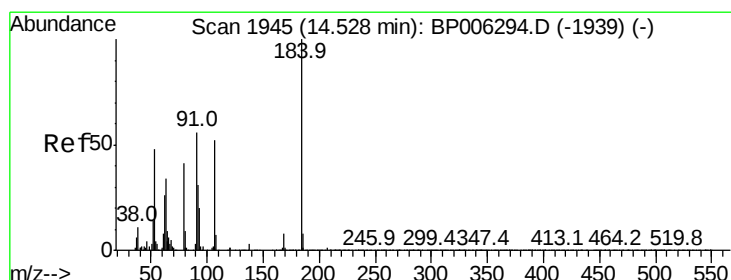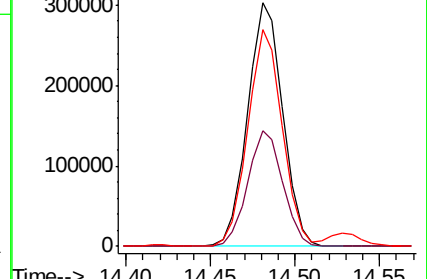

#53

2,4-Dinitrophenol

Concen: 5.231 ng/ul

RT: 14.53 min Scan# 1945

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:184 Resp: 36572

Ion Ratio Lower Upper

184 100

63 77.6 63.0 94.4



154 68.7 54.6 82.0




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BP0

Ion 154.00 (153.70 to 154.70): E




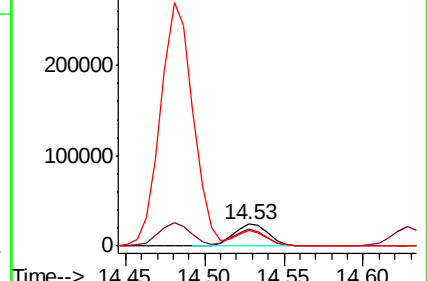




#55
4-Nitrophenol
Concen: 8.351 ng/ul
RT: 14.63 min Scan# 1962
Delta R.T. -0.01 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:109 Resp: 70782
Ion Ratio Lower Upper
109 100
139 129.2 106.2 159.2
65 139.2 108.4 162.6

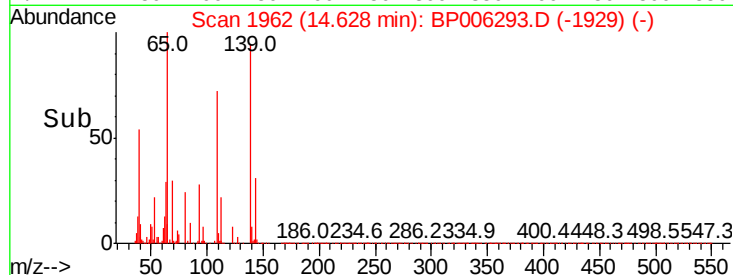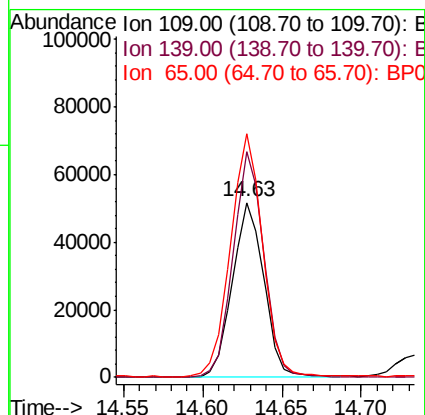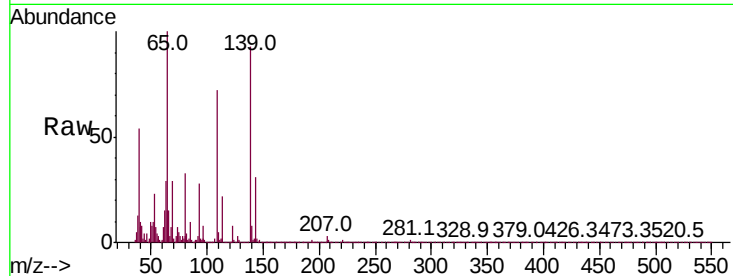

#56
Dibenzofuran
Concen: 9.324 ng/ul
RT: 14.82 min Scan# 1995
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion:168 Resp: 590296
Ion Ratio Lower Upper
168 100
139 41.6 32.6 49.0




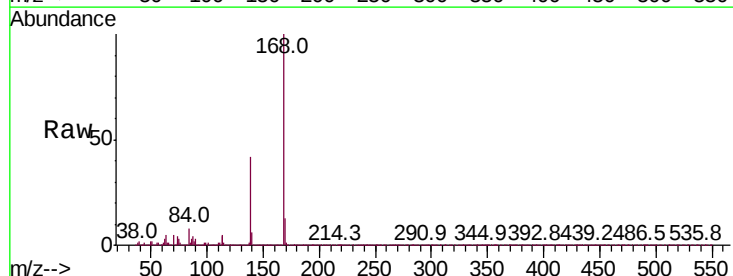


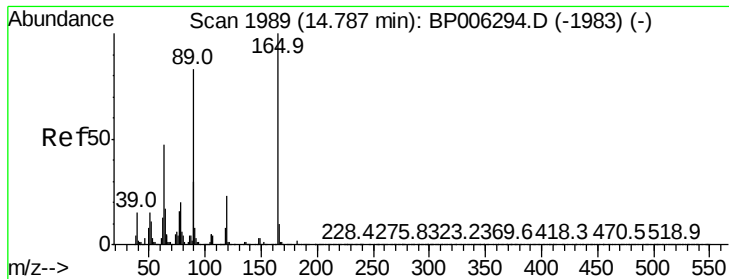

#57
 2,4-Dinitrotoluene
 Concen: 7.638 ng/ul
 RT: 14.79 min Scan# 1989
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602


Tot Ion:165 Resp: 115132
 Ion Ratio Lower Upper
 165 100
 63 47.3 37.4 56.0
 182 2.9 2.6 3.8

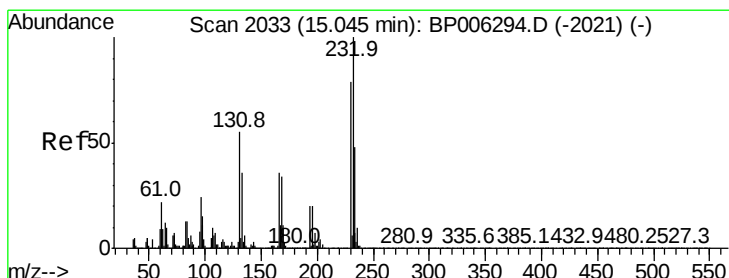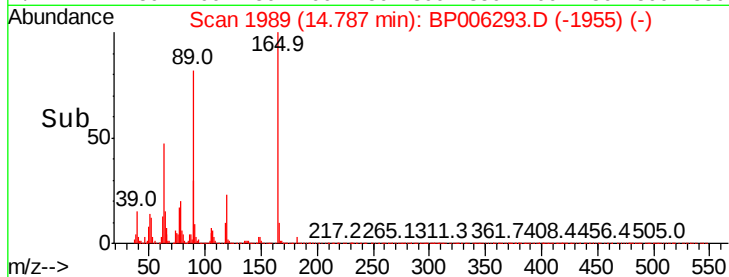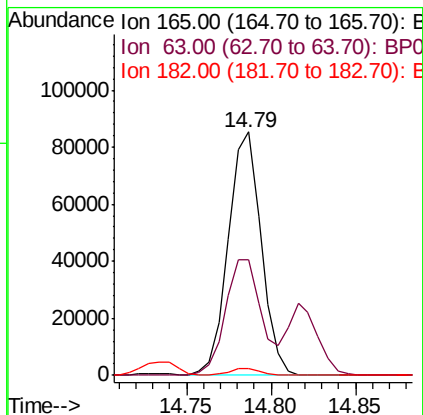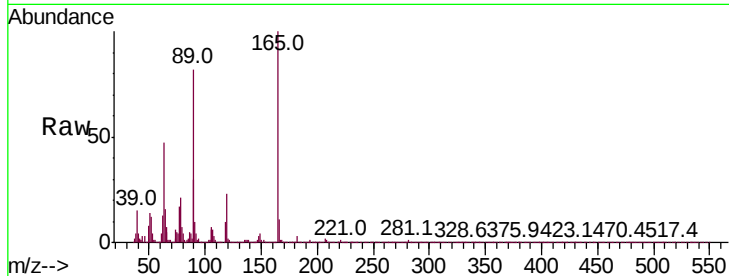

#58
 2,3,4,6-Tetrachlorophenol
 Concen: 6.470 ng/ul
 RT: 15.05 min Scan# 2033
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43

Tgt Ion:232 Resp: 92928
 Ion Ratio Lower Upper
 232 100
 131 57.3 43.8 65.8
 130 3.3 2.6 3.8
 166 35.7 28.5 42.7


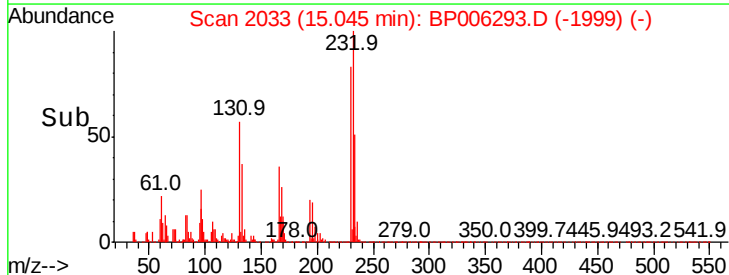
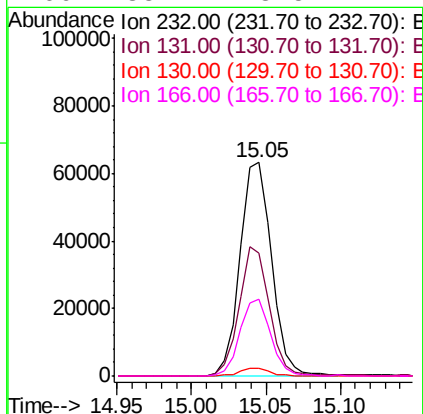
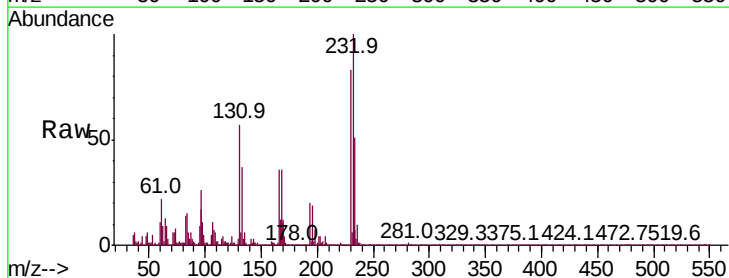




#59
Diethylphthalate
Concen: 9.723 ng/ul
RT: 15.26 min Scan# 2069
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:149 Resp: 501937
Ion Ratio Lower Upper
149 100
177 19.8 16.1 24.1
150 12.1 9.8 14.6

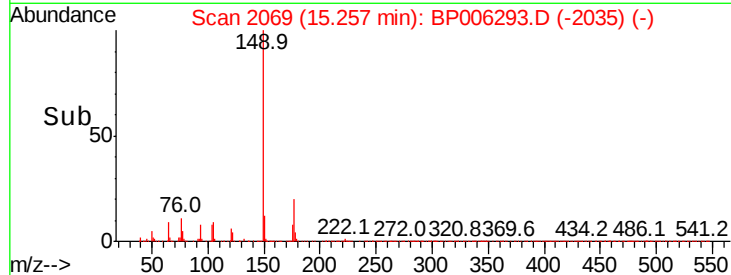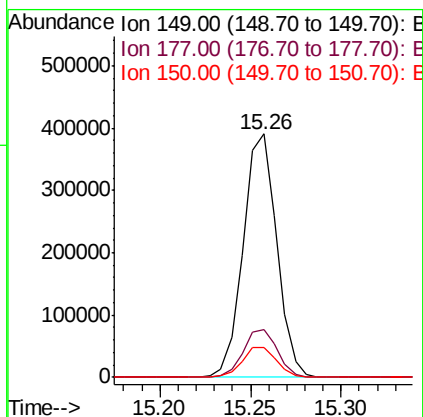

#61
Fluorene
Concen: 9.229 ng/ul
RT: 15.47 min Scan# 2105
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion:166 Resp: 482944
Ion Ratio Lower Upper
166 100
165 99.3 79.2 118.8
167 13.0 10.7 16.1

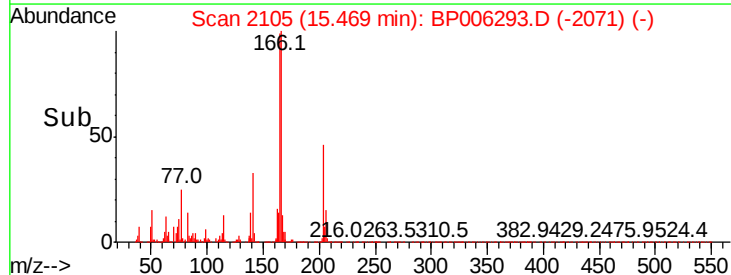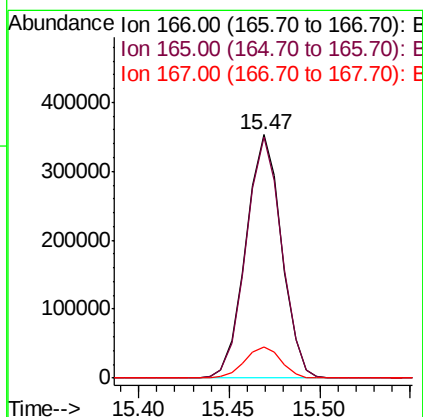



#62

4-Chlorophenyl-phenylether

Concen: 7.888 ng/ul

RT: 15.47 min Scan# 2105

Delta R.T. -0.00 min





Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion: 204 Resp: 223880

Ion	Ratio	Lower	Upper
204	100		
206	33.4	25.5	38.3
141	71.3	57.0	85.4



#63

4-Nitroaniline

Concen: 8.011 ng/ul

RT: 15.49 min Scan# 2108




Delta R.T. -0.01 min


Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion: 138 Resp: 77966

Ion	Ratio	Lower	Upper
138	100		
92	59.9	46.5	69.7
108	83.3	67.8	101.6


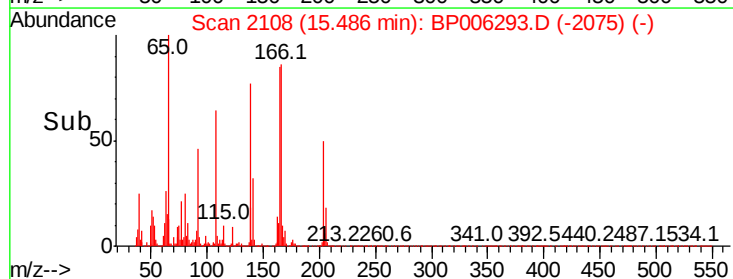






#66
 4,6-Dinitro-2-methylphenol
 Concen: 6.217 ng/ul
 RT: 15.55 min Scan# 2118
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602


Tot Ion	198	Resp	57355
Ion Ratio	100	Lower	Upper
182	5.6	4.6	6.8
77	31.7	25.6	38.4

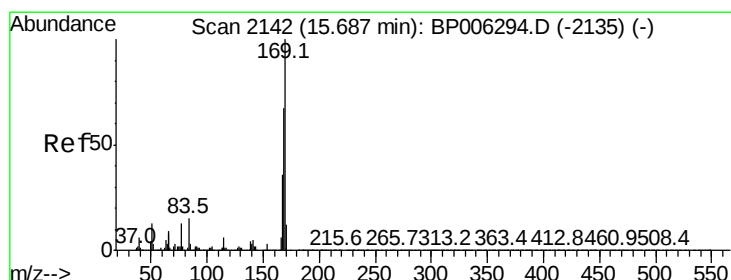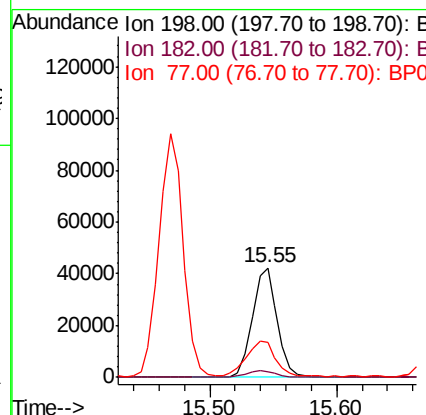

#67
 N-Nitrosodiphenylamine
 Concen: 10.216 ng/ul
 RT: 15.69 min Scan# 2142
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43

Tgt Ion	169	Resp	402969
Ion Ratio	100	Lower	Upper
168	68.0	53.8	80.8
167	37.1	29.1	43.7


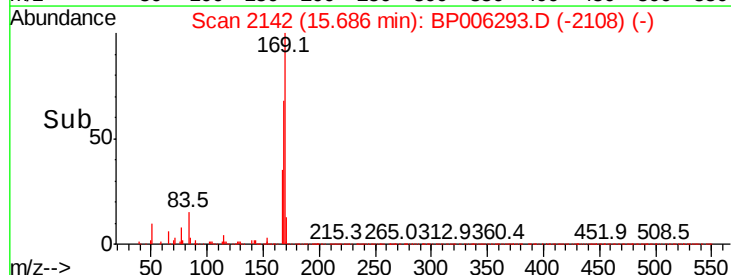
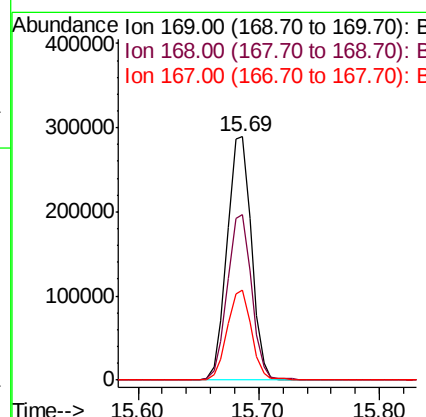





#68
4-Bromophenyl-phenylether
Concen: 6.828 ng/ul
RT: 16.37 min Scan# 2258
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion:248 Resp: 105272
Ion Ratio Lower Upper
248 100
250 98.1 79.4 119.2
141 88.7 70.3 105.5

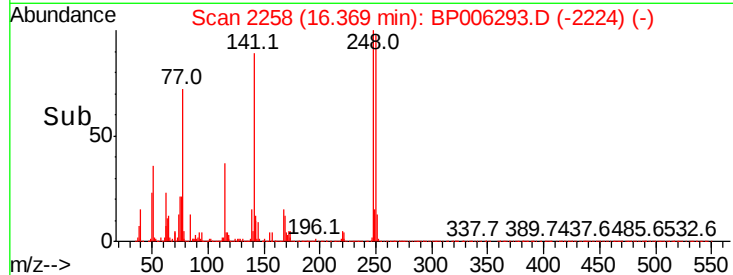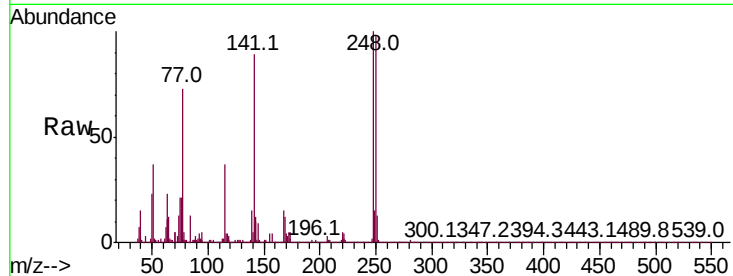

#69
Hexachlorobenzene
Concen: 8.350 ng/ul
RT: 16.47 min Scan# 2275
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion:284 Resp: 144440
Ion Ratio Lower Upper
284 100
142 43.4 35.5 53.3
249 32.5 26.7 40.1

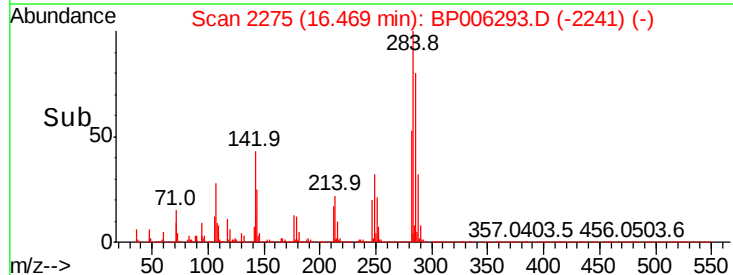


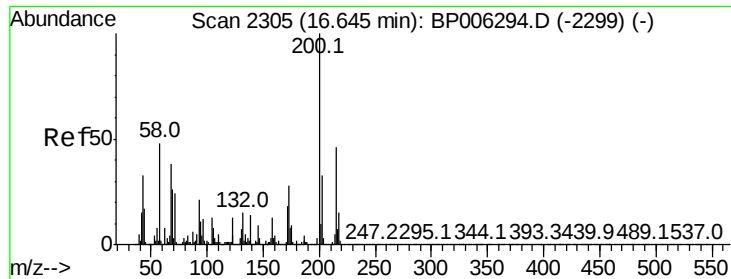

#70
Atrazine
Concen: 8.198 ng/ul
RT: 16.65 min Scan# 2305
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion	Ratio	Lower	Upper
200	100		
173	26.3	22.4	33.6
215	45.5	37.0	55.4






Abundance

Ion 200.00 (199.70 to 200.70): E


Ion 173.00 (172.70 to 173.70): E

Ion 215.00 (214.70 to 215.70): E

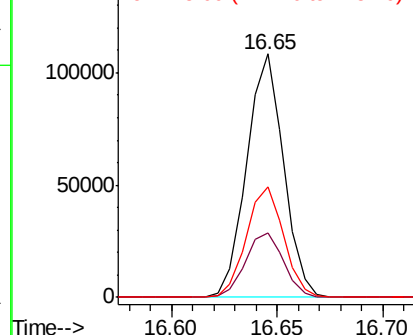

#71
Pentachlorophenol
Concen: 6.597 ng/ul
RT: 16.82 min Scan# 2334
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
266	100		
264	64.2	49.6	74.4
268	65.8	50.7	76.1






Abundance

Ion 265.70 (265.40 to 266.40): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E

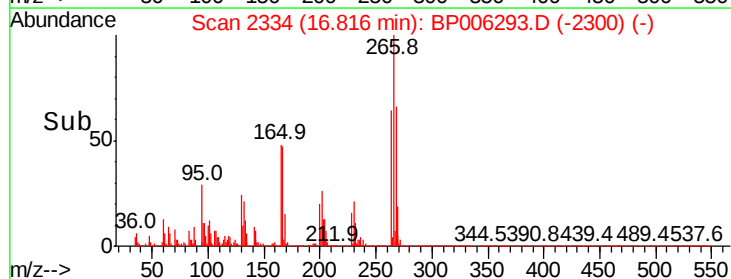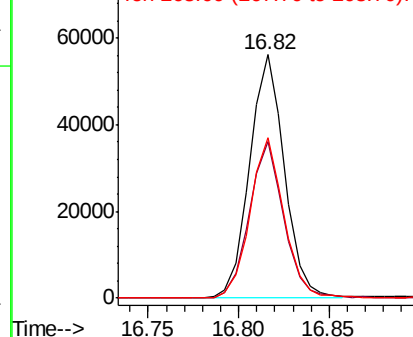



#72

Phenanthrene

Concen: 9.828 ng/ul

RT: 17.21 min Scan# 2401

Delta R.T. -0.01 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:178 Resp: 733162

Ion Ratio Lower Upper

178 100

179 15.5 12.0 18.0




176 18.8 15.0 22.6



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

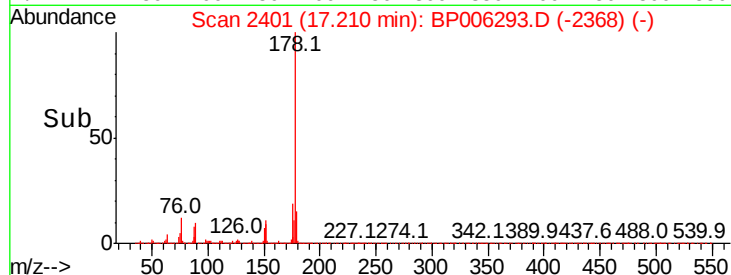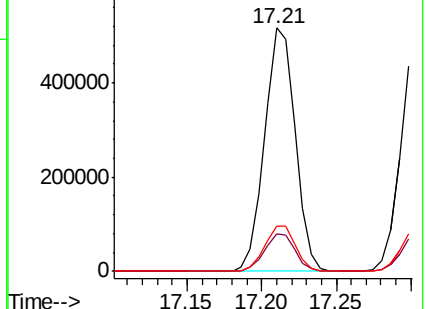

#74

Anthracene

Concen: 9.879 ng/ul

RT: 17.30 min Scan# 2417

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:178 Resp: 744431

Ion Ratio Lower Upper

178 100

179 15.1 12.2 18.4



176 18.5 14.8 22.2




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

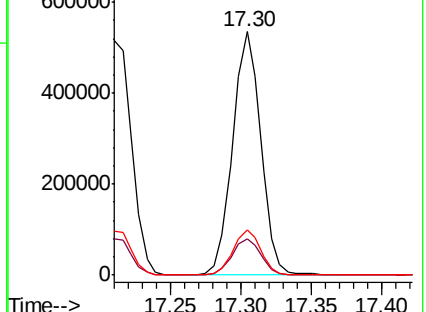



#75

1,2,3,4-Tetrachlorobenzene

Concen: 8.283 ng/uL

RT: 13.22 min Scan# 1722

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :


BNA_P

ClientSampleId :

SSTD010602

Tot Ion:216 Resp: 182810

Ion	Ratio	Lower	Upper
216	100		
214	76.6	62.4	93.6
218	49.5	37.8	56.6






Abundance

Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

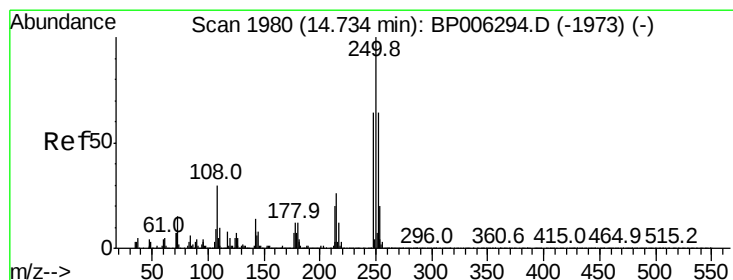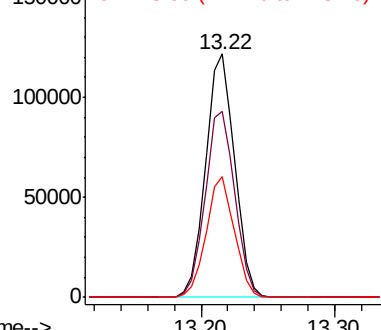

#76

Pentachlorobenzene

Concen: 8.045 ng/uL

RT: 14.73 min Scan# 1980


Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion:250 Resp: 178081

Ion	Ratio	Lower	Upper
250	100		
248	62.8	51.3	76.9
252	63.3	51.0	76.6






Abundance

Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

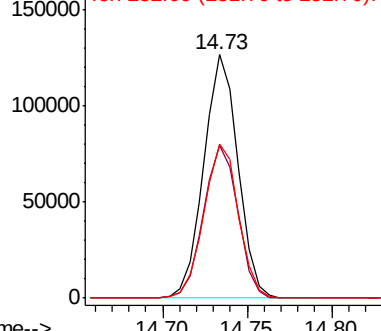

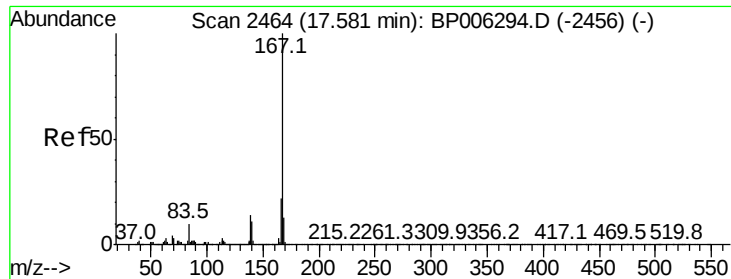

#77

Carbazole

Concen: 10.031 ng/ul

RT: 17.57 min Scan# 2463

Delta R.T. -0.01 min





Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion:167 Resp: 663667

Ion	Ratio	Lower	Upper
167	100		
166	21.4	17.2	25.8
139	14.2	11.3	16.9

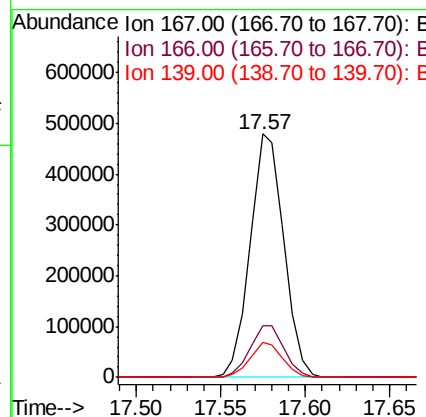

#78

Di-n-butylphthalate

Concen: 10.250 ng/ul

RT: 18.15 min Scan# 2560




Delta R.T. -0.01 min


Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Tgt Ion:149 Resp: 772699

Ion	Ratio	Lower	Upper
149	100		
150	9.1	7.4	11.0
104	5.9	4.4	6.6

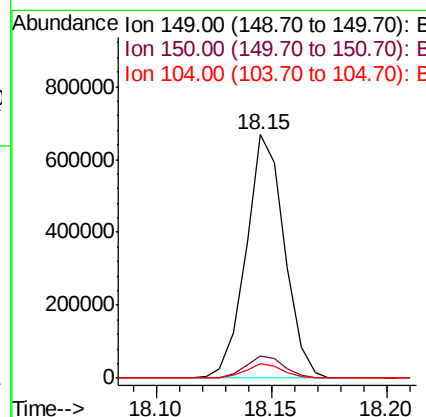



#80

Fluoranthene

Concen: 10.434 ng/ul

RT: 19.19 min Scan# 2737

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:202 Resp: 798432

Ion Ratio Lower Upper

202 100

101 13.6 11.0 16.6




100 10.7 8.8 13.2



Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BF

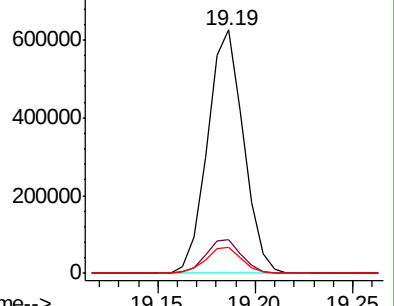

#82

Pyrene

Concen: 10.635 ng/ul

RT: 19.54 min Scan# 2797

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:202 Resp: 841595

Ion Ratio Lower Upper

202 100

101 16.0 13.0 19.4



100 13.8 11.0 16.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): BF




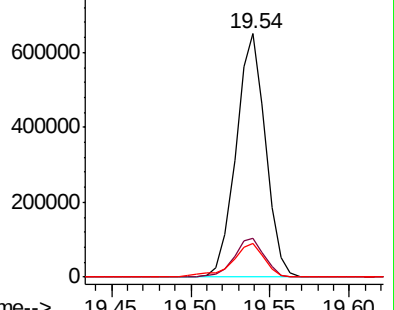




#83
 Butylbenzylphthalate
 Concen: 10.998 ng/ul
 RT: 20.43 min Scan# 2949
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43




Instrument :
 BNA_P
 ClientSampleId :
 SSTD010602


Tot Ion	Ratio	Lower	Upper
149	100		
91	78.1	61.8	92.8
206	18.5	15.0	22.6

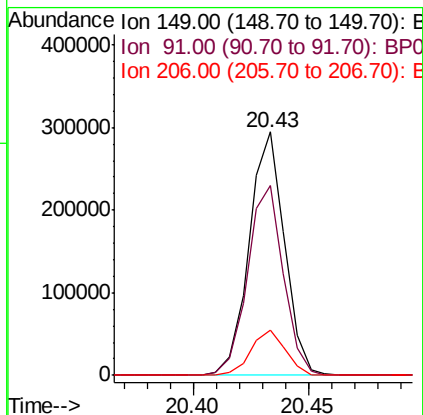

#84
 3,3'-Dichlorobenzidine
 Concen: 8.552 ng/ul
 RT: 21.19 min Scan# 3078
 Delta R.T. -0.00 min
 Lab File: BP006293.D
 Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
252	100		
254	64.7	51.4	77.0
126	14.1	11.3	16.9

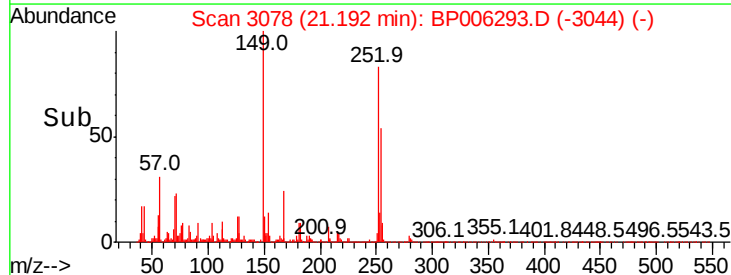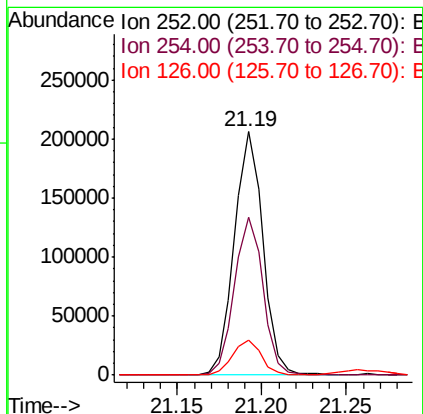



#85

Benzo(a)anthracene

Concen: 9.969 ng/ul

RT: 21.25 min Scan# 3088

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:228 Resp: 789414

Ion Ratio Lower Upper

228 100

229 20.0 15.9 23.9

226 27.1 21.6 32.4






Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 229.00 (228.70 to 229.70): E

Ion 226.00 (225.70 to 226.70): E

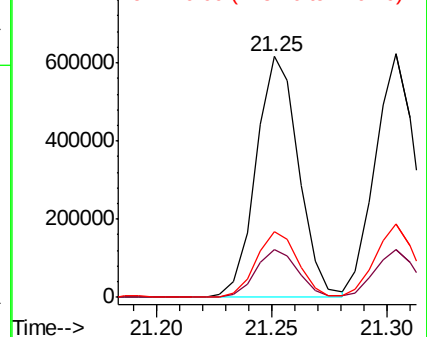

#86

Bis(2-ethylhexyl)phthalate

Concen: 11.504 ng/ul

RT: 21.20 min Scan# 3079

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:149 Resp: 499685

Ion Ratio Lower Upper

149 100

167 25.1 20.3 30.5

279 3.5 2.7 4.1






Abundance

Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

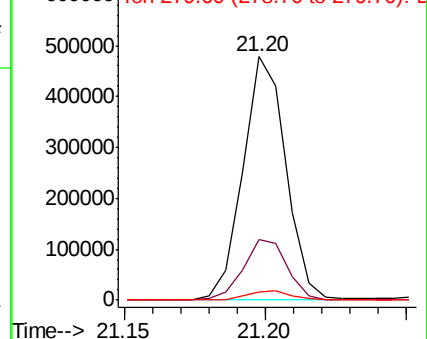



#87

Chrysene

Concen: 9.703 ng/ul

RT: 21.30 min Scan# 3097

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:228 Resp: 753608

Ion Ratio Lower Upper

228 100

226 30.1 24.1 36.1




229 19.7 15.8 23.6



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

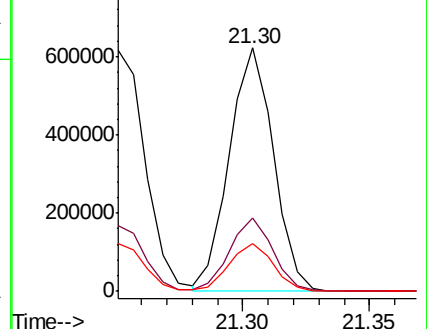

#89

Di-n-octyl phthalate

Concen: 9.945 ng/ul


RT: 22.11 min Scan# 3234

Delta R.T. -0.01 min



Lab File: BP006293.D


Acq: 23 Jul 2021 18:43

Tgt Ion:149 Resp: 795739



Abundance Ion 149.00 (148.70 to 149.70): E



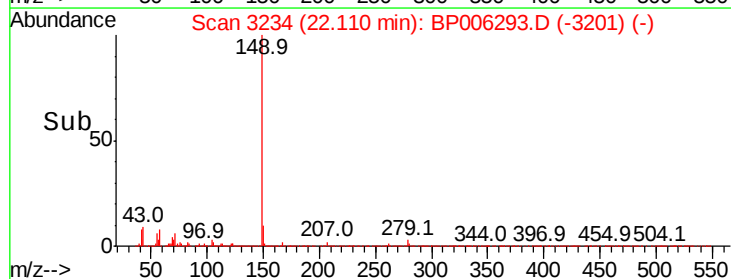
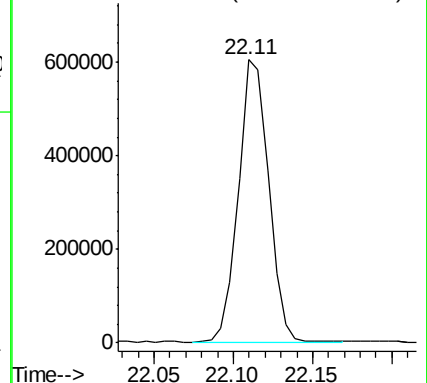


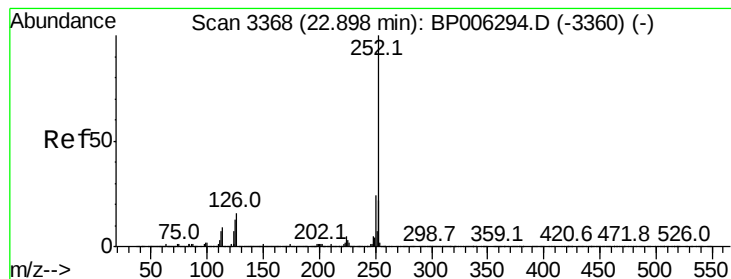

#90
Benzo(b)fluoranthene
Concen: 9.848 ng/ul
RT: 22.90 min Scan# 3368
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43




Instrument :
BNA_P
ClientSampleId :
SSTD010602


Tot Ion	Ratio	Lower	Upper
252	100		
253	22.5	17.7	26.5
125	13.1	10.6	16.0

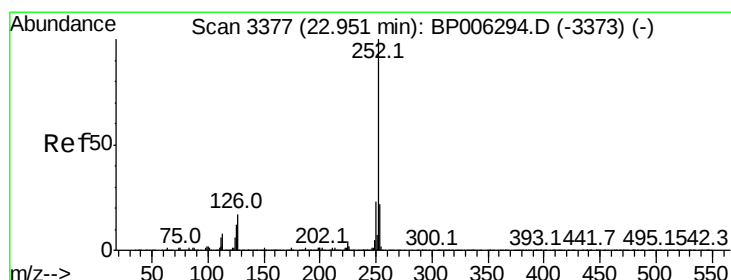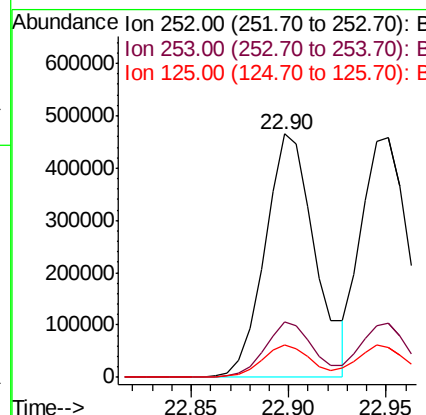

#91
Benzo(k)fluoranthene
Concen: 9.207 ng/ul
RT: 22.95 min Scan# 3377
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
252	100		
253	22.6	17.5	26.3
125	12.7	10.3	15.5

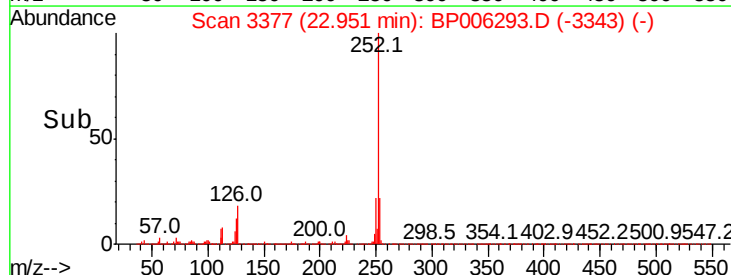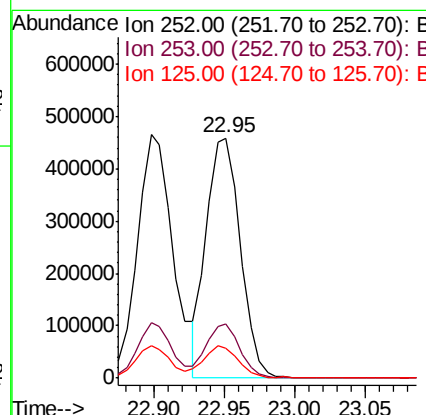



#93

Benzo(a)pyrene

Concen: 9.614 ng/ul

RT: 23.51 min Scan# 3472

Delta R.T. -0.00 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43

Instrument :

BNA_P

ClientSampleId :

SSTD010602


Tot Ion:252 Resp: 706848

Ion Ratio Lower Upper

252 100

253 21.8 17.6 26.4




125 13.9 11.8 17.8



Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

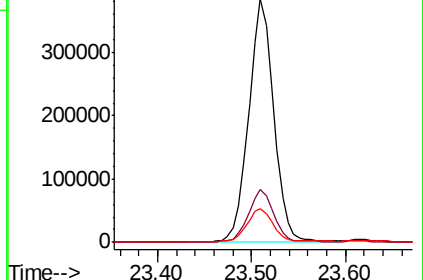

#94

Indeno(1,2,3-cd)pyrene

Concen: 9.646 ng/ul

RT: 26.04 min Scan# 3902

Delta R.T. -0.01 min

Lab File: BP006293.D

Acq: 23 Jul 2021 18:43


Tgt Ion:276 Resp: 896286

Ion Ratio Lower Upper

276 100

138 26.9 21.8 32.6



277 25.1 19.6 29.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E



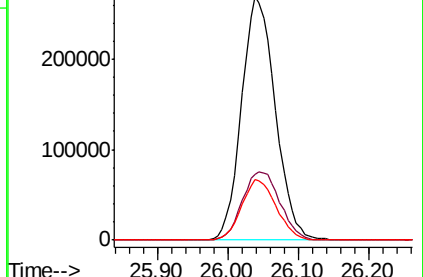





#95
Dibenzo(a,h)anthracene
Concen: 9.856 ng/ul
RT: 26.07 min Scan# 3907
Delta R.T. -0.00 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Instrument :
BNA_P
ClientSampleId :
SSTD010602

Tot Ion	Ratio	Lower	Upper
278	100		
139	17.9	15.8	23.6
279	24.2	18.8	28.2

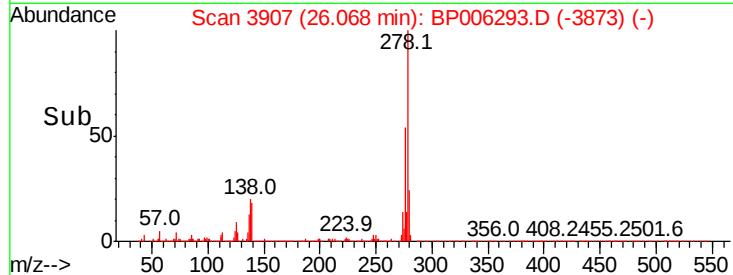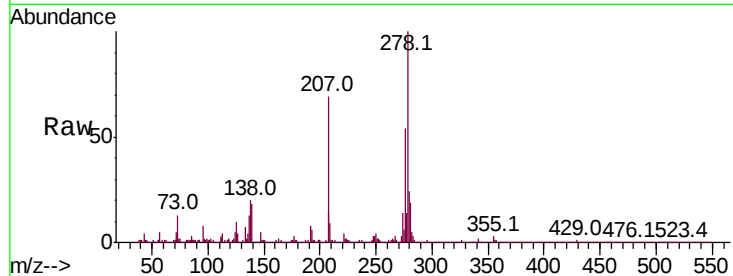

#96
Benzo(g,h,i)perylene
Concen: 9.518 ng/ul
RT: 26.79 min Scan# 4029
Delta R.T. -0.01 min
Lab File: BP006293.D
Acq: 23 Jul 2021 18:43

Tgt Ion	Ratio	Lower	Upper
276	100		
138	27.5	20.2	30.4
277	23.8	18.6	27.8

