

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006326.D
 Acq On : 25 Jul 2021 03:03
 Operator : CG/JU
 Sample : M3063-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AW9

Quant Time: Jul 26 01:11:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	270538	20.000	ng/u1	0.00
20) Naphthalene-d8	10.575	136	1163212	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.416	164	674894	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	1336075	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1253260	20.000	ng/u1	0.00
88) Perylene-d12	23.604	264	1283899	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	34775	4.798	ng/uL	0.00
4) Pyridine-d5	3.711	84	171359	7.964	ng/u1	0.00
7) Phenol-d5	6.958	99	202905	7.986	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.134	67	529831	33.513	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	529432	28.046	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	370885	18.562	ng/u1	0.00
21) Nitrobenzene-d5	8.946	128	321541	37.124	ng/u1	0.00
24) 2-Nitrophenol-d4	9.657	143	319571	38.642	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	523991	32.334	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	789647	29.597	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	1929360	40.167	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	2260424	38.303	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	77253	8.100	ng/u1	0.00
60) Fluorene-d10	15.410	176	1587190	39.306	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	264444	35.504	ng/u1	0.00
73) Anthracene-d10	17.263	188	2577505	42.736	ng/u1	0.00
81) Pyrene-d10	19.504	212	2856733	44.317	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.457	264	2802655	42.956	ng/u1	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.940	77	64194	4.631	ng/u1	97
16) Acetophenone	8.610	105	31211	1.016	ng/u1	97
59) Diethylphthalate	15.251	149	54998	1.126	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006326.D
Acq On : 25 Jul 2021 03:03
Operator : CG/JU
Sample : M3063-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AW9

Quant Time: Jul 26 01:11:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration




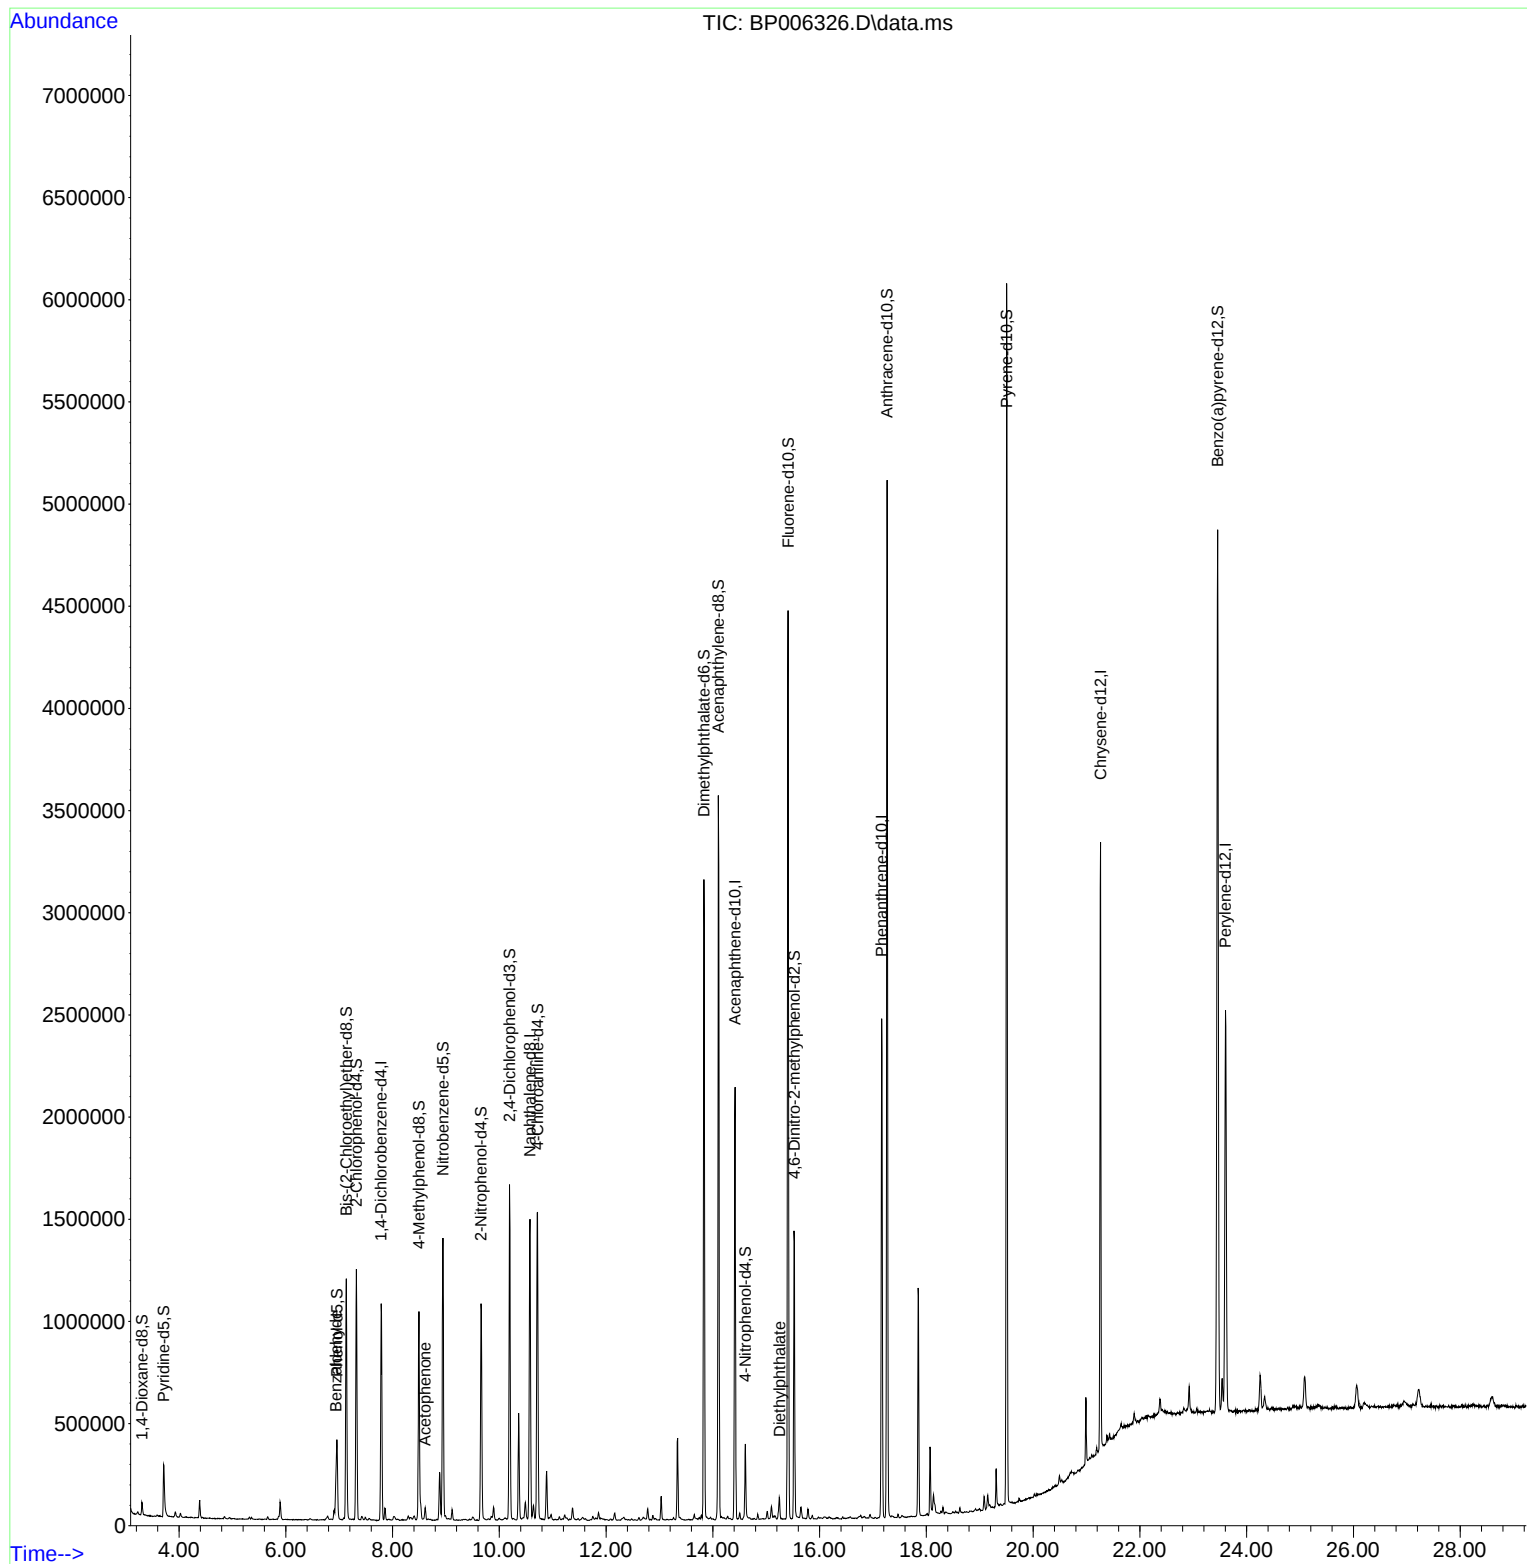


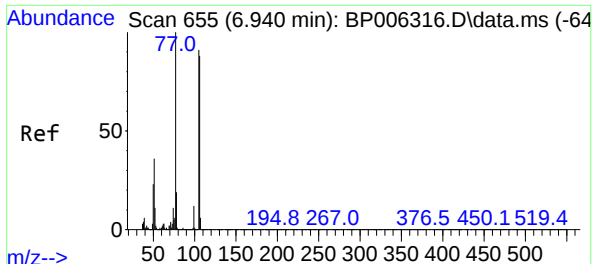

#6
Benzaldehyde
Concen: 4.631 ng/ul
RT: 6.940 min Scan# 655
Delta R.T. -0.006 min
Lab File: BP006326.D
Acq: 25 Jul 2021 03:03




Instrument :
BNA_P
ClientSampleId :
C0AW9


Tgt Ion: 77 Resp: 64194
Ion Ratio Lower Upper
77 100
105 90.3 74.5 111.7
106 86.4 71.0 106.4

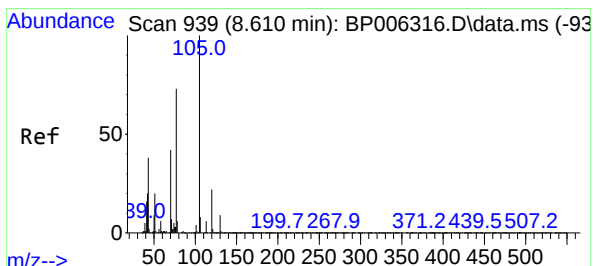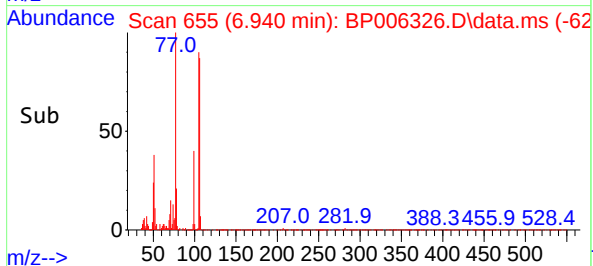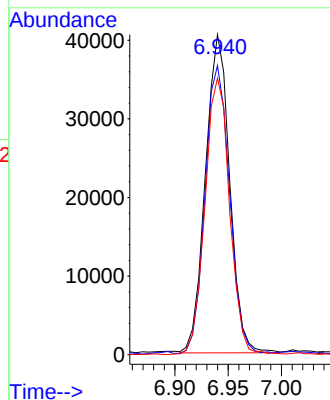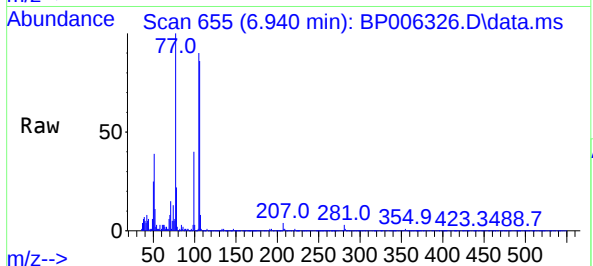

#16
Acetophenone
Concen: 1.016 ng/ul
RT: 8.610 min Scan# 939
Delta R.T. -0.006 min
Lab File: BP006326.D
Acq: 25 Jul 2021 03:03

Tgt Ion: 105 Resp: 31211
Ion Ratio Lower Upper
105 100
77 77.8 65.0 97.4
51 22.7 17.9 26.9

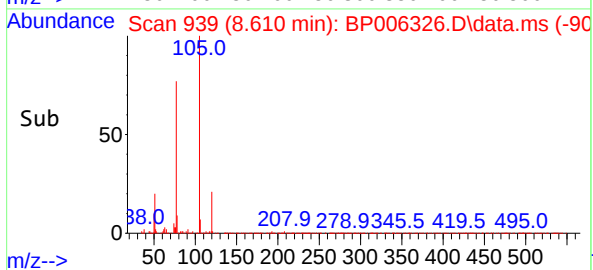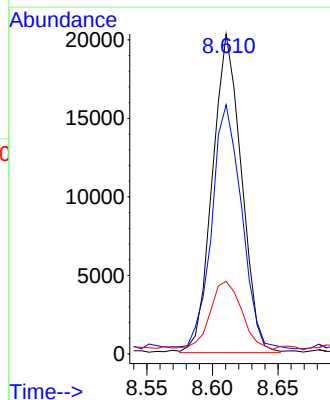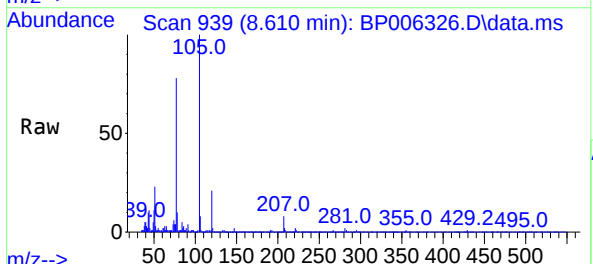

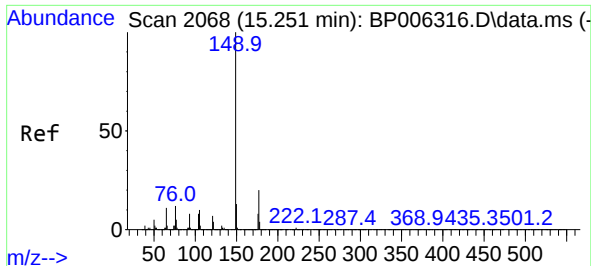

#59
Diethylphthalate
Concen: 1.126 ng/ul
RT: 15.251 min Scan# 2068
Delta R.T. -0.006 min
Lab File: BP006326.D
Acq: 25 Jul 2021 03:03

Instrument :
BNA_P
ClientSampleId :
C0AW9

Tgt Ion:	149	Resp:	54998
Ion	Ratio	Lower	Upper
149	100		
177	20.8	16.1	24.1
150	13.8	9.8	14.6

