

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006310.D
 Acq On : 24 Jul 2021 17:22
 Operator : CG/JU
 Sample : M2973-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006310.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	33	36	43	rVB	29481	38013	1.08%	0.104%
2	3.710	102	106	120	rBV	212809	346755	9.89%	0.947%
3	3.928	140	143	150	rVB4	8990	15266	0.44%	0.042%
4	4.022	155	159	169	rVB	20150	31718	0.90%	0.087%
5	4.928	311	313	317	rVB5	3811	4216	0.12%	0.012%
6	5.822	463	465	468	rVB3	3350	3535	0.10%	0.010%
7	6.416	563	566	569	rBV5	2971	4144	0.12%	0.011%
8	6.740	616	621	622	rVV5	2909	4360	0.12%	0.012%
9	6.793	625	630	636	rVB8	5830	11373	0.32%	0.031%
10	6.957	652	658	671	rBV	420763	715087	20.40%	1.952%
11	7.040	671	672	677	rVB5	4009	4399	0.13%	0.012%
12	7.134	680	688	702	rBV	388039	610108	17.41%	1.666%
13	7.322	712	720	729	rBV	458881	708972	20.23%	1.936%
14	7.422	732	737	740	rBV6	7861	10190	0.29%	0.028%
15	7.792	791	800	807	rBV	946579	1481772	42.28%	4.045%
16	7.863	807	812	819	rVB2	21029	30937	0.88%	0.084%
17	7.928	819	823	826	rBV6	3073	4240	0.12%	0.012%
18	8.028	835	840	844	rBV4	9034	15790	0.45%	0.043%
19	8.334	886	892	896	rBV3	7171	11967	0.34%	0.033%
20	8.492	911	919	927	rBV	542926	865881	24.71%	2.364%
21	8.545	927	928	934	rVV4	7250	9933	0.28%	0.027%
22	8.610	935	939	944	rVB2	12588	19145	0.55%	0.052%
23	8.945	988	996	1006	rBV	419398	678955	19.37%	1.854%
24	9.063	1009	1016	1021	rVV2	14212	26631	0.76%	0.073%
25	9.122	1021	1026	1033	rVB2	6195	12836	0.37%	0.035%
26	9.663	1110	1118	1127	rBV	287123	476074	13.58%	1.300%
27	9.892	1152	1157	1162	rVV9	3848	6306	0.18%	0.017%
28	10.092	1186	1191	1195	rVB7	2715	5324	0.15%	0.015%
29	10.192	1201	1208	1217	rBV	463379	760327	21.69%	2.076%
30	10.369	1230	1238	1246	rBV	68370	115029	3.28%	0.314%
31	10.575	1265	1273	1280	rBV	1274844	2142975	61.14%	5.851%
32	10.622	1280	1281	1285	rVB4	5638	5571	0.16%	0.015%
33	10.716	1288	1297	1308	rBV	517824	864943	24.68%	2.361%
34	11.104	1357	1363	1373	rBV10	11954	25611	0.73%	0.070%
35	11.228	1376	1384	1385	rBV8	3263	6093	0.17%	0.017%
36	11.369	1404	1408	1414	rBV9	5413	9233	0.26%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006310.D
 Acq On : 24 Jul 2021 17:22
 Operator : CG/JU
 Sample : M2973-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	11.616	1445	1450	1456	rBV4	7307	14588	0.42%	0.040%
38	11.928	1499	1503	1505	rBV5	2981	3932	0.11%	0.011%
39	12.163	1536	1543	1548	rVB2	11294	18473	0.53%	0.050%
40	12.375	1574	1579	1583	rBV8	2231	3657	0.10%	0.010%
41	12.428	1585	1588	1593	rVV4	4516	7557	0.22%	0.021%
42	12.780	1645	1648	1652	rVB3	7021	9030	0.26%	0.025%
43	13.033	1683	1691	1696	rBV3	12007	21068	0.60%	0.058%
44	13.145	1706	1710	1714	rVB6	2777	3595	0.10%	0.010%
45	13.263	1725	1730	1735	rVB9	5817	9397	0.27%	0.026%
46	13.327	1735	1741	1746	rBV10	4513	8647	0.25%	0.024%
47	13.386	1746	1751	1754	rVV7	4127	5407	0.15%	0.015%
48	13.751	1808	1813	1815	rVB6	2890	4932	0.14%	0.013%
49	13.833	1821	1827	1838	rBV	956698	1328271	37.90%	3.626%
50	14.110	1864	1874	1886	rBV	887577	1368948	39.06%	3.737%
51	14.210	1888	1891	1898	rVB9	6712	11914	0.34%	0.033%
52	14.333	1907	1912	1916	rBV7	3351	4957	0.14%	0.014%
53	14.416	1916	1926	1933	rBV	1890687	2749292	78.44%	7.506%
54	14.474	1935	1936	1942	rVB6	4927	5281	0.15%	0.014%
55	14.610	1951	1959	1972	rBV	396462	588094	16.78%	1.606%
56	14.774	1984	1987	1991	rBV6	2568	4033	0.12%	0.011%
57	14.845	1995	1999	2003	rVV6	10547	14999	0.43%	0.041%
58	14.892	2006	2007	2014	rVB7	3676	3866	0.11%	0.011%
59	14.957	2014	2018	2022	rBV7	3469	4977	0.14%	0.014%
60	15.233	2062	2065	2066	rBV2	4169	4805	0.14%	0.013%
61	15.286	2071	2074	2077	rVB5	5361	5545	0.16%	0.015%
62	15.410	2088	2095	2101	rBV	1333876	1920270	54.79%	5.243%
63	15.521	2108	2114	2125	rBV	309675	453695	12.94%	1.239%
64	15.651	2131	2136	2140	rVB2	15030	21241	0.61%	0.058%
65	15.974	2188	2191	2192	rBV3	4242	3935	0.11%	0.011%
66	16.210	2227	2231	2236	rVB5	14423	20480	0.58%	0.056%
67	16.321	2246	2250	2252	rBV5	5456	7893	0.23%	0.022%
68	16.574	2289	2293	2299	rVB8	7684	12653	0.36%	0.035%
69	16.916	2344	2351	2354	rBV3	22624	37156	1.06%	0.101%
70	16.951	2354	2357	2360	rVB3	11982	15342	0.44%	0.042%
71	17.045	2370	2373	2376	rBV5	4179	6006	0.17%	0.016%
72	17.168	2387	2394	2399	rBV	2212535	3163678	90.27%	8.637%
73	17.204	2399	2400	2405	rVV	45169	53767	1.53%	0.147%
74	17.263	2405	2410	2422	rVV2	1421240	2064427	58.90%	5.636%
75	17.363	2423	2427	2434	rVB10	14632	29147	0.83%	0.080%
76	17.574	2460	2463	2468	rVB6	8021	9685	0.28%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006310.D
 Acq On : 24 Jul 2021 17:22
 Operator : CG/JU
 Sample : M2973-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	17.863	2508	2512	2516	rBV	31662	37158	1.06%	0.101%
78	18.039	2538	2542	2544	rBV4	14629	20039	0.57%	0.055%
79	18.074	2544	2548	2556	rVB2	124481	179718	5.13%	0.491%
80	18.145	2557	2560	2561	rBV	9256	10366	0.30%	0.028%
81	18.227	2570	2574	2577	rBV3	21001	28974	0.83%	0.079%
82	18.480	2613	2617	2621	rBV	36368	44692	1.28%	0.122%
83	18.527	2622	2625	2630	rVB4	13255	16549	0.47%	0.045%
84	18.927	2687	2693	2696	rBV7	27002	47724	1.36%	0.130%
85	18.998	2702	2705	2708	rVB4	33849	36503	1.04%	0.100%
86	19.086	2716	2720	2724	rVB3	22398	30525	0.87%	0.083%
87	19.180	2728	2736	2745	rVV	216803	317675	9.06%	0.867%
88	19.310	2755	2758	2766	rVB3	64128	85819	2.45%	0.234%
89	19.504	2786	2791	2804	rBV	1392108	1999189	57.04%	5.458%
90	20.021	2876	2879	2883	rVB	45061	49131	1.40%	0.134%
91	20.115	2893	2895	2899	rVB2	37956	43108	1.23%	0.118%
92	20.504	2956	2961	2965	rBV	935247	1017188	29.02%	2.777%
93	20.880	3022	3025	3030	rBV3	101674	145821	4.16%	0.398%
94	20.992	3041	3044	3046	rBV3	103332	132599	3.78%	0.362%
95	21.021	3046	3049	3053	rVB	273829	312903	8.93%	0.854%
96	21.262	3085	3090	3094	rBV	2838472	3445588	98.31%	9.407%
97	23.456	3458	3463	3473	rVB2	543030	1013620	28.92%	2.767%
98	23.609	3483	3489	3499	rVB2	1770148	3504861	100.00%	9.569%




Sum of corrected areas: 36628099

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006310.D
Acq On : 24 Jul 2021 17:22
Operator : CG/JU
Sample : M2973-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

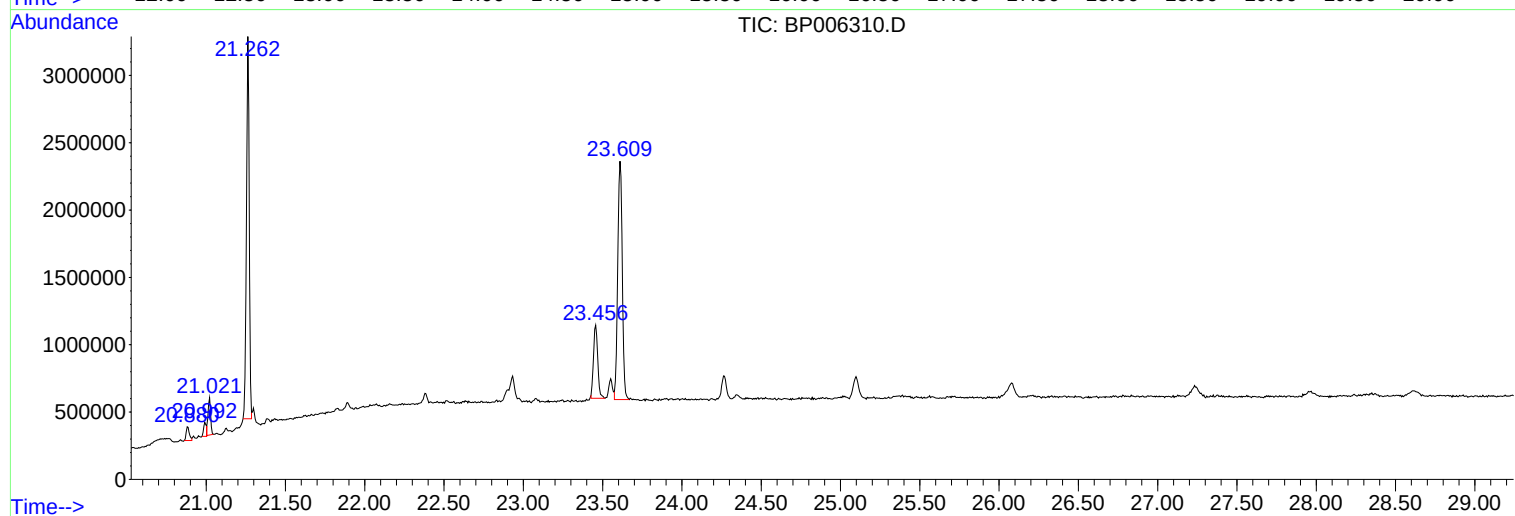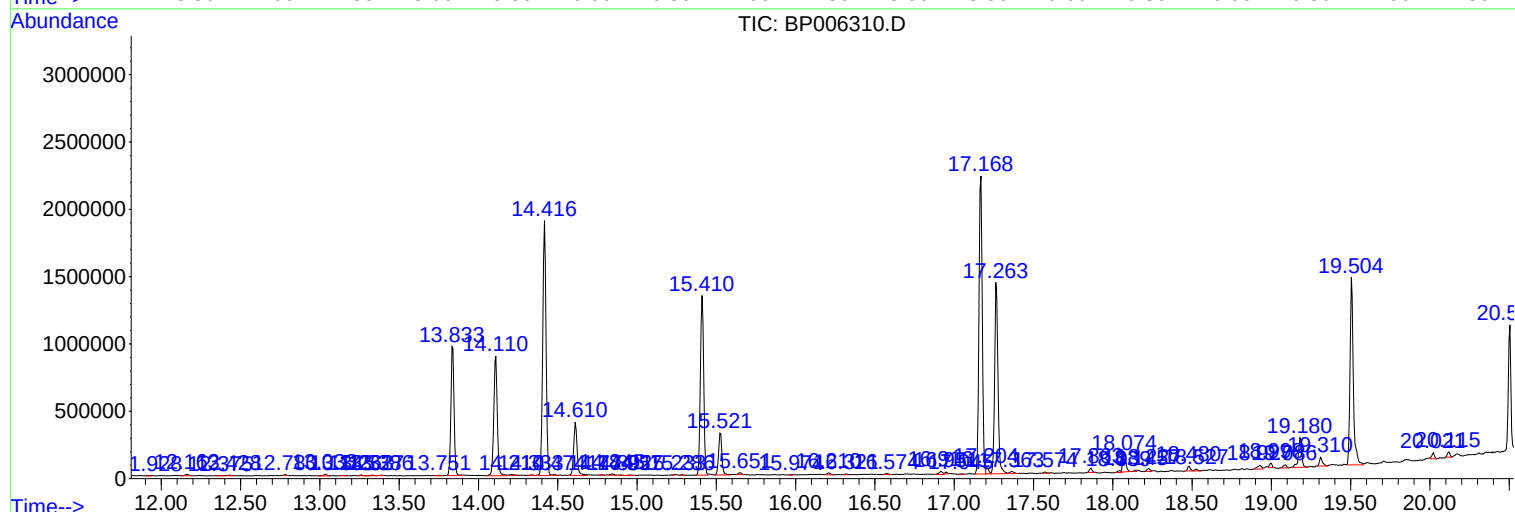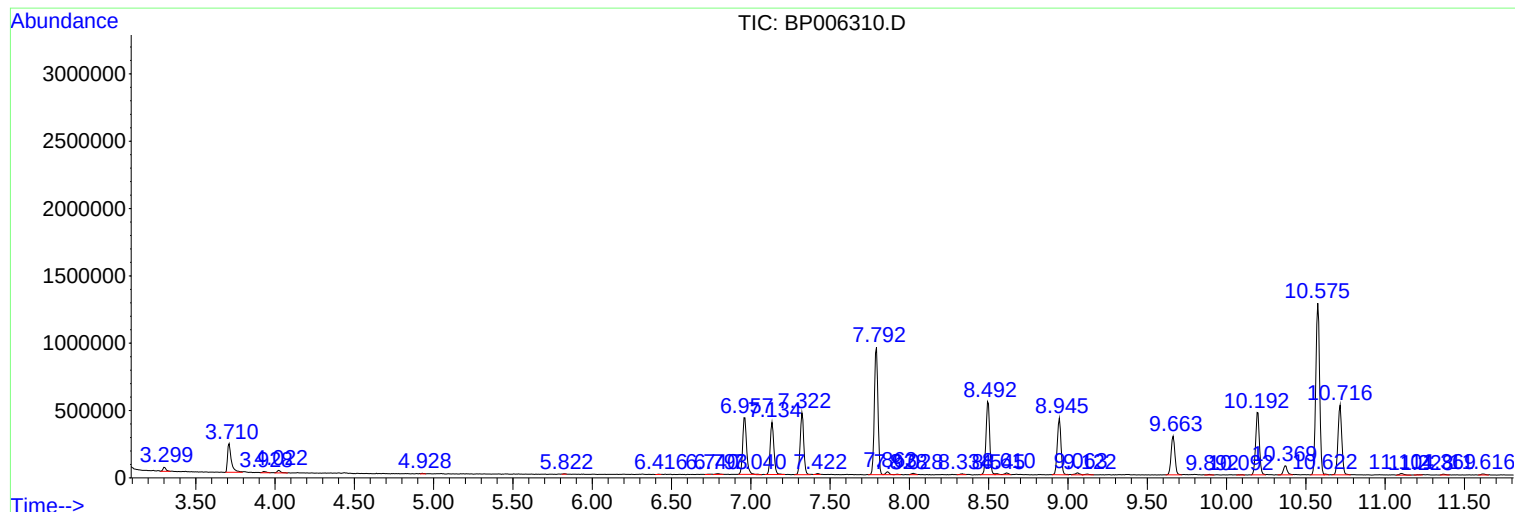

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006310.D
Acq On : 24 Jul 2021 17:22
Operator : CG/JU
Sample : M2973-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC4










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Adipic acid, 2-ethylhexyl o... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.500	5.90 ng/ul	1017190	Chrysene-d12	21.262

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	91
2			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	87
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	86
4			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	83
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	83

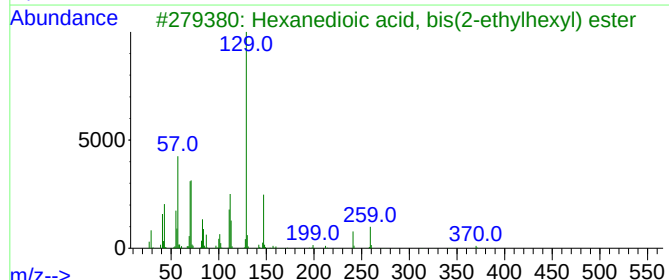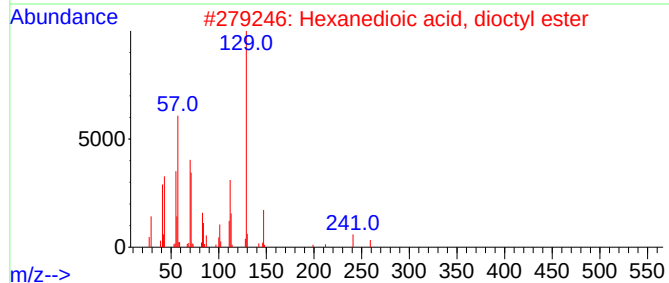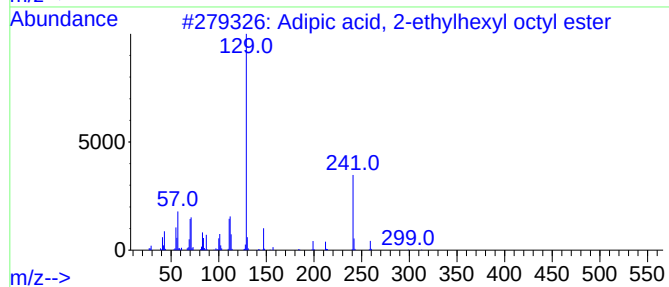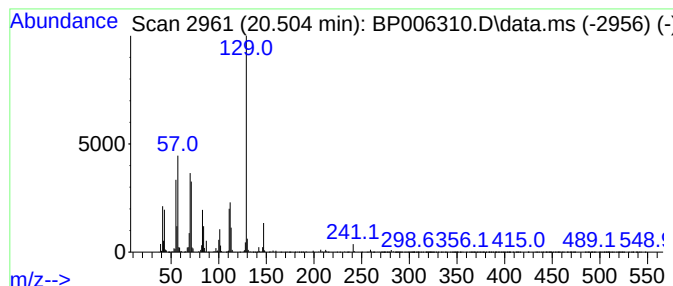

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006310.D
Acq On : 24 Jul 2021 17:22
Operator : CG/JU
Sample : M2973-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC4

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Adipic acid, 2-...	20.500	5.9	ng/ul	1017190	5	21.262	3445590	20.0