

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006320.D
 Acq On : 24 Jul 2021 23:38
 Operator : CG/JU
 Sample : M2973-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006320.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.311	34	38	44	rVB	32055	47214	0.98%	0.098%
2	3.717	103	107	122	rBV	243678	419782	8.74%	0.873%
3	3.817	122	124	133	rVB7	12191	19461	0.41%	0.040%
4	3.934	141	144	149	rVB	9849	14913	0.31%	0.031%
5	4.028	156	160	165	rVB	20744	30296	0.63%	0.063%
6	6.787	624	629	634	rBV9	5748	10722	0.22%	0.022%
7	6.964	651	659	670	rBV	489428	809047	16.84%	1.682%
8	7.134	682	688	699	rBV	449006	696202	14.49%	1.448%
9	7.322	712	720	728	rBV	531961	823224	17.13%	1.712%
10	7.422	733	737	745	rVB6	7124	11758	0.24%	0.024%
11	7.793	792	800	807	rBV	1132537	1821483	37.91%	3.788%
12	8.022	833	839	845	rBV4	13752	25712	0.54%	0.053%
13	8.328	886	891	894	rBV6	9464	15261	0.32%	0.032%
14	8.493	911	919	930	rBV	637874	995075	20.71%	2.069%
15	8.610	933	939	946	rVV	17743	31271	0.65%	0.065%
16	8.946	988	996	1004	rBV	475517	782601	16.29%	1.627%
17	9.663	1111	1118	1130	rBV	340984	559337	11.64%	1.163%
18	10.193	1199	1208	1217	rBV	530799	876414	18.24%	1.822%
19	10.369	1231	1238	1248	rBV	97435	168423	3.51%	0.350%
20	10.575	1265	1273	1280	rVV	1588661	2613488	54.40%	5.434%
21	10.622	1280	1281	1288	rVV	10946	13434	0.28%	0.028%
22	10.716	1288	1297	1310	rVB	542939	930601	19.37%	1.935%
23	11.104	1357	1363	1371	rBV	6529	13321	0.28%	0.028%
24	11.369	1403	1408	1413	rBV7	8730	14243	0.30%	0.030%
25	12.163	1537	1543	1548	rBV2	12812	23116	0.48%	0.048%
26	12.781	1641	1648	1653	rBV4	11596	17198	0.36%	0.036%
27	13.034	1686	1691	1695	rBV4	13638	20839	0.43%	0.043%
28	13.257	1722	1729	1736	rVB4	6873	14126	0.29%	0.029%
29	13.387	1747	1751	1756	rVB8	6197	10378	0.22%	0.022%
30	13.746	1805	1812	1815	rVB6	8420	14777	0.31%	0.031%
31	13.834	1821	1827	1838	rBV	1100435	1459013	30.37%	3.034%
32	14.104	1863	1873	1886	rBV	1005390	1568749	32.65%	3.262%
33	14.416	1919	1926	1933	rVV	2243826	3299299	68.67%	6.861%
34	14.475	1933	1936	1945	rVB3	18204	32396	0.67%	0.067%
35	14.610	1952	1959	1970	rBV	358265	527976	10.99%	1.098%
36	14.810	1990	1993	1996	rVV4	13479	19908	0.41%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006320.D
 Acq On : 24 Jul 2021 23:38
 Operator : CG/JU
 Sample : M2973-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	14.840	1996	1998	2002	rVV5	10730	12924	0.27%	0.027%
38	14.893	2002	2007	2013	rVB3	12761	18806	0.39%	0.039%
39	15.034	2026	2031	2035	rBV8	9976	18709	0.39%	0.039%
40	15.087	2035	2040	2045	rVB4	9244	16737	0.35%	0.035%
41	15.204	2054	2060	2061	rBV6	10670	14826	0.31%	0.031%
42	15.281	2071	2073	2079	rVB4	8749	11261	0.23%	0.023%
43	15.410	2088	2095	2100	rVV	1465833	2120725	44.14%	4.410%
44	15.457	2100	2103	2109	rVB3	34178	54170	1.13%	0.113%
45	15.522	2109	2114	2123	rBV	320093	447304	9.31%	0.930%
46	15.645	2128	2135	2140	rBV6	14140	29533	0.61%	0.061%
47	15.757	2150	2154	2163	rVB2	23409	39667	0.83%	0.082%
48	15.904	2176	2179	2187	rVB2	22408	43603	0.91%	0.091%
49	15.987	2187	2193	2194	rBV6	6938	10933	0.23%	0.023%
50	16.204	2227	2230	2235	rVB3	14718	17037	0.35%	0.035%
51	16.322	2245	2250	2255	rVB9	8791	12950	0.27%	0.027%
52	16.475	2267	2276	2280	rBV3	24218	49944	1.04%	0.104%
53	16.516	2280	2283	2288	rVB3	10195	13532	0.28%	0.028%
54	16.569	2288	2292	2296	rVB7	9022	13531	0.28%	0.028%
55	16.622	2297	2301	2306	rVB4	13715	20416	0.42%	0.042%
56	16.704	2309	2315	2318	rBV3	20563	34664	0.72%	0.072%
57	16.739	2318	2321	2326	rVB5	20100	28167	0.59%	0.059%
58	16.834	2333	2337	2343	rVB7	11640	18458	0.38%	0.038%
59	16.916	2344	2351	2354	rVV4	32209	68738	1.43%	0.143%
60	16.951	2354	2357	2359	rVV3	20817	27890	0.58%	0.058%
61	16.981	2359	2362	2369	rVV2	27723	54092	1.13%	0.112%
62	17.163	2387	2393	2398	rBV	2592713	3766379	78.39%	7.832%
63	17.204	2398	2400	2405	rVV	494469	640570	13.33%	1.332%
64	17.263	2405	2410	2414	rVV2	1437816	2085005	43.40%	4.336%
65	17.298	2414	2416	2423	rVV	221157	279044	5.81%	0.580%
66	17.363	2423	2427	2431	rVB6	23945	39141	0.81%	0.081%
67	17.616	2465	2470	2474	rBV7	12444	20847	0.43%	0.043%
68	17.692	2479	2483	2487	rBV2	18127	28574	0.59%	0.059%
69	17.745	2490	2492	2498	rVB6	8237	14241	0.30%	0.030%
70	17.857	2507	2511	2514	rBV	36403	48461	1.01%	0.101%
71	18.034	2537	2541	2544	rBV	90667	126770	2.64%	0.264%
72	18.081	2544	2549	2555	rVV2	158203	282569	5.88%	0.588%
73	18.163	2557	2563	2568	rVV2	59355	99108	2.06%	0.206%
74	18.222	2568	2573	2577	rVV2	144015	252954	5.26%	0.526%
75	18.257	2577	2579	2585	rVB2	64332	79846	1.66%	0.166%
76	18.481	2612	2617	2621	rBV	105395	138906	2.89%	0.289%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
 Data File : BP006320.D
 Acq On : 24 Jul 2021 23:38
 Operator : CG/JU
 Sample : M2973-10
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGEC7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	18.528	2621	2625	2630	rVB	70883	97429	2.03%	0.203%
78	18.763	2662	2665	2669	rBV4	18647	21393	0.45%	0.044%
79	18.810	2670	2673	2676	rBV2	29136	30485	0.63%	0.063%
80	18.845	2676	2679	2684	rVB3	22009	27976	0.58%	0.058%
81	18.928	2688	2693	2697	rBV2	78161	121598	2.53%	0.253%
82	19.057	2712	2715	2716	rBV3	18655	19636	0.41%	0.041%
83	19.181	2731	2736	2742	rVB	1014268	1277935	26.60%	2.657%
84	19.328	2755	2761	2765	rVB	67474	115634	2.41%	0.240%
85	19.504	2786	2791	2794	rBV	1416046	1933146	40.24%	4.020%
86	19.533	2794	2796	2805	rVV	447986	523291	10.89%	1.088%
87	19.604	2805	2808	2815	rVB3	41978	71604	1.49%	0.149%
88	19.710	2823	2826	2831	rVB	56556	68562	1.43%	0.143%
89	19.857	2845	2851	2857	rBV3	62851	147116	3.06%	0.306%
90	19.986	2868	2873	2874	rBV3	44514	72722	1.51%	0.151%
91	20.016	2875	2878	2883	rVB	192983	236411	4.92%	0.492%
92	20.116	2891	2895	2899	rBV2	185476	237067	4.93%	0.493%
93	20.169	2901	2904	2909	rVB2	77922	119692	2.49%	0.249%
94	20.498	2956	2960	2965	rBV	2596621	2684245	55.87%	5.582%
95	20.992	3040	3044	3053	rBV6	127988	246569	5.13%	0.513%
96	21.263	3083	3090	3094	rBV2	3277142	4804501	100.00%	9.990%
97	21.298	3094	3096	3104	rVB	389900	455598	9.48%	0.947%
98	22.892	3364	3367	3369	rBV	164650	233421	4.86%	0.485%
99	23.451	3458	3462	3468	rVB2	423024	692389	14.41%	1.440%
100	23.604	3482	3488	3500	rVB2	2025359	4000690	83.27%	8.319%




Sum of corrected areas: 48091200

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006320.D
Acq On : 24 Jul 2021 23:38
Operator : CG/JU
Sample : M2973-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

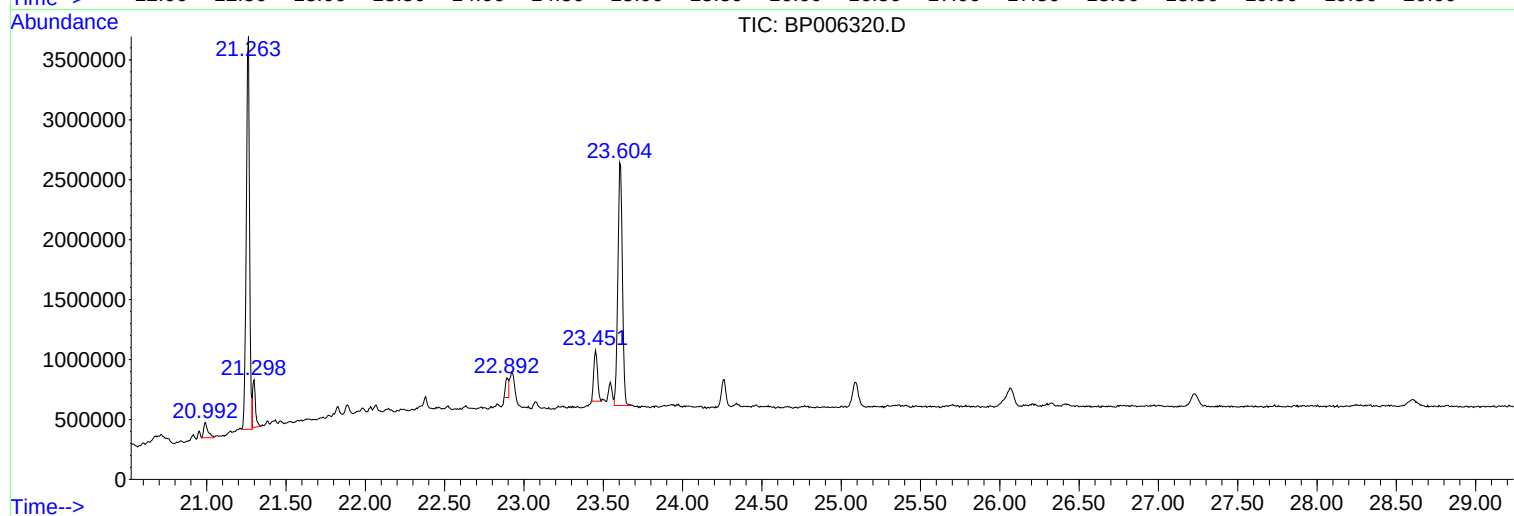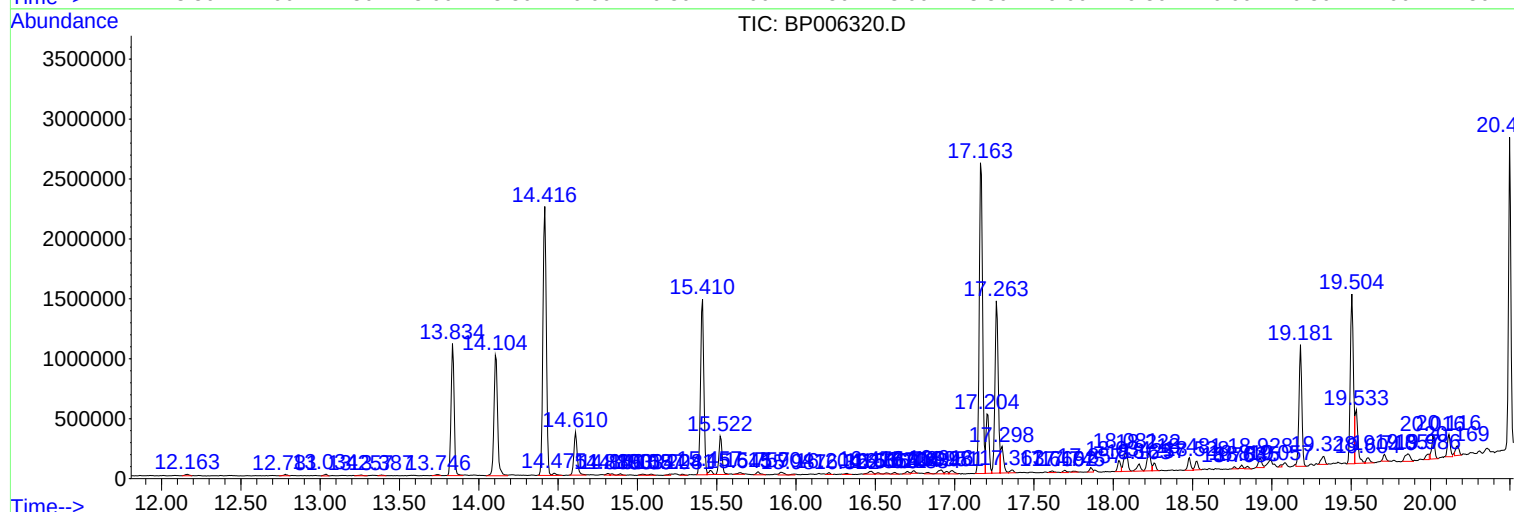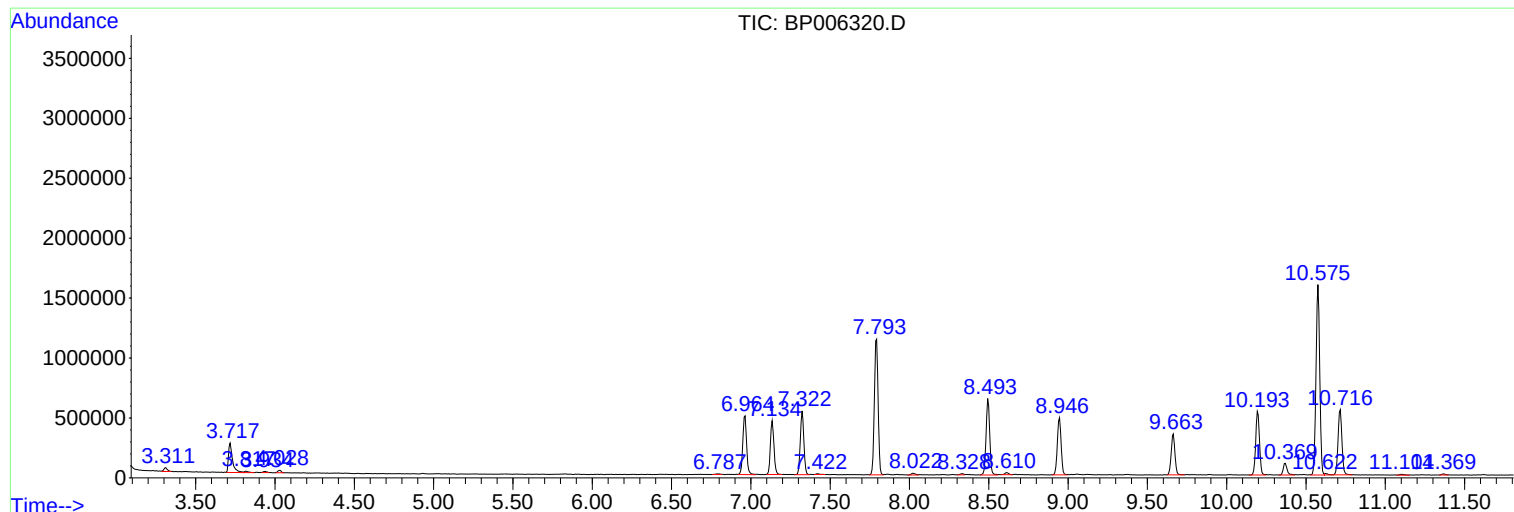

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006320.D
Acq On : 24 Jul 2021 23:38
Operator : CG/JU
Sample : M2973-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC7










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diisooctyl adipate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.500	11.17 ng/ul	2684250	Chrysene-d12	21.263

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diisooctyl adipate	370	C22H42O4	001330-86-5	90
2			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	87
3			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	83
4			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	64
5			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	62

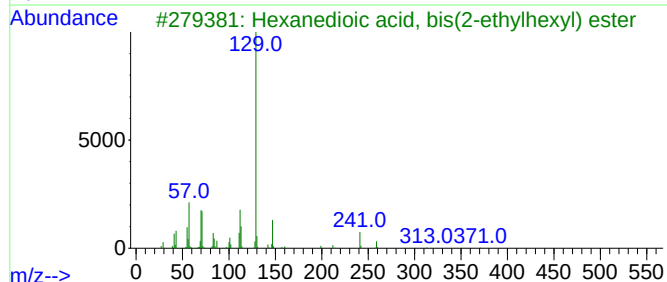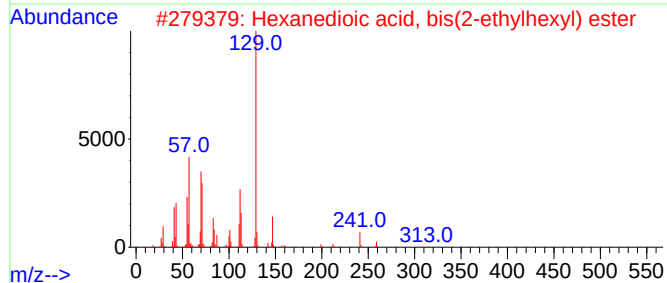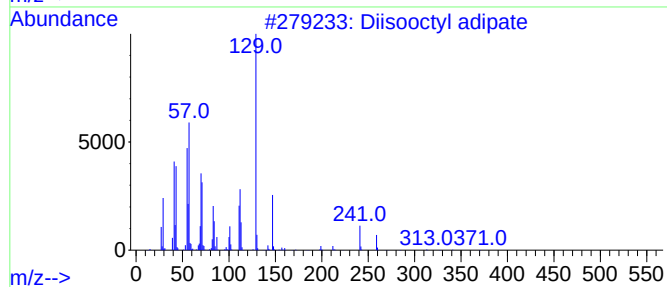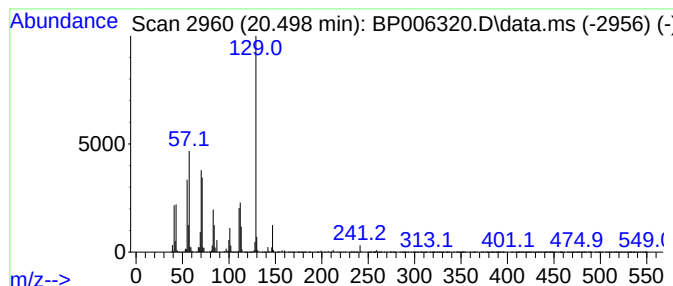

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072421\
Data File : BP006320.D
Acq On : 24 Jul 2021 23:38
Operator : CG/JU
Sample : M2973-10
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGEC7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diisooctyl adipate	20.500	11.2	ng/ul	2684250	5	21.263	4804500	20.0