

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021134.D
 Acq On : 24 Jul 2024 20:56
 Operator : MA/JU
 Sample : P3244-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	38	rBV	43966	55966	1.16%	0.105%
2	3.605	103	105	120	rBV	257245	398208	8.25%	0.748%
3	3.905	154	156	161	rVB	12906	14900	0.31%	0.028%
4	4.317	222	226	236	rVB3	10175	22322	0.46%	0.042%
5	4.452	247	249	255	rVB7	4274	6210	0.13%	0.012%
6	4.805	305	309	316	rVB	16164	26810	0.56%	0.050%
7	6.758	636	641	646	rVV3	7618	13383	0.28%	0.025%
8	6.875	654	661	675	rBV	227201	445477	9.23%	0.837%
9	6.999	675	682	698	rVB	762788	1243000	25.75%	2.335%
10	7.205	710	717	734	rBV	946370	1537285	31.84%	2.887%
11	7.646	784	792	801	rBV	990415	1491704	30.90%	2.802%
12	8.381	910	917	934	rBV	686763	1272908	26.37%	2.391%
13	8.805	981	989	1007	rBV	886395	1573474	32.59%	2.955%
14	9.152	1043	1048	1051	rBV4	5720	6894	0.14%	0.013%
15	9.516	1102	1110	1126	rBV	733519	1393296	28.86%	2.617%
16	9.816	1155	1161	1166	rBV10	4523	11550	0.24%	0.022%
17	10.075	1198	1205	1227	rBV	1073695	2092197	43.34%	3.930%
18	10.416	1254	1263	1275	rBV	1212674	2084217	43.17%	3.915%
19	10.569	1282	1289	1308	rBV	616285	1341883	27.80%	2.520%
20	11.193	1389	1395	1399	rBV6	10243	22255	0.46%	0.042%
21	11.257	1401	1406	1414	rVB4	16317	33256	0.69%	0.062%
22	12.016	1530	1535	1544	rBV2	16390	32251	0.67%	0.061%
23	12.622	1635	1638	1643	rVB7	3903	5766	0.12%	0.011%
24	12.722	1652	1655	1660	rBV6	2668	5010	0.10%	0.009%
25	12.887	1675	1683	1684	rBV7	5210	8509	0.18%	0.016%
26	13.116	1719	1722	1726	rBV6	3746	4920	0.10%	0.009%
27	13.163	1726	1730	1735	rVB8	3159	6558	0.14%	0.012%
28	13.240	1740	1743	1752	rVB10	4229	9435	0.20%	0.018%
29	13.469	1775	1782	1786	rBV10	2765	7019	0.15%	0.013%
30	13.698	1814	1821	1835	rBV	2054087	2942295	60.95%	5.526%
31	13.981	1862	1869	1884	rBV2	2218519	3509761	72.70%	6.592%
32	14.169	1897	1901	1902	rBV4	3826	5285	0.11%	0.010%
33	14.210	1902	1908	1914	rVV5	11192	27285	0.57%	0.051%
34	14.292	1915	1922	1931	rVV	1711722	2671034	55.33%	5.017%
35	14.422	1940	1944	1949	rBV7	10302	17340	0.36%	0.033%
36	14.504	1953	1958	1959	rBV3	23097	30242	0.63%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021134.D
 Acq On : 24 Jul 2024 20:56
 Operator : MA/JU
 Sample : P3244-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	14.622	1972	1978	1986	rBV	98918	218976	4.54%	0.411%
38	14.722	1992	1995	2006	rVB	13544	32530	0.67%	0.061%
39	15.145	2064	2067	2069	rBV4	3636	5788	0.12%	0.011%
40	15.251	2082	2085	2088	rBV5	3855	6298	0.13%	0.012%
41	15.310	2088	2095	2104	rVV	3087531	4325110	89.59%	8.124%
42	15.381	2105	2107	2114	rVB3	24523	32060	0.66%	0.060%
43	15.469	2116	2122	2133	rBV	698882	1300773	26.95%	2.443%
44	16.498	2294	2297	2302	rBV7	7118	11909	0.25%	0.022%
45	17.116	2394	2402	2412	rBV	2100698	3110733	64.44%	5.843%
46	17.210	2412	2418	2430	rVV2	2995583	4486298	92.93%	8.426%
47	18.033	2554	2558	2568	rBV	178401	304281	6.30%	0.572%
48	19.133	2743	2745	2751	rVB	39596	51145	1.06%	0.096%
49	19.369	2782	2785	2792	rBV2	131797	185372	3.84%	0.348%
50	19.592	2817	2823	2831	rBV	3830749	4827468	100.00%	9.067%
51	21.545	3150	3155	3167	rVB	1676959	2563452	53.10%	4.815%
52	24.621	3669	3678	3692	rVB	1651902	4429272	91.75%	8.319%
53	24.851	3709	3717	3731	rVB	1073693	2979969	61.73%	5.597%




Sum of corrected areas: 53241339

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021134.D
Acq On : 24 Jul 2024 20:56
Operator : MA/JU
Sample : P3244-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

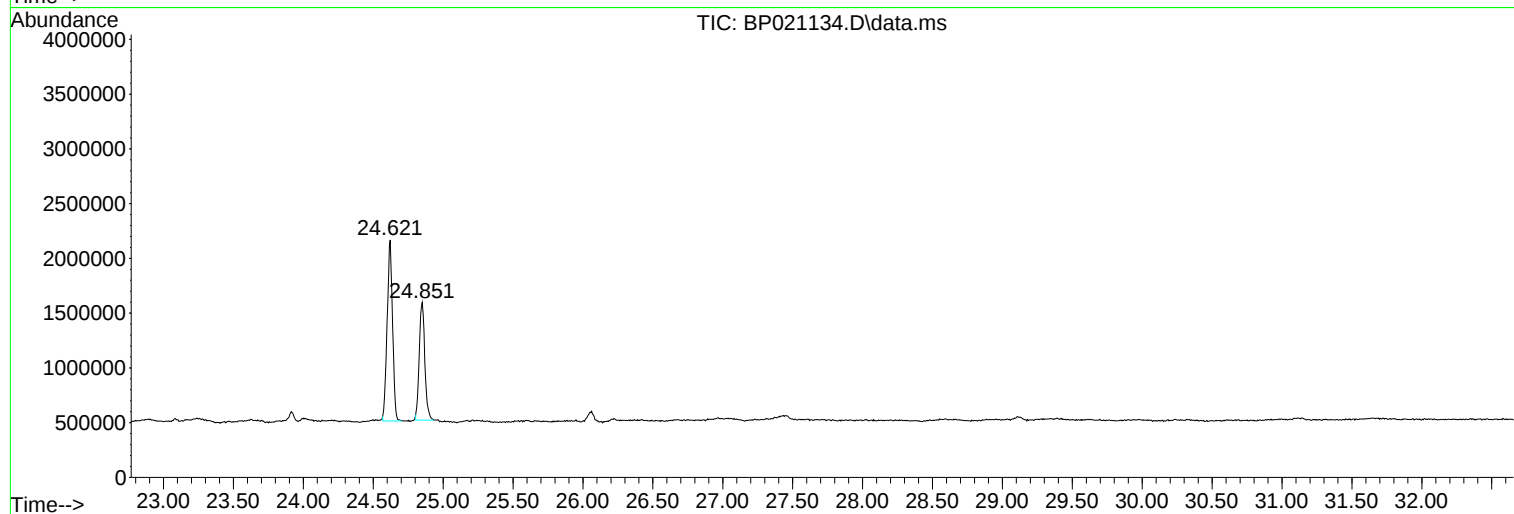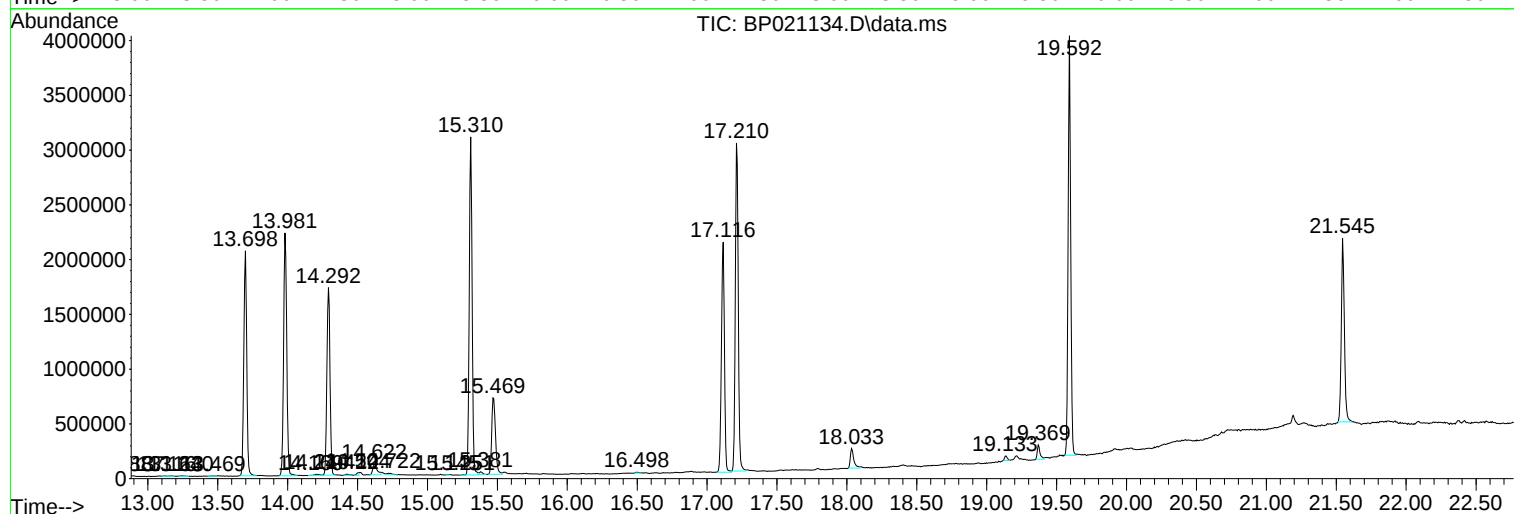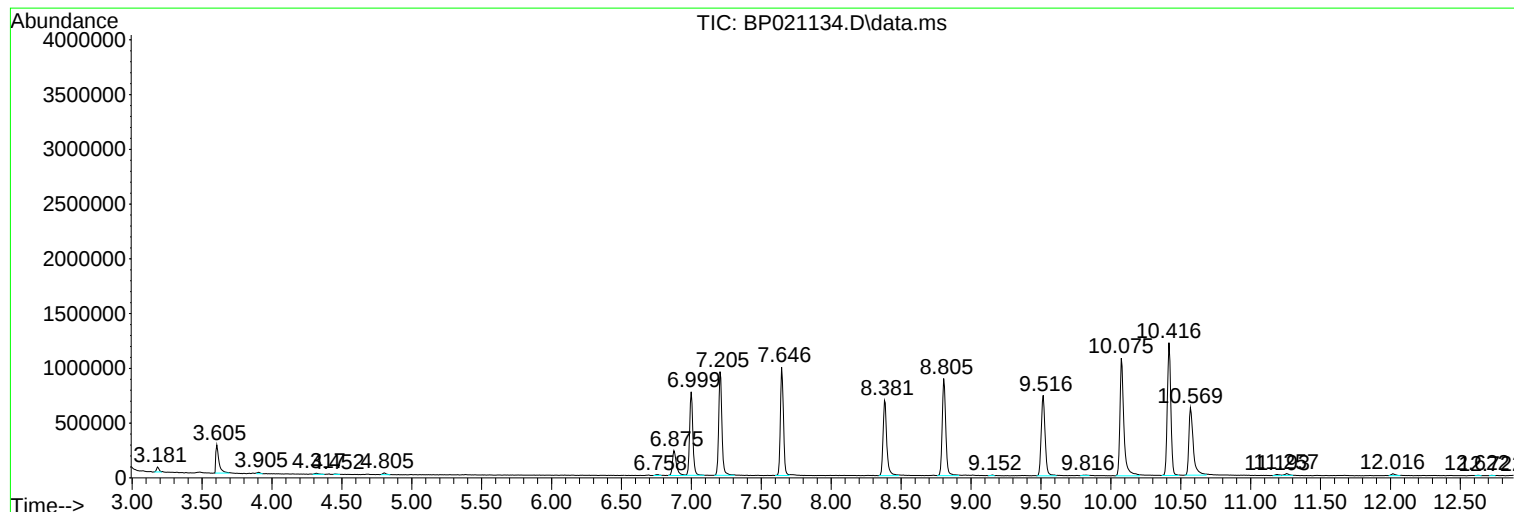

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021134.D
Acq On : 24 Jul 2024 20:56
Operator : MA/JU
Sample : P3244-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021134.D
Acq On : 24 Jul 2024 20:56
Operator : MA/JU
Sample : P3244-09
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
