

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021136.D
 Acq On : 24 Jul 2024 22:23
 Operator : MA/JU
 Sample : P3244-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021136.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	29	33	40	rVB	42974	57355	1.21%	0.126%
2	3.605	102	105	122	rBV	201018	323007	6.83%	0.710%
3	3.905	152	156	161	rVB	13263	17776	0.38%	0.039%
4	4.317	223	226	233	rVB4	7132	12088	0.26%	0.027%
5	4.446	246	248	253	rVB6	3127	4851	0.10%	0.011%
6	4.693	287	290	293	rVB5	3630	5000	0.11%	0.011%
7	4.805	304	309	313	rBV	14337	22449	0.47%	0.049%
8	5.781	471	475	480	rBV7	4497	6829	0.14%	0.015%
9	6.758	637	641	646	rBV3	9229	13544	0.29%	0.030%
10	6.875	654	661	674	rBV	198593	393127	8.31%	0.864%
11	7.005	677	683	698	rVB	578779	979058	20.69%	2.151%
12	7.205	710	717	732	rBV	736722	1263167	26.69%	2.776%
13	7.658	787	794	805	rBV	883317	1428800	30.19%	3.140%
14	8.387	912	918	939	rBV	590782	1095938	23.16%	2.408%
15	8.811	982	990	1004	rBV	683914	1215975	25.70%	2.672%
16	9.016	1020	1025	1032	rVB	14828	23645	0.50%	0.052%
17	9.158	1043	1049	1055	rBV7	5855	10778	0.23%	0.024%
18	9.375	1079	1086	1093	rVB4	12193	24934	0.53%	0.055%
19	9.528	1104	1112	1131	rBV	571429	1065234	22.51%	2.341%
20	9.828	1157	1163	1164	rBV6	3830	5166	0.11%	0.011%
21	10.075	1197	1205	1226	rBV	726310	1626744	34.38%	3.575%
22	10.269	1237	1238	1245	rVB7	2752	4780	0.10%	0.011%
23	10.422	1256	1264	1279	rBV	1028365	1871882	39.56%	4.113%
24	10.581	1283	1291	1313	rBV	634738	1297455	27.42%	2.851%
25	11.193	1389	1395	1403	rBV5	9956	28684	0.61%	0.063%
26	12.028	1531	1537	1543	rBV3	13115	25725	0.54%	0.057%
27	13.087	1712	1717	1724	rBV4	12150	20736	0.44%	0.046%
28	13.399	1768	1770	1777	rVB8	2978	5322	0.11%	0.012%
29	13.463	1777	1781	1784	rBV6	2957	4781	0.10%	0.011%
30	13.704	1812	1822	1835	rBV	1407736	2150739	45.45%	4.726%
31	13.987	1863	1870	1880	rBV	1717061	2572669	54.37%	5.653%
32	14.181	1898	1903	1916	rBV	11422	36686	0.78%	0.081%
33	14.298	1916	1923	1933	rBV	1560166	2297350	48.55%	5.048%
34	14.434	1942	1946	1952	rBV9	3956	8055	0.17%	0.018%
35	14.634	1973	1980	1988	rBV2	74680	194136	4.10%	0.427%
36	14.734	1995	1997	2003	rVB7	11072	18748	0.40%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021136.D
 Acq On : 24 Jul 2024 22:23
 Operator : MA/JU
 Sample : P3244-11
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	15.087	2055	2057	2064	rBV8	3633	5335	0.11%	0.012%
38	15.145	2064	2067	2072	rBV7	6057	8833	0.19%	0.019%
39	15.304	2087	2094	2103	rBV	1990502	3110308	65.73%	6.835%
40	15.469	2116	2122	2133	rBV	478611	924345	19.53%	2.031%
41	17.110	2394	2401	2412	rBV	1749155	2543379	53.75%	5.589%
42	17.216	2412	2419	2431	rBV	2272642	3285107	69.42%	7.219%
43	18.039	2555	2559	2565	rBV	154337	239964	5.07%	0.527%
44	19.139	2743	2746	2750	rBV2	29508	43147	0.91%	0.095%
45	19.216	2757	2759	2763	rBV2	28137	45211	0.96%	0.099%
46	19.369	2782	2785	2791	rBV3	85749	113017	2.39%	0.248%
47	19.598	2818	2824	2832	rBV2	2675513	4016236	84.87%	8.826%
48	19.663	2833	2835	2840	rVB	66745	89423	1.89%	0.197%
49	21.557	3151	3157	3166	rBV	1809521	2788717	58.93%	6.128%
50	24.633	3672	3680	3702	rVB	1746285	4731988	100.00%	10.399%
51	24.869	3711	3720	3733	rVB	1187807	3427803	72.44%	7.533%


Sum of corrected areas: 45506026

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021136.D
Acq On : 24 Jul 2024 22:23
Operator : MA/JU
Sample : P3244-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

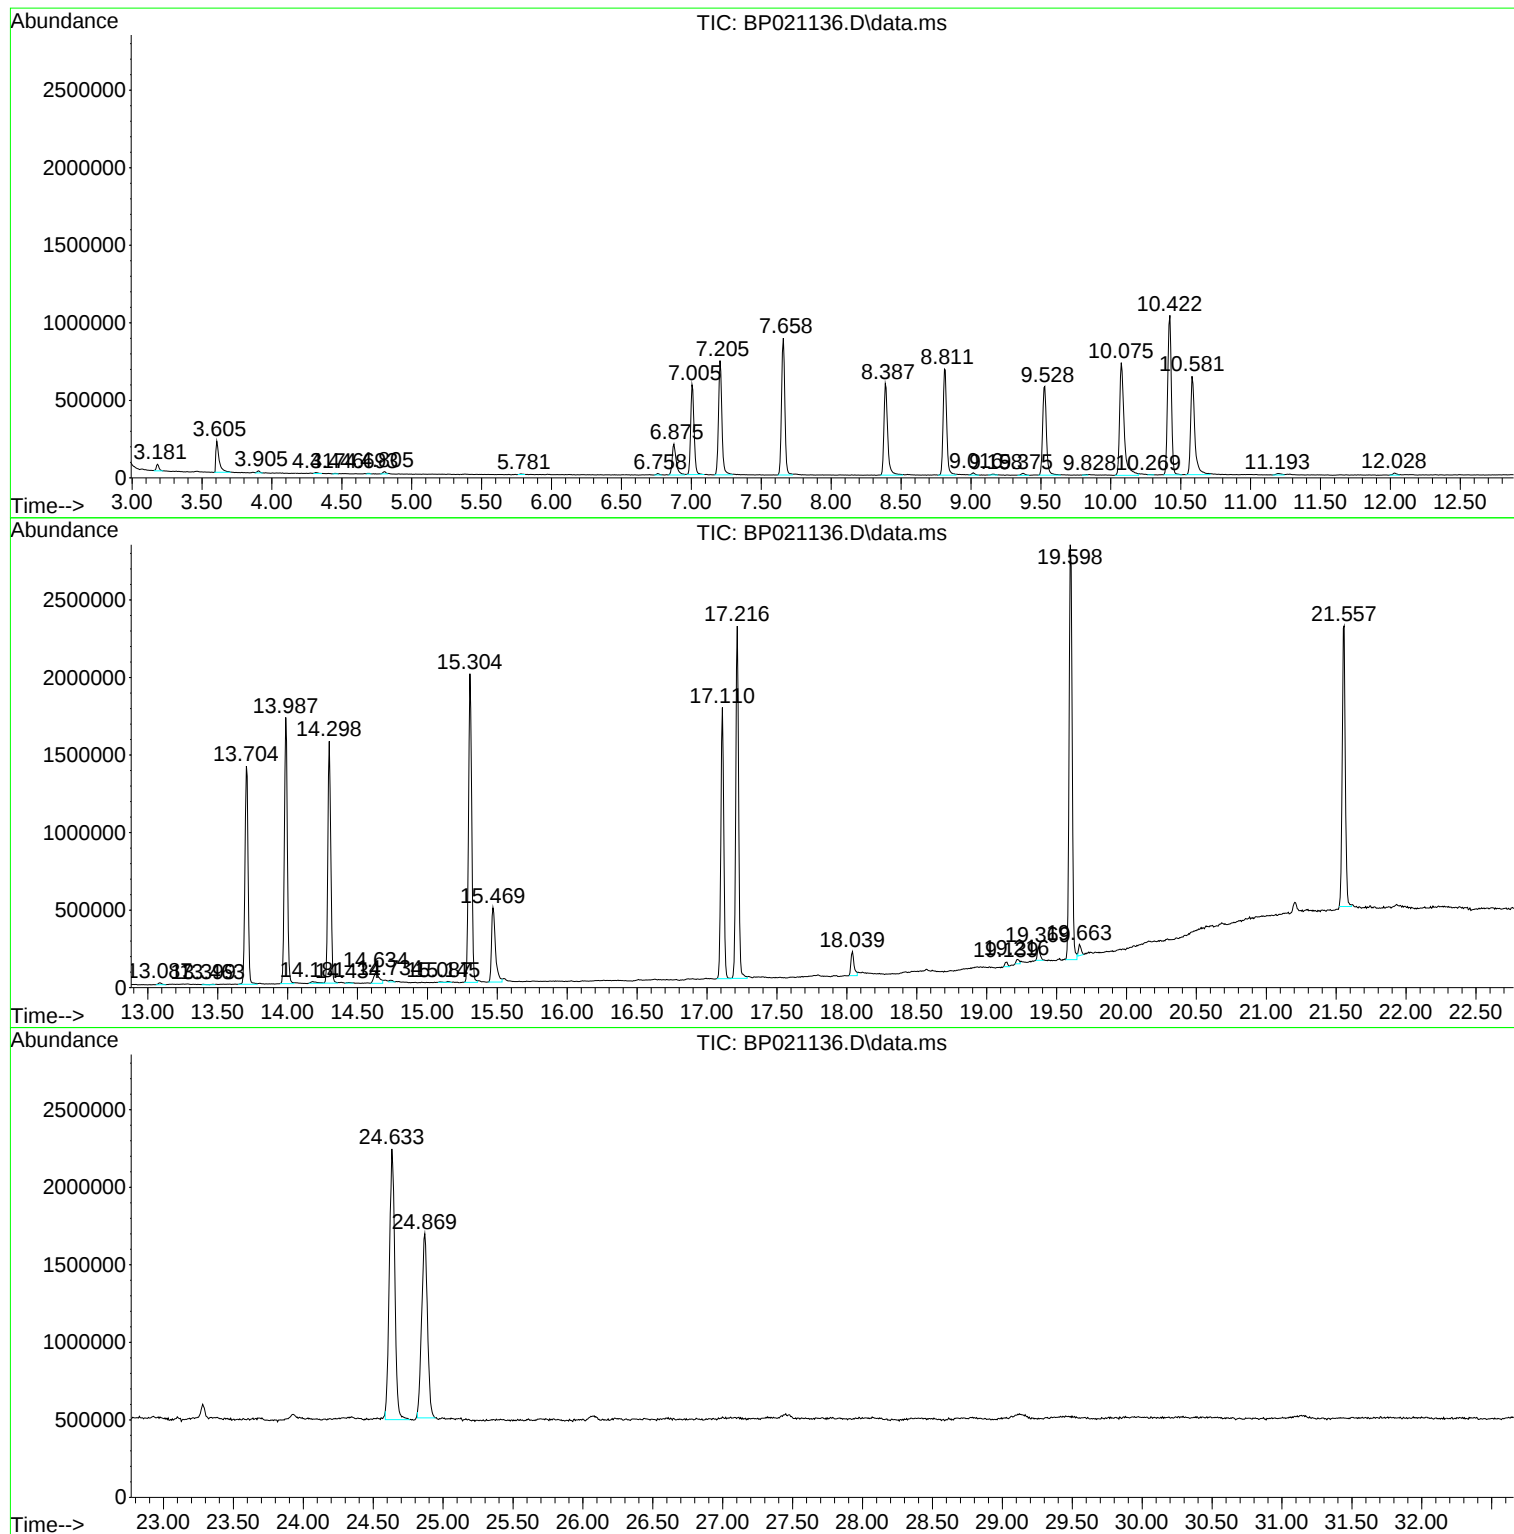

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021136.D
Acq On : 24 Jul 2024 22:23
Operator : MA/JU
Sample : P3244-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021136.D
Acq On : 24 Jul 2024 22:23
Operator : MA/JU
Sample : P3244-11
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc