

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021137.D
 Acq On : 24 Jul 2024 23:06
 Operator : MA/JU
 Sample : P3244-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	29	32	44	rVB	39864	60154	1.59%	0.154%
2	3.293	50	52	57	rBV6	3615	4831	0.13%	0.012%
3	3.605	102	105	119	rBV	193959	320565	8.49%	0.820%
4	3.899	152	155	165	rVB	12312	19354	0.51%	0.049%
5	4.317	224	226	230	rVB3	6798	8338	0.22%	0.021%
6	4.417	238	243	247	rBV5	11014	17973	0.48%	0.046%
7	4.452	247	249	255	rVB6	4896	5749	0.15%	0.015%
8	4.693	286	290	296	rVB9	4820	8078	0.21%	0.021%
9	4.805	304	309	318	rVB	14575	25043	0.66%	0.064%
10	4.987	333	340	352	rBV	39727	70836	1.88%	0.181%
11	5.964	503	506	512	rVB	4976	7813	0.21%	0.020%
12	6.311	561	565	570	rVB8	3471	6716	0.18%	0.017%
13	6.758	635	641	644	rVV4	4217	6654	0.18%	0.017%
14	6.881	654	662	676	rBV	158853	349288	9.25%	0.893%
15	6.999	676	682	698	rVB	537201	862986	22.86%	2.206%
16	7.211	708	718	733	rBV	622462	1103230	29.23%	2.820%
17	7.652	786	793	805	rBV	851418	1248695	33.08%	3.192%
18	8.387	911	918	932	rBV	439765	847789	22.46%	2.167%
19	8.810	982	990	1004	rBV	631343	1077565	28.55%	2.755%
20	9.152	1041	1048	1054	rVB7	4828	8752	0.23%	0.022%
21	9.375	1079	1086	1093	rBV7	7978	16359	0.43%	0.042%
22	9.458	1093	1100	1103	rBV4	4467	7283	0.19%	0.019%
23	9.522	1103	1111	1127	rBV	502779	951486	25.21%	2.433%
24	9.828	1156	1163	1171	rBV	2799	7321	0.19%	0.019%
25	10.081	1196	1206	1232	rBV	647977	1439641	38.14%	3.681%
26	10.428	1255	1265	1281	rBV	888267	1684184	44.62%	4.306%
27	10.581	1283	1291	1307	rBV	418704	832945	22.07%	2.129%
28	11.199	1391	1396	1400	rBV2	8259	16338	0.43%	0.042%
29	11.257	1400	1406	1415	rVV2	42737	99793	2.64%	0.255%
30	11.634	1468	1470	1478	rVB9	3648	5241	0.14%	0.013%
31	12.028	1532	1537	1544	rBV4	10426	21092	0.56%	0.054%
32	13.698	1815	1821	1831	rBV	1391167	1960245	51.93%	5.011%
33	13.769	1831	1833	1837	rVB4	4454	5916	0.16%	0.015%
34	13.981	1862	1869	1885	rBV	1505798	2308160	61.15%	5.901%
35	14.198	1900	1906	1913	rBV8	8295	20109	0.53%	0.051%
36	14.287	1914	1921	1930	rVV	1353408	2029845	53.77%	5.189%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
 Data File : BP021137.D
 Acq On : 24 Jul 2024 23:06
 Operator : MA/JU
 Sample : P3244-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZG3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

37	14.616	1970	1977	1992	rBV	58673	188590	5.00%	0.482%
38	14.722	1992	1995	2001	rVB8	5353	11892	0.32%	0.030%
39	15.075	2052	2055	2056	rBV3	3686	4294	0.11%	0.011%
40	15.140	2063	2066	2068	rVB4	3886	4161	0.11%	0.011%
41	15.304	2087	2094	2101	rBV	1852712	2841818	75.28%	7.265%
42	15.381	2103	2107	2116	rVB	112370	165026	4.37%	0.422%
43	15.469	2116	2122	2133	rBV	406632	795444	21.07%	2.034%
44	16.028	2214	2217	2223	rBV7	6446	11644	0.31%	0.030%
45	16.498	2293	2297	2298	rBV3	4112	5054	0.13%	0.013%
46	16.981	2375	2379	2382	rVB3	6380	9538	0.25%	0.024%
47	17.110	2395	2401	2409	rBV	1542172	2232865	59.15%	5.708%
48	17.210	2412	2418	2429	rVV	1920119	2914994	77.22%	7.452%
49	17.786	2514	2516	2521	rVB6	11287	16963	0.45%	0.043%
50	17.910	2533	2537	2540	rBV6	9144	14191	0.38%	0.036%
51	18.034	2553	2558	2568	rBV2	49768	111586	2.96%	0.285%
52	19.139	2743	2746	2752	rBV4	25561	34602	0.92%	0.088%
53	19.592	2817	2823	2836	rBV	2487200	3407846	90.28%	8.712%
54	21.545	3150	3155	3166	rBV2	1263159	2160564	57.24%	5.524%
55	24.627	3671	3679	3694	rVB2	1238828	3774754	100.00%	9.650%
56	24.845	3708	3716	3735	rVB2	925595	2943003	77.97%	7.524%




Sum of corrected areas: 39115196

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021137.D
Acq On : 24 Jul 2024 23:06
Operator : MA/JU
Sample : P3244-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

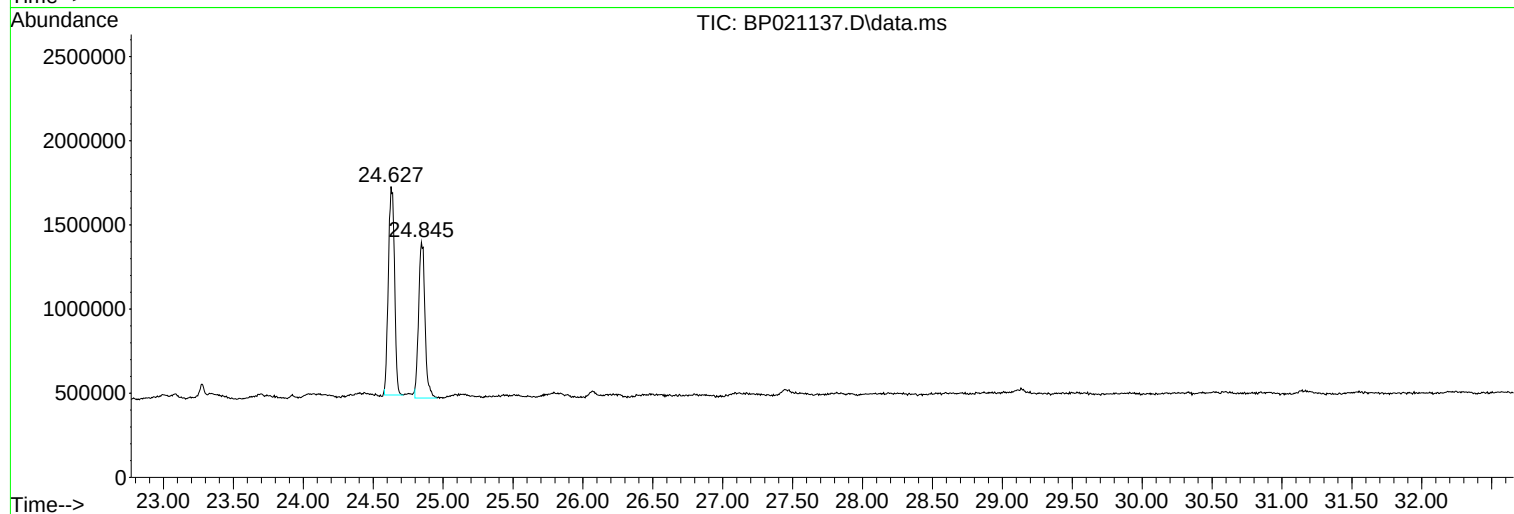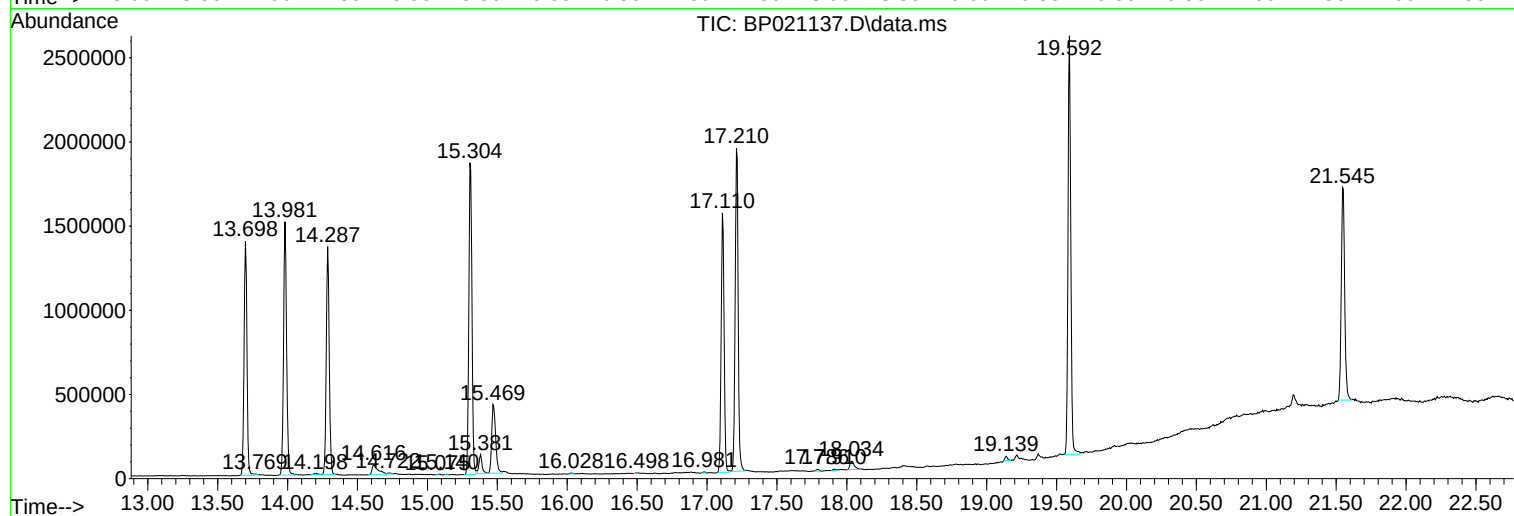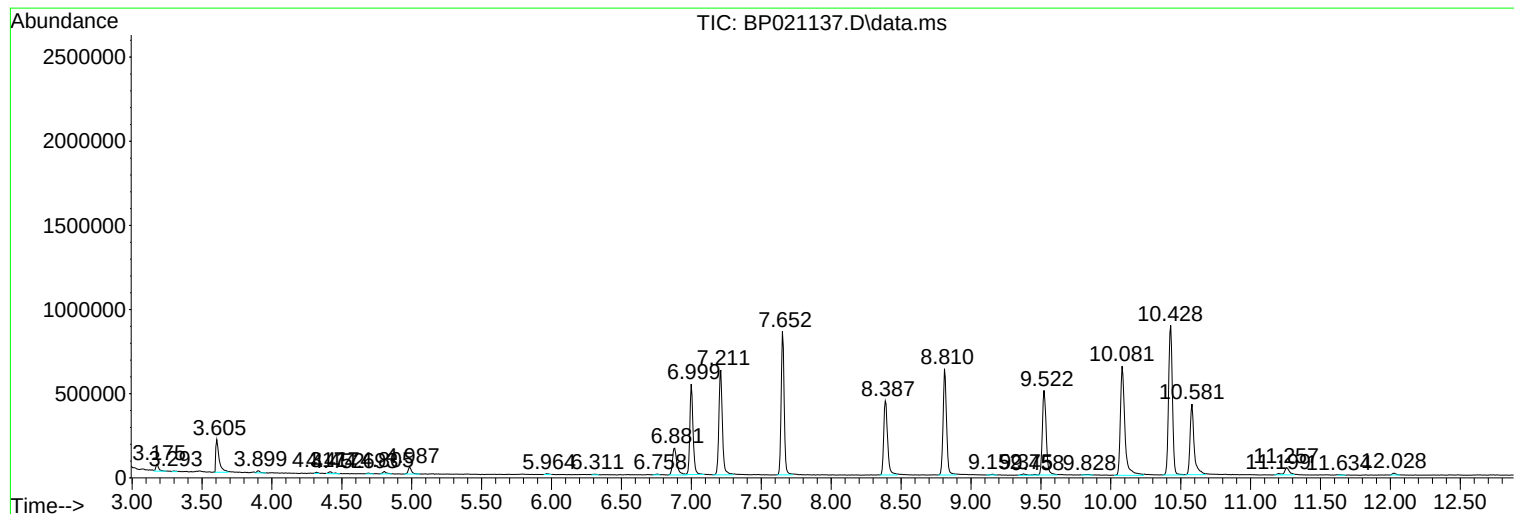

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021137.D
Acq On : 24 Jul 2024 23:06
Operator : MA/JU
Sample : P3244-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072424\
Data File : BP021137.D
Acq On : 24 Jul 2024 23:06
Operator : MA/JU
Sample : P3244-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZG3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------