
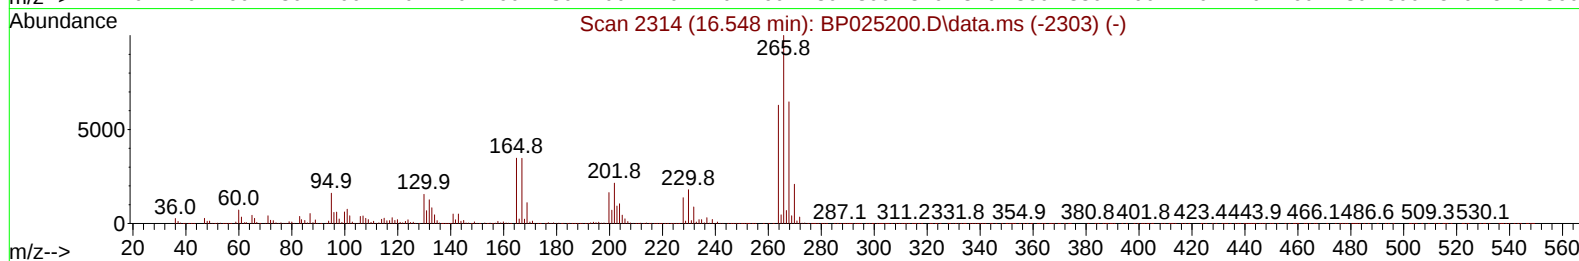
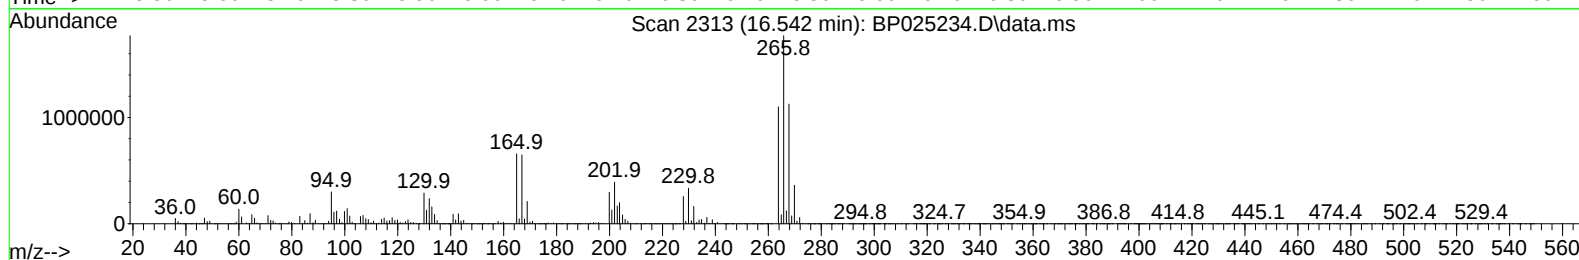


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072425\
Data File : BP025234.D
Acq On : 24 Jul 2025 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 24 10:37:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

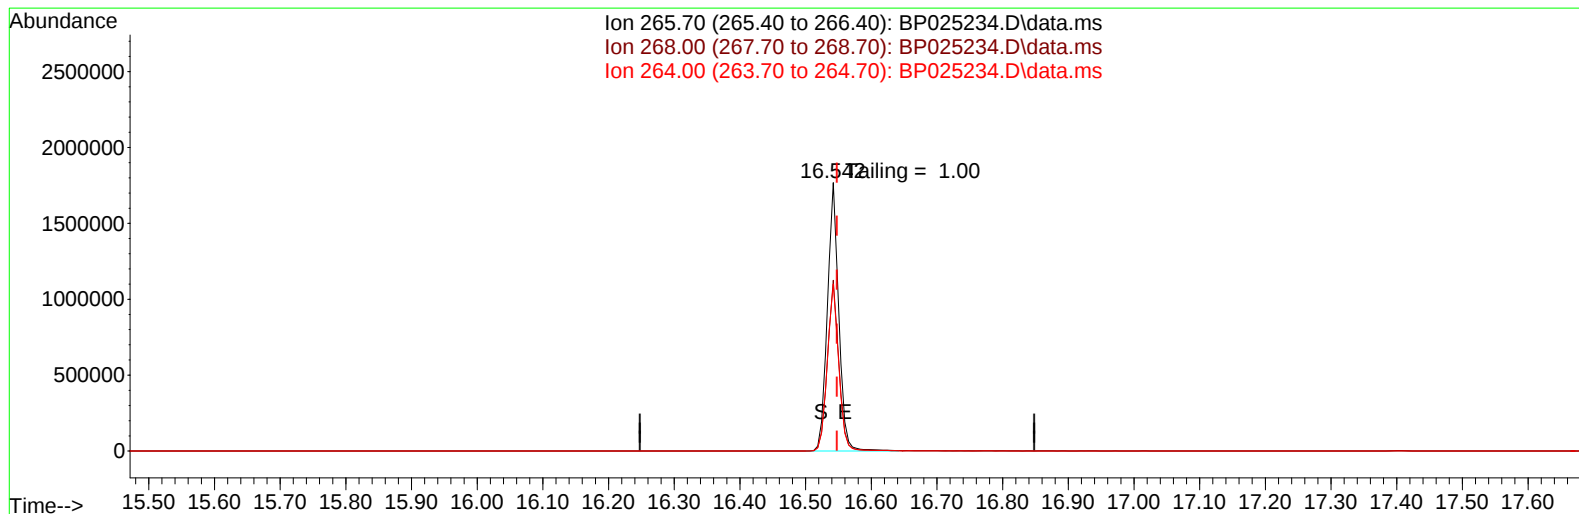

TIC: BP025234.D\data.ms




(70) Pentachlorophenol (C)

16.542min (-0.006) 1737965.32 ng

response 2129379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.64
264.00	62.90	62.25
0.00	0.00	0.00

Quant Time: Jul 24 10:37:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

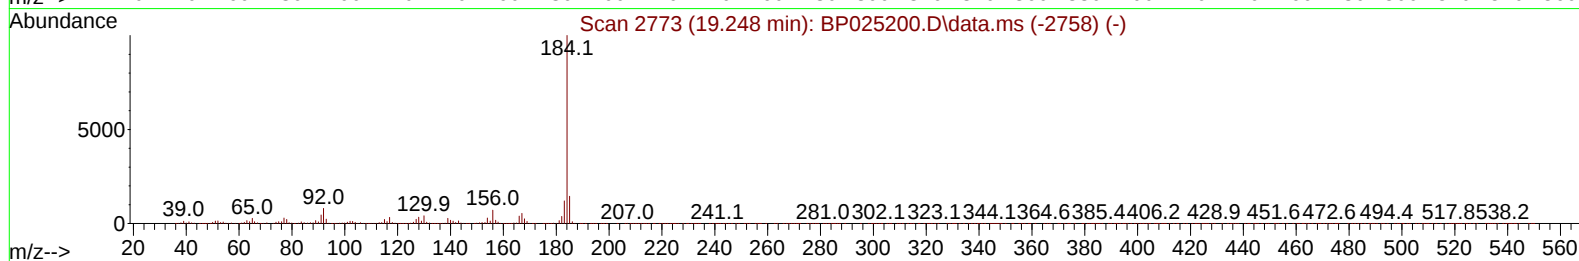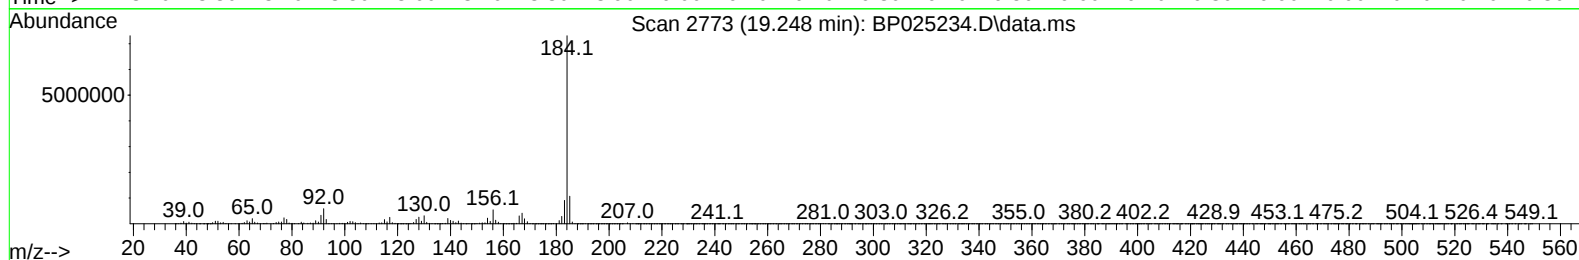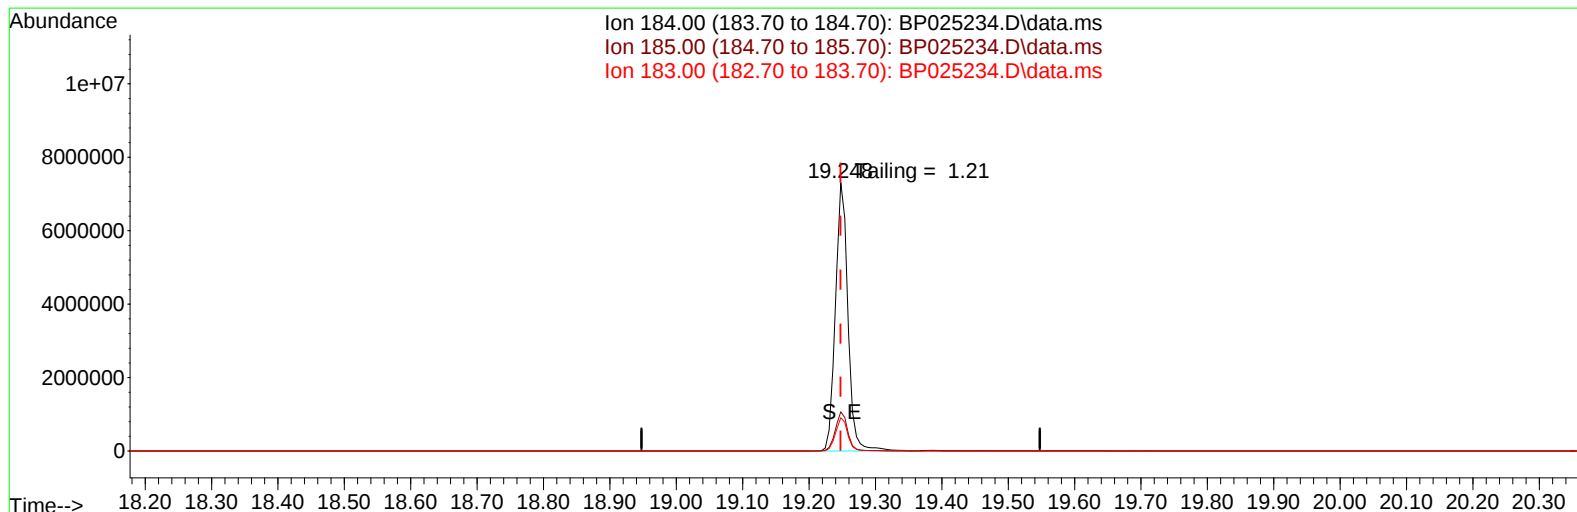

TIC: BP025234.D\data.ms

(77) Benzidine

19.248min (+ 0.000) 510916.31 ng

response **9578469**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.64
183.00	12.00	12.42
0.00	0.00	0.00