
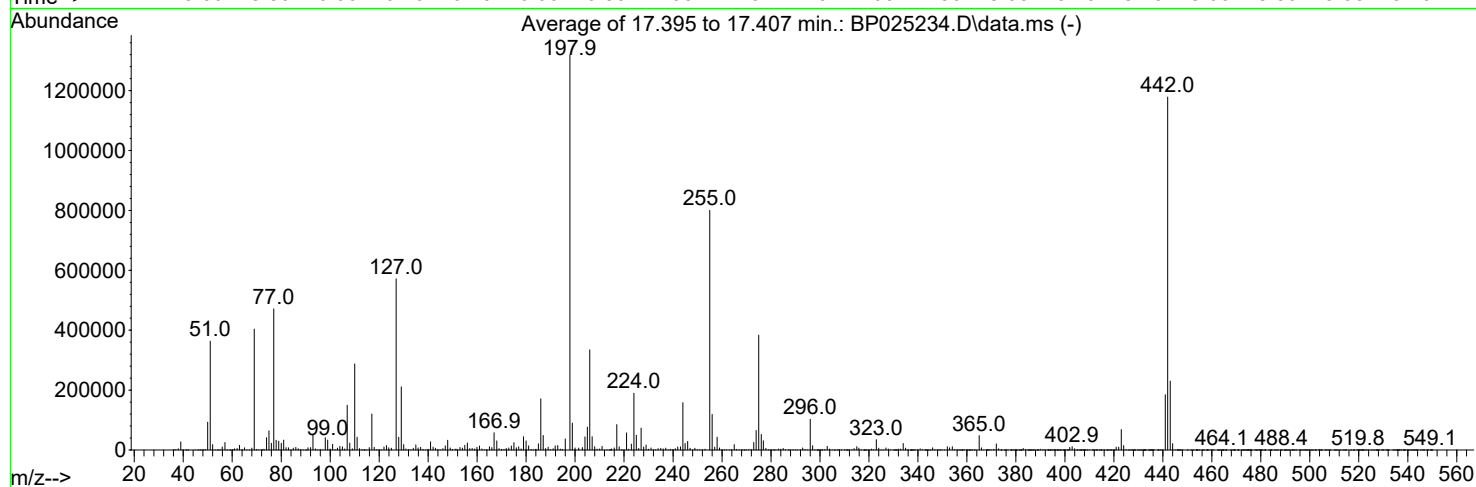


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072425\
Data File : BP025234.D
Acq On : 24 Jul 2025 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 22 02:55:21 2025

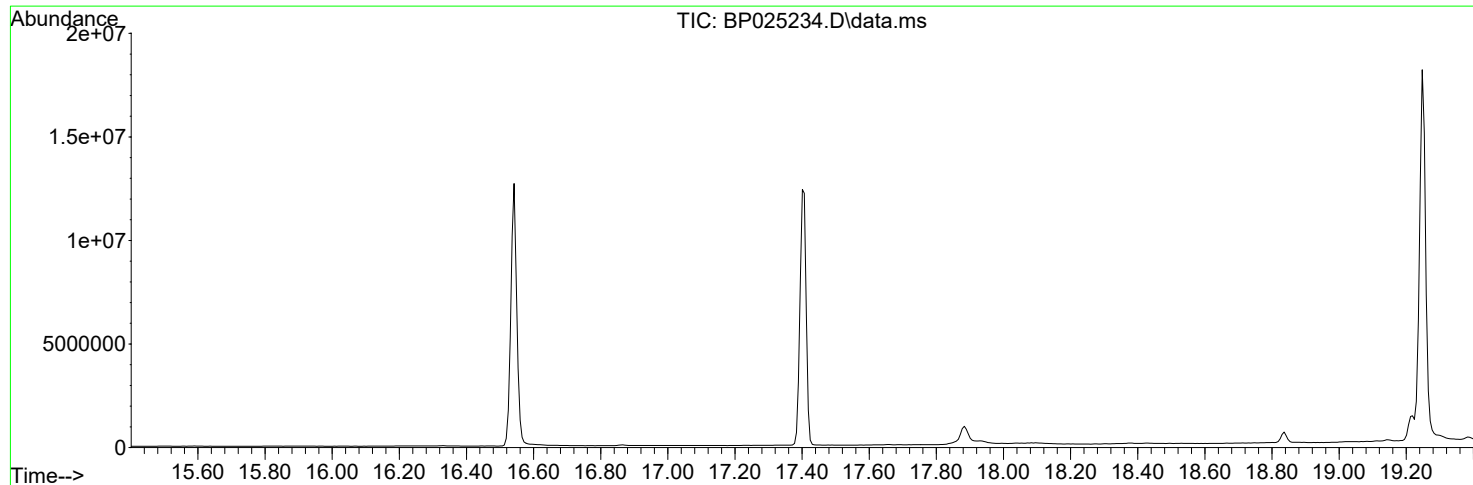

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2449

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	6288	PASS
69	69	100	100	100.0	404093	PASS
70	69	0.00	2	0.5	1966	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1318428	PASS
199	198	5	9	6.8	89717	PASS
365	198	1	100	3.7	48161	PASS
441	443	0.01	150	80.2	184677	PASS
442	442	100	100	100.0	1178647	PASS
443	442	15	24	19.5	230369	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/24/2025	BNA_P	<u>BP025232.D</u>
Compound Name	Response	Retention Time
DDT	4769480	20.565
DDD	147539	20.107
DDE	6793	19.565
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
154332	4923812	3.13

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072425\
Data File : BP025234.D
Acq On : 24 Jul 2025 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 24 10:37:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

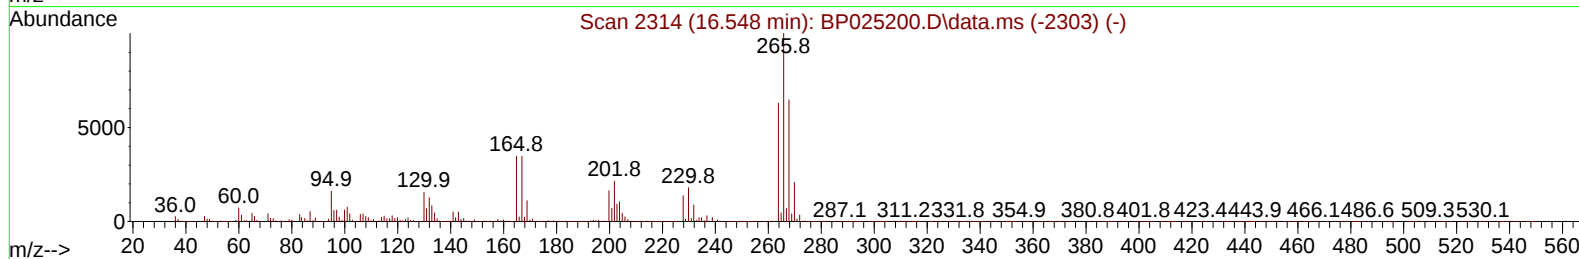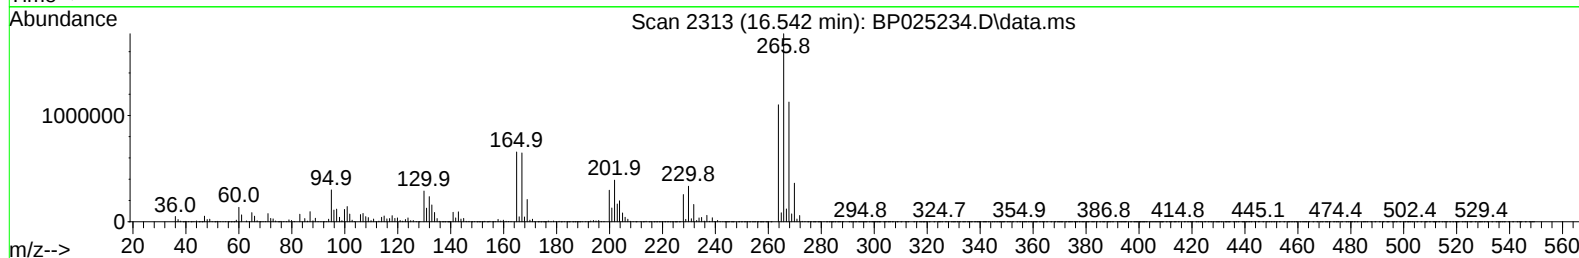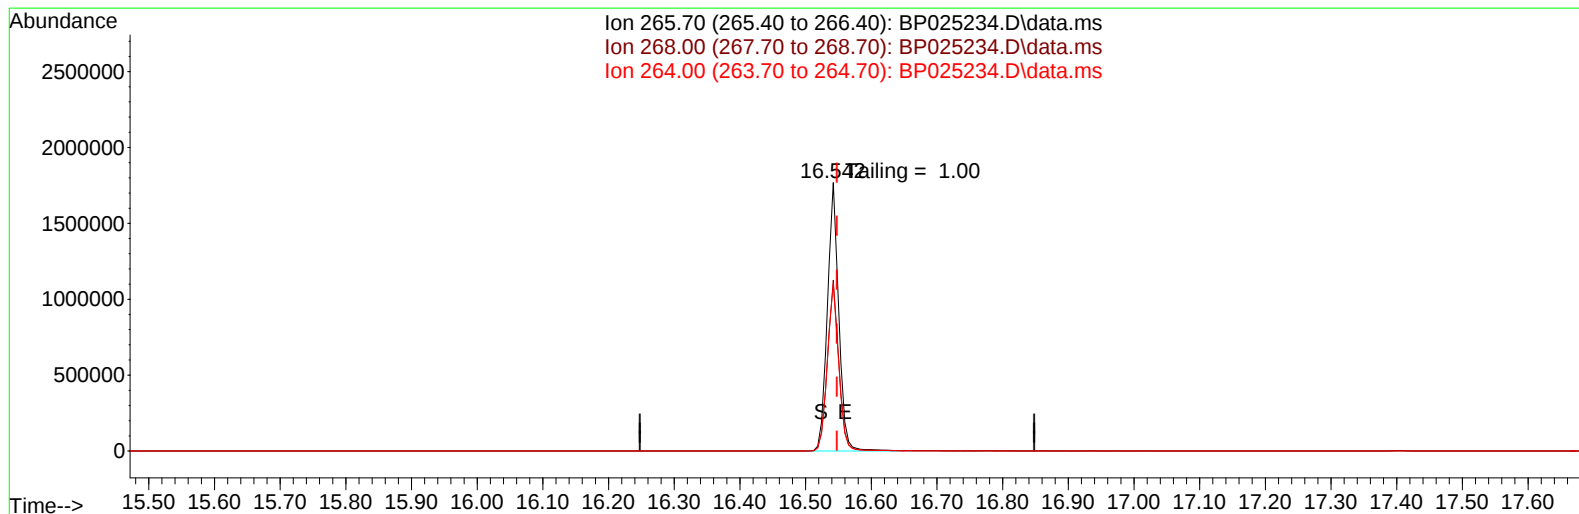

TIC: BP025234.D\data.ms

(70) Pentachlorophenol (C)

16.542min (-0.006) 1737965.32 ng




response 2129379

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	63.64
264.00	62.90	62.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072425\
Data File : BP025234.D
Acq On : 24 Jul 2025 09:13
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 24 10:37:50 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 22 02:55:21 2025
Response via : Initial Calibration

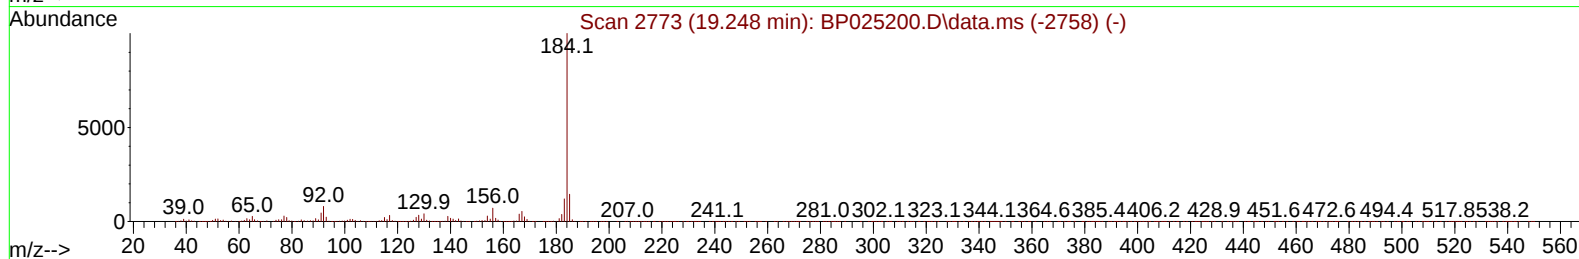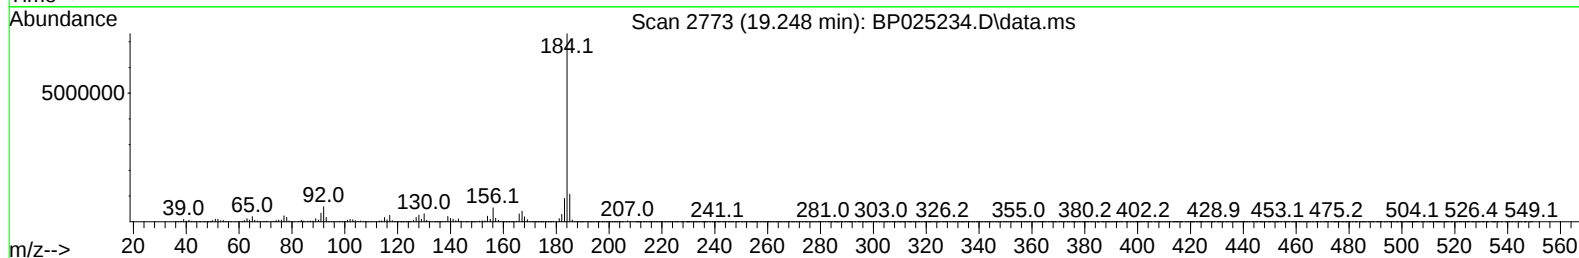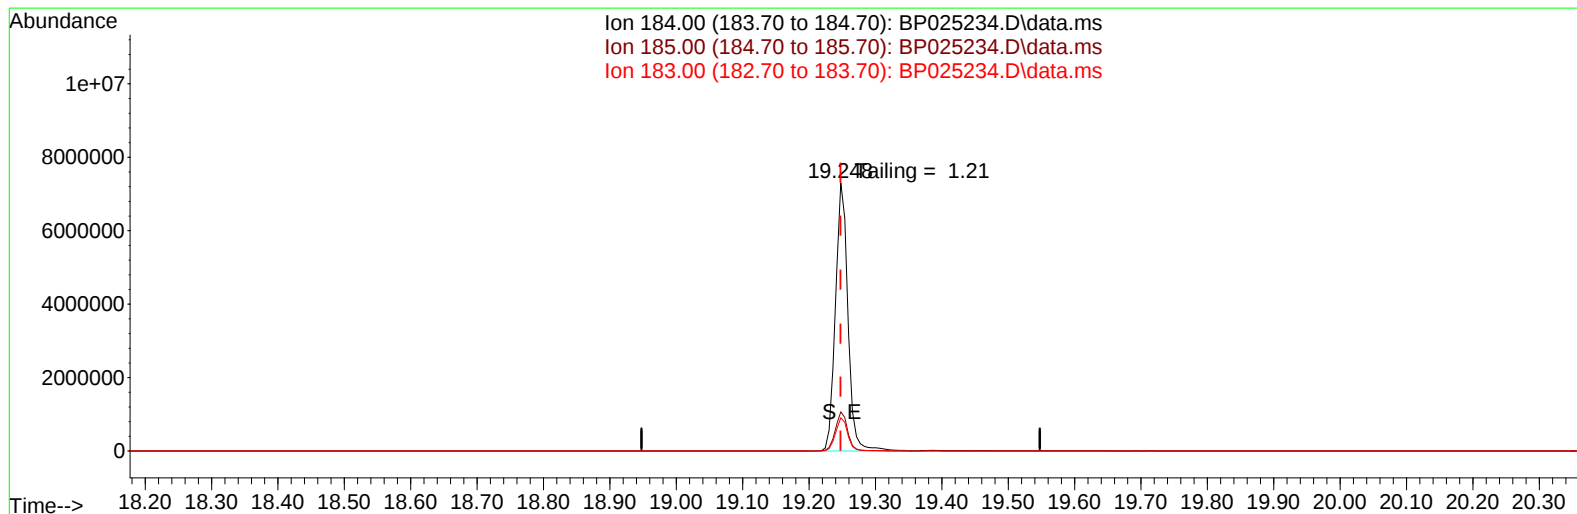

TIC: BP025234.D\data.ms

(77) Benzidine

19.248min (+ 0.000) 510916.31 ng

response 9578469

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.64
183.00	12.00	12.42
0.00	0.00	0.00