

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011085.D
 Acq On : 25 Jul 2022 10:59
 Operator : CG/JU
 Sample : N3801-12
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX5

Quant Time: Jul 25 11:54:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.669	152	477937	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.463	136	2224298	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.334	164	1359611	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	2621810	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.216	240	1753784	20.000	ng/u1	#-0.01
88) Perylene-d12	23.557	264	1390031	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.164	96	78329	5.908	ng/uL	-0.02
4) Pyridine-d5	3.575	84	1139011	33.240	ng/u1	-0.02
7) Phenol-d5	6.846	99	1436807	36.623	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.011	67	977603	38.751	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.199	132	1176392	37.109	ng/u1	-0.01
15) 4-Methylphenol-d8	8.387	113	1211779	38.582	ng/u1	-0.01
21) Nitrobenzene-d5	8.834	128	623719	38.478	ng/u1	0.00
24) 2-Nitrophenol-d4	9.552	143	687241	42.847	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	1062530	36.223	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.610	131	1722266	35.615	ng/u1	0.00
46) Dimethylphthalate-d6	13.751	166	3808966	40.990	ng/u1	-0.01
49) Acenaphthylene-d8	14.022	160	4431902	40.422	ng/u1	0.00
54) 4-Nitrophenol-d4	14.551	143	588049	31.268	ng/u1	0.00
60) Fluorene-d10	15.334	176	3000271	37.985	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	488373	37.644	ng/u1	0.00
73) Anthracene-d10	17.198	188	4421458	39.669	ng/u1	0.00
81) Pyrene-d10	19.451	212	4476027	48.595	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.410	264	2788912	41.774	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.199	88	48497	3.486	ng/uL#	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011085.D
Acq On : 25 Jul 2022 10:59
Operator : CG/JU
Sample : N3801-12
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX5

Quant Time: Jul 25 11:54:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

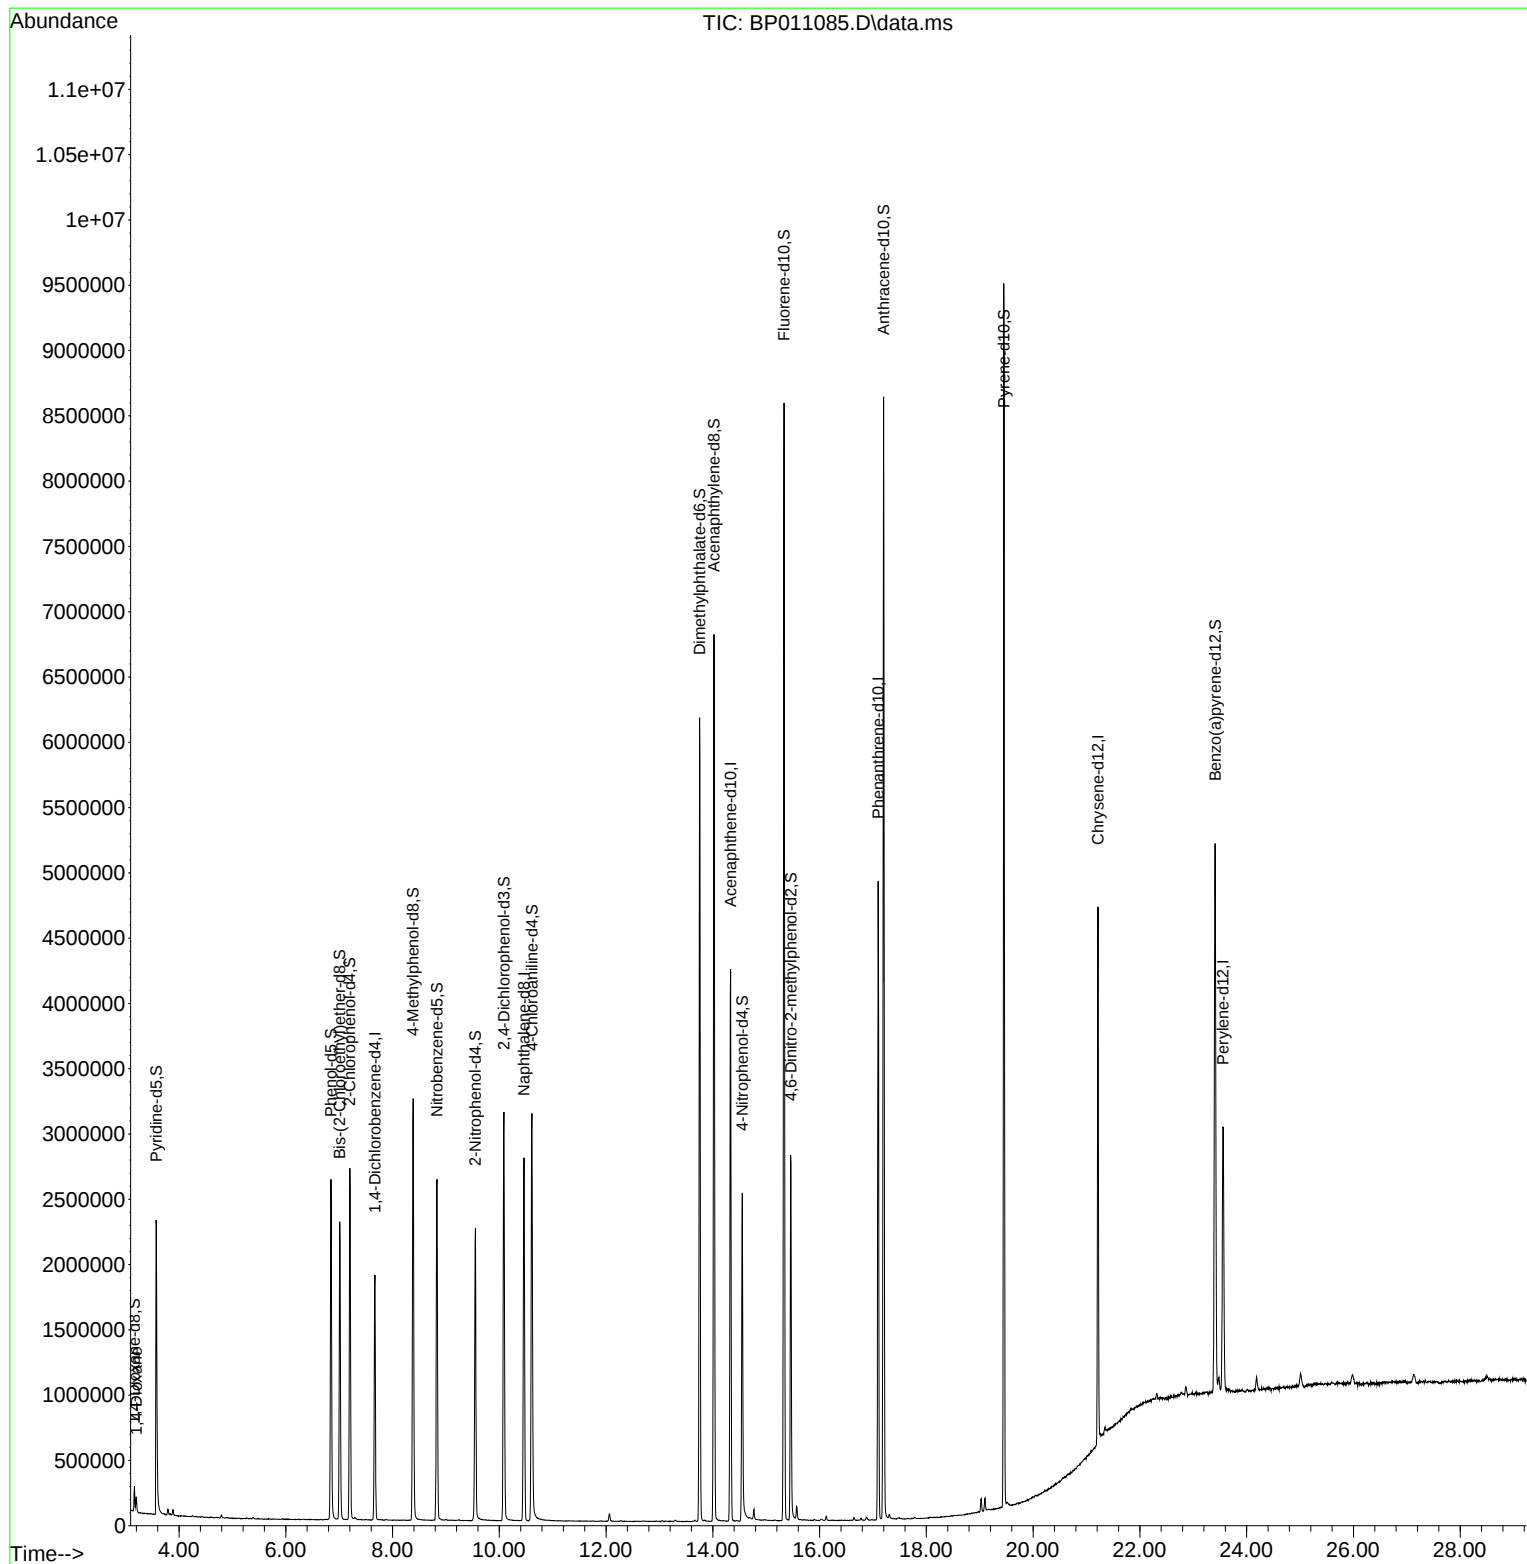

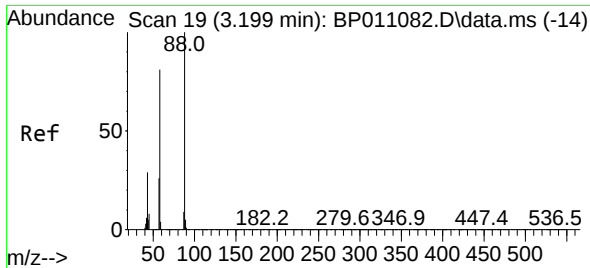

#2
 1,4-Dioxane
 Concen: 3.486 ng/uL
 RT: 3.199 min Scan# 19
 Delta R.T. -0.018 min
 Lab File: BP011085.D
 Acq: 25 Jul 2022 10:59

Instrument :
 BNA_P
 ClientSampleId :
 GBHX5

Tgt Ion: 88 Resp: 48497
 Ion Ratio Lower Upper
 88 100
 43 35.3 35.8 53.6#
 58 83.3 68.1 102.1

