

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011089.D
 Acq On : 25 Jul 2022 13:17
 Operator : CG/JU
 Sample : N3801-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	10	rBV	64105	79736	0.59%	0.063%
2	3.164	10	13	23	rVB	154815	203844	1.52%	0.161%
3	3.575	80	83	101	rBV	715127	1029809	7.68%	0.812%
4	3.793	116	120	125	rVB	62154	87962	0.66%	0.069%
5	3.887	132	136	140	rVB	42780	57077	0.43%	0.045%
6	4.399	220	223	228	rVB4	23198	30129	0.22%	0.024%
7	4.793	287	290	295	rVB2	10157	13677	0.10%	0.011%
8	5.387	388	391	400	rVB	16873	29982	0.22%	0.024%
9	6.805	627	632	633	rBV3	12475	15438	0.12%	0.012%
10	6.846	633	639	651	rVB	438571	709551	5.29%	0.560%
11	7.010	660	667	679	rBV	1989638	3054251	22.76%	2.409%
12	7.199	692	699	711	rBV	1758031	2701262	20.13%	2.130%
13	7.287	711	714	719	rVB7	11579	18039	0.13%	0.014%
14	7.669	771	779	789	rBV	1813388	2829438	21.09%	2.231%
15	8.381	893	900	918	rBV	1333209	2253144	16.79%	1.777%
16	8.828	969	976	992	rBV	2398712	3928726	29.28%	3.098%
17	9.246	1040	1047	1055	rBV	60939	92812	0.69%	0.073%
18	9.551	1091	1099	1114	rBV	1743586	2939872	21.91%	2.319%
19	10.087	1180	1190	1203	rBV	2474287	4134010	30.81%	3.260%
20	10.463	1243	1254	1270	rVB	2681025	4573560	34.09%	3.607%
21	10.610	1270	1279	1298	rBV	2789439	4878594	36.36%	3.848%
22	11.745	1466	1472	1477	rBV	60174	88699	0.66%	0.070%
23	12.063	1518	1526	1534	rBV2	50155	96155	0.72%	0.076%
24	12.687	1625	1632	1638	rBV6	11257	24891	0.19%	0.020%
25	12.940	1671	1675	1680	rBV7	13144	21205	0.16%	0.017%
26	13.240	1718	1726	1730	rBV8	9181	17328	0.13%	0.014%
27	13.751	1807	1813	1826	rBV	6114792	8402510	62.62%	6.627%
28	14.022	1851	1859	1876	rBV	6934888	9628545	71.76%	7.594%
29	14.334	1904	1912	1926	rBV	4307451	6256512	46.63%	4.934%
30	14.551	1941	1949	1963	rBV	238871	500675	3.73%	0.395%
31	14.769	1984	1986	1990	rVB5	11379	15072	0.11%	0.012%
32	14.969	2014	2020	2026	rVB10	9194	16374	0.12%	0.013%
33	15.145	2045	2050	2058	rBV2	36993	59546	0.44%	0.047%
34	15.334	2075	2082	2089	rBV	8985057	12275623	91.49%	9.681%
35	15.457	2097	2103	2118	rBV	2768601	3729473	27.80%	2.941%
36	15.575	2118	2123	2135	rVB	110370	183101	1.36%	0.144%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011089.D
 Acq On : 25 Jul 2022 13:17
 Operator : CG/JU
 Sample : N3801-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHW6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.122	2212	2216	2223	rVB3	32214	50442	0.38%	0.040%
38	16.398	2260	2263	2270	rVB9	9389	15659	0.12%	0.012%
39	16.575	2287	2293	2298	rVB10	16811	27757	0.21%	0.022%
40	16.775	2323	2327	2332	rVB5	19036	24930	0.19%	0.020%
41	16.880	2337	2345	2350	rBV7	19530	40729	0.30%	0.032%
42	17.098	2376	2382	2392	rBV	4974048	6923581	51.60%	5.460%
43	17.198	2392	2399	2414	rVV2	9189216	12959669	96.59%	10.221%
44	17.404	2430	2434	2438	rVB	21087	27607	0.21%	0.022%
45	17.792	2495	2500	2504	rVB4	33047	45656	0.34%	0.036%
46	18.010	2533	2537	2540	rBV5	17499	24289	0.18%	0.019%
47	18.080	2546	2549	2553	rVB	31774	36983	0.28%	0.029%
48	19.027	2706	2710	2714	rBV2	124755	156218	1.16%	0.123%
49	19.098	2718	2722	2726	rVV	91193	123617	0.92%	0.097%
50	19.398	2771	2773	2776	rVB4	32415	27641	0.21%	0.022%
51	19.451	2776	2782	2789	rBV	9860546	13417680	100.00%	10.582%
52	21.216	3077	3082	3090	rBV	4274363	5305565	39.54%	4.184%
53	23.410	3448	3455	3463	rBV2	4417340	8422755	62.77%	6.643%
54	23.562	3475	3481	3489	rVB2	2097716	4188598	31.22%	3.303%




Sum of corrected areas: 126795998

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011089.D
Acq On : 25 Jul 2022 13:17
Operator : CG/JU
Sample : N3801-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

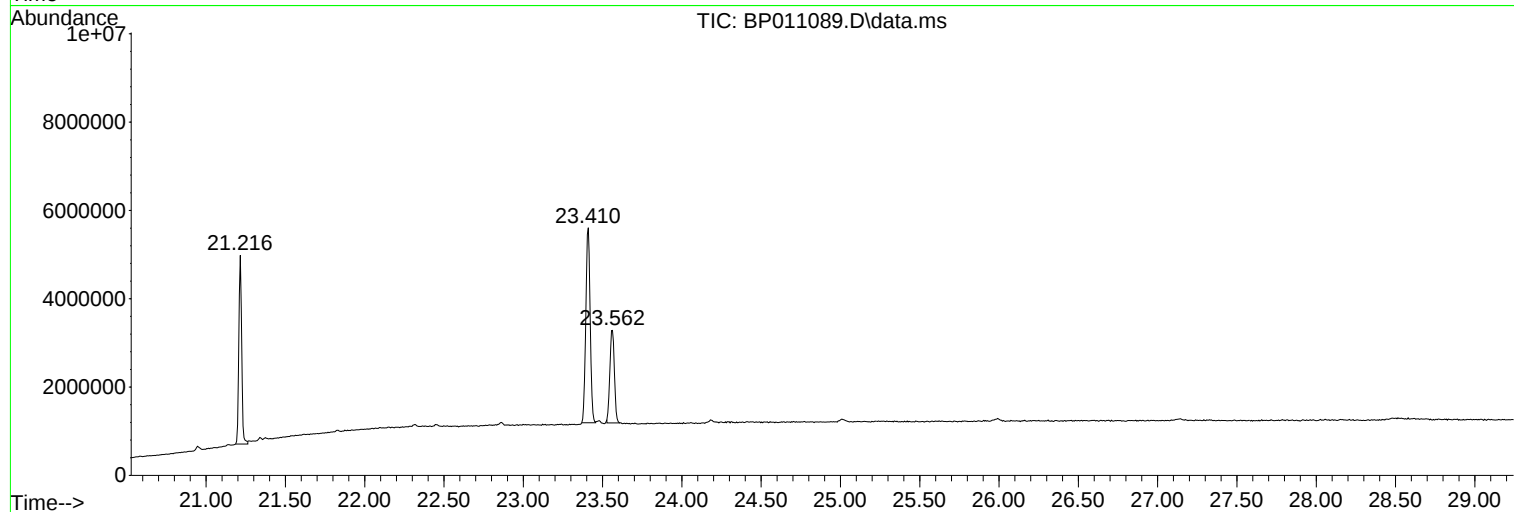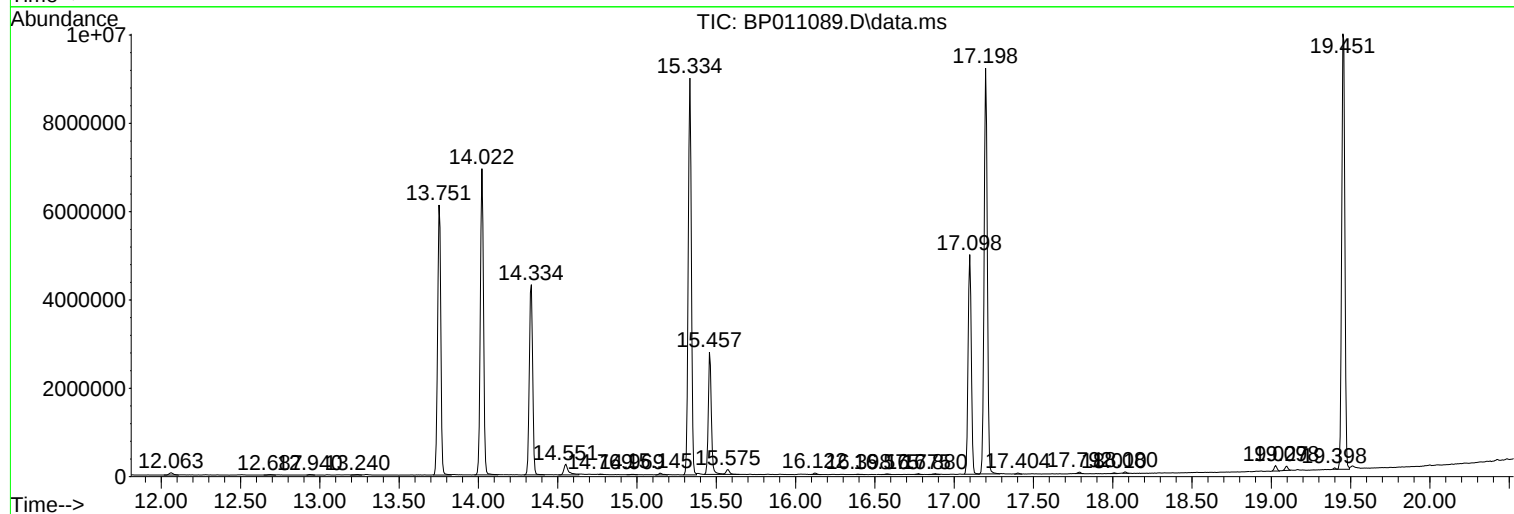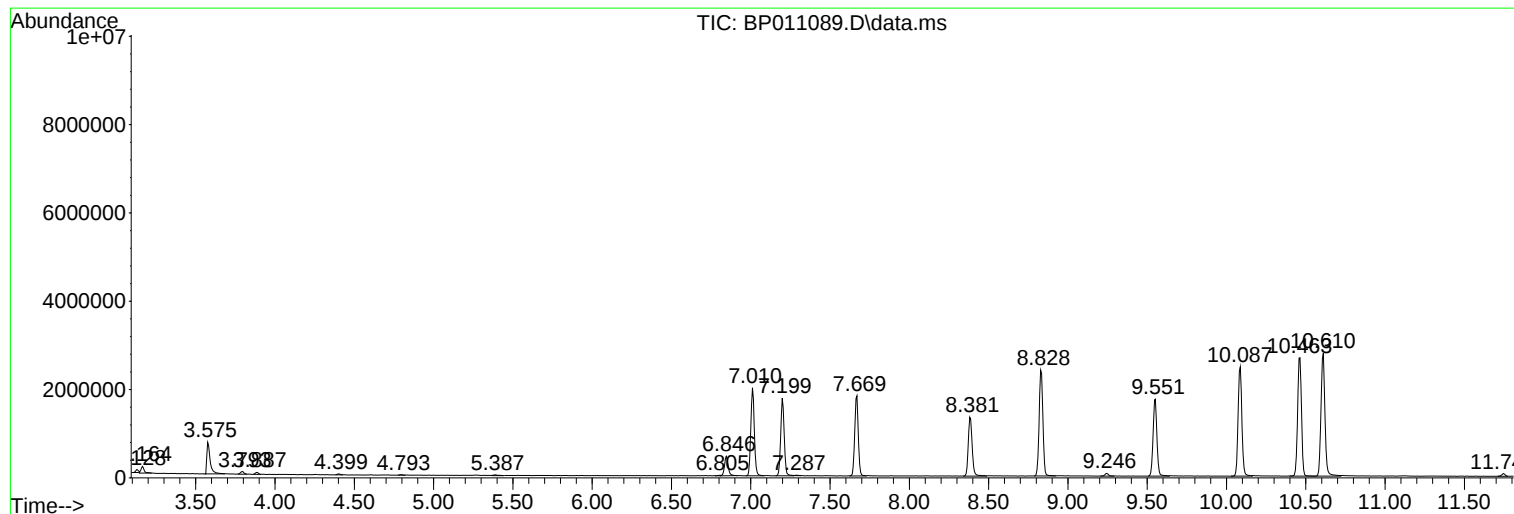

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011089.D
Acq On : 25 Jul 2022 13:17
Operator : CG/JU
Sample : N3801-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011089.D
Acq On : 25 Jul 2022 13:17
Operator : CG/JU
Sample : N3801-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc