

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011090.D
 Acq On : 25 Jul 2022 13:52
 Operator : CG/JU
 Sample : N3801-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011090.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.129	3	7	11	rBV	578363	738048	5.25%	0.567%
2	3.164	11	13	17	rVB	141006	142343	1.01%	0.109%
3	3.581	81	84	97	rBV	484405	735570	5.23%	0.565%
4	3.793	114	120	125	rBV2	63016	101066	0.72%	0.078%
5	3.887	132	136	142	rVB	37092	47005	0.33%	0.036%
6	5.387	388	391	396	rVB	13600	18817	0.13%	0.014%
7	6.846	630	639	652	rBV	444755	718793	5.11%	0.553%
8	7.011	660	667	680	rBV	2150723	3252296	23.13%	2.500%
9	7.199	692	699	712	rBV	1882820	2915685	20.73%	2.241%
10	7.287	712	714	719	rVB6	10657	14303	0.10%	0.011%
11	7.669	771	779	789	rBV	1690911	2676461	19.03%	2.057%
12	8.381	893	900	914	rBV	1405311	2316185	16.47%	1.780%
13	8.828	969	976	989	rBV	2559040	4167062	29.63%	3.203%
14	9.240	1042	1046	1054	rVB3	16502	30589	0.22%	0.024%
15	9.546	1092	1098	1118	rBV	1912422	3211646	22.84%	2.469%
16	10.087	1183	1190	1205	rBV	2672106	4454434	31.68%	3.424%
17	10.463	1245	1254	1267	rVB	2502640	4258628	30.28%	3.274%
18	10.610	1269	1279	1299	rBV	2686019	4670341	33.21%	3.590%
19	11.287	1388	1394	1400	rBV9	10958	24907	0.18%	0.019%
20	11.746	1466	1472	1477	rBV3	14896	25809	0.18%	0.020%
21	12.063	1519	1526	1534	rBV2	49109	91224	0.65%	0.070%
22	12.687	1625	1632	1639	rBV8	13457	30843	0.22%	0.024%
23	12.940	1668	1675	1681	rBV3	18209	30774	0.22%	0.024%
24	13.234	1720	1725	1730	rBV5	18658	30559	0.22%	0.023%
25	13.293	1730	1735	1742	rVB6	9371	23843	0.17%	0.018%
26	13.751	1805	1813	1826	rBV	6180405	8571126	60.95%	6.589%
27	13.863	1826	1832	1838	rVB	12984	31192	0.22%	0.024%
28	14.022	1850	1859	1869	rBV	6953117	10013013	71.21%	7.697%
29	14.328	1905	1911	1920	rBV	3922455	5842280	41.55%	4.491%
30	14.551	1943	1949	1967	rBV2	249406	620648	4.41%	0.477%
31	14.769	1982	1986	1993	rVB8	13507	23410	0.17%	0.018%
32	15.146	2045	2050	2053	rBV	97043	138436	0.98%	0.106%
33	15.169	2053	2054	2062	rVB	66765	73546	0.52%	0.057%
34	15.334	2075	2082	2088	rBV	8874167	12664683	90.06%	9.735%
35	15.381	2088	2090	2097	rVV3	43351	68781	0.49%	0.053%
36	15.457	2097	2103	2117	rVV	2969877	3957712	28.14%	3.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011090.D
 Acq On : 25 Jul 2022 13:52
 Operator : CG/JU
 Sample : N3801-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.575	2117	2123	2130	rVB	105162	172117	1.22%	0.132%
38	15.904	2175	2179	2184	rVB8	8144	14476	0.10%	0.011%
39	16.028	2195	2200	2201	rBV5	13265	15621	0.11%	0.012%
40	16.069	2204	2207	2211	rVV4	15084	23849	0.17%	0.018%
41	16.122	2211	2216	2223	rVB3	34909	53042	0.38%	0.041%
42	16.245	2232	2237	2244	rVB10	8935	20782	0.15%	0.016%
43	16.581	2290	2294	2298	rVB5	12453	18857	0.13%	0.014%
44	16.775	2323	2327	2331	rVB3	16367	22863	0.16%	0.018%
45	16.875	2339	2344	2348	rBV6	29562	56336	0.40%	0.043%
46	17.098	2375	2382	2392	rVV	4791250	6585505	46.83%	5.062%
47	17.198	2392	2399	2413	rVV	9905557	13379023	95.14%	10.284%
48	17.304	2415	2417	2423	rVB7	15205	23005	0.16%	0.018%
49	17.404	2429	2434	2438	rBV	27929	40350	0.29%	0.031%
50	17.616	2467	2470	2473	rVB4	12677	14362	0.10%	0.011%
51	17.781	2494	2498	2504	rVB6	40632	56418	0.40%	0.043%
52	18.004	2533	2536	2539	rBV5	15060	22156	0.16%	0.017%
53	18.081	2545	2549	2553	rVB	54715	65341	0.46%	0.050%
54	18.292	2583	2585	2590	rBV6	11294	16317	0.12%	0.013%
55	19.028	2705	2710	2714	rBV2	126266	170270	1.21%	0.131%
56	19.098	2718	2722	2726	rVV	100440	135514	0.96%	0.104%
57	19.192	2735	2738	2742	rVB	51598	56861	0.40%	0.044%
58	19.451	2776	2782	2789	rBV	10599901	14062074	100.00%	10.809%
59	21.216	3077	3082	3091	rBV	4110679	5225433	37.16%	4.017%
60	23.410	3448	3455	3463	rBV2	4691341	8961858	63.73%	6.889%
61	23.557	3474	3480	3490	rVB2	2048226	4146938	29.49%	3.188%




Sum of corrected areas: 130091426

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011090.D
Acq On : 25 Jul 2022 13:52
Operator : CG/JU
Sample : N3801-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

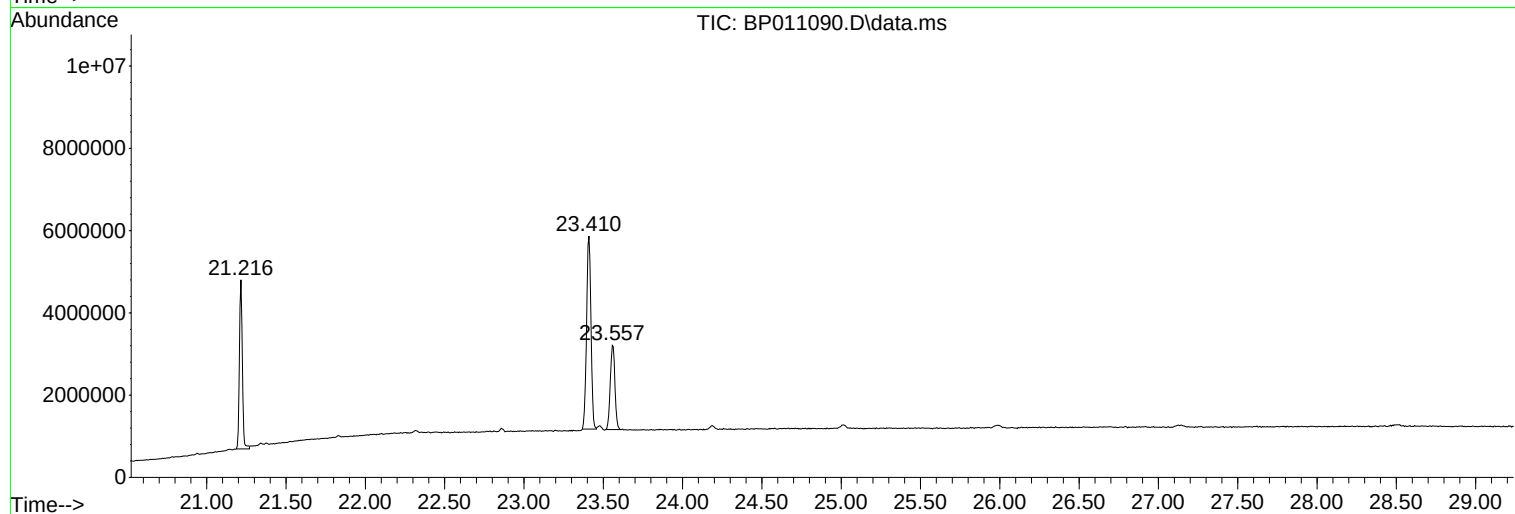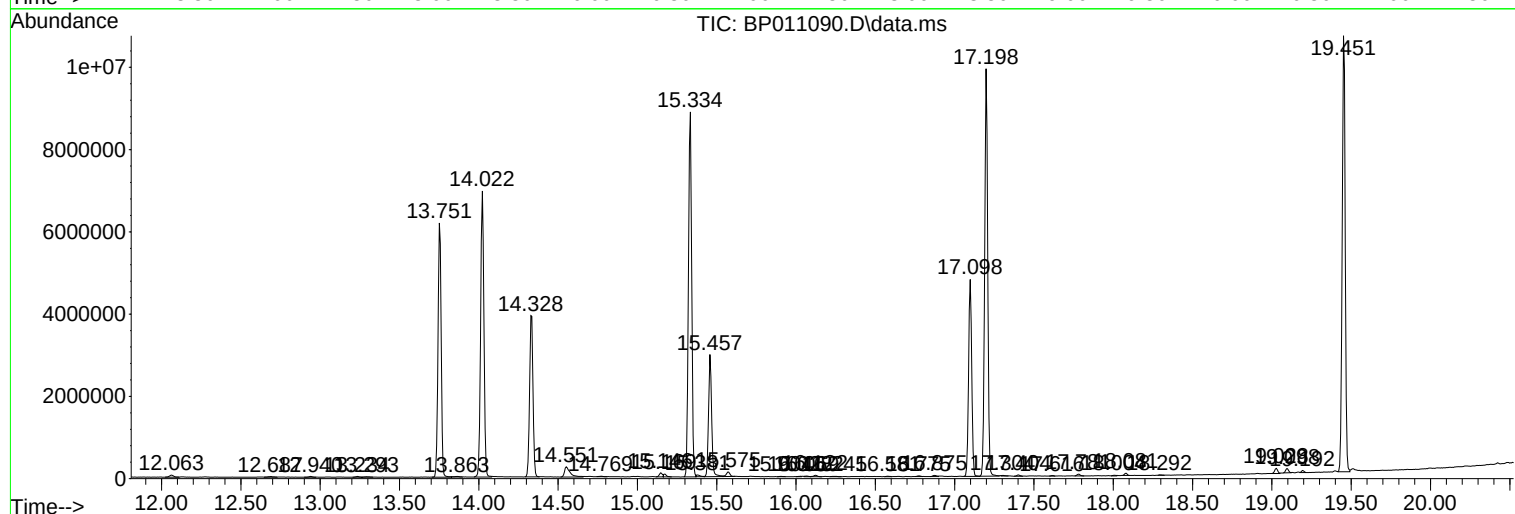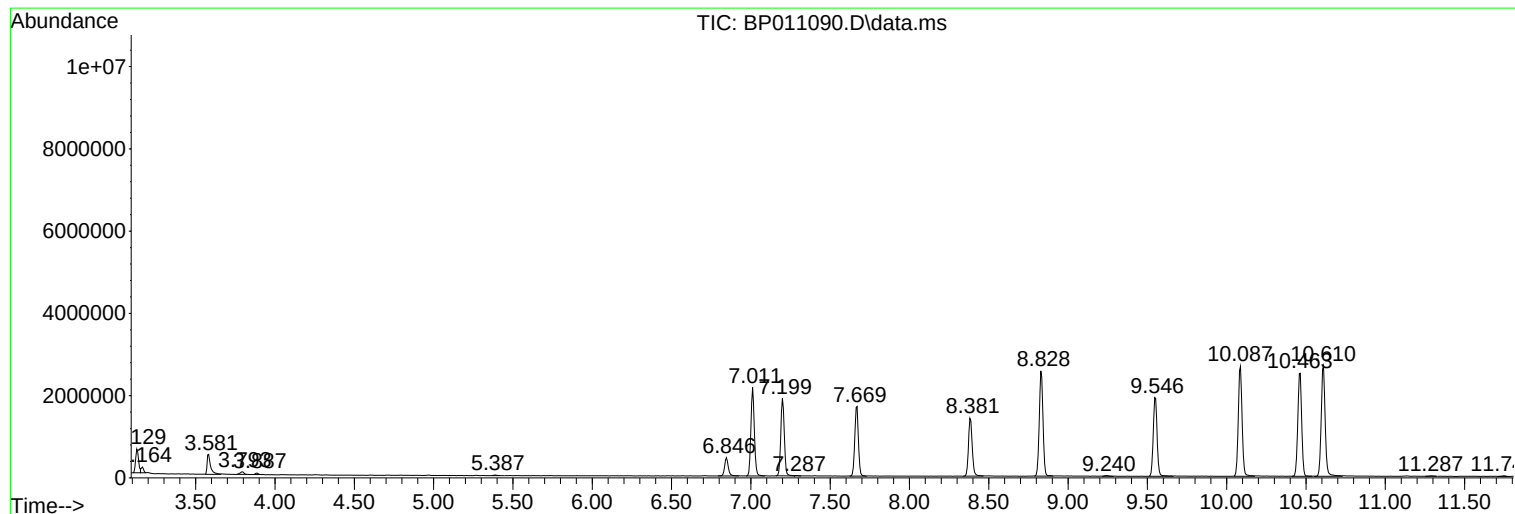

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011090.D
Acq On : 25 Jul 2022 13:52
Operator : CG/JU
Sample : N3801-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011090.D
Acq On : 25 Jul 2022 13:52
Operator : CG/JU
Sample : N3801-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc