

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011091.D
 Acq On : 25 Jul 2022 14:26
 Operator : CG/JU
 Sample : N3801-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rBV	337978	449767	2.82%	0.325%
2	3.164	11	13	19	rVB	144053	150725	0.94%	0.109%
3	3.581	81	84	102	rVB	437491	645733	4.04%	0.467%
4	3.793	114	120	128	rVB	84129	140702	0.88%	0.102%
5	3.887	132	136	146	rVB	45893	66910	0.42%	0.048%
6	4.399	218	223	237	rVB	535764	775519	4.86%	0.561%
7	4.969	317	320	327	rVB3	18242	27932	0.17%	0.020%
8	5.387	387	391	396	rBV	18031	25944	0.16%	0.019%
9	6.846	633	639	651	rVB	594900	939054	5.88%	0.679%
10	7.010	660	667	680	rBV	2448370	3667701	22.96%	2.652%
11	7.199	690	699	711	rBV	2210659	3398275	21.28%	2.457%
12	7.663	772	778	790	rVB	1632465	2567241	16.07%	1.856%
13	8.381	893	900	916	rBV	1813325	2903418	18.18%	2.099%
14	8.828	969	976	986	rBV	2861504	4662097	29.19%	3.371%
15	9.246	1040	1047	1052	rBV	53913	86884	0.54%	0.063%
16	9.546	1090	1098	1115	rBV	2166328	3658770	22.91%	2.645%
17	10.087	1181	1190	1206	rBV	2964990	5006769	31.35%	3.620%
18	10.457	1245	1253	1261	rBV	2457965	4072375	25.50%	2.944%
19	10.604	1271	1278	1299	rBV	2767987	4861862	30.44%	3.515%
20	11.745	1466	1472	1478	rVB2	34757	51981	0.33%	0.038%
21	12.063	1521	1526	1533	rBV2	50957	91505	0.57%	0.066%
22	12.681	1627	1631	1639	rBV4	12781	25737	0.16%	0.019%
23	12.940	1669	1675	1686	rBV3	32017	63448	0.40%	0.046%
24	13.751	1806	1813	1826	rBV	6536065	9113032	57.05%	6.589%
25	14.022	1850	1859	1876	rBV	7282911	10621767	66.50%	7.680%
26	14.334	1905	1912	1926	rBV	3725687	5411802	33.88%	3.913%
27	14.545	1942	1948	1967	rBV	357383	693694	4.34%	0.502%
28	14.769	1981	1986	1995	rVB10	18607	36103	0.23%	0.026%
29	15.145	2045	2050	2060	rBV	94846	139400	0.87%	0.101%
30	15.334	2075	2082	2097	rBV	9121895	12985319	81.30%	9.389%
31	15.457	2097	2103	2117	rVV	3165811	4316906	27.03%	3.121%
32	15.569	2117	2122	2128	rVV	115472	192774	1.21%	0.139%
33	16.057	2201	2205	2210	rVV6	17507	34438	0.22%	0.025%
34	16.122	2210	2216	2222	rVB3	35224	59178	0.37%	0.043%
35	16.581	2289	2294	2300	rBV10	12993	21893	0.14%	0.016%
36	16.775	2323	2327	2332	rBV3	20214	24667	0.15%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011091.D
Acq On : 25 Jul 2022 14:26
Operator : CG/JU
Sample : N3801-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	16.875	2340	2344	2349	rBV4	15987	27870	0.17%	0.020%
38	17.098	2375	2382	2392	rBV	4205280	5987937	37.49%	4.329%
39	17.198	2392	2399	2412	rVV2	9688880	13332951	83.47%	9.640%
40	17.404	2430	2434	2438	rVB	15749	17326	0.11%	0.013%
41	18.004	2533	2536	2539	rBV5	12090	16495	0.10%	0.012%
42	18.080	2546	2549	2553	rVB	18948	19957	0.12%	0.014%
43	19.027	2705	2710	2717	rBV2	145014	212844	1.33%	0.154%
44	19.098	2717	2722	2729	rVV	125216	194851	1.22%	0.141%
45	19.451	2776	2782	2789	rBV	11716718	15972736	100.00%	11.549%
46	21.216	3077	3082	3090	rBV	4403967	5525660	34.59%	3.995%
47	23.410	3448	3455	3462	rBV2	5768442	10627541	66.54%	7.684%
48	23.557	3475	3480	3489	rVB2	2237078	4381869	27.43%	3.168%




Sum of corrected areas: 138309359

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011091.D
Acq On : 25 Jul 2022 14:26
Operator : CG/JU
Sample : N3801-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

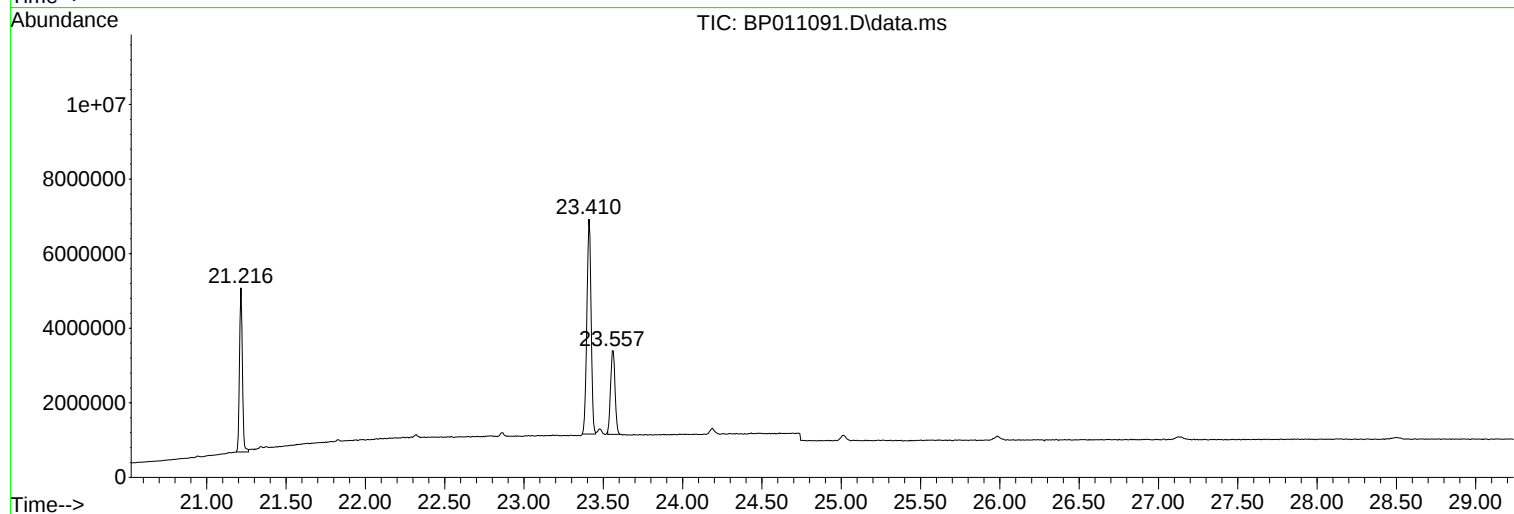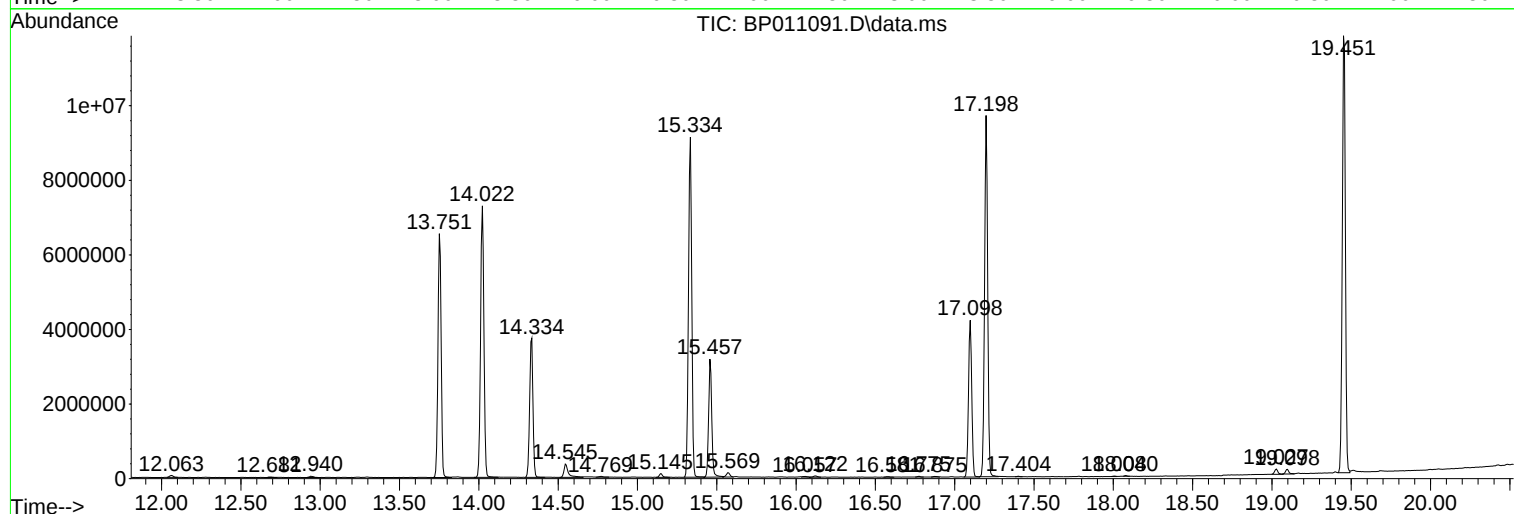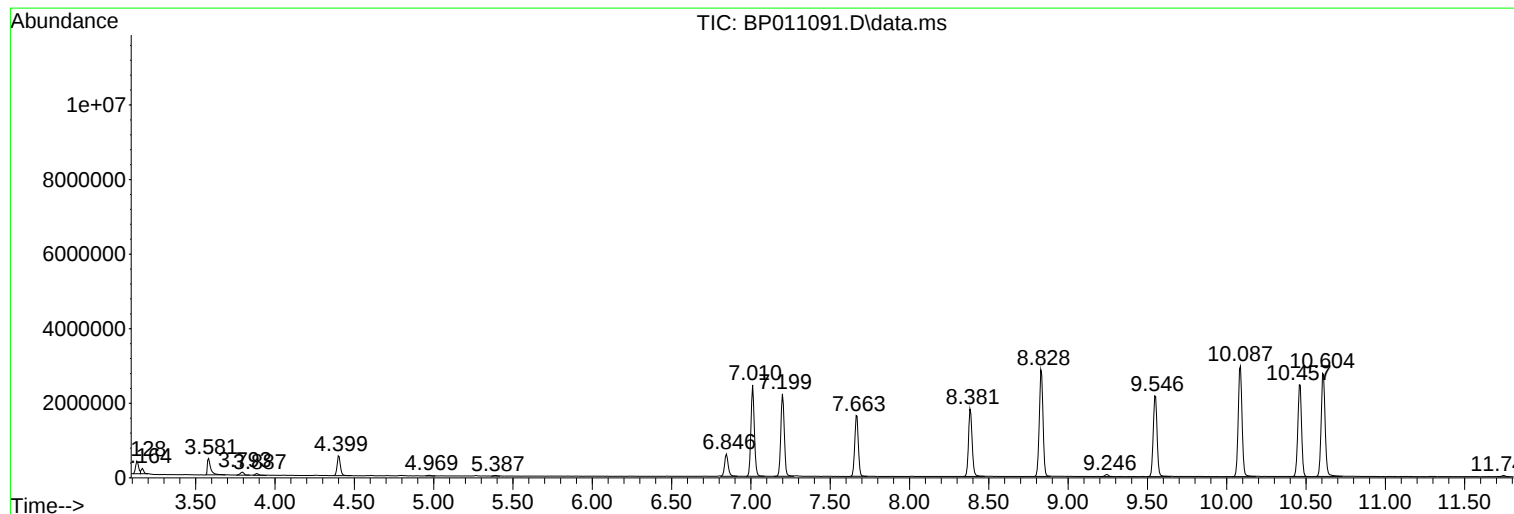

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011091.D
Acq On : 25 Jul 2022 14:26
Operator : CG/JU
Sample : N3801-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW9










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetrachloroethylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.399	6.04 ng/ul	775519	1,4-Dichlorobenzene-d4	7.669

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
2			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
3			Tetrachloroethylene	164	C2Cl4	000127-18-4	98
4			Tetrachloroethylene	164	C2Cl4	000127-18-4	97
5			Pyrimidine, 5-fluoro-2,4-dichloro-	166	C4HC12FN2	002927-71-1	32

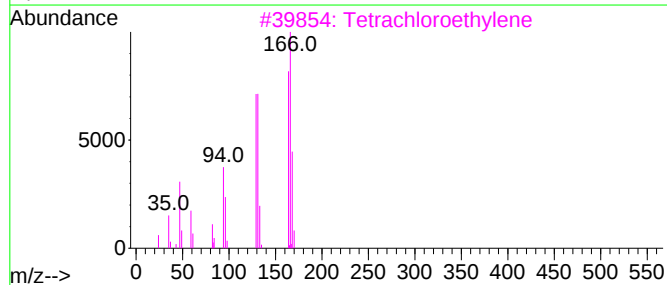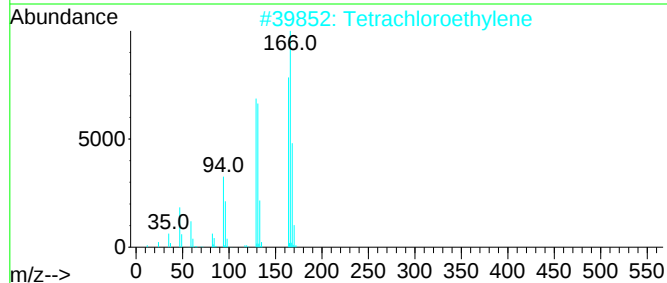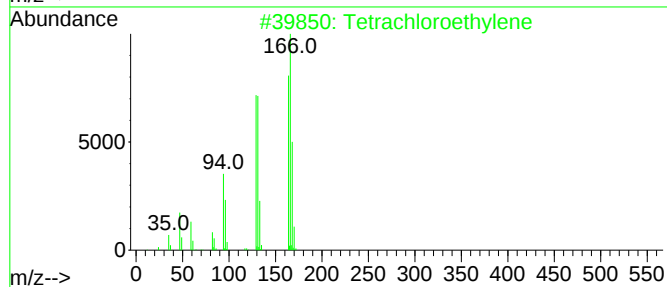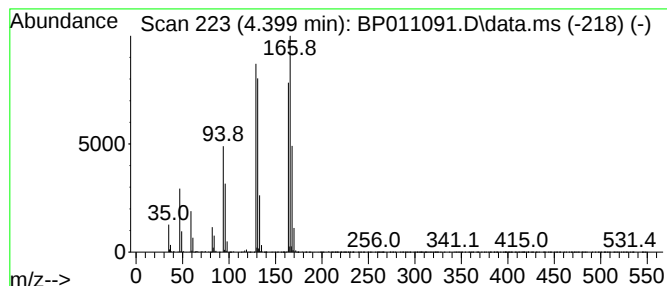

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011091.D
Acq On : 25 Jul 2022 14:26
Operator : CG/JU
Sample : N3801-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetrachloroethy...	4.399	6.0	ng/u1	775519	1	7.669	2567240	20.0