

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011092.D
 Acq On : 25 Jul 2022 15:01
 Operator : CG/JU
 Sample : N3801-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011092.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	10	rBV	35676	47567	0.33%	0.036%
2	3.164	10	13	29	rVB	133030	212757	1.47%	0.163%
3	3.575	81	83	108	rVB	661291	999492	6.92%	0.764%
4	3.793	114	120	128	rVB3	70729	139404	0.97%	0.107%
5	3.887	132	136	141	rVB	34794	48303	0.33%	0.037%
6	5.387	388	391	398	rVB2	17305	27567	0.19%	0.021%
7	5.534	412	416	419	rBV	18049	22993	0.16%	0.018%
8	6.846	631	639	649	rBV	434856	706727	4.89%	0.540%
9	7.010	659	667	680	rBV	2095824	3232716	22.39%	2.471%
10	7.199	692	699	711	rBV	1839496	2887960	20.00%	2.207%
11	7.287	711	714	722	rVB7	13953	23847	0.17%	0.018%
12	7.663	771	778	788	rBV	1671347	2621510	18.15%	2.004%
13	8.381	893	900	918	rBV	1423296	2312354	16.01%	1.767%
14	8.828	969	976	989	rBV	2518914	4106357	28.44%	3.139%
15	9.246	1042	1047	1054	rVB4	10015	17911	0.12%	0.014%
16	9.546	1091	1098	1114	rBV	1937090	3202000	22.18%	2.447%
17	10.081	1182	1189	1209	rBV	2606617	4373139	30.29%	3.342%
18	10.457	1245	1253	1261	rBV	2470419	4149861	28.74%	3.172%
19	10.604	1270	1278	1309	rBV	2605862	4697847	32.53%	3.591%
20	11.128	1358	1367	1372	rBV2	20127	44003	0.30%	0.034%
21	11.751	1467	1473	1477	rVB4	8354	14609	0.10%	0.011%
22	12.063	1519	1526	1535	rBV	48058	88945	0.62%	0.068%
23	12.681	1626	1631	1636	rBV5	12549	23415	0.16%	0.018%
24	12.940	1671	1675	1680	rBV3	19397	29921	0.21%	0.023%
25	13.240	1721	1726	1729	rBV6	9447	16956	0.12%	0.013%
26	13.298	1732	1736	1742	rVB7	9906	17139	0.12%	0.013%
27	13.751	1805	1813	1825	rBV	5898589	8135926	56.34%	6.218%
28	14.022	1849	1859	1876	rBV	6625699	9392711	65.05%	7.179%
29	14.334	1902	1912	1923	rBV	3666887	5549777	38.43%	4.242%
30	14.551	1941	1949	1968	rBV	269770	581813	4.03%	0.445%
31	14.769	1981	1986	1993	rVB	14923	26178	0.18%	0.020%
32	14.969	2016	2020	2024	rBV2	23607	30424	0.21%	0.023%
33	15.145	2045	2050	2054	rBV	66326	98466	0.68%	0.075%
34	15.334	2075	2082	2097	rBV	8312053	11851721	82.08%	9.058%
35	15.457	2097	2103	2117	rVV	2984451	4064497	28.15%	3.107%
36	15.575	2118	2123	2134	rVB	103192	178459	1.24%	0.136%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011092.D
 Acq On : 25 Jul 2022 15:01
 Operator : CG/JU
 Sample : N3801-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.898	2175	2178	2184	rVB8	9856	16264	0.11%	0.012%
38	16.045	2194	2203	2210	rBV9	13841	44780	0.31%	0.034%
39	16.122	2211	2216	2221	rVB3	33143	47177	0.33%	0.036%
40	16.775	2321	2327	2331	rBV5	16159	27762	0.19%	0.021%
41	16.875	2340	2344	2351	rBV3	25356	49395	0.34%	0.038%
42	17.098	2375	2382	2392	rBV	4794194	6494990	44.98%	4.964%
43	17.198	2392	2399	2412	rBV2	9136340	12844320	88.95%	9.817%
44	17.398	2430	2433	2439	rVB	16432	22278	0.15%	0.017%
45	17.786	2495	2499	2503	rVB6	16907	23939	0.17%	0.018%
46	18.080	2545	2549	2552	rVB	32024	36501	0.25%	0.028%
47	18.475	2612	2616	2619	rBV5	9916	15431	0.11%	0.012%
48	19.027	2706	2710	2716	rBV2	117147	156780	1.09%	0.120%
49	19.098	2717	2722	2727	rBV	106540	158651	1.10%	0.121%
50	19.398	2771	2773	2776	rVB3	23373	21928	0.15%	0.017%
51	19.451	2776	2782	2789	rBV	10248740	14439638	100.00%	11.036%
52	21.216	3077	3082	3091	rBV	5048864	6290353	43.56%	4.808%
53	23.410	3448	3455	3462	rBV2	5712181	10951142	75.84%	8.370%
54	23.563	3474	3481	3492	rVB2	2665013	5221544	36.16%	3.991%




Sum of corrected areas: 130838145

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011092.D
Acq On : 25 Jul 2022 15:01
Operator : CG/JU
Sample : N3801-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

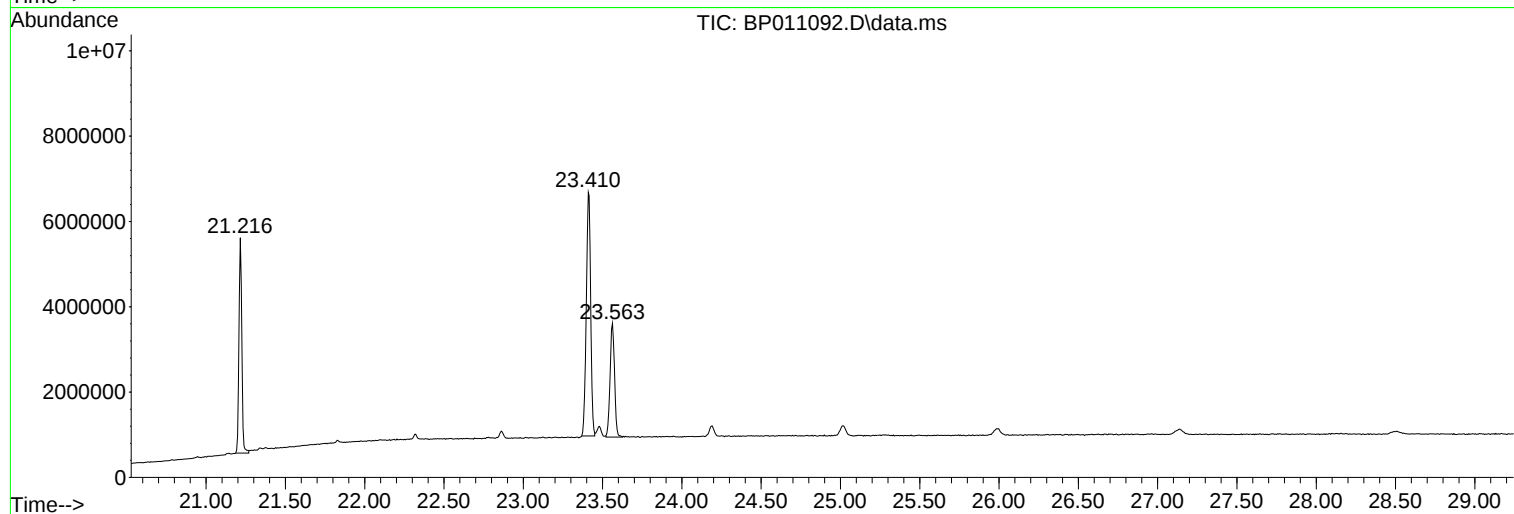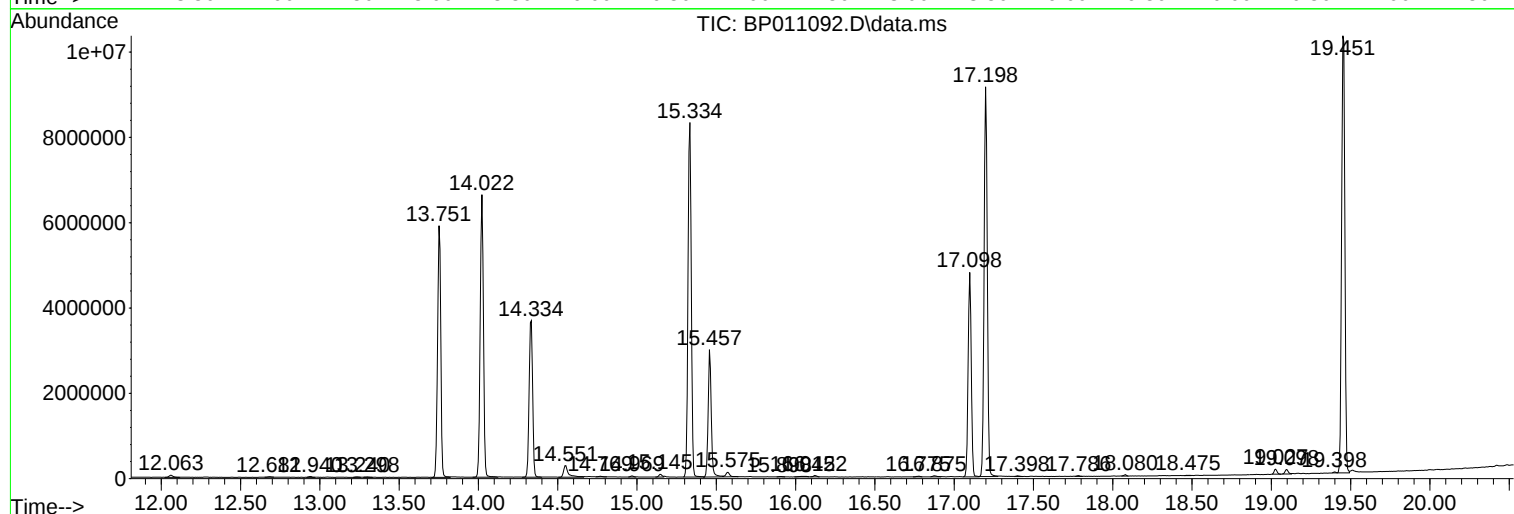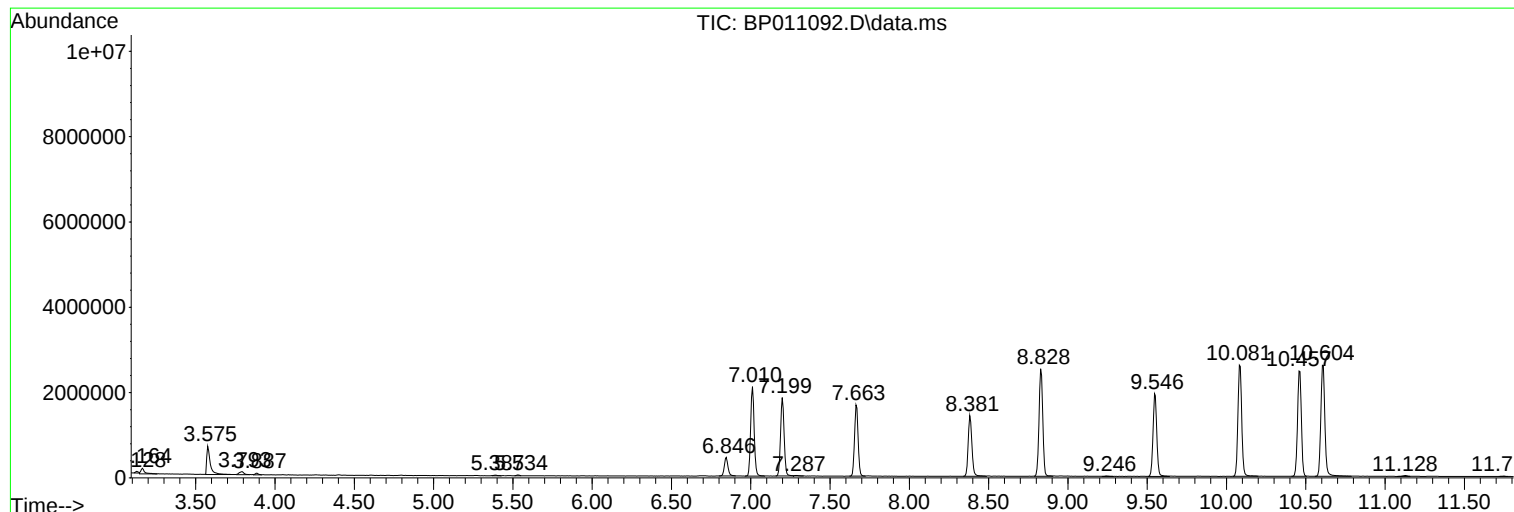

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011092.D
Acq On : 25 Jul 2022 15:01
Operator : CG/JU
Sample : N3801-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011092.D
Acq On : 25 Jul 2022 15:01
Operator : CG/JU
Sample : N3801-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc