

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011093.D
 Acq On : 25 Jul 2022 15:35
 Operator : CG/JU
 Sample : N3801-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011093.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	11	rBV	288301	379899	2.51%	0.288%
2	3.164	11	13	20	rVB	140787	163122	1.08%	0.124%
3	3.575	80	83	99	rBV	448760	693572	4.58%	0.525%
4	3.793	115	120	126	rVB	64395	104153	0.69%	0.079%
5	3.887	132	136	142	rVB	39927	55192	0.36%	0.042%
6	4.399	219	223	228	rBV	27805	35718	0.24%	0.027%
7	4.793	286	290	294	rBV4	10836	17203	0.11%	0.013%
8	5.387	388	391	395	rVB	15633	19425	0.13%	0.015%
9	6.846	632	639	654	rVB	479581	778170	5.14%	0.589%
10	7.011	660	667	681	rBV	2100624	3195022	21.11%	2.419%
11	7.199	692	699	710	rBV	1891476	2907012	19.21%	2.201%
12	7.287	711	714	722	rVB8	11647	23081	0.15%	0.017%
13	7.663	771	778	788	rBV	1471750	2325489	15.37%	1.761%
14	8.381	893	900	913	rBV	1521761	2489725	16.45%	1.885%
15	8.828	969	976	995	rBV	2589879	4204350	27.78%	3.183%
16	9.246	1042	1047	1053	rVB	26108	42848	0.28%	0.032%
17	9.546	1090	1098	1111	rBV	1977329	3303503	21.83%	2.501%
18	10.087	1181	1190	1210	rBV	2675502	4554707	30.10%	3.449%
19	10.457	1246	1253	1261	rBV	2264859	3735256	24.68%	2.828%
20	10.610	1266	1279	1297	rBV	2518822	4455447	29.44%	3.373%
21	11.746	1465	1472	1478	rBV	31994	51124	0.34%	0.039%
22	12.063	1520	1526	1533	rBV	54570	97759	0.65%	0.074%
23	12.687	1626	1632	1638	rBV6	11302	20761	0.14%	0.016%
24	12.940	1669	1675	1681	rBV6	14174	22263	0.15%	0.017%
25	13.240	1721	1726	1730	rVB3	11629	15575	0.10%	0.012%
26	13.751	1806	1813	1825	rBV	6610104	8879046	58.67%	6.723%
27	13.845	1825	1829	1839	rVB	9552	24029	0.16%	0.018%
28	14.022	1849	1859	1868	rBV	7064744	10255080	67.76%	7.765%
29	14.328	1904	1911	1922	rBV	3522542	5138276	33.95%	3.890%
30	14.545	1939	1948	1962	rBV	346030	644885	4.26%	0.488%
31	14.775	1982	1987	1993	rVB10	11487	22326	0.15%	0.017%
32	15.145	2045	2050	2064	rVB2	46293	79165	0.52%	0.060%
33	15.334	2074	2082	2096	rBV	8892772	12819477	84.71%	9.706%
34	15.457	2097	2103	2118	rVV	3269473	4424403	29.24%	3.350%
35	15.569	2118	2122	2130	rVB2	112575	171812	1.14%	0.130%
36	16.051	2195	2204	2211	rBV7	20482	55249	0.37%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011093.D
 Acq On : 25 Jul 2022 15:35
 Operator : CG/JU
 Sample : N3801-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHW8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.122	2211	2216	2221	rVB2	35058	49574	0.33%	0.038%
38	16.769	2322	2326	2332	rVB6	17946	26350	0.17%	0.020%
39	16.875	2340	2344	2354	rVB5	17467	36387	0.24%	0.028%
40	17.098	2375	2382	2392	rBV	4137692	5934277	39.21%	4.493%
41	17.198	2392	2399	2413	rVV	9923154	13732790	90.74%	10.398%
42	17.398	2430	2433	2438	rVB2	19991	25036	0.17%	0.019%
43	17.781	2494	2498	2502	rVB6	15508	22458	0.15%	0.017%
44	18.004	2532	2536	2541	rBV7	15645	27172	0.18%	0.021%
45	18.075	2545	2548	2553	rVB	25870	35056	0.23%	0.027%
46	19.028	2705	2710	2714	rBV	126540	183821	1.21%	0.139%
47	19.092	2717	2721	2730	rVV	117035	175489	1.16%	0.133%
48	19.398	2770	2773	2776	rBV4	28231	34016	0.22%	0.026%
49	19.451	2776	2782	2789	rBV	11490202	15133678	100.00%	11.458%
50	21.216	3077	3082	3090	rBV	4135008	5336605	35.26%	4.041%
51	23.404	3447	3454	3462	rBV2	5633837	10787396	71.28%	8.168%
52	23.557	3473	3480	3489	rVB2	2143271	4330416	28.61%	3.279%




Sum of corrected areas: 132074645

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011093.D
Acq On : 25 Jul 2022 15:35
Operator : CG/JU
Sample : N3801-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

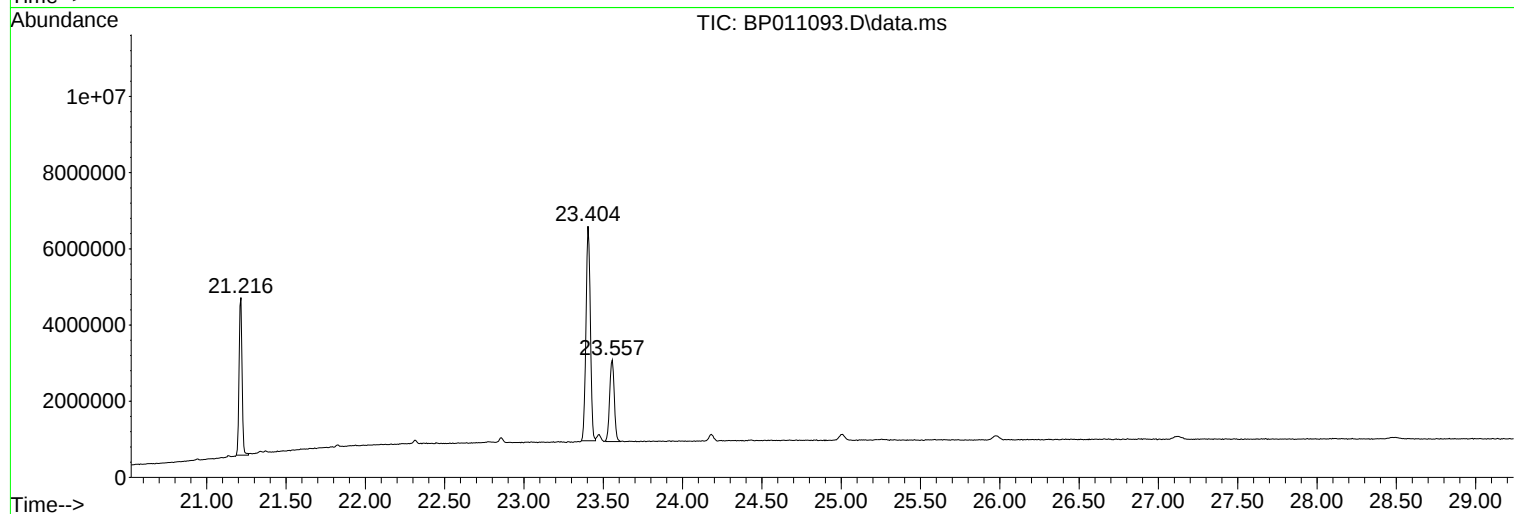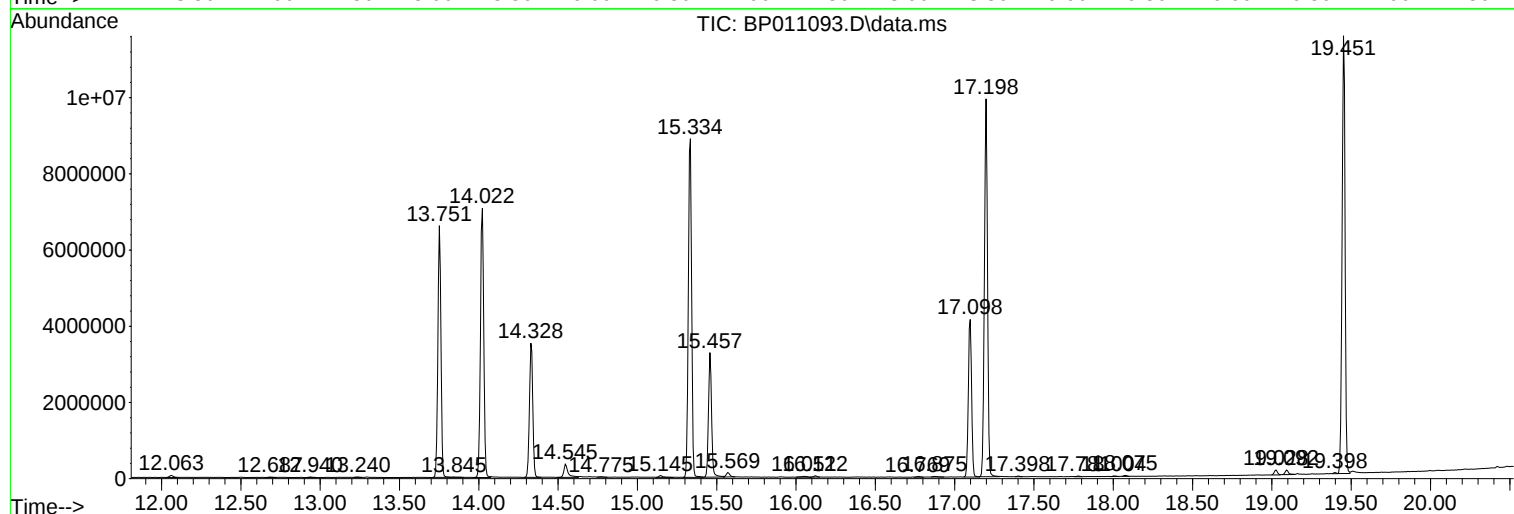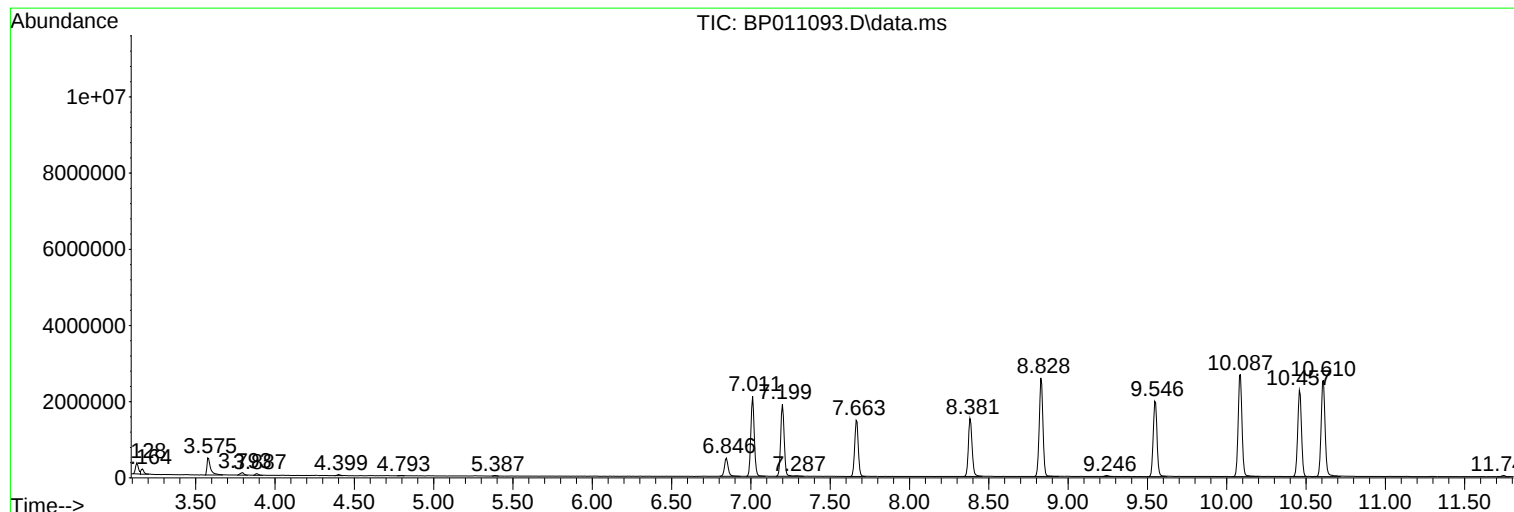

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011093.D
Acq On : 25 Jul 2022 15:35
Operator : CG/JU
Sample : N3801-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011093.D
Acq On : 25 Jul 2022 15:35
Operator : CG/JU
Sample : N3801-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHW8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------