

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011094.D
 Acq On : 25 Jul 2022 16:10
 Operator : CG/JU
 Sample : N3801-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011094.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	10	13	21	rVB	134772	164452	1.37%	0.137%
2	3.581	81	84	98	rBV	355179	530084	4.40%	0.440%
3	3.793	114	120	125	rVB2	64691	117487	0.98%	0.098%
4	3.887	132	136	147	rVB	44253	66179	0.55%	0.055%
5	4.793	288	290	295	rVB4	11238	13138	0.11%	0.011%
6	5.264	366	370	376	rVB5	8824	14073	0.12%	0.012%
7	5.393	386	392	400	rVB	14321	25334	0.21%	0.021%
8	6.105	509	513	520	rBV9	8001	16819	0.14%	0.014%
9	6.846	632	639	652	rVB	435042	718513	5.97%	0.597%
10	7.011	660	667	680	rBV	2023711	3088613	25.66%	2.566%
11	7.199	691	699	711	rBV	1842418	2827681	23.49%	2.349%
12	7.287	711	714	721	rVB7	13811	22651	0.19%	0.019%
13	7.663	771	778	788	rBV	1867641	2934863	24.39%	2.438%
14	8.381	893	900	916	rBV	1345443	2149848	17.86%	1.786%
15	8.828	969	976	987	rBV	2463014	3908987	32.48%	3.248%
16	9.246	1042	1047	1051	rVB4	10760	15938	0.13%	0.013%
17	9.546	1089	1098	1109	rBV	1912010	3059685	25.42%	2.542%
18	10.081	1182	1189	1209	rBV	2548616	4272125	35.50%	3.549%
19	10.457	1244	1253	1263	rBV	2836119	4663391	38.75%	3.875%
20	10.604	1270	1278	1297	rBV	1765721	3144398	26.13%	2.612%
21	11.293	1388	1395	1400	rBV8	15118	33858	0.28%	0.028%
22	11.746	1467	1472	1476	rVB3	11116	17482	0.15%	0.015%
23	12.057	1518	1525	1534	rBV2	46270	85470	0.71%	0.071%
24	12.681	1624	1631	1636	rBV7	13912	27114	0.23%	0.023%
25	12.940	1668	1675	1683	rBV8	20240	37689	0.31%	0.031%
26	13.051	1688	1694	1700	rVB8	8540	14866	0.12%	0.012%
27	13.234	1720	1725	1729	rBV5	14121	23859	0.20%	0.020%
28	13.293	1729	1735	1739	rVV6	8598	14759	0.12%	0.012%
29	13.751	1806	1813	1824	rBV	6053118	8169410	67.88%	6.787%
30	14.022	1849	1859	1873	rBV	6197308	9255509	76.90%	7.690%
31	14.328	1904	1911	1921	rBV	4525151	6375389	52.97%	5.297%
32	14.545	1943	1948	1965	rBV	226465	483565	4.02%	0.402%
33	14.763	1979	1985	1992	rVB	13736	28201	0.23%	0.023%
34	15.145	2044	2050	2064	rVB2	123217	203919	1.69%	0.169%
35	15.328	2074	2081	2088	rBV	8064896	11717746	97.36%	9.736%
36	15.375	2088	2089	2096	rVV5	42380	63150	0.52%	0.052%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011094.D
 Acq On : 25 Jul 2022 16:10
 Operator : CG/JU
 Sample : N3801-16
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.457	2096	2103	2117	rVV	2600558	3622537	30.10%	3.010%
38	15.569	2117	2122	2128	rVB2	100683	153054	1.27%	0.127%
39	15.904	2174	2179	2186	rVB8	9714	17773	0.15%	0.015%
40	16.028	2194	2200	2204	rBV9	13248	25801	0.21%	0.021%
41	16.122	2212	2216	2221	rVB3	29495	45005	0.37%	0.037%
42	16.228	2230	2234	2240	rBV9	5247	12699	0.11%	0.011%
43	16.286	2240	2244	2251	rVB9	7460	13734	0.11%	0.011%
44	16.645	2301	2305	2311	rVB8	9381	12193	0.10%	0.010%
45	16.775	2323	2327	2331	rVB5	16012	21554	0.18%	0.018%
46	16.875	2340	2344	2356	rVB6	21533	51051	0.42%	0.042%
47	17.092	2375	2381	2392	rBV	4915792	7074413	58.78%	5.878%
48	17.198	2392	2399	2411	rVV	7745408	11278505	93.71%	9.371%
49	17.398	2429	2433	2438	rBV	20385	25464	0.21%	0.021%
50	17.775	2494	2497	2503	rVB8	23613	32299	0.27%	0.027%
51	18.075	2545	2548	2552	rVB	39601	47451	0.39%	0.039%
52	18.322	2586	2590	2598	rBV8	12774	26709	0.22%	0.022%
53	18.475	2612	2616	2621	rBV3	23049	39298	0.33%	0.033%
54	19.022	2705	2709	2714	rBV	107703	144430	1.20%	0.120%
55	19.092	2717	2721	2726	rBV	123760	167718	1.39%	0.139%
56	19.451	2776	2782	2789	rBV	9051337	12035520	100.00%	10.000%
57	21.210	3077	3081	3091	rBV	3985263	5204864	43.25%	4.324%
58	23.404	3447	3454	3462	rBV	4018022	7663950	63.68%	6.368%
59	23.551	3473	3479	3490	rVB2	2168697	4338028	36.04%	3.604%




Sum of corrected areas: 120360295

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011094.D
Acq On : 25 Jul 2022 16:10
Operator : CG/JU
Sample : N3801-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

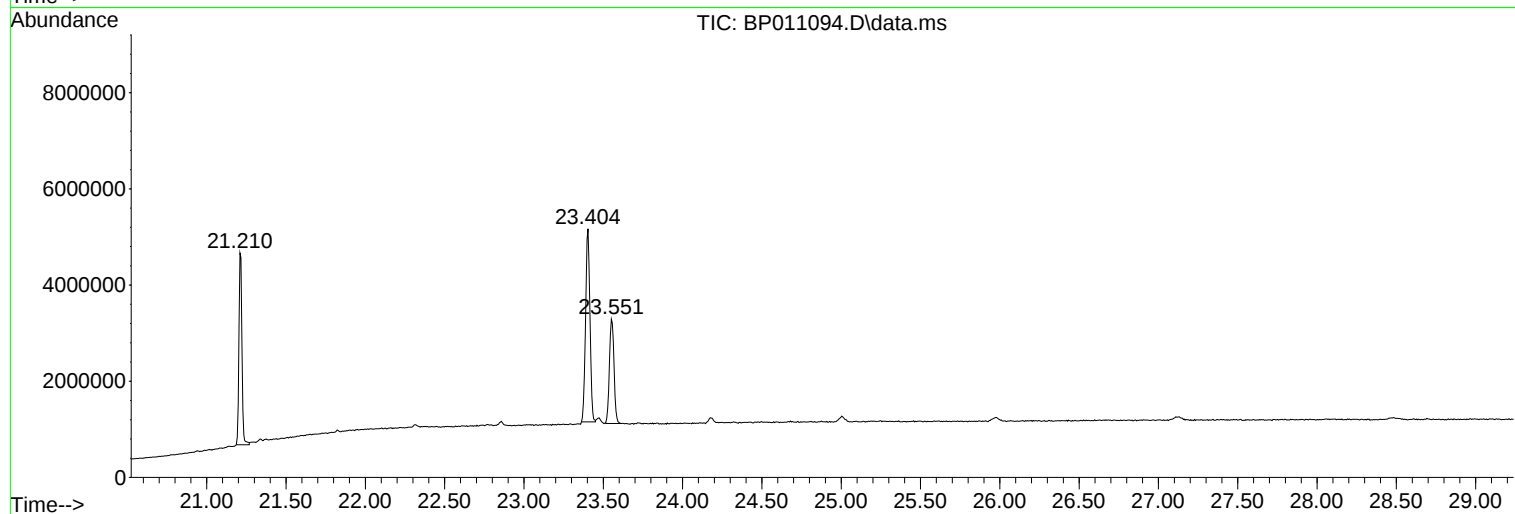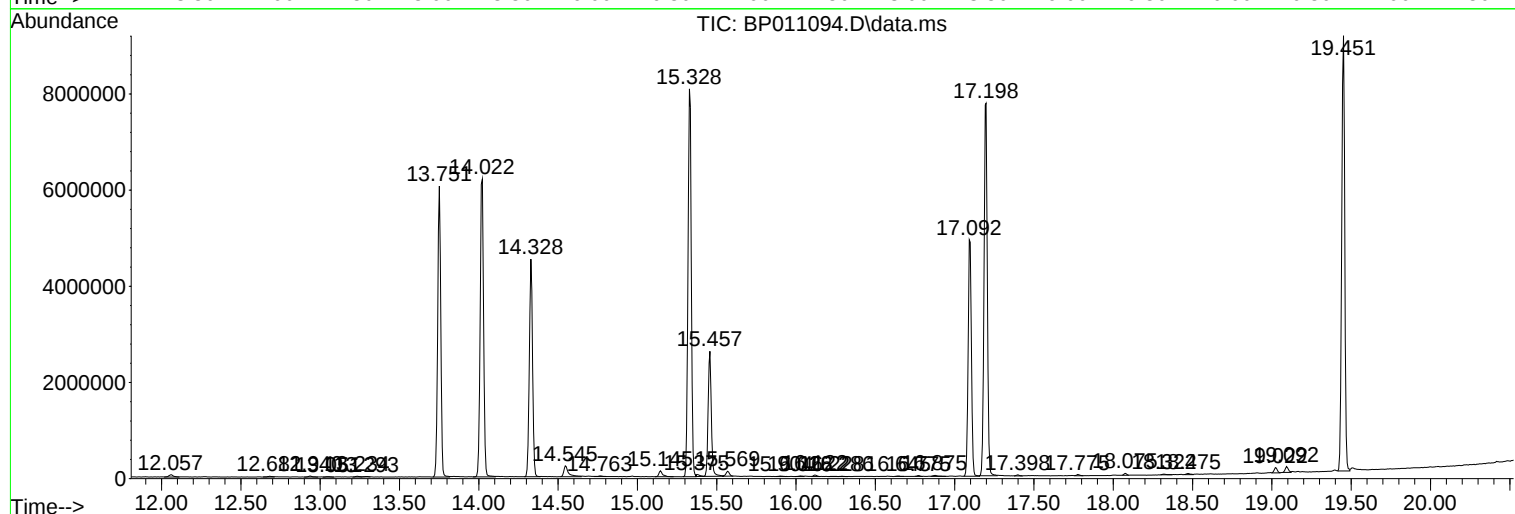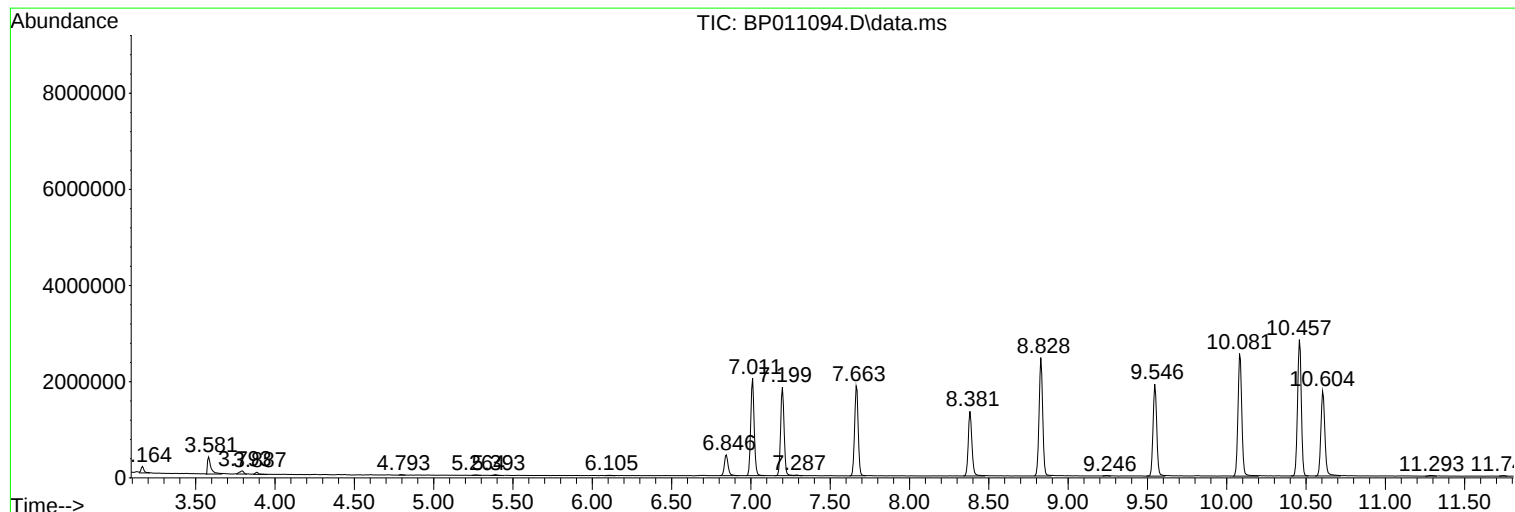

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011094.D
Acq On : 25 Jul 2022 16:10
Operator : CG/JU
Sample : N3801-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011094.D
Acq On : 25 Jul 2022 16:10
Operator : CG/JU
Sample : N3801-16
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc