

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011095.D
 Acq On : 25 Jul 2022 16:45
 Operator : CG/JU
 Sample : N3801-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011095.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	26	rVB	148472	221360	1.41%	0.148%
2	3.576	81	83	108	rVB	734469	1073263	6.83%	0.719%
3	3.793	115	120	126	rVB	69706	107637	0.69%	0.072%
4	3.887	132	136	141	rVB	42005	53145	0.34%	0.036%
5	4.799	287	291	298	rVB3	9335	17810	0.11%	0.012%
6	5.387	388	391	396	rVB	15859	22446	0.14%	0.015%
7	6.846	629	639	652	rBV	515305	852415	5.43%	0.571%
8	7.011	660	667	680	rVB	2494179	3756841	23.92%	2.517%
9	7.199	692	699	711	rBV	2187779	3343855	21.29%	2.240%
10	7.287	711	714	724	rVB9	13984	27403	0.17%	0.018%
11	7.664	771	778	789	rBV	2055857	3176487	20.23%	2.128%
12	8.381	893	900	914	rBV	1703510	2720599	17.32%	1.823%
13	8.828	968	976	994	rBV	3053691	4852923	30.90%	3.252%
14	9.240	1042	1046	1056	rVB2	39548	58830	0.37%	0.039%
15	9.546	1090	1098	1117	rBV	2298844	3724121	23.71%	2.495%
16	10.081	1180	1189	1205	rBV	3092133	5164768	32.89%	3.460%
17	10.458	1245	1253	1266	rVB	3143150	5080531	32.35%	3.404%
18	10.605	1269	1278	1303	rBV	3214334	5593731	35.62%	3.748%
19	11.740	1465	1471	1477	rVB3	26348	45232	0.29%	0.030%
20	12.057	1518	1525	1535	rBV2	60075	112110	0.71%	0.075%
21	12.681	1624	1631	1640	rBV10	13272	33726	0.21%	0.023%
22	12.934	1670	1674	1681	rBV2	21141	35045	0.22%	0.023%
23	13.228	1718	1724	1729	rBV8	11731	20710	0.13%	0.014%
24	13.293	1729	1735	1742	rVB3	12053	23674	0.15%	0.016%
25	13.751	1806	1813	1825	rBV	7139851	9878347	62.90%	6.619%
26	14.022	1849	1859	1877	rBV	7595527	11570786	73.68%	7.753%
27	14.328	1902	1911	1922	rBV	4821674	7018286	44.69%	4.702%
28	14.546	1942	1948	1969	rBV	290679	599111	3.81%	0.401%
29	14.698	1971	1974	1979	rVV6	10505	20303	0.13%	0.014%
30	14.769	1983	1986	1990	rVB6	12879	18135	0.12%	0.012%
31	15.146	2045	2050	2057	rBV	98883	141047	0.90%	0.095%
32	15.328	2074	2081	2096	rBV	10083756	14364956	91.47%	9.625%
33	15.457	2096	2103	2116	rVV	3250395	4386522	27.93%	2.939%
34	15.569	2117	2122	2128	rVB	125317	184953	1.18%	0.124%
35	16.028	2195	2200	2201	rBV5	12683	18658	0.12%	0.013%
36	16.051	2202	2204	2210	rVV5	17494	29546	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
 Data File : BP011095.D
 Acq On : 25 Jul 2022 16:45
 Operator : CG/JU
 Sample : N3801-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.116	2211	2215	2224	rVB2	41710	63733	0.41%	0.043%
38	16.769	2318	2326	2330	rBV6	22769	41223	0.26%	0.028%
39	16.875	2339	2344	2348	rBV5	20538	37174	0.24%	0.025%
40	17.092	2374	2381	2392	rBV	5625928	8011685	51.01%	5.368%
41	17.198	2392	2399	2414	rVV	10307783	14806180	94.28%	9.920%
42	17.392	2430	2432	2439	rVB2	14806	23581	0.15%	0.016%
43	17.781	2494	2498	2502	rBV7	15868	22818	0.15%	0.015%
44	18.075	2545	2548	2552	rVB	25064	30319	0.19%	0.020%
45	19.022	2705	2709	2714	rBV2	133552	188408	1.20%	0.126%
46	19.092	2717	2721	2726	rVV	122568	163594	1.04%	0.110%
47	19.451	2776	2782	2789	rBV	12054652	15704778	100.00%	10.522%
48	21.210	3076	3081	3089	rBV	5057984	6524623	41.55%	4.372%
49	23.404	3447	3454	3462	rBV2	5251445	10151741	64.64%	6.802%
50	23.551	3473	3479	3493	rVB2	2587195	5131722	32.68%	3.438%




Sum of corrected areas: 149250891

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011095.D
Acq On : 25 Jul 2022 16:45
Operator : CG/JU
Sample : N3801-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

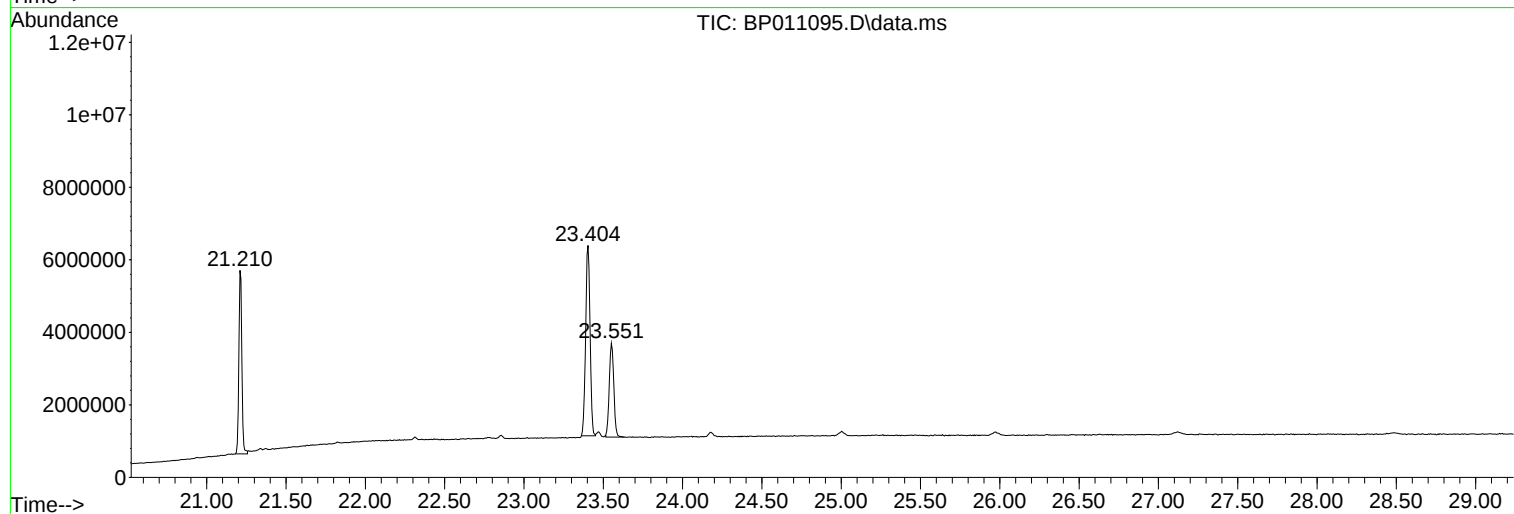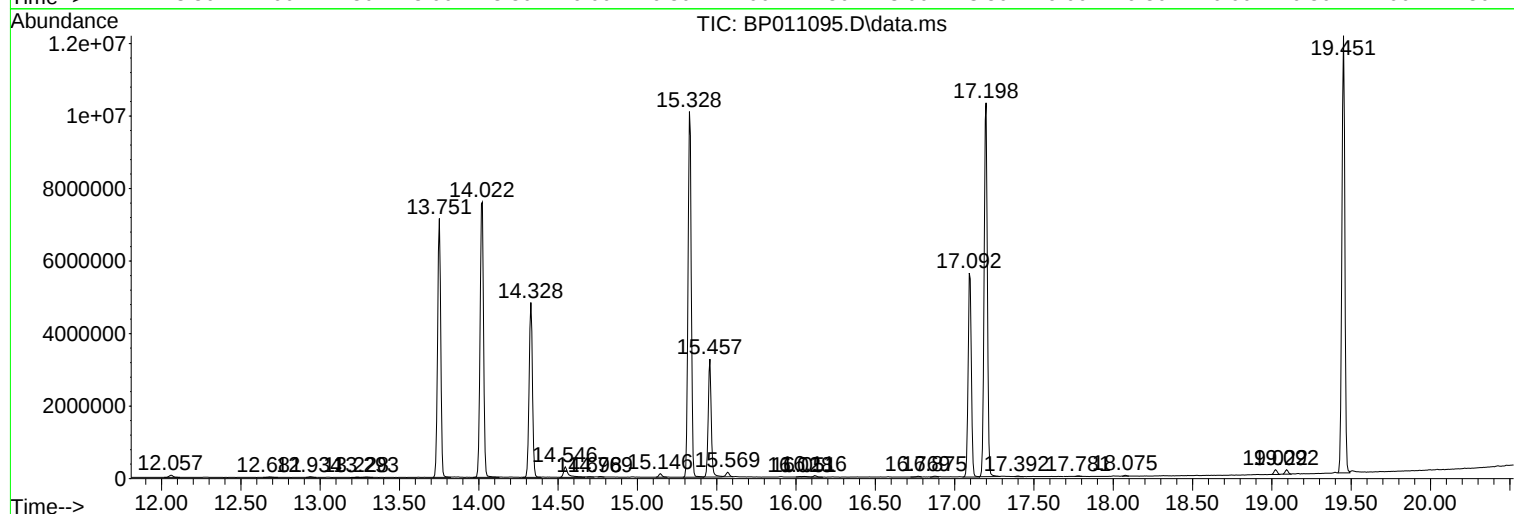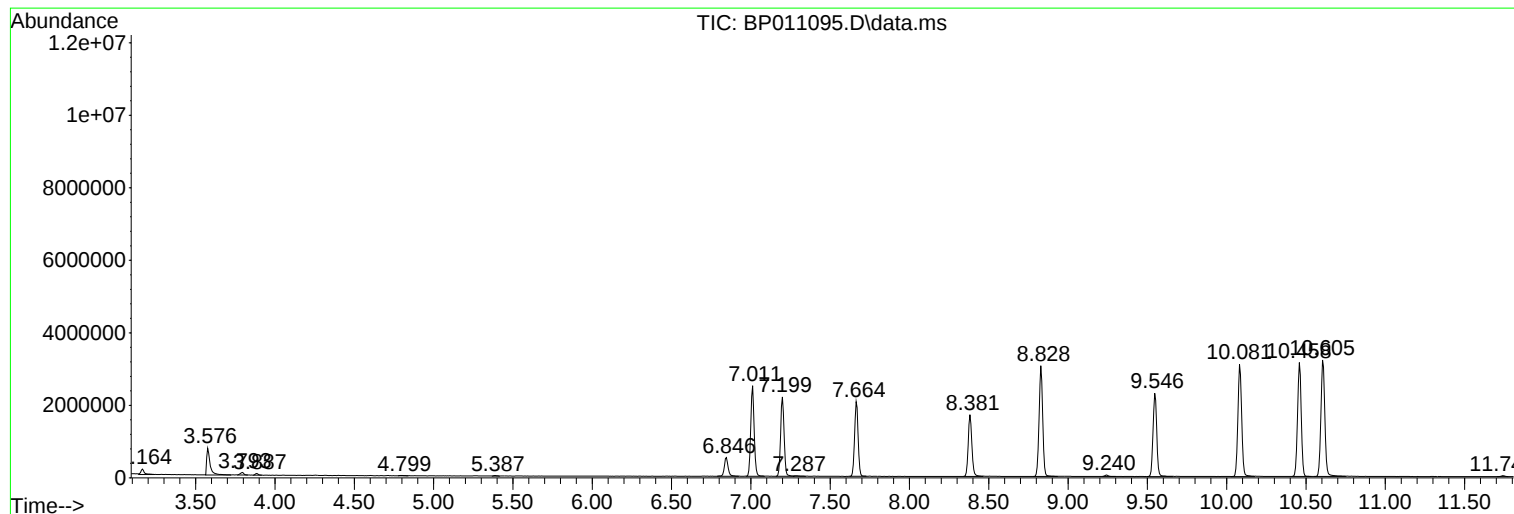

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011095.D
Acq On : 25 Jul 2022 16:45
Operator : CG/JU
Sample : N3801-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072522\
Data File : BP011095.D
Acq On : 25 Jul 2022 16:45
Operator : CG/JU
Sample : N3801-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc