




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021147.D
 Acq On : 25 Jul 2024 14:31
 Operator : MA/JU
 Sample : P3325-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B34

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:39:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

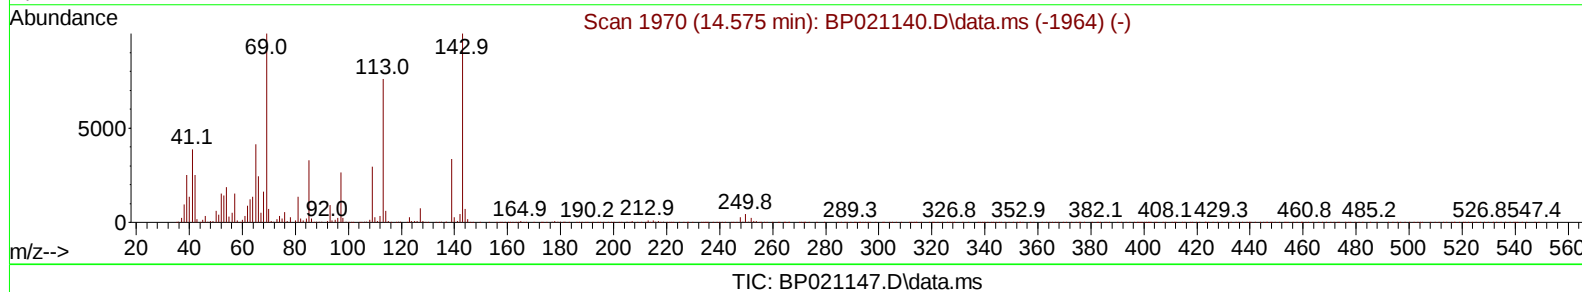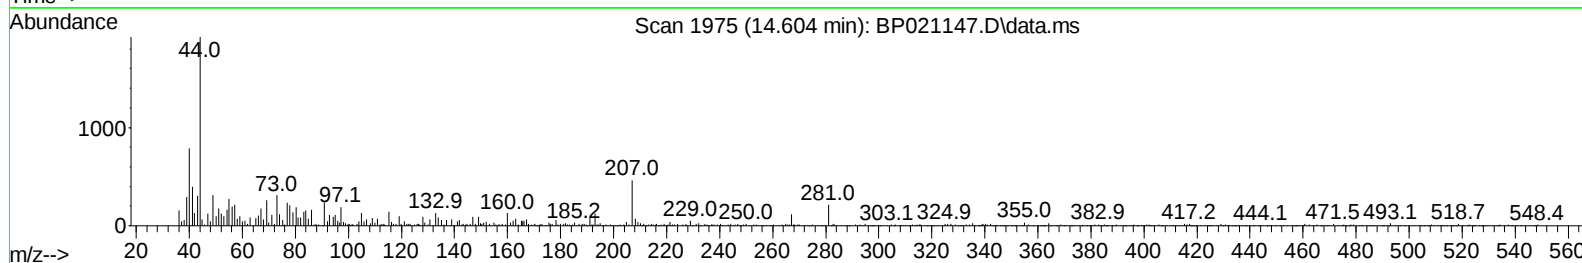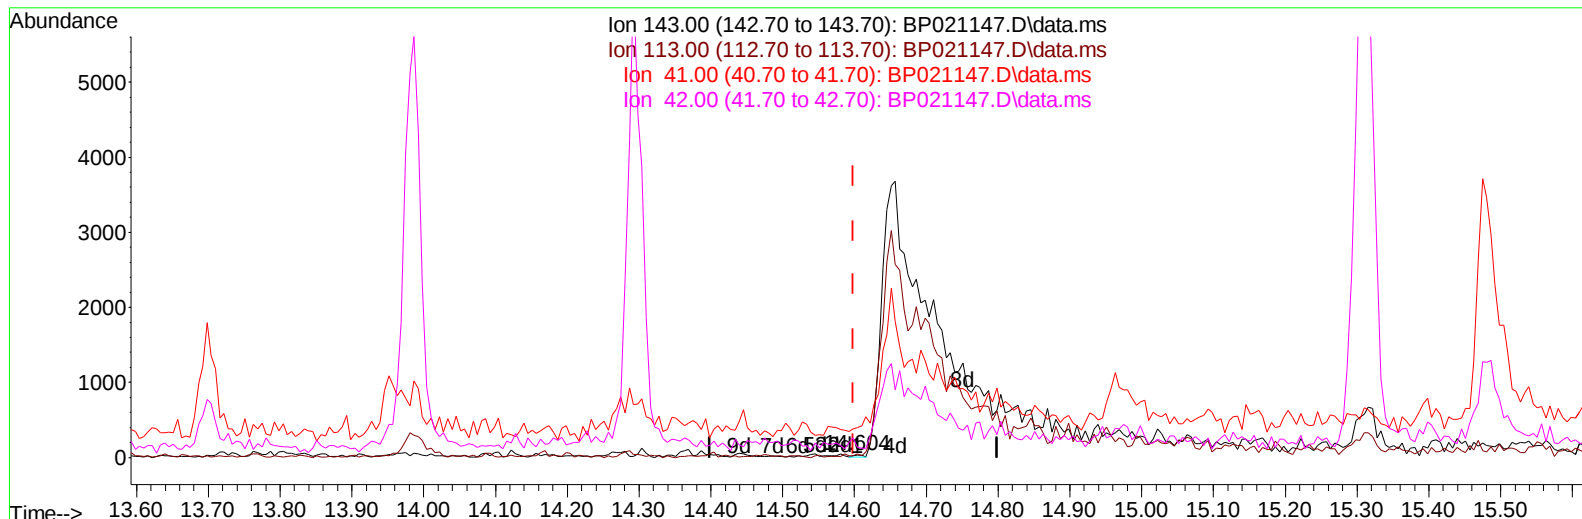

(54) 4-Nitrophenol-d4 (S)

14.604min (+ 0.006) 0.01 ng/u1

response 26

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	147.06#
41.00	37.90	1176.47#
42.00	27.10	385.29#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021147.D
 Acq On : 25 Jul 2024 14:31
 Operator : MA/JU
 Sample : P3325-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B34

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:39:03 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

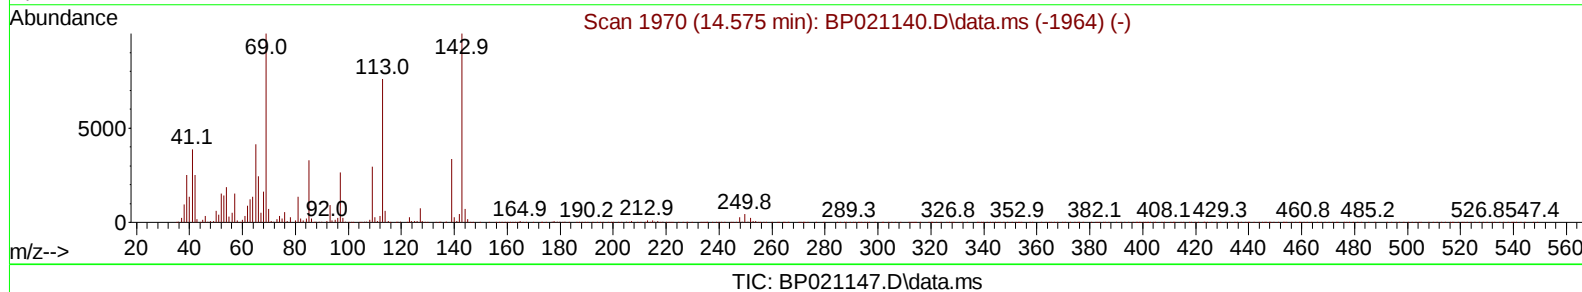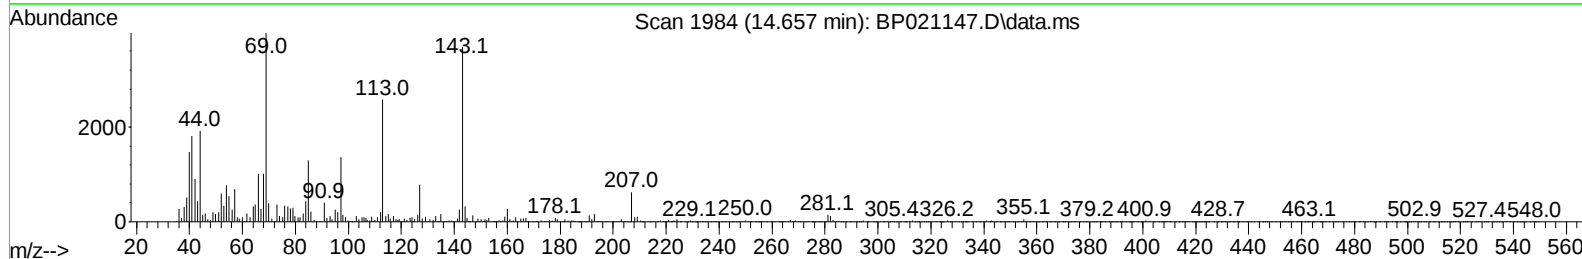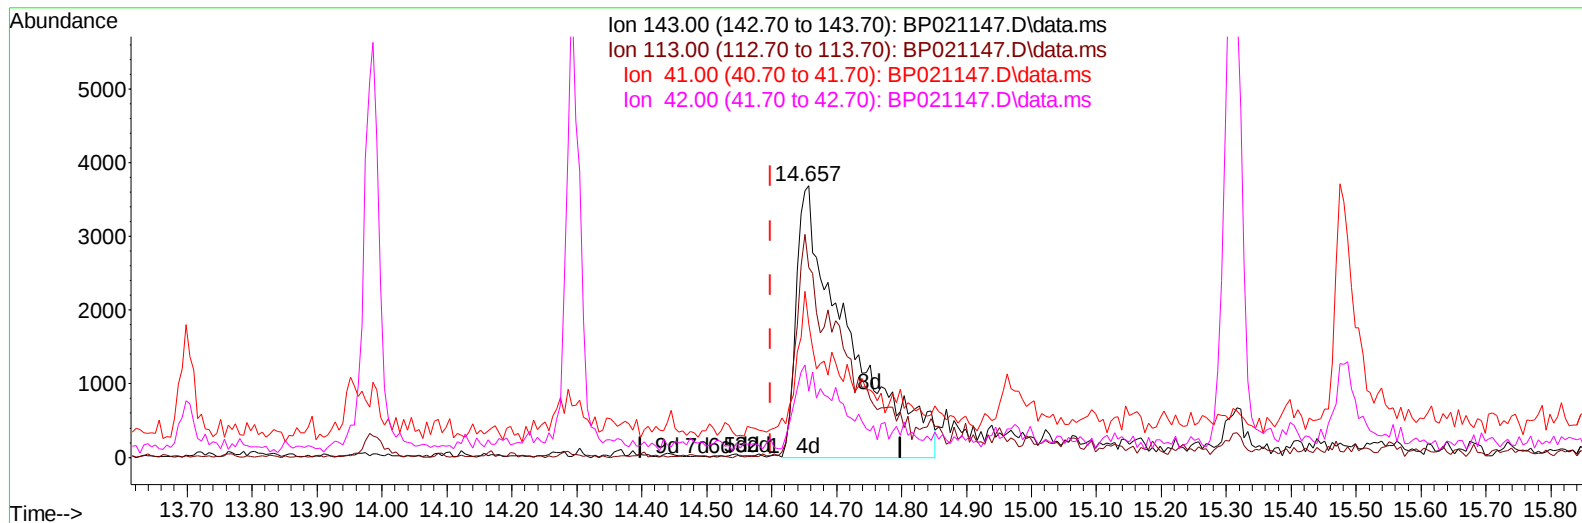

(54) 4-Nitrophenol-d4 (S)

14.657min (+ 0.059) 6.97 ng/ul m

response 20355

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	69.88
41.00	37.90	49.17#
42.00	27.10	24.42

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021147.D
 Acq On : 25 Jul 2024 14:31
 Operator : MA/JU
 Sample : P3325-06
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B34

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

Quant Time: Jul 25 22:59:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.651	152		130524	20.000	ng/ul	0.00
20) Naphthalene-d8	10.422	136		482129	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.292	164		282262	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188		567097	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240		562816	20.000	ng/ul	0.00
88) Perylene-d12	24.874	264		764558	20.000	ng/ul	0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.181	96		16387	5.713	ng/uL	0.00
4) Pyridine-d5	3.616	84		43856	5.281	ng/ul	0.02
7) Phenol-d5	6.875	99		86300	8.110	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.999	67		195376	30.296	ng/ul	0.00
11) 2-Chlorophenol-d4	7.204	132		242751	27.688	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113		150452	17.023	ng/ul	0.00
21) Nitrobenzene-d5	8.810	128		120764	32.249	ng/ul	0.00
24) 2-Nitrophenol-d4	9.528	143		136016	31.734	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.081	165		217613	28.078	ng/ul	0.00
31) 4-Chloroaniline-d4	10.587	131		200143	19.493	ng/ul	0.02
46) Dimethylphthalate-d6	13.698	166		656532	31.996	ng/ul	0.00
49) Acenaphthylene-d8	13.986	160		751504	32.617	ng/ul	0.00
54) 4-Nitrophenol-d4	14.657	143		20355m	6.972	ng/ul	0.06
60) Fluorene-d10	15.310	176		567685	33.723	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.475	200		83251	24.263	ng/ul	0.00
73) Anthracene-d10	17.216	188		911678	36.195	ng/ul	0.01
81) Pyrene-d10	19.604	212		1082760	31.118	ng/ul	0.02
92) Benzo(a)pyrene-d12	24.645	264		1416584	37.567	ng/ul	0.00
Target Compounds							
2) 1,4-Dioxane	3.216	88		7068	2.241	ng/uL	Qvalue 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021147.D
Acq On : 25 Jul 2024 14:31
Operator : MA/JU
Sample : P3325-06
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B34

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:59:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

