




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

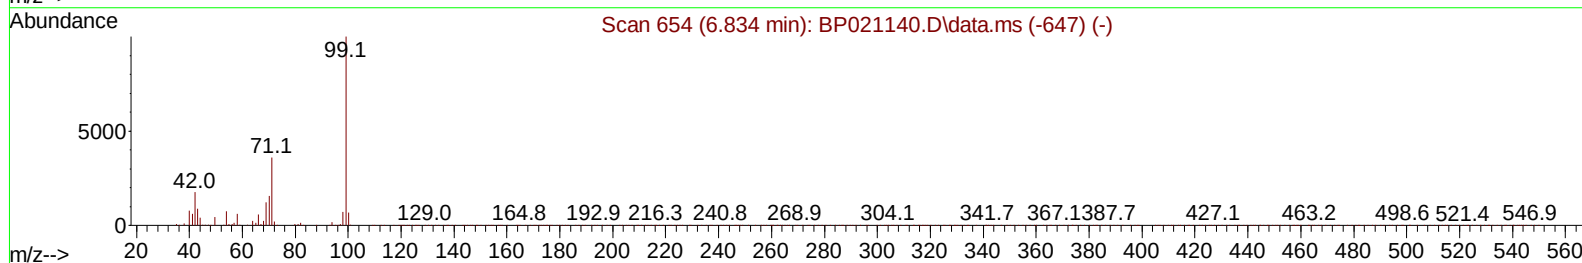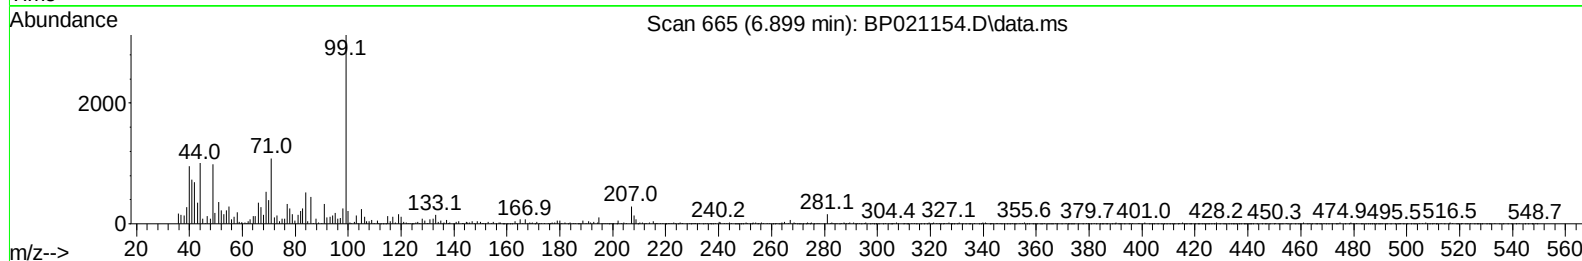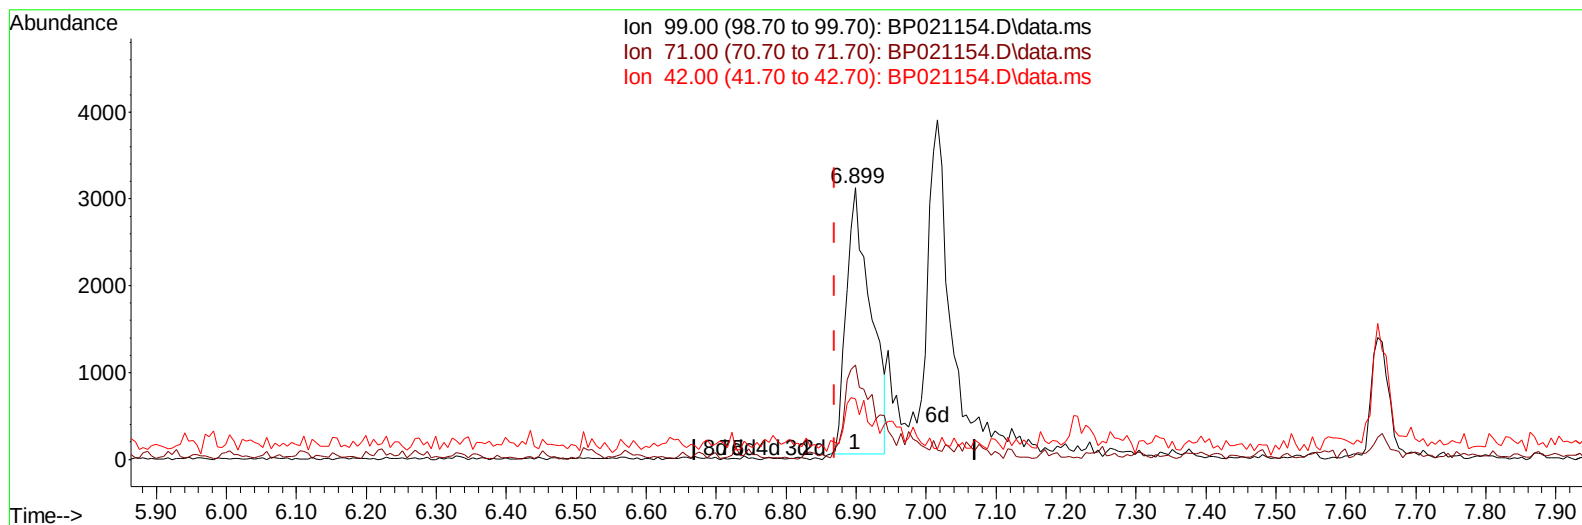

TIC: BP021154.D\data.ms

(7) Phenol-d5 (S)

6.899min (+ 0.029) 0.45 ng/u1

response 7322

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.60	34.74
42.00	19.30	22.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

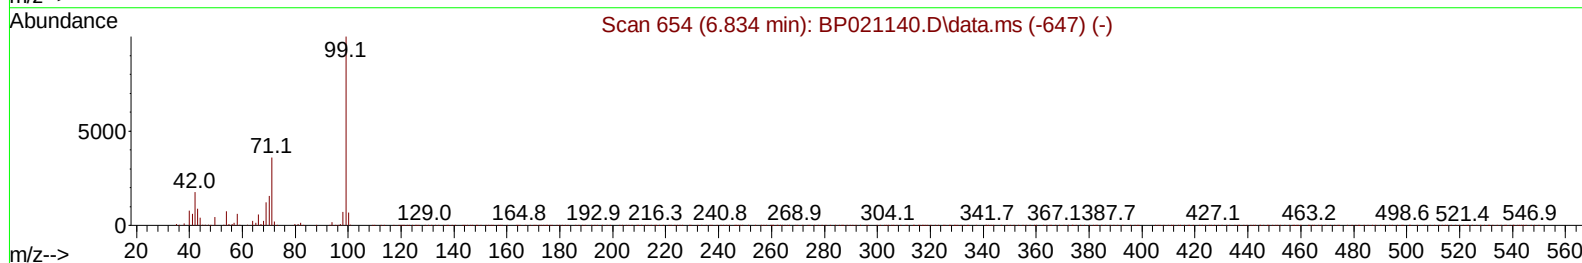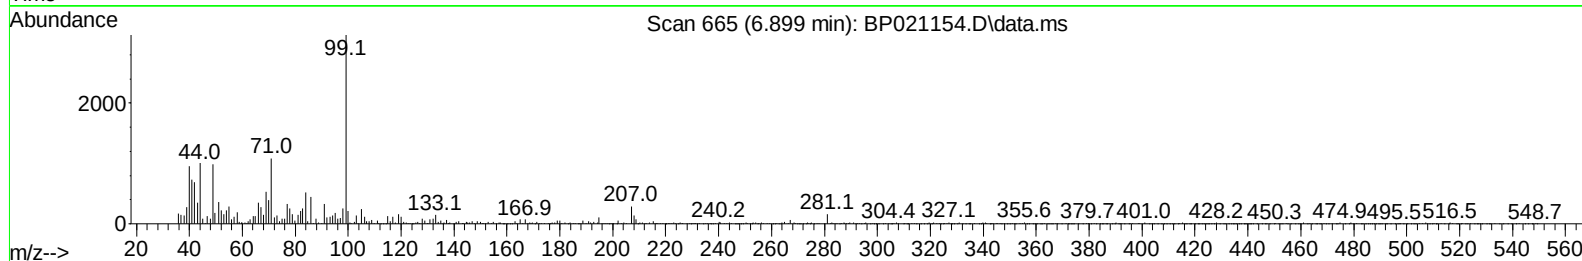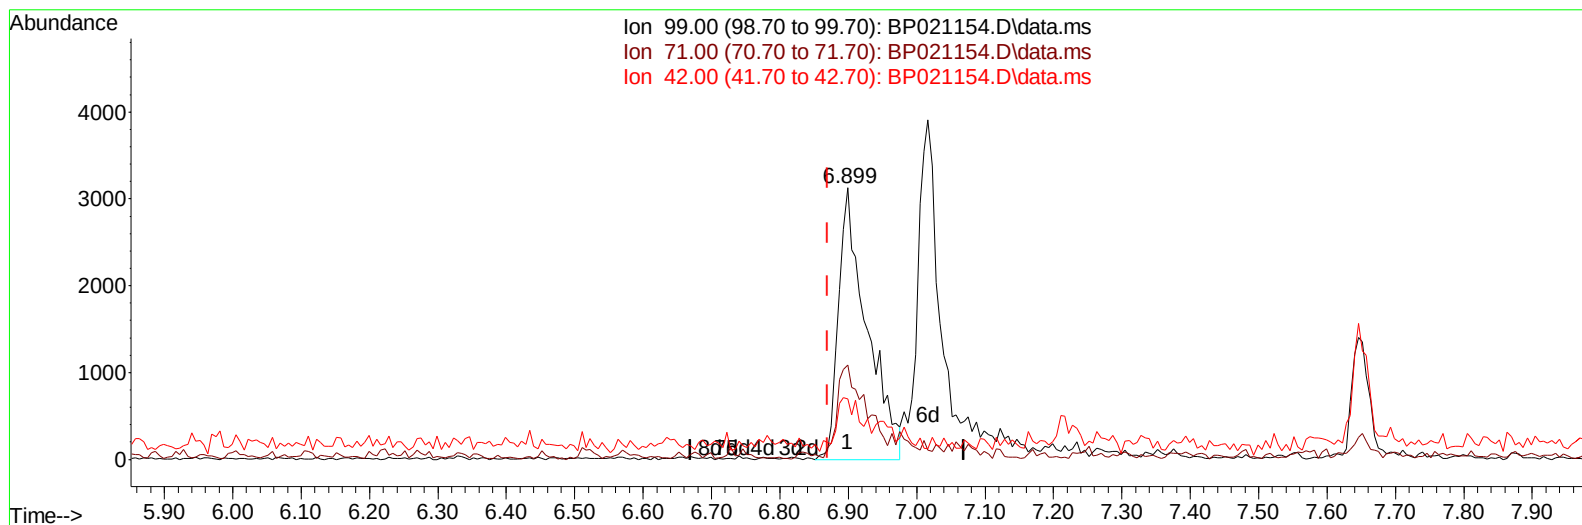

TIC: BP021154.D\data.ms

(7) Phenol-d5 (S)

6.899min (+ 0.029) 0.55 ng/ul m

response 8990

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	35.60	34.74
42.00	19.30	22.20
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

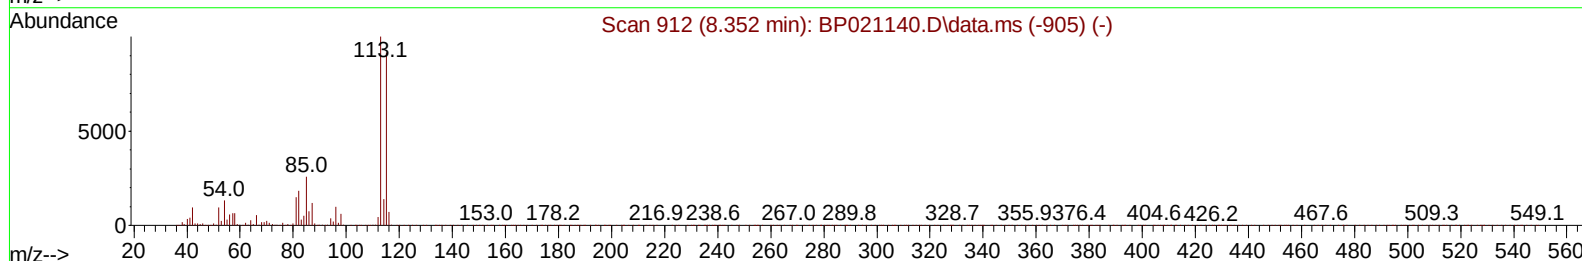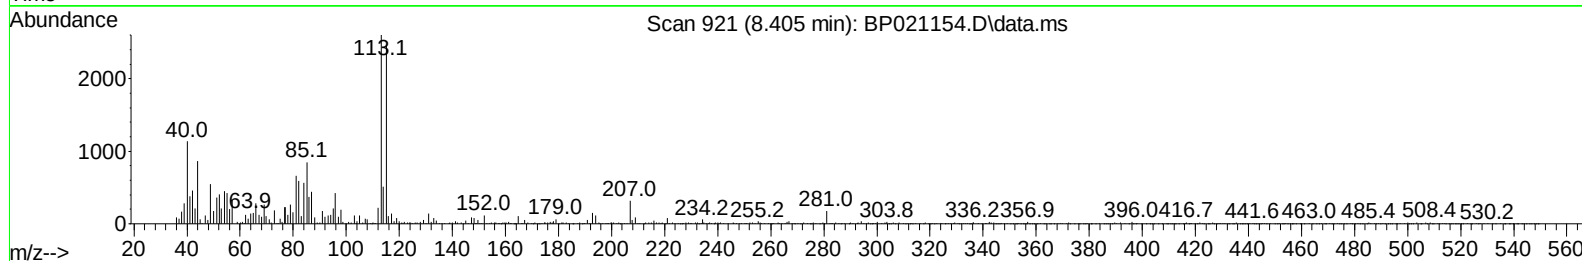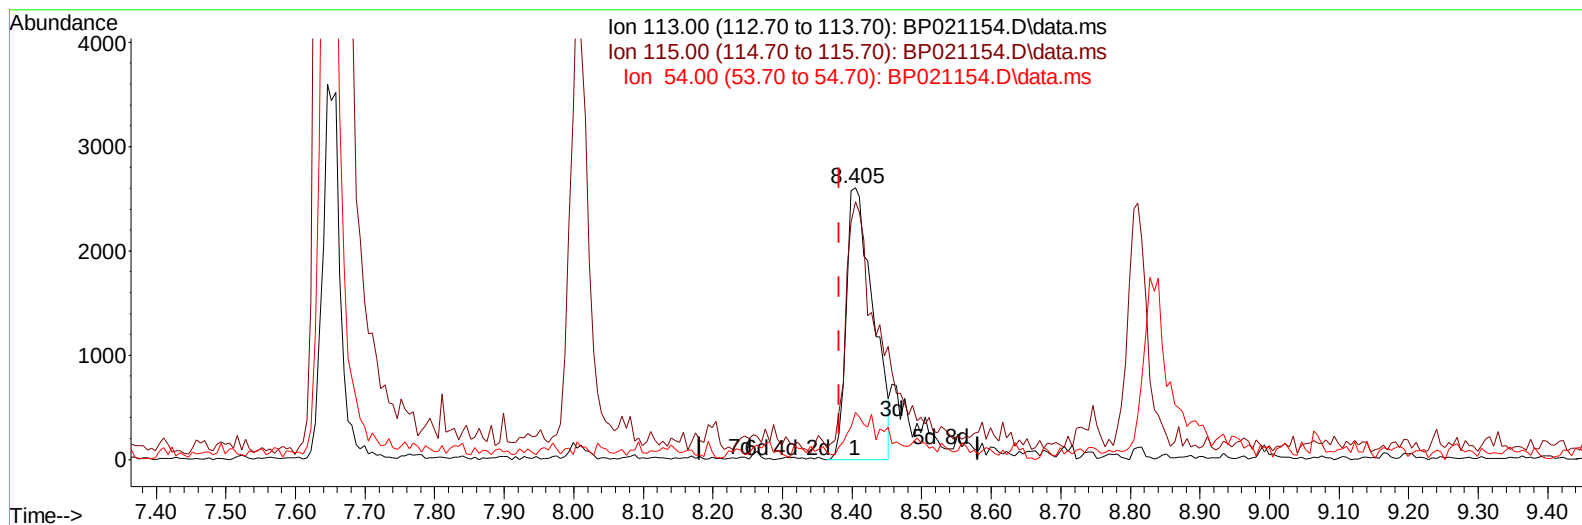

TIC: BP021154.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.405min (+ 0.024) 0.51 ng/uL

response 6918

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	95.01
54.00	13.70	17.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

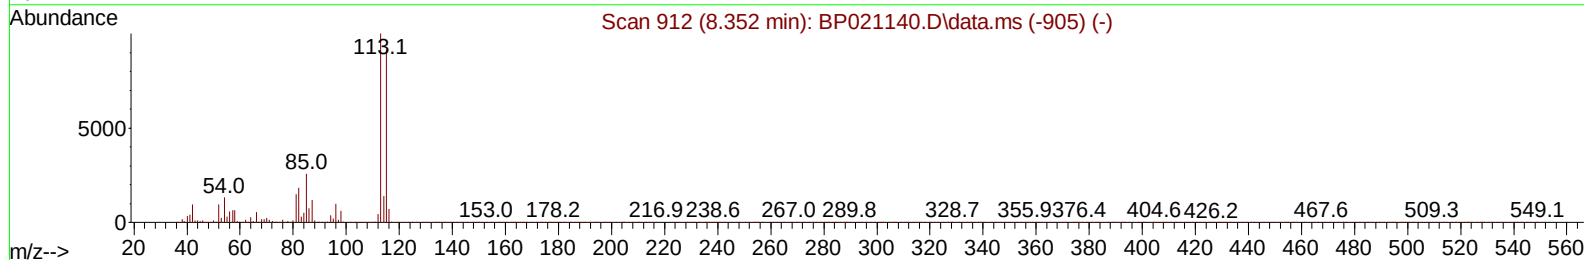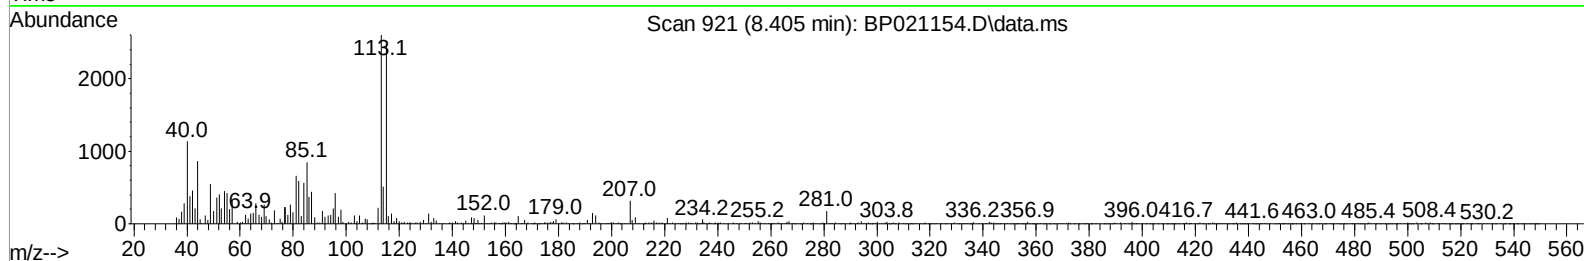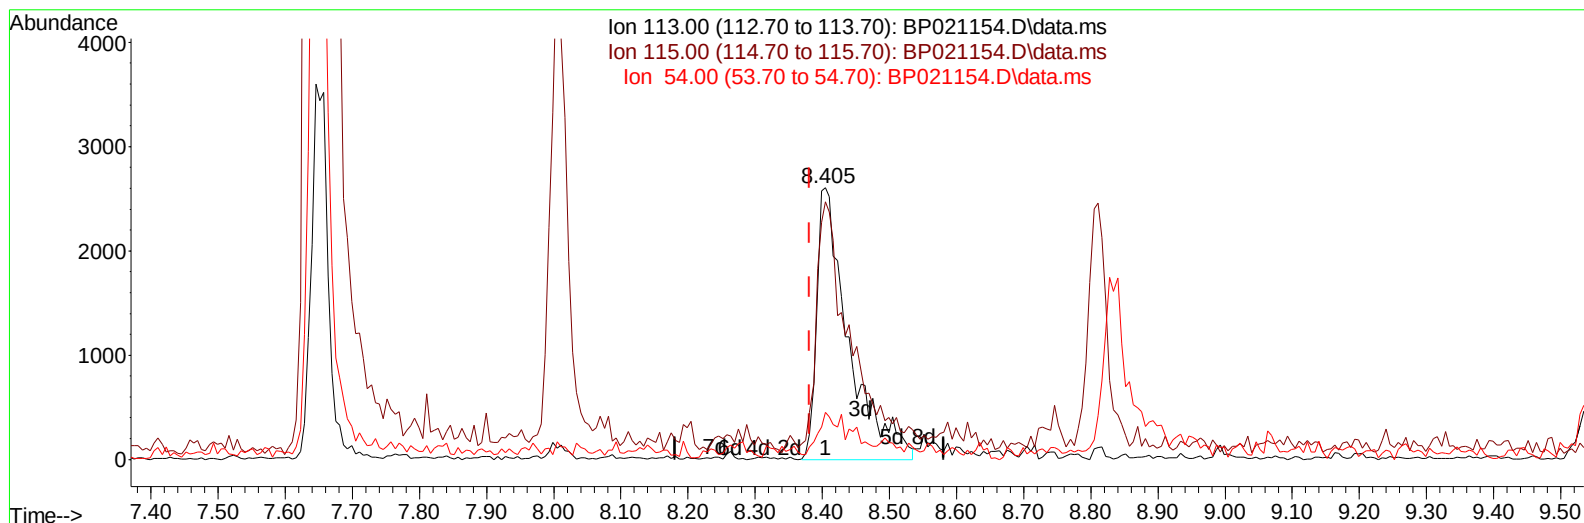

TIC: BP021154.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.405min (+ 0.024) 0.64 ng/ul m

response 8644

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	93.20	95.01
54.00	13.70	17.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

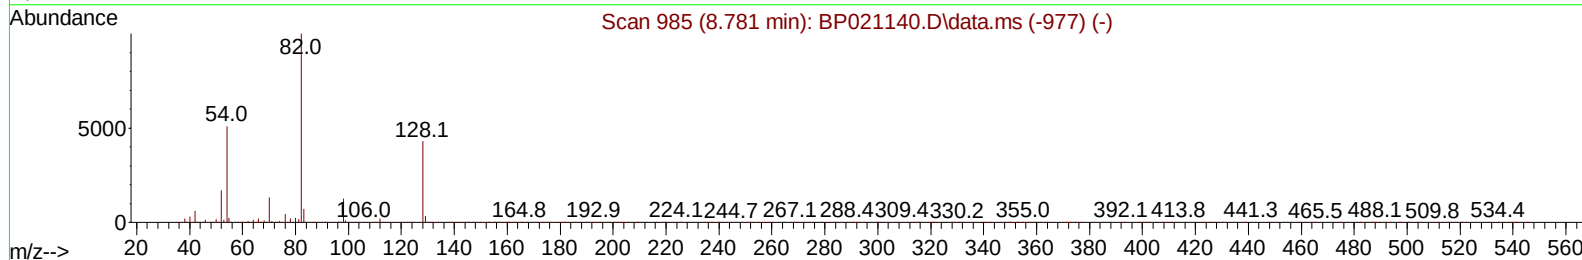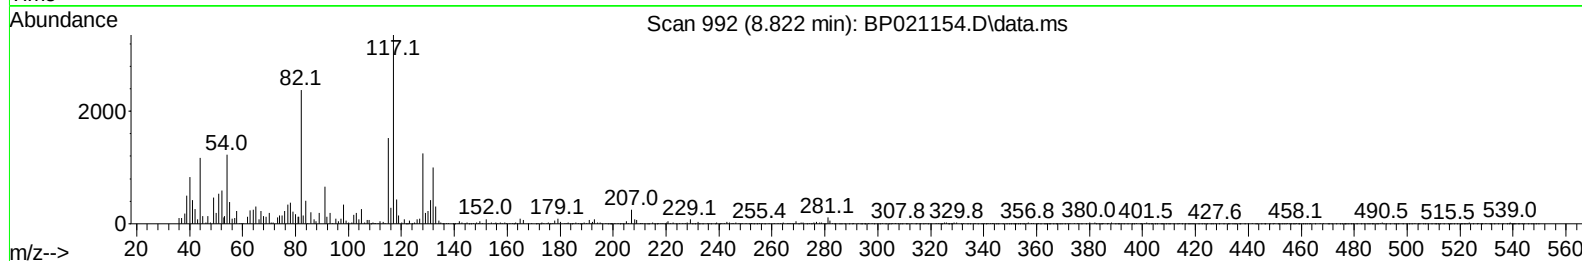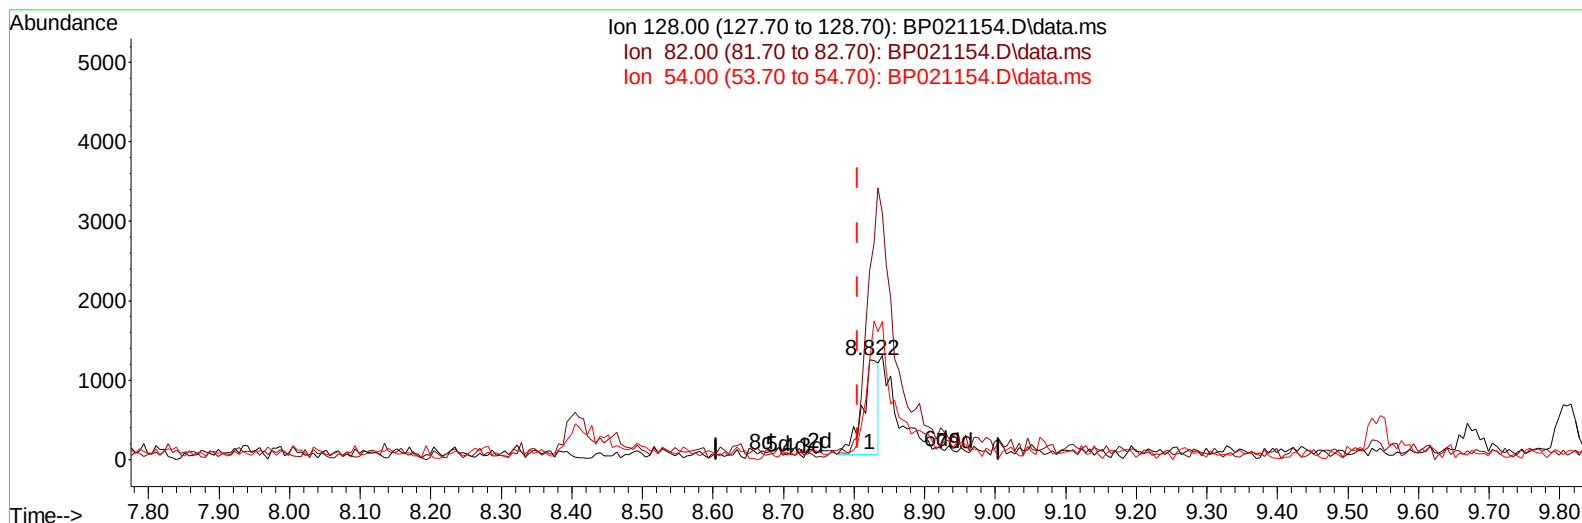

TIC: BP021154.D\data.ms

(21) Nitrobenzene-d5 (S)

8.822min (+ 0.018) 0.32 ng/uL

response 1952

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	190.01
54.00	125.70	98.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

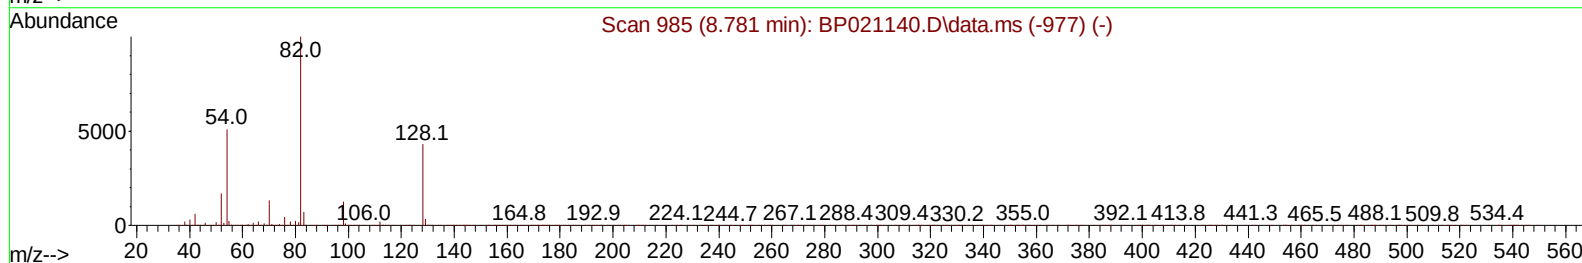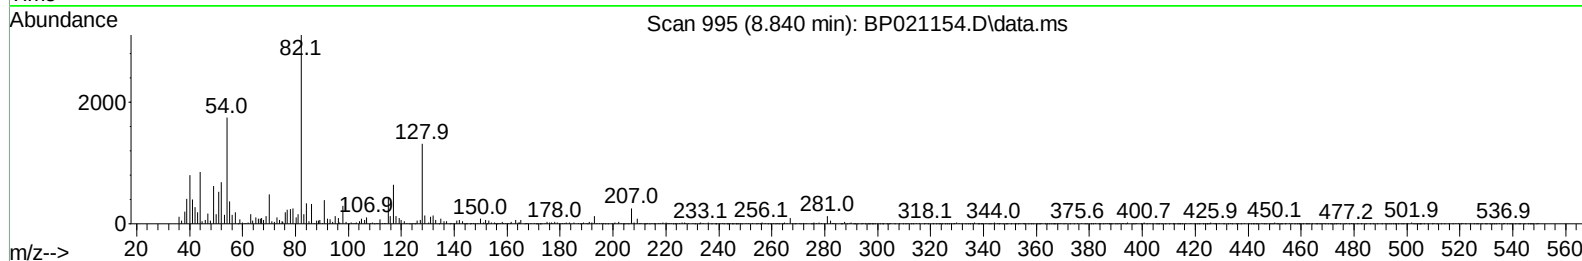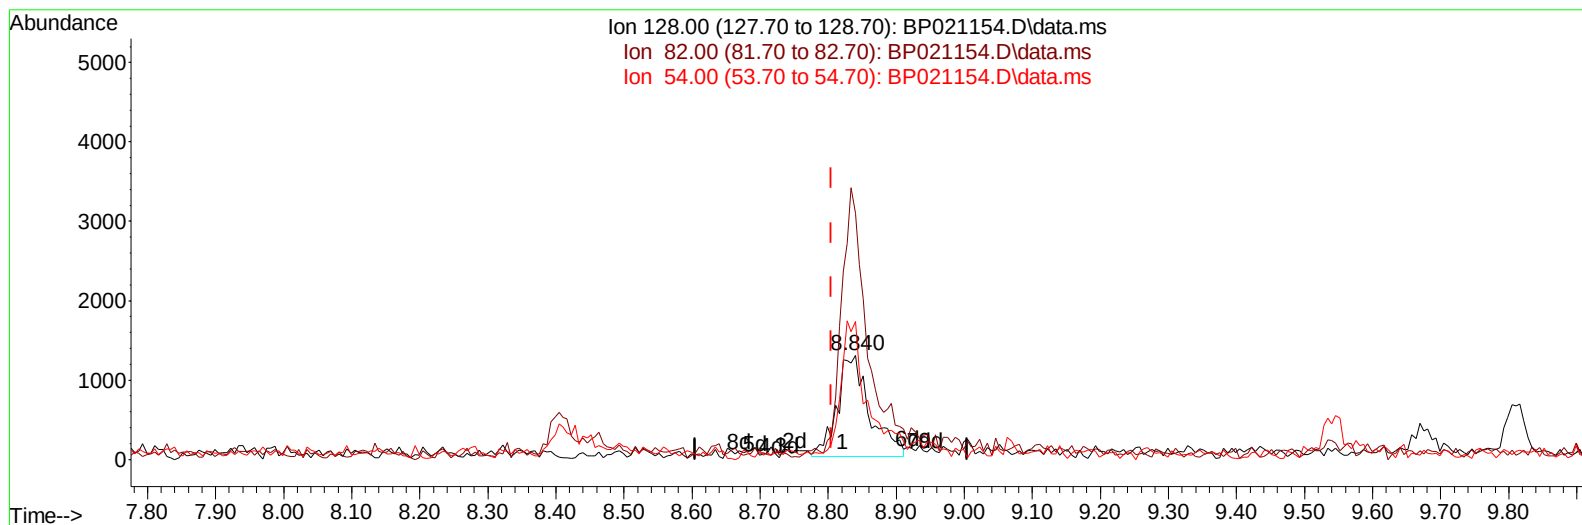

TIC: BP021154.D\data.ms

(21) Nitrobenzene-d5 (S)

8.840min (+ 0.035) 0.68 ng/ul m

response 4209

Ion	Exp%	Act%
128.00	100.00	100.00
82.00	236.60	236.15
54.00	125.70	132.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

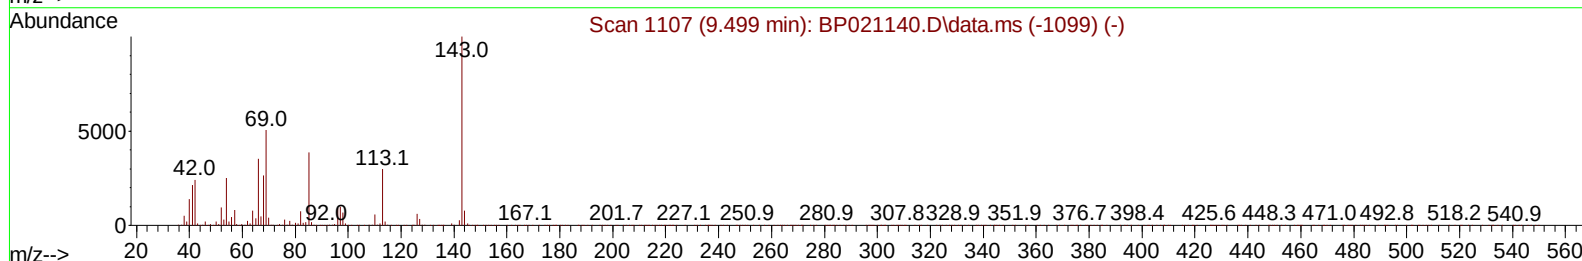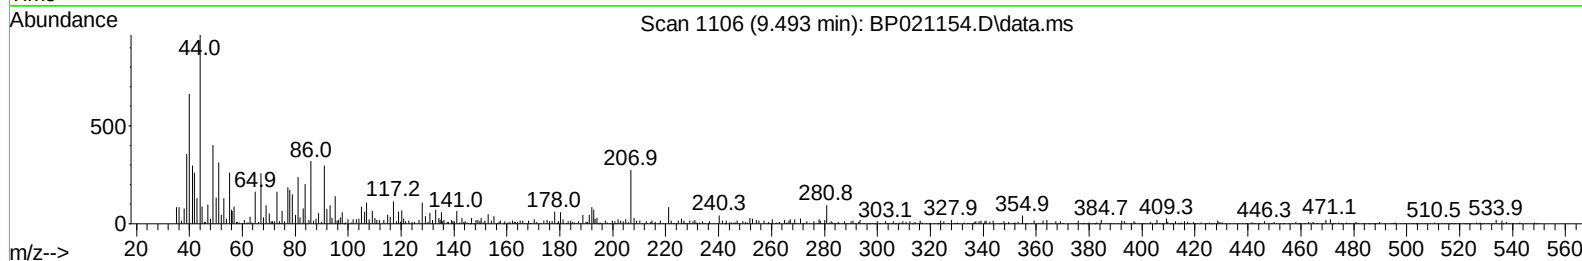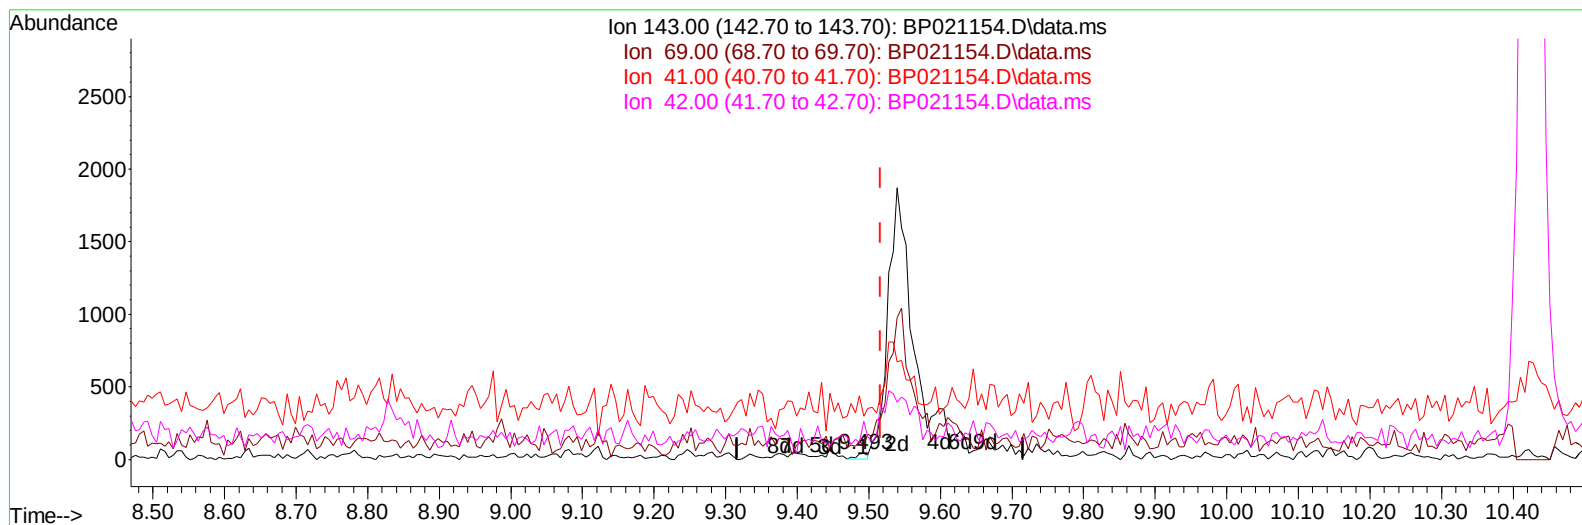

TIC: BP021154.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.493min (-0.024) 0.01 ng/ul

response 40

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	231.71#
41.00	22.70	724.39#
42.00	22.10	636.59#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

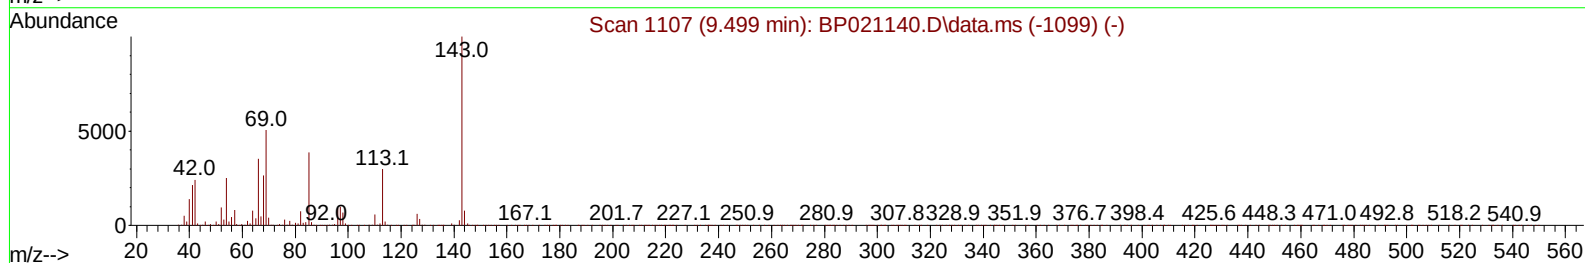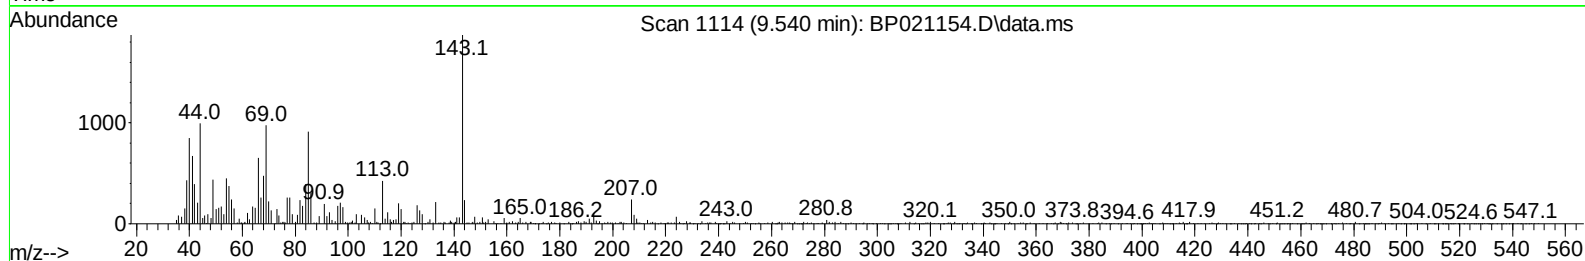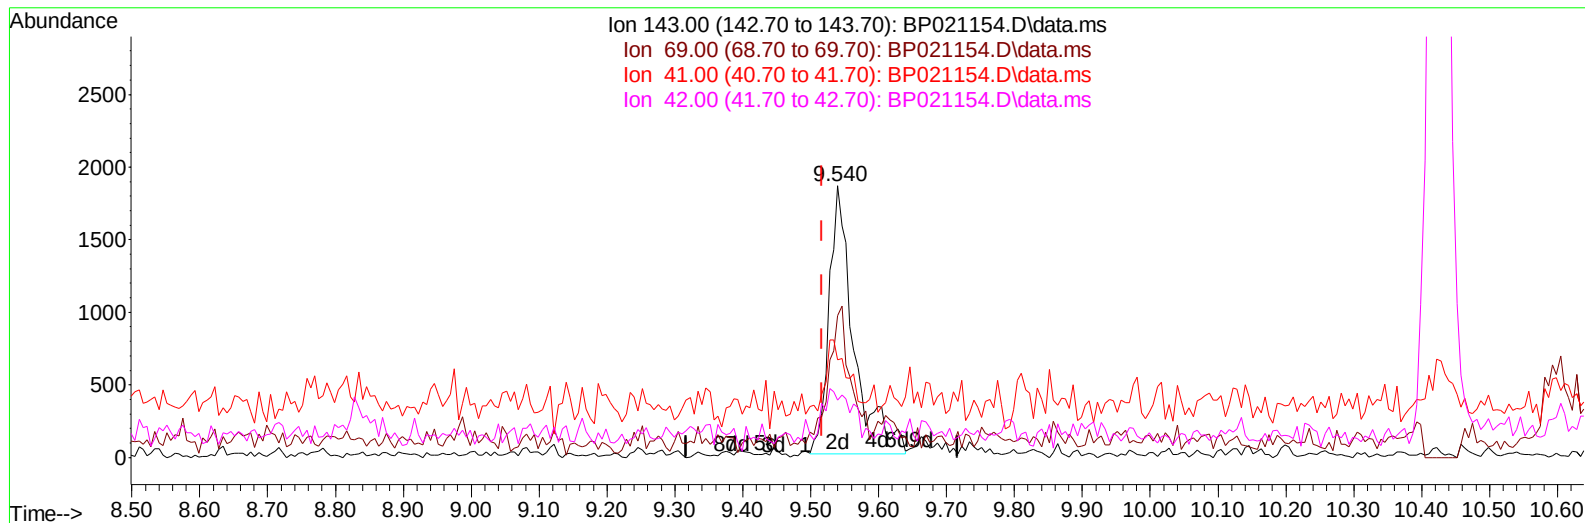

TIC: BP021154.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.540min (+ 0.024) 0.67 ng/ul m

response 4703

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	50.20	52.14
41.00	22.70	35.88#
42.00	22.10	21.07




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

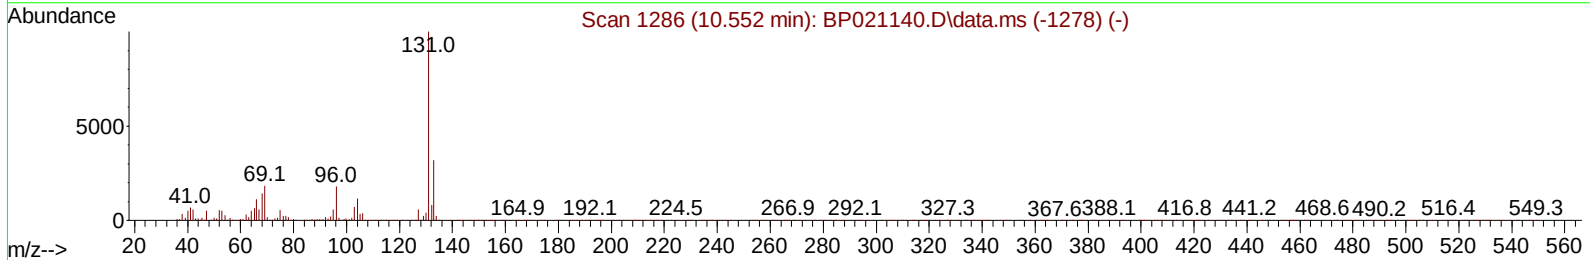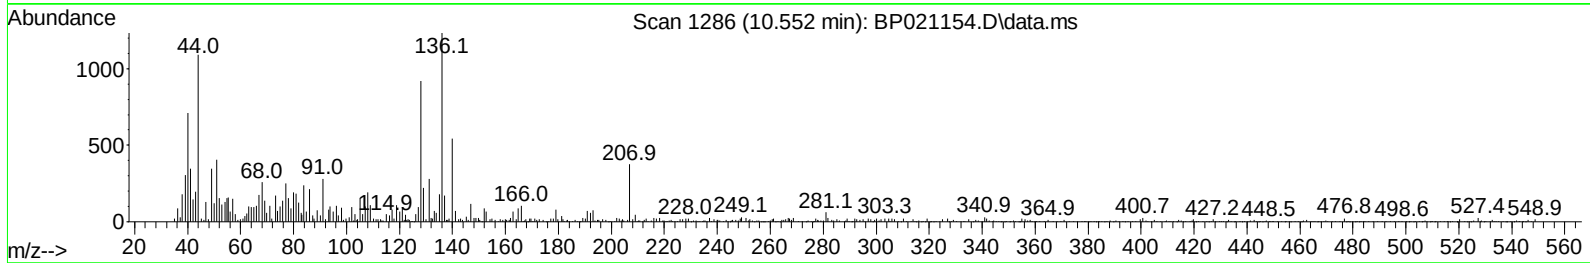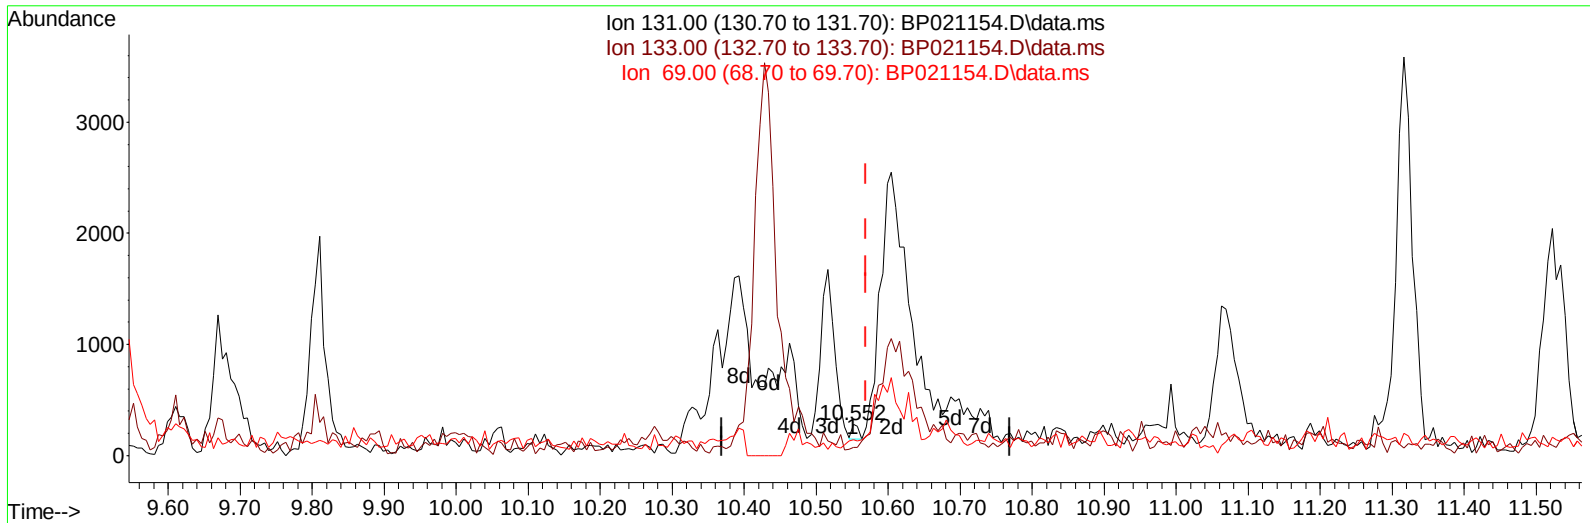

TIC: BP021154.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.552min (-0.018) 0.01 ng/ul

response 86

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	26.16
69.00	17.40	50.18#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

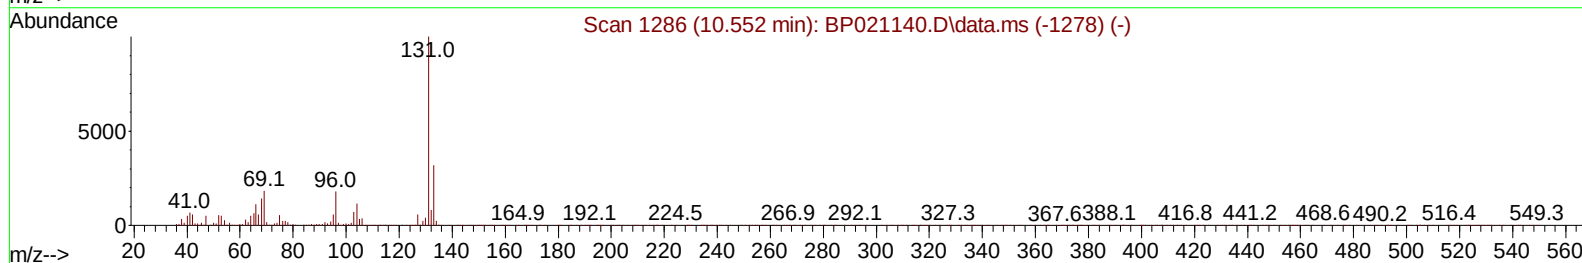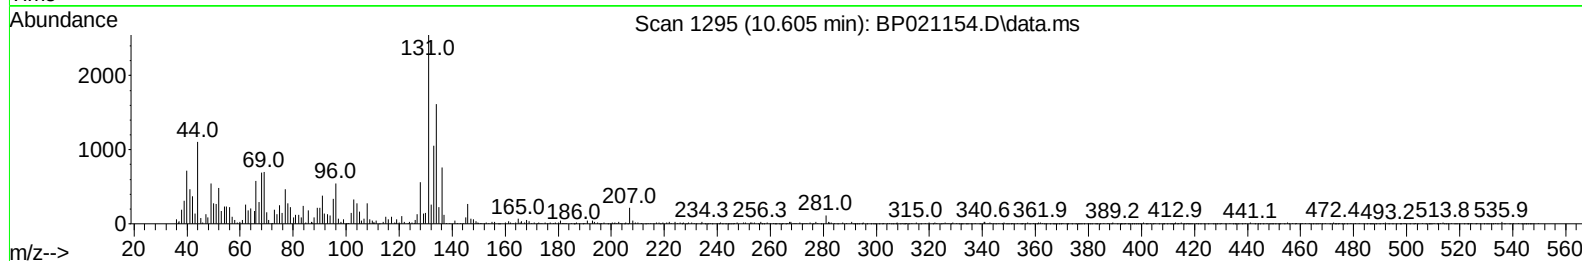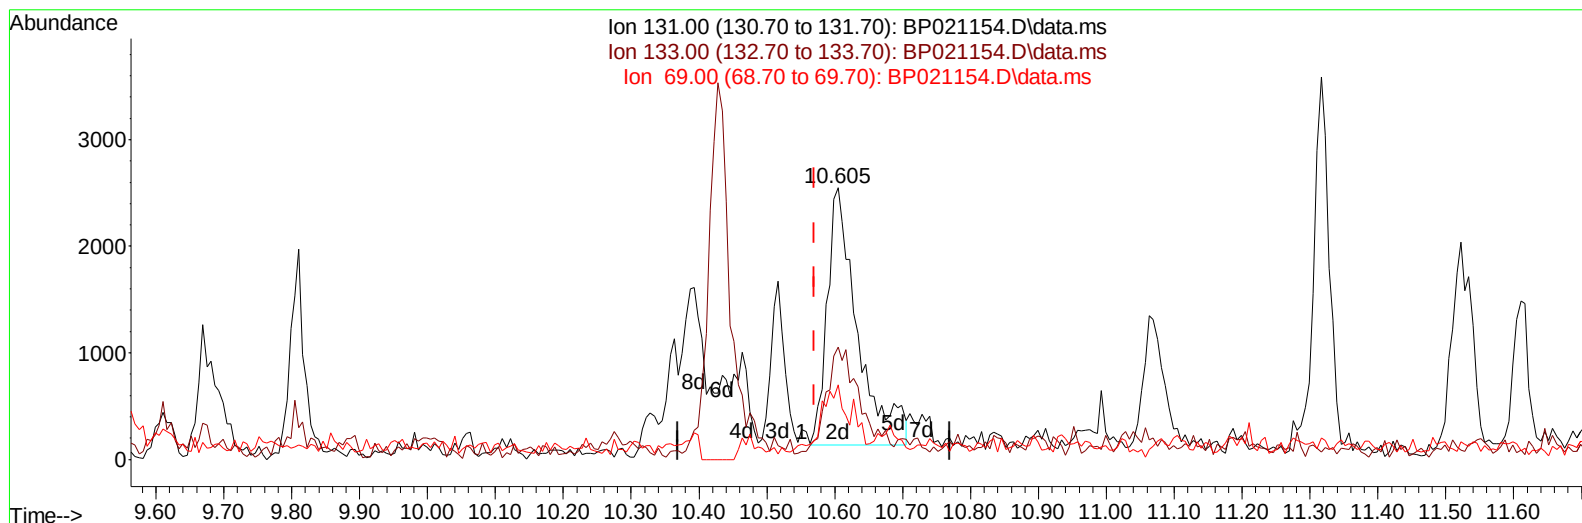

TIC: BP021154.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.605min (+ 0.035) 0.44 ng/ul m

response 7509

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.50	41.34#
69.00	17.40	27.40#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

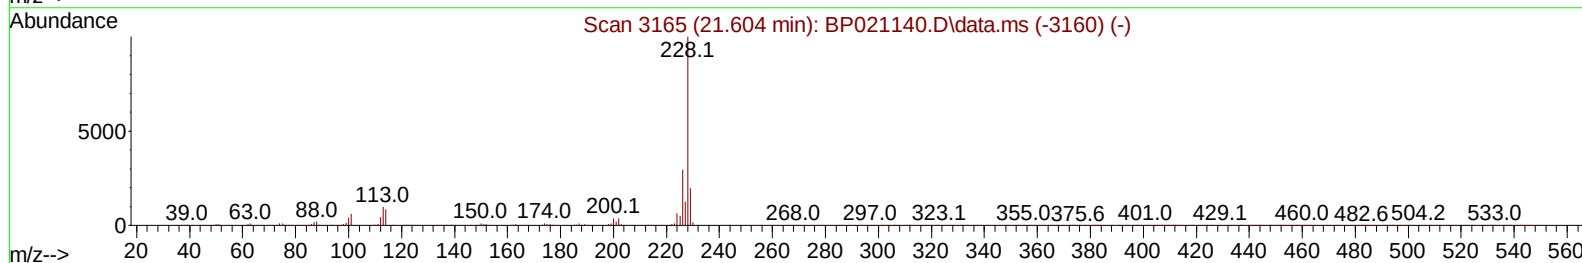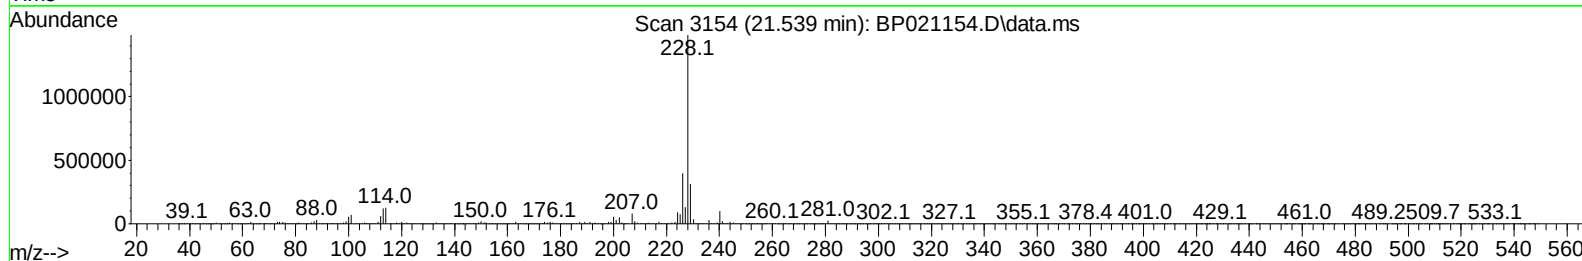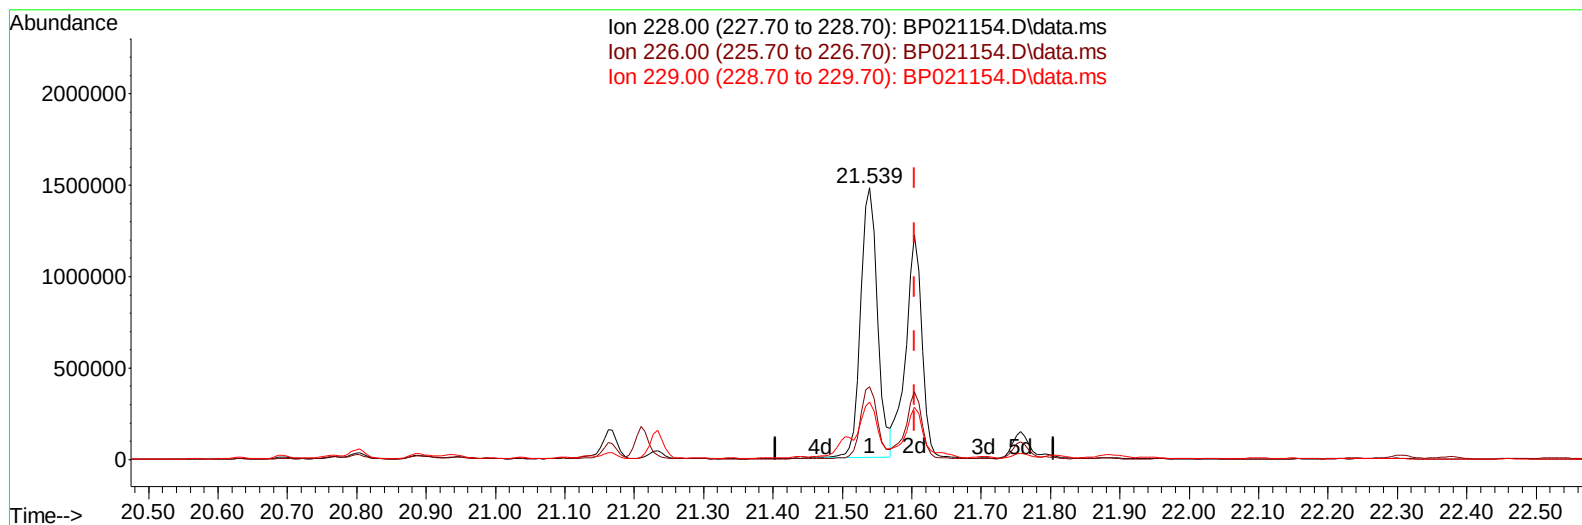

TIC: BP021154.D\data.ms

(87) Chrysene

21.539min (-0.065) 48.14 ng/u1

response 2489636

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.50	26.83
229.00	19.40	21.17
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

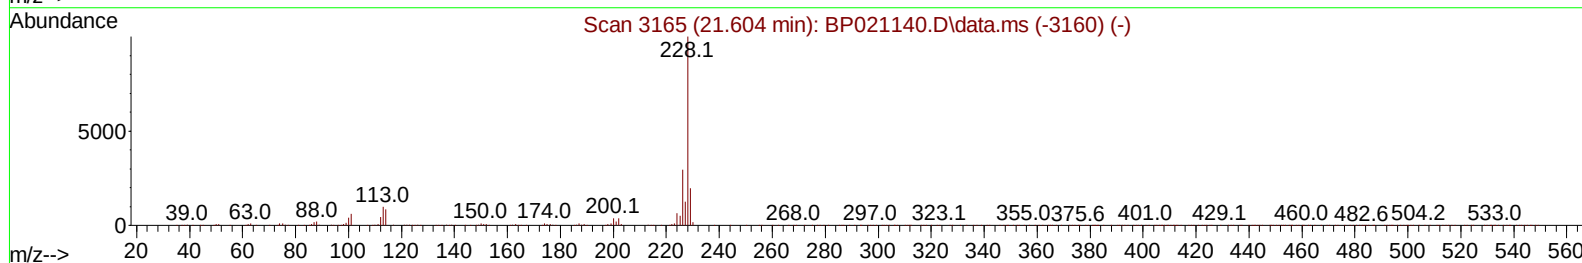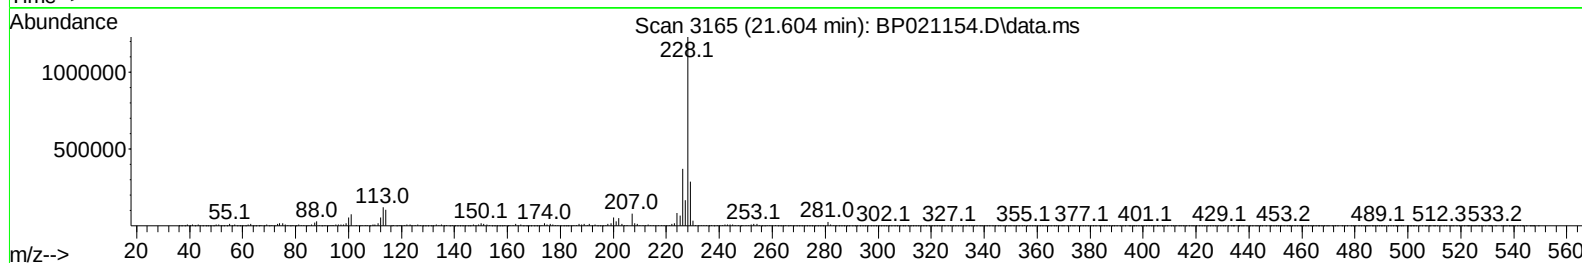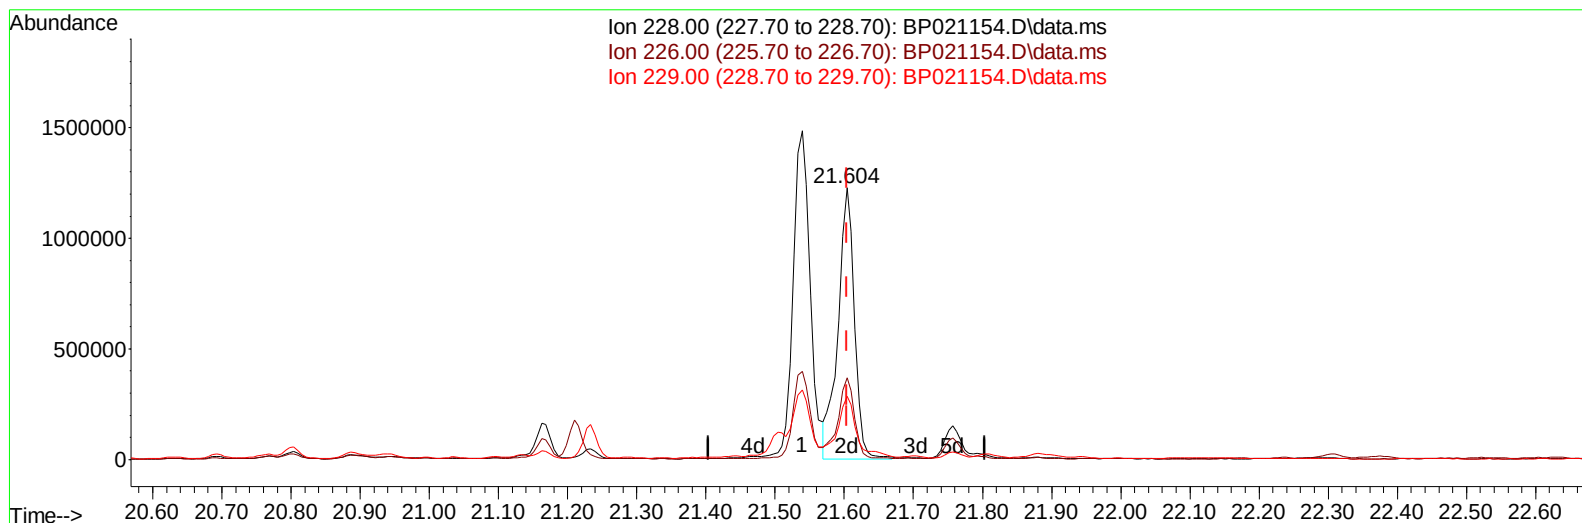

TIC: BP021154.D\data.ms

(87) Chrysene

21.604min (-0.000) 39.44 ng/ul m

response 2039765

Ion	Exp%	Act%
228.00	100.00	100.00
226.00	29.50	30.08
229.00	19.40	23.29#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

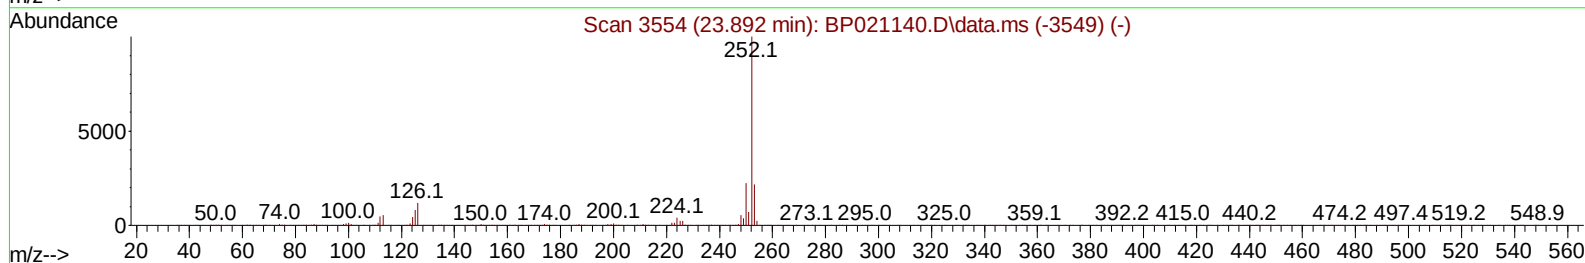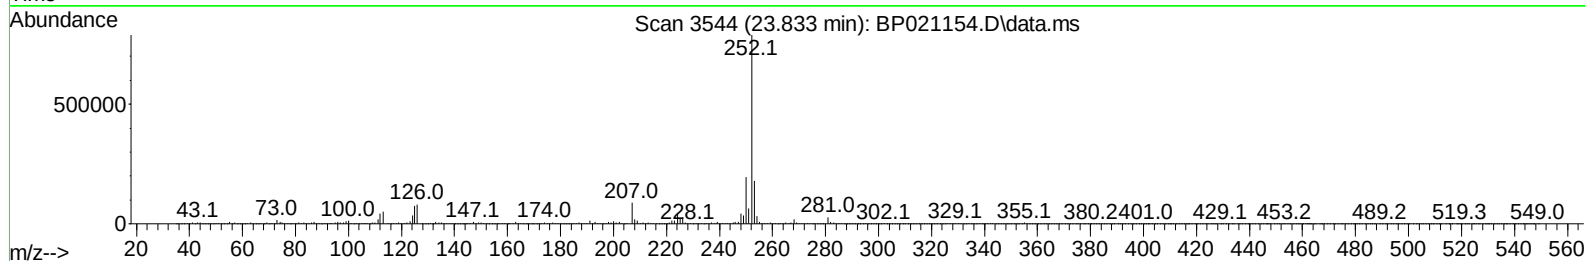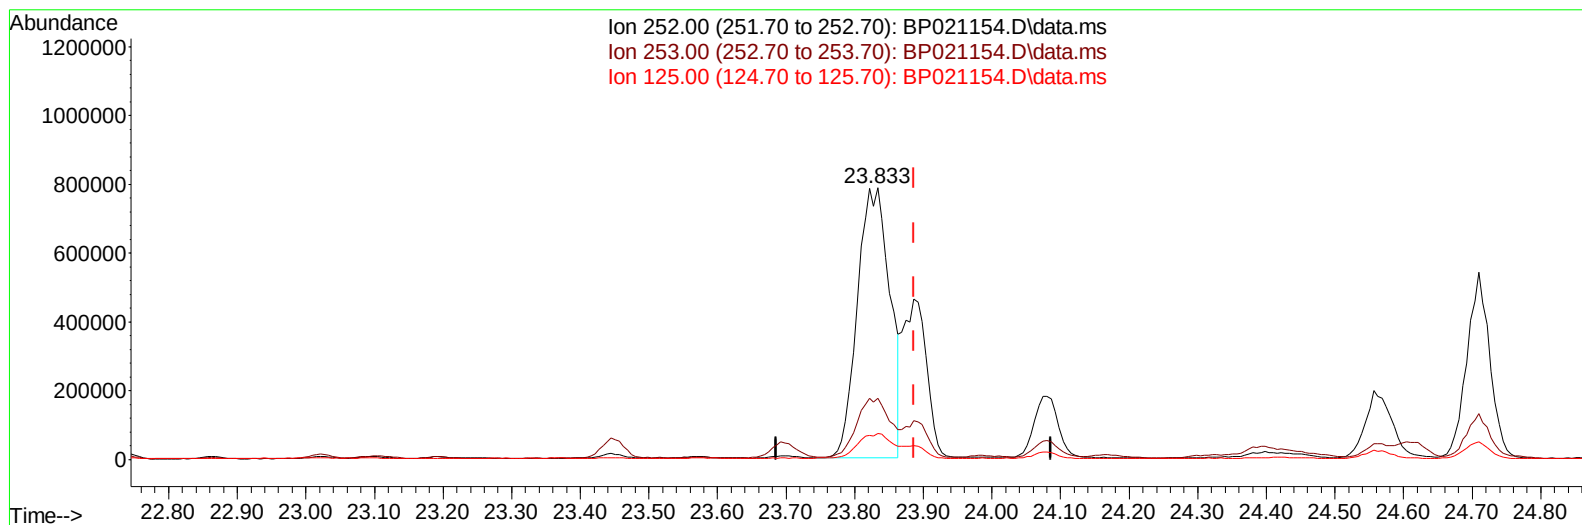

TIC: BP021154.D\data.ms

(91) Benzo(k)fluoranthene

23.833min (-0.053) 38.13 ng/u1

response 2579688

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	22.56
125.00	9.20	9.48
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

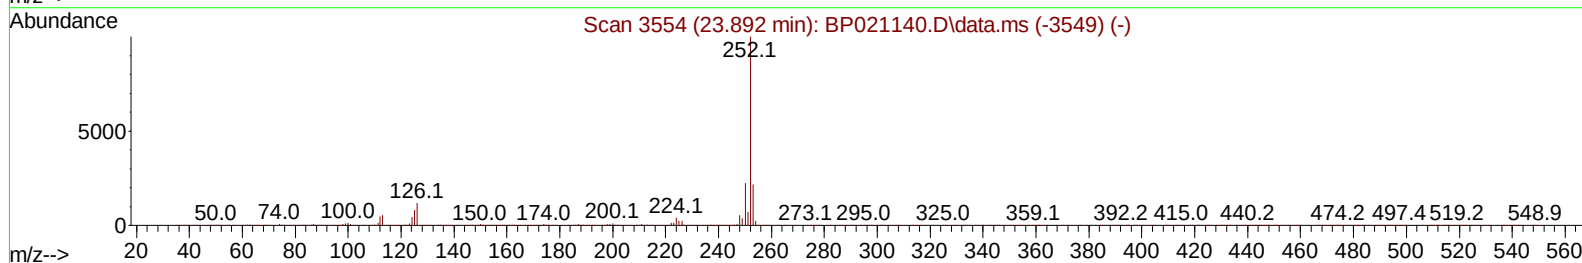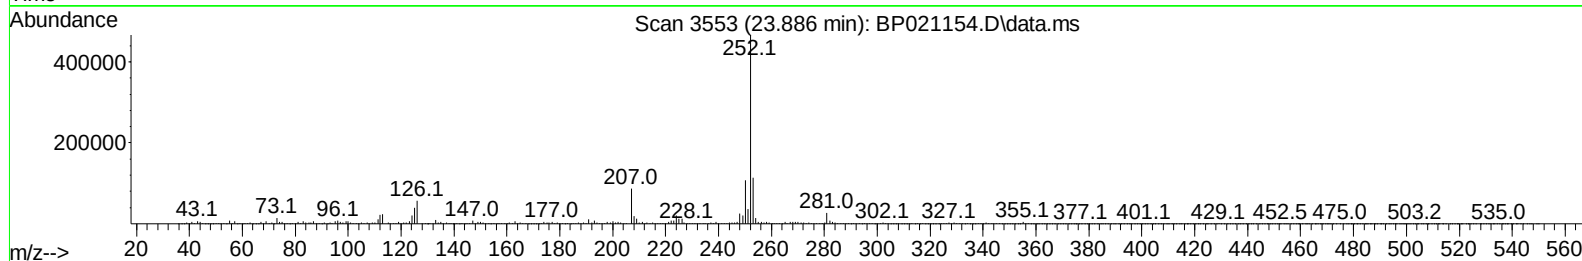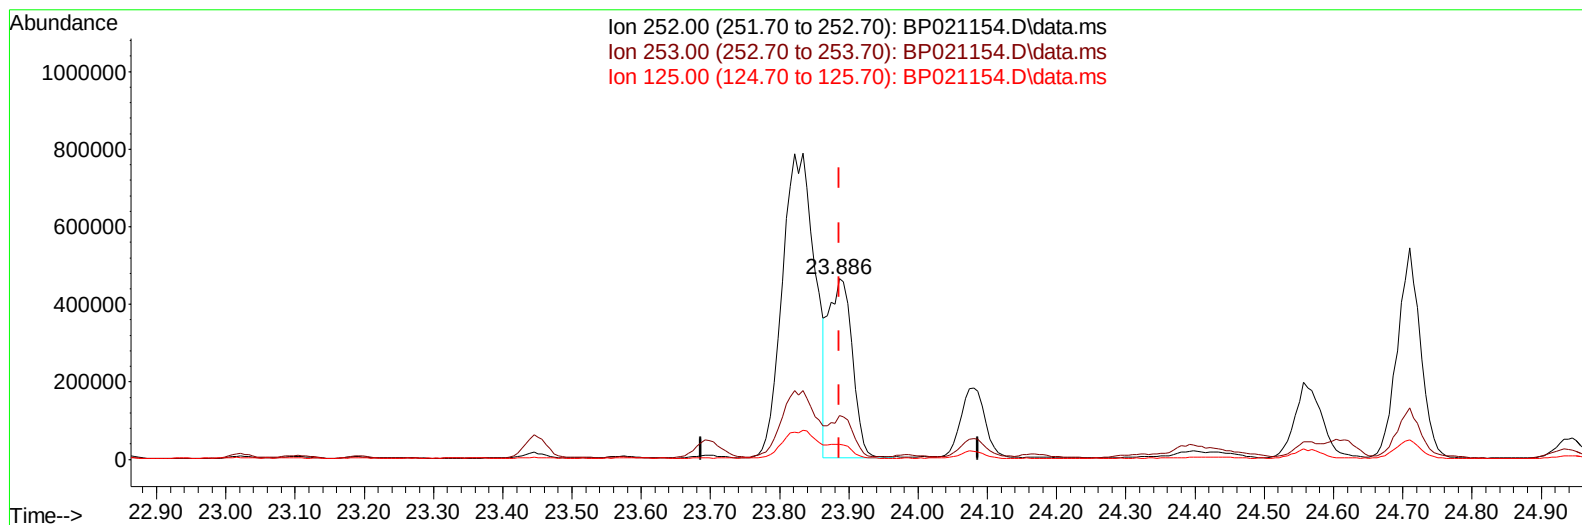

TIC: BP021154.D\data.ms

(91) Benzo(k)fluoranthene

23.886min (-0.000) 16.27 ng/ul m

response 1100942

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	21.80	24.36
125.00	9.20	8.52
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

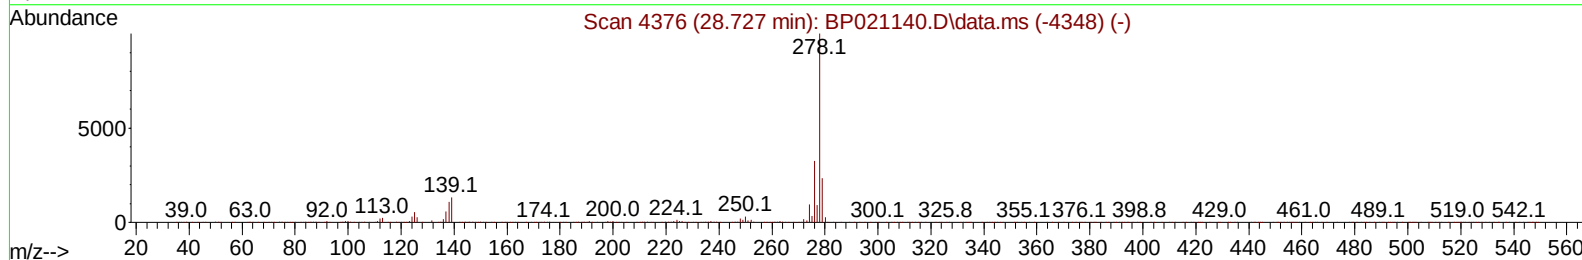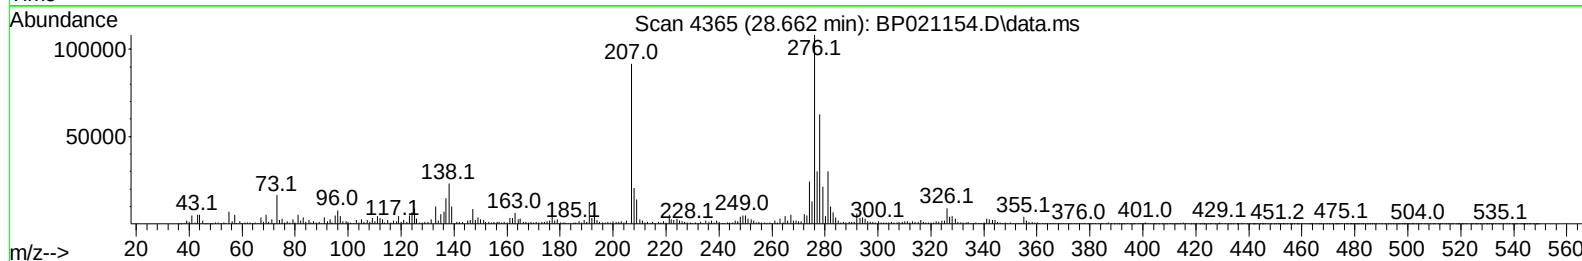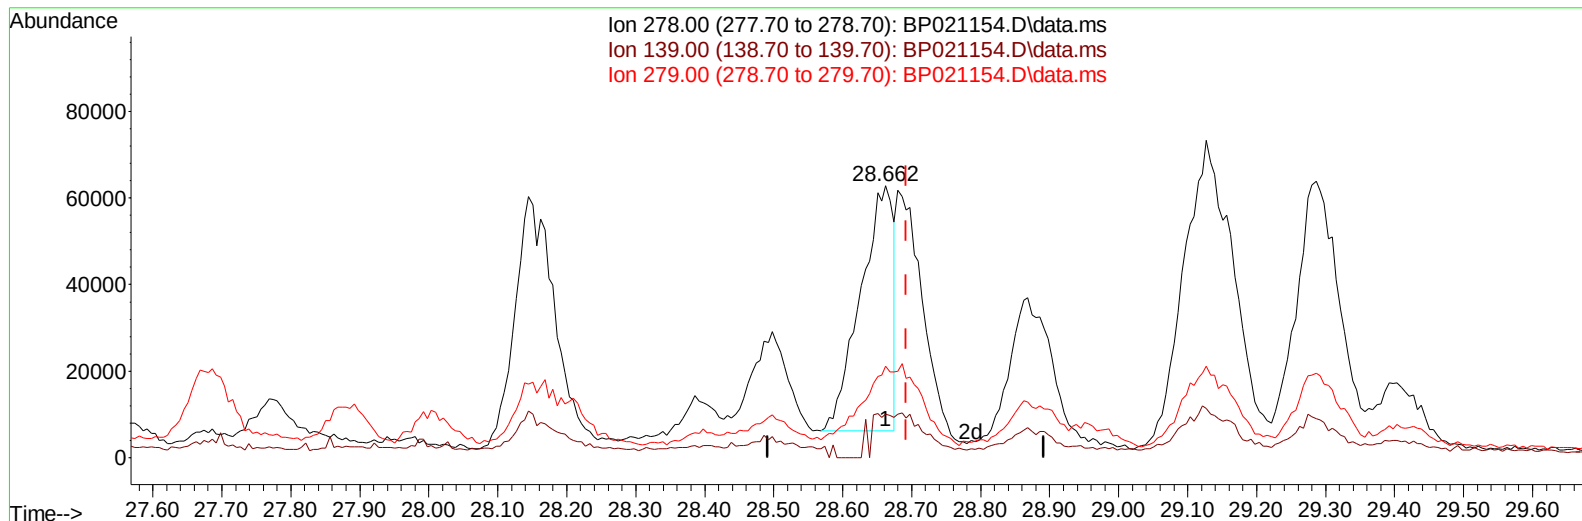

TIC: BP021154.D\data.ms

(95) Dibenzo(a,h)anthracene

28.662min (-0.029) 2.74 ng/u1

response 187181

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.60	15.85
279.00	24.20	33.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

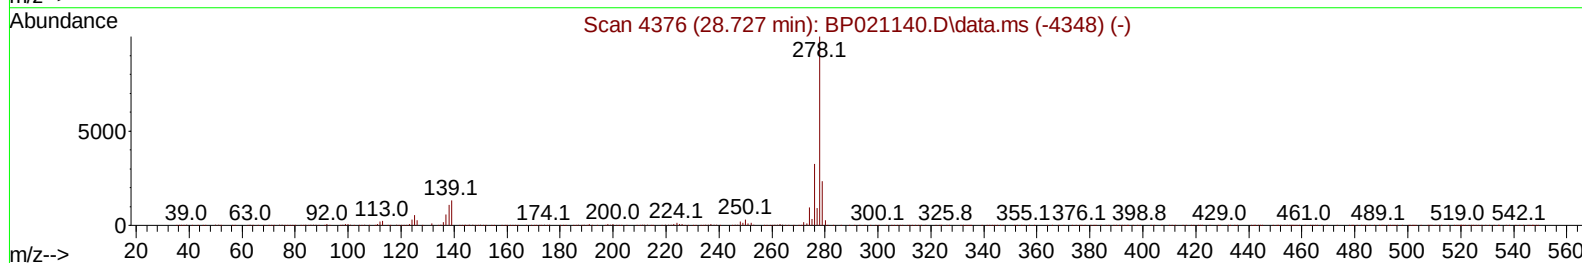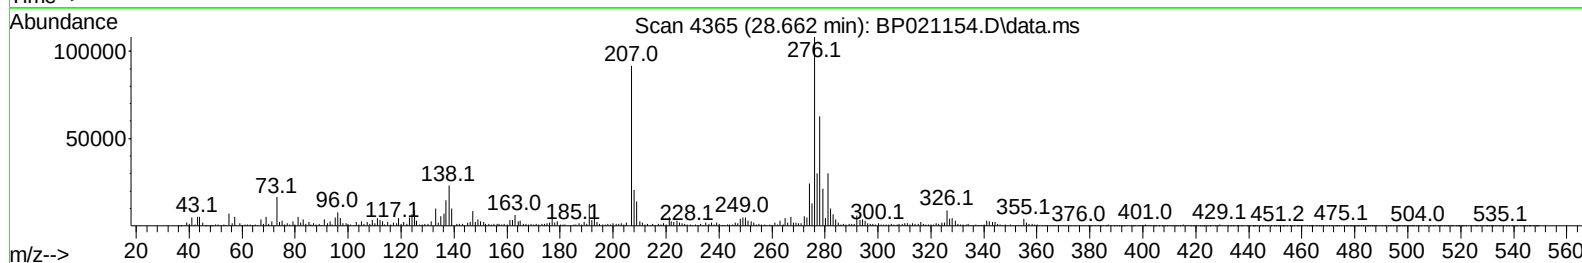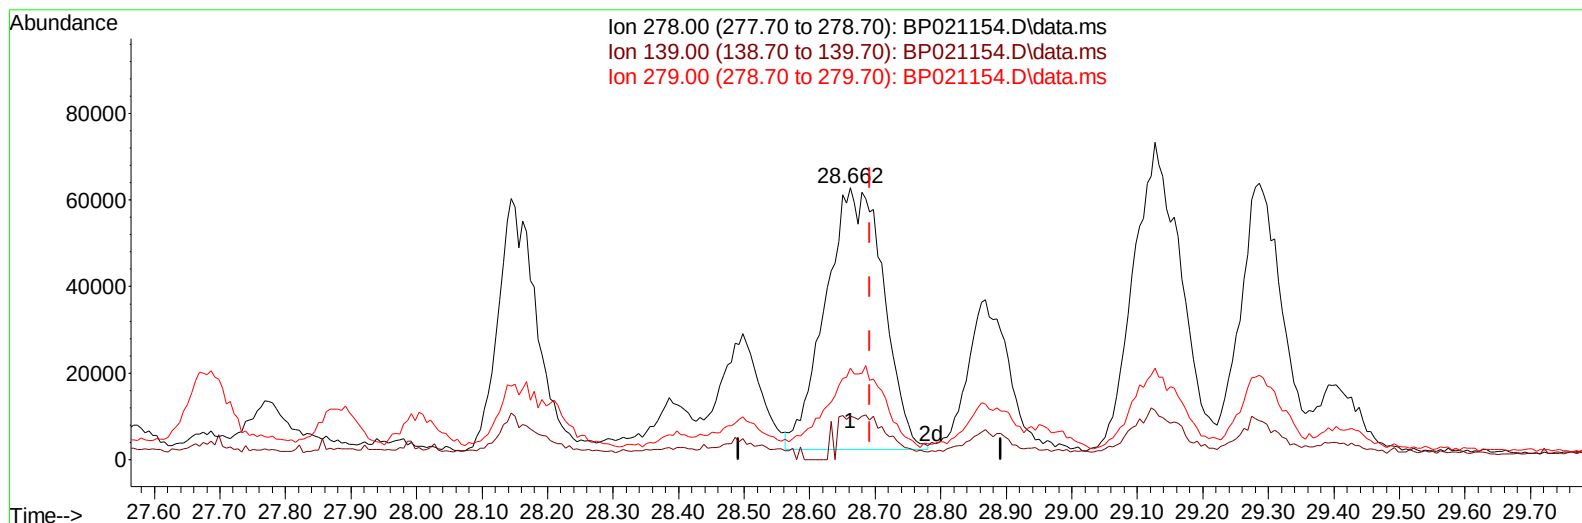

TIC: BP021154.D\data.ms

(95) Dibenzo(a,h)anthracene

28.662min (-0.029) 5.44 ng/ul m

response 372061

Ion	Exp%	Act%
278.00	100.00	100.00
139.00	13.60	15.85
279.00	24.20	33.60#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

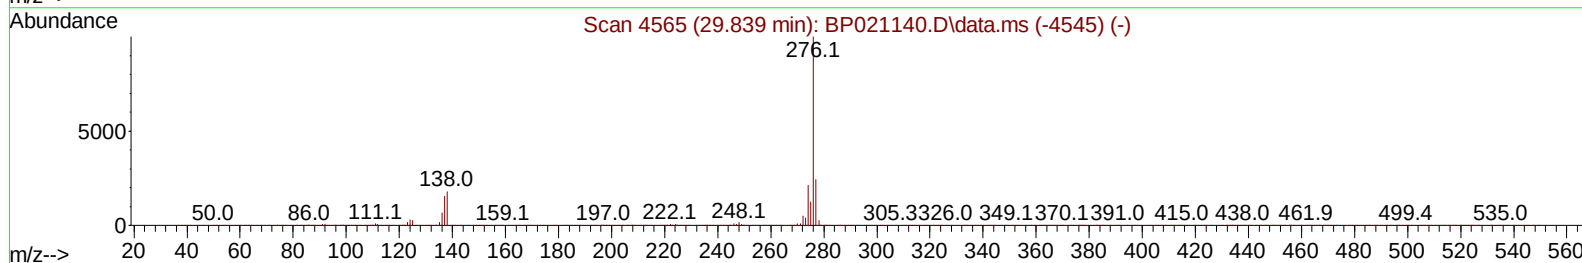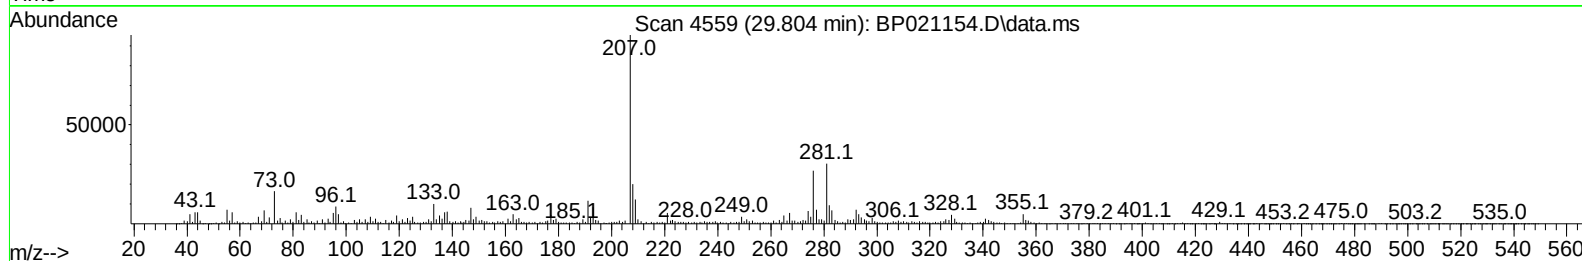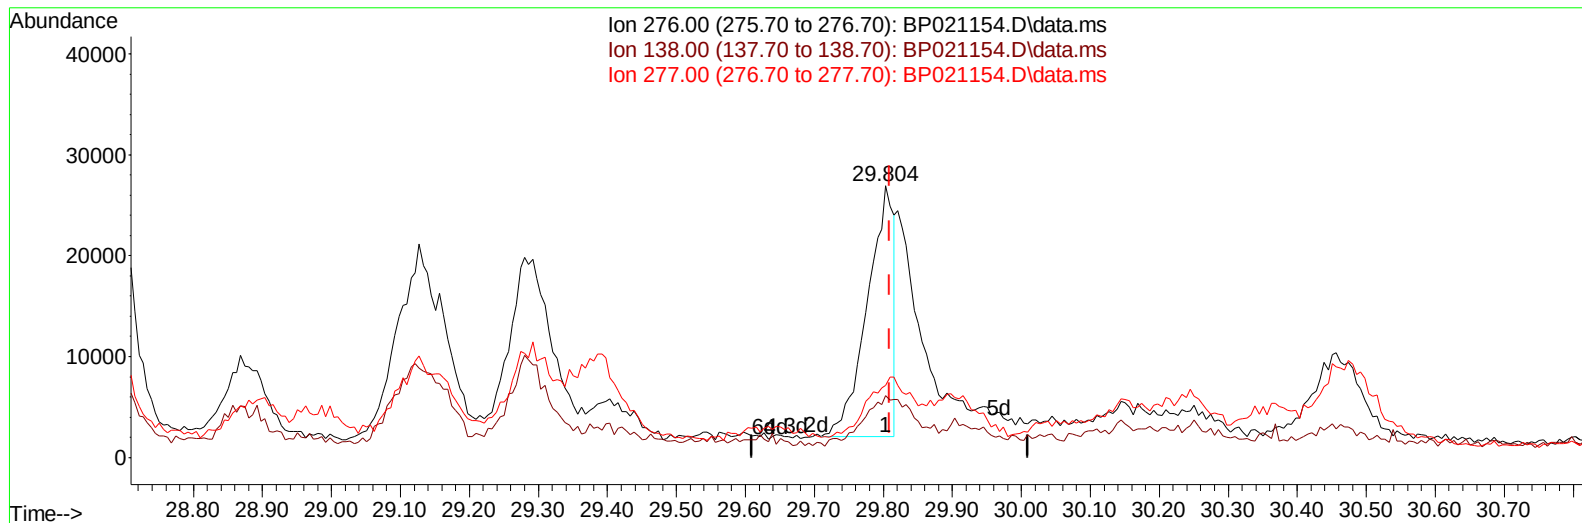

TIC: BP021154.D\data.ms

(96) Benzo(g,h,i)perylene

29.804min (-0.006) 0.99 ng/u1

response 66351

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	22.82
277.00	22.70	26.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 22:41:04 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

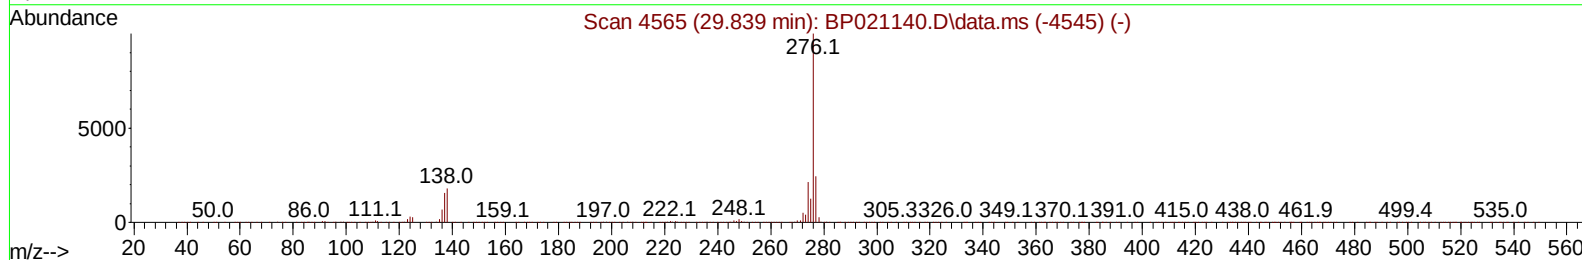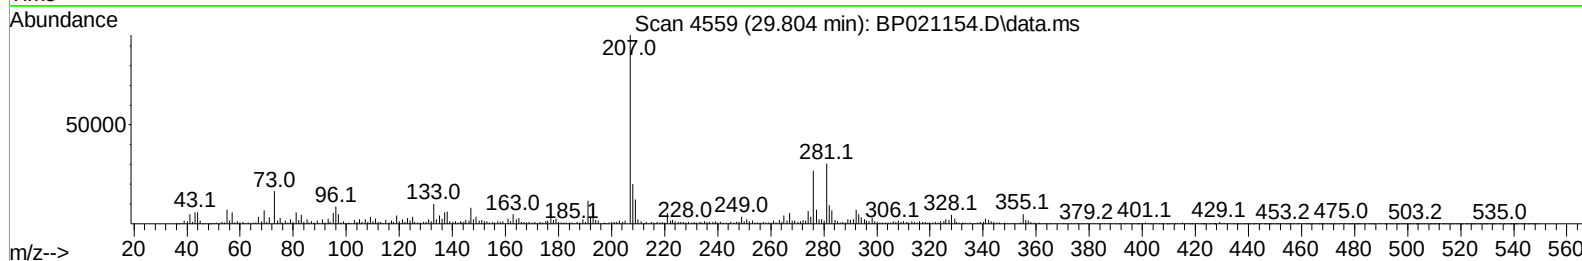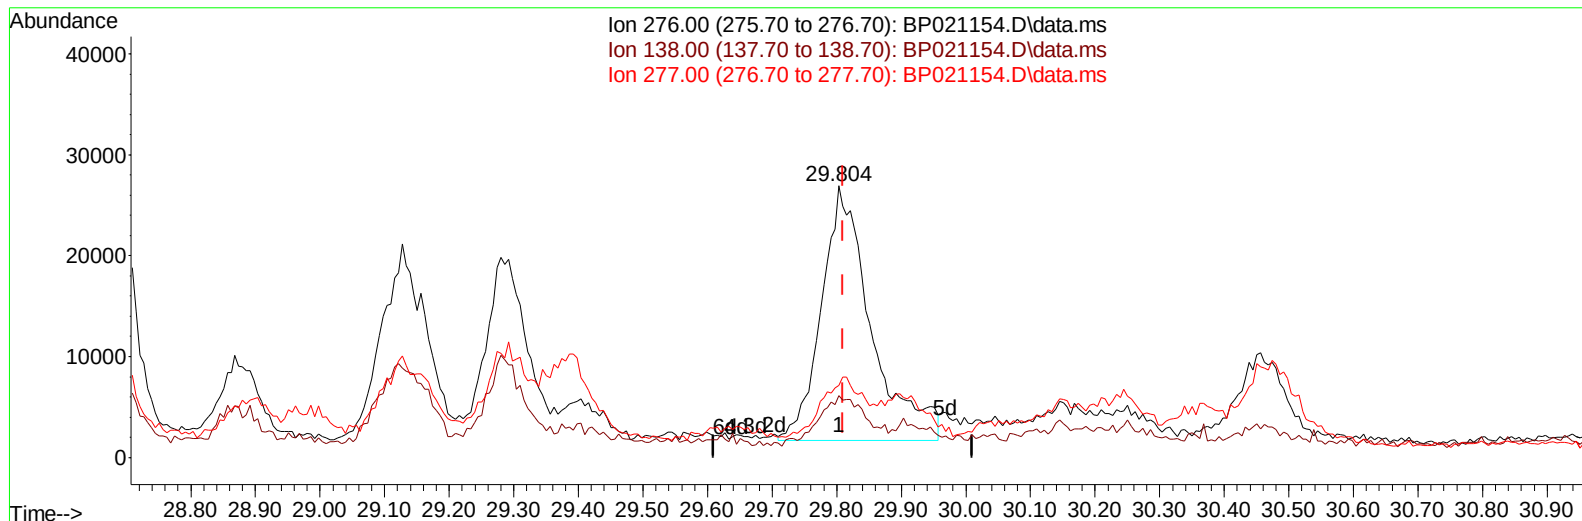

TIC: BP021154.D\data.ms

(96) Benzo(g,h,i)perylene

29.804min (-0.006) 2.00 ng/ul m

response 134153

Ion	Exp%	Act%
276.00	100.00	100.00
138.00	19.10	22.82
277.00	22.70	26.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021154.D
 Acq On : 25 Jul 2024 19:33
 Operator : MA/JU
 Sample : P3263-04DL 30X
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BA6DL

Manual IntegrationsAPPROVED

Quant Time: Jul 25 23:31:39 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jul 25 00:15:24 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/26/2024
 Supervised By :mohammad ahmed 07/27/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.652	152	199956	20.000	ng/ul	0.00
20) Naphthalene-d8	10.428	136	793644	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.293	164	492042	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.110	188	917240	20.000	ng/ul	0.00
79) Chrysene-d12	21.557	240	794578	20.000	ng/ul	0.00
88) Perylene-d12	24.863	264	1117061	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.899	99	8990m	0.551	ng/ul	0.03
9) Bis-(2-Chloroethyl)eth...	7.016	67	6351	0.643	ng/ul	0.02
11) 2-Chlorophenol-d4	7.216	132	8791	0.655	ng/ul	0.01
15) 4-Methylphenol-d8	8.405	113	8644m	0.638	ng/ul	0.02
21) Nitrobenzene-d5	8.840	128	4209m	0.683	ng/ul	0.04
24) 2-Nitrophenol-d4	9.540	143	4703m	0.667	ng/ul	0.02
28) 2,4-Dichlorophenol-d3	10.110	165	7961	0.624	ng/ul	0.04
31) 4-Chloroaniline-d4	10.605	131	7509m	0.444	ng/ul	0.04
46) Dimethylphthalate-d6	13.698	166	31001	0.867	ng/ul	0.00
49) Acenaphthylene-d8	13.987	160	33421	0.832	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.310	176	26721	0.911	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	17.210	188	37804	0.928	ng/ul	0.00
81) Pyrene-d10	19.592	212	35174	0.716	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.639	264	37138	0.674	ng/ul	-0.01
Target Compounds						
					Qvalue	
30) Naphthalene	10.475	128	341791	8.187	ng/ul	99
36) 2-Methylnaphthalene	12.087	142	232897	8.127	ng/ul	99
37) 1-Methylnaphthalene	12.310	142	157399	5.341	ng/ul	98
43) 1,1'-Biphenyl	13.110	154	65090	1.810	ng/ul	97
52) Acenaphthene	14.357	153	913275	30.259	ng/ul	99
56) Dibenzofuran	14.698	168	739712	17.897	ng/ul	97
61) Fluorene	15.363	166	1026866	30.446	ng/ul	100
72) Phenanthrene	17.157	178	6328625	133.002	ng/ul	99
74) Anthracene	17.245	178	2061264	42.493	ng/ul	100
77) Carbazole	17.545	167	708416	17.865	ng/ul	99
80) Fluoranthene	19.245	202	5144867	86.724	ng/ul	100
82) Pyrene	19.622	202	3404766	56.400	ng/ul	100
85) Benzo(a)anthracene	21.539	228	2521547	45.302	ng/ul	98
87) Chrysene	21.604	228	2039765m	39.438	ng/ul	
90) Benzo(b)fluoranthene	23.833	252	2579688	38.055	ng/ul	98
91) Benzo(k)fluoranthene	23.886	252	1100942m	16.274	ng/ul	
93) Benzo(a)pyrene	24.710	252	1262223	19.704	ng/ul	96
94) Indeno(1,2,3-cd)pyrene	28.627	276	931412	11.284	ng/ul	98
95) Dibenzo(a,h)anthracene	28.662	278	372061m	5.443	ng/ul	
96) Benzo(g,h,i)perylene	29.804	276	134153m	1.996	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

BNA_P

ClientSampleId :

A4BA6DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021154.D
Acq On : 25 Jul 2024 19:33
Operator : MA/JU
Sample : P3263-04DL 30X
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BA6DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/26/2024
Supervised By :mohammad ahmed 07/27/2024

Quant Time: Jul 25 23:31:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jul 25 00:15:24 2024
Response via : Initial Calibration

