

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021141.D
 Acq On : 25 Jul 2024 10:18
 Operator : MA/JU
 Sample : PB162100BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK100

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021141.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	27	30	41	rVB	56508	79707	1.87%	0.168%
2	3.581	98	101	118	rBV	536028	853537	20.03%	1.796%
3	3.887	149	153	158	rVB	13545	20577	0.48%	0.043%
4	6.746	636	639	645	rVB8	2531	4278	0.10%	0.009%
5	6.846	649	656	674	rBV	675038	1299463	30.50%	2.734%
6	6.987	674	680	697	rVB	641476	1005899	23.61%	2.117%
7	7.187	706	714	730	rBV	752459	1336039	31.36%	2.811%
8	7.640	782	791	803	rBV	870655	1380978	32.41%	2.906%
9	8.363	906	914	935	rBV	725898	1602038	37.60%	3.371%
10	8.799	978	988	1000	rBV	744432	1258657	29.54%	2.648%
11	9.510	1102	1109	1125	rBV	612569	1101589	25.86%	2.318%
12	9.781	1151	1155	1160	rVB7	2468	4333	0.10%	0.009%
13	10.057	1195	1202	1224	rBV	729421	1613419	37.87%	3.395%
14	10.405	1253	1261	1272	rBV	1121198	1862960	43.73%	3.920%
15	10.569	1281	1289	1314	rBV	690301	1506888	35.37%	3.171%
16	12.022	1530	1536	1545	rBV6	7753	24601	0.58%	0.052%
17	13.257	1739	1746	1749	rBV8	4054	6769	0.16%	0.014%
18	13.704	1812	1822	1834	rBV	1279875	2227905	52.29%	4.688%
19	13.787	1834	1836	1845	rVB7	5593	8089	0.19%	0.017%
20	13.975	1861	1868	1883	rBV	1692897	2731853	64.12%	5.748%
21	14.287	1914	1921	1938	rBV	1487507	2429763	57.03%	5.112%
22	14.593	1965	1973	1980	rBV2	239652	640045	15.02%	1.347%
23	14.963	2033	2036	2042	rVB8	2565	4644	0.11%	0.010%
24	15.298	2086	2093	2115	rBV	1912839	3343082	78.47%	7.034%
25	15.469	2115	2122	2134	rBV	580406	945610	22.20%	1.990%
26	15.834	2180	2184	2188	rVB6	4868	6844	0.16%	0.014%
27	16.104	2223	2230	2235	rBV7	7118	13094	0.31%	0.028%
28	16.892	2360	2364	2368	rBV4	5263	8585	0.20%	0.018%
29	17.104	2394	2400	2411	rBV	2008934	2859945	67.13%	6.018%
30	17.210	2411	2418	2436	rVV	2142997	3631805	85.25%	7.642%
31	19.145	2742	2747	2753	rVB6	28593	47654	1.12%	0.100%
32	19.222	2757	2760	2765	rVV	24474	35558	0.83%	0.075%
33	19.598	2818	2824	2835	rBV	2833505	4260370	100.00%	8.964%
34	21.569	3153	3159	3168	rBV2	1603258	2729271	64.06%	5.743%
35	24.657	3676	3684	3702	rVB2	1363437	3694305	86.71%	7.773%
36	24.886	3715	3723	3741	rVB	959071	2946125	69.15%	6.199%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021141.D
Acq On : 25 Jul 2024 10:18
Operator : MA/JU
Sample : PB162100BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK100

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47526279

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021141.D
Acq On : 25 Jul 2024 10:18
Operator : MA/JU
Sample : PB162100BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

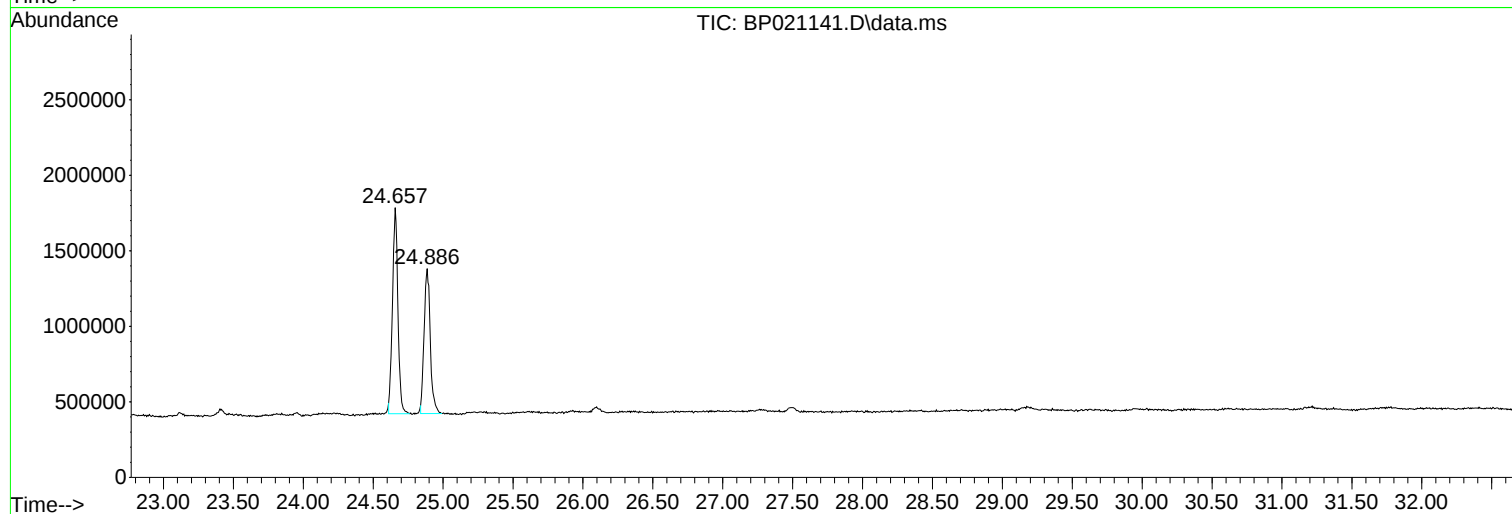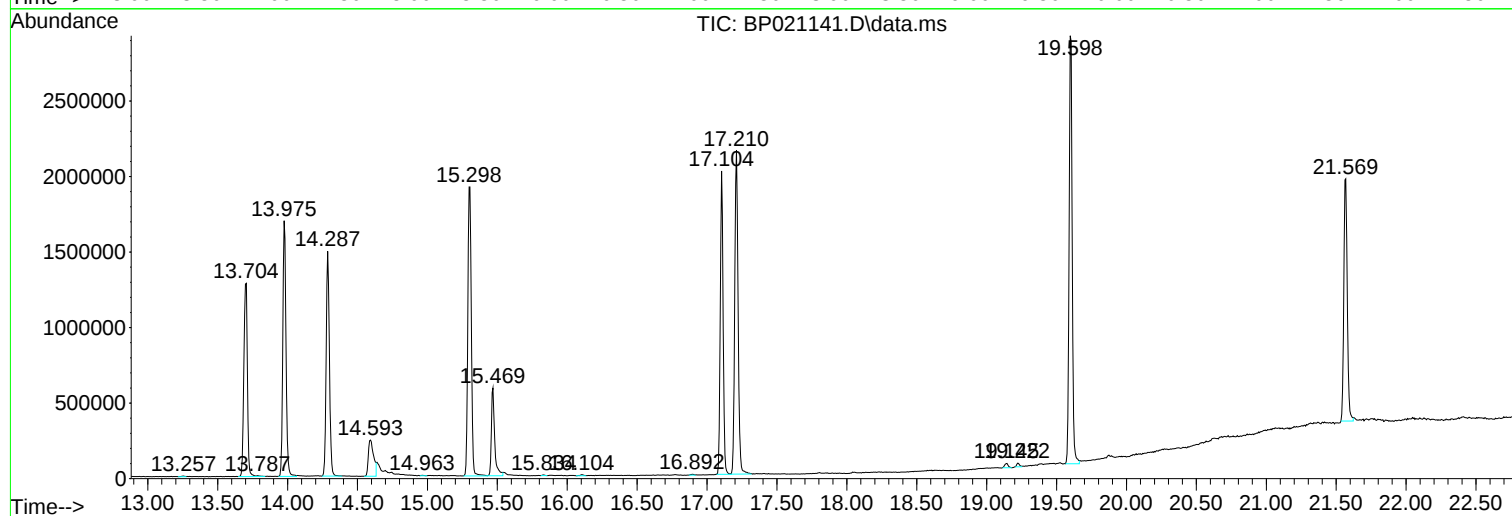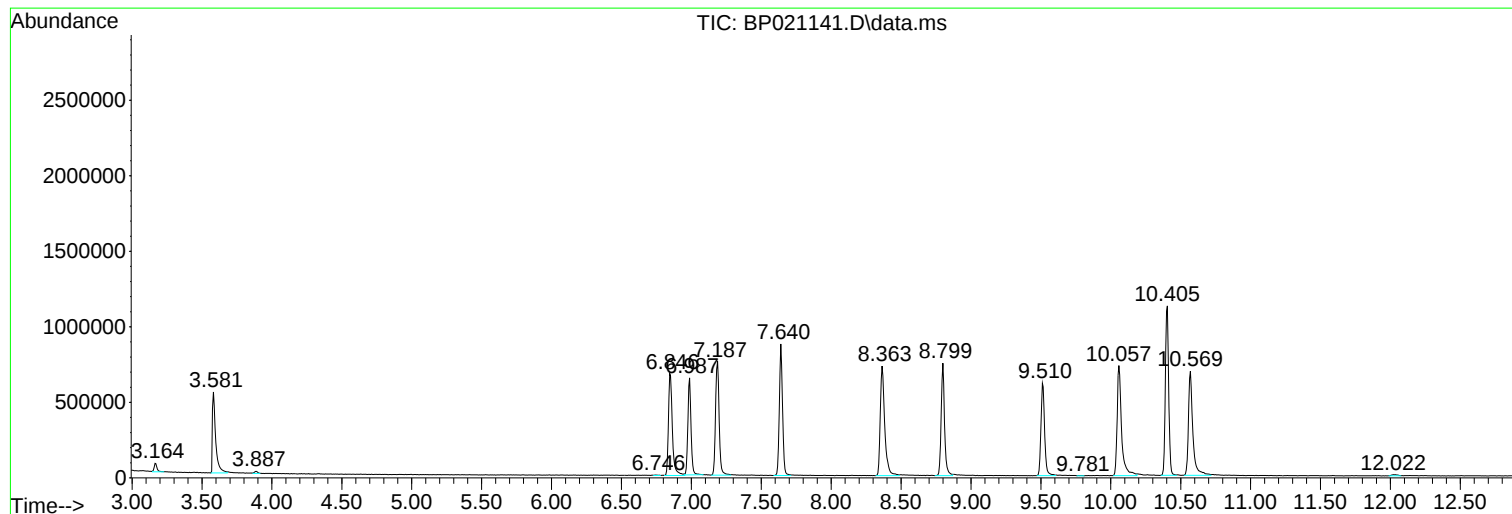

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021141.D
Acq On : 25 Jul 2024 10:18
Operator : MA/JU
Sample : PB162100BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021141.D
Acq On : 25 Jul 2024 10:18
Operator : MA/JU
Sample : PB162100BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK100

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------