

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
 Data File : BP021151.D
 Acq On : 25 Jul 2024 17:22
 Operator : MA/JU
 Sample : PB162259BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK259

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP021151.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	41	rVB	46454	63508	1.97%	0.185%
2	3.605	101	105	130	rBV	502699	839542	26.03%	2.448%
3	3.905	153	156	162	rVB2	11358	16191	0.50%	0.047%
4	6.864	652	659	676	rBV	464430	995519	30.87%	2.903%
5	7.005	676	683	693	rVB	461846	750044	23.26%	2.187%
6	7.199	709	716	739	rBV	577973	1047056	32.46%	3.053%
7	7.658	786	794	809	rBV	598623	1042648	32.33%	3.040%
8	8.381	910	917	935	rBV	587318	1204116	37.33%	3.511%
9	8.510	937	939	944	rVB5	2882	4153	0.13%	0.012%
10	8.810	983	990	1008	rBV	544111	945357	29.31%	2.756%
11	9.522	1104	1111	1135	rBV	441150	828476	25.69%	2.416%
12	9.875	1165	1171	1173	rBV7	1741	3229	0.10%	0.009%
13	10.075	1197	1205	1225	rBV	460315	1168796	36.24%	3.408%
14	10.416	1255	1263	1275	rBV	755165	1355531	42.03%	3.952%
15	10.581	1282	1291	1310	rBV	490057	1150992	35.69%	3.356%
16	12.051	1533	1541	1548	rBV5	6419	15587	0.48%	0.045%
17	13.710	1817	1823	1837	rBV	1012853	1531381	47.48%	4.465%
18	13.987	1863	1870	1883	rBV2	1163584	1914726	59.37%	5.583%
19	14.298	1914	1923	1934	rBV	1065280	1652231	51.23%	4.817%
20	14.622	1971	1978	1989	rBV2	118369	434942	13.49%	1.268%
21	14.704	1990	1992	1996	rVB2	21077	26983	0.84%	0.079%
22	15.316	2086	2096	2105	rBV	1373114	2314176	71.75%	6.747%
23	15.481	2116	2124	2150	rBV	275313	622841	19.31%	1.816%
24	16.122	2230	2233	2237	rVB6	4249	5708	0.18%	0.017%
25	16.898	2363	2365	2369	rBV4	3219	3665	0.11%	0.011%
26	17.116	2395	2402	2413	rBV	1157039	1805272	55.97%	5.264%
27	17.222	2413	2420	2441	rVV	1552159	2409077	74.69%	7.024%
28	18.228	2589	2591	2592	rBV2	5351	4845	0.15%	0.014%
29	19.151	2744	2748	2753	rBV4	18917	30303	0.94%	0.088%
30	19.604	2819	2825	2835	rBV	1857959	2709268	84.00%	7.899%
31	21.563	3153	3158	3171	rVB	1075295	1805766	55.99%	5.265%
32	24.645	3673	3682	3701	rVB2	1019618	3225252	100.00%	9.404%
33	24.880	3714	3722	3736	rVB	857184	2370288	73.49%	6.911%




Sum of corrected areas: 34297469

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021151.D
Acq On : 25 Jul 2024 17:22
Operator : MA/JU
Sample : PB162259BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK259

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

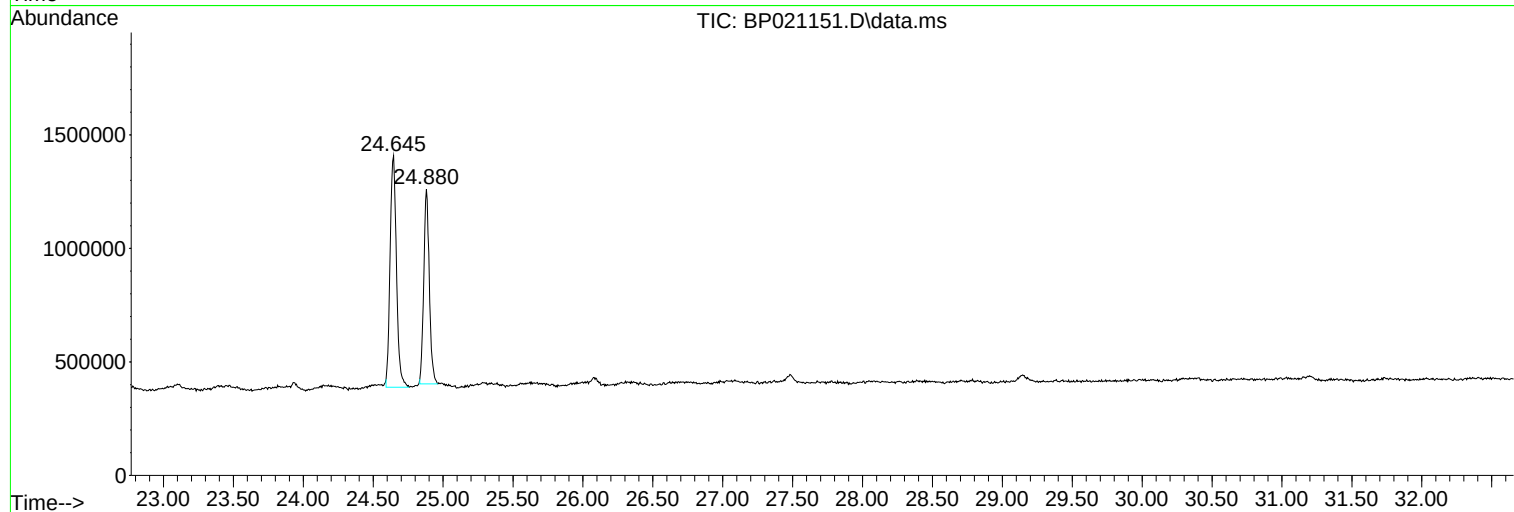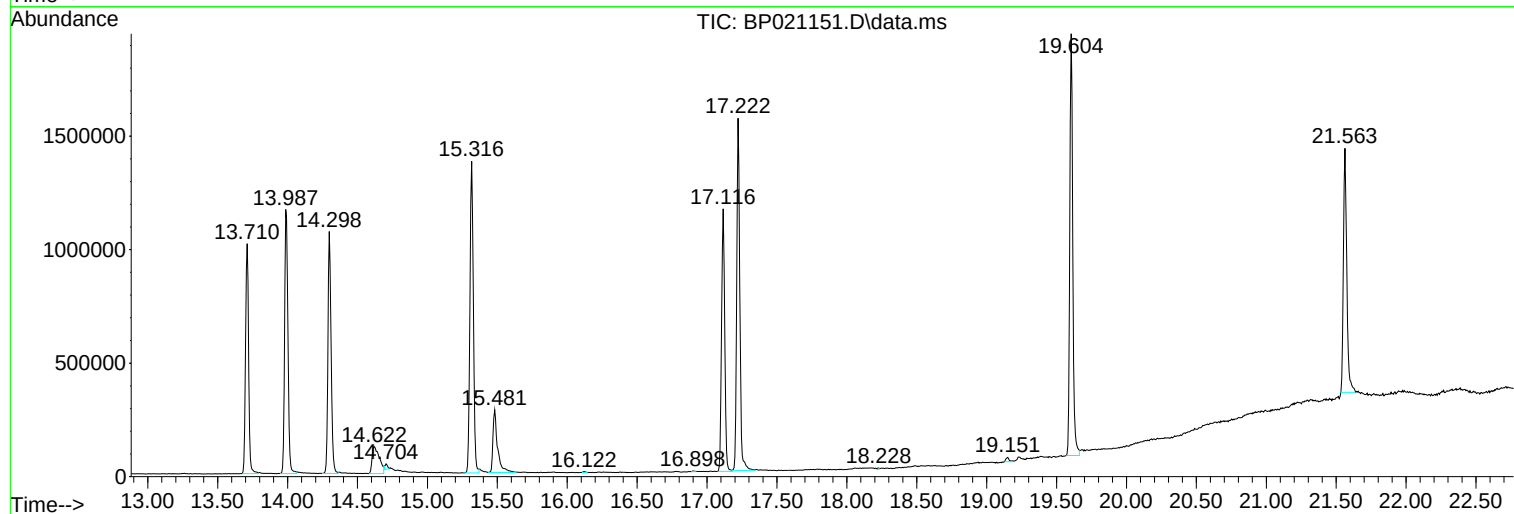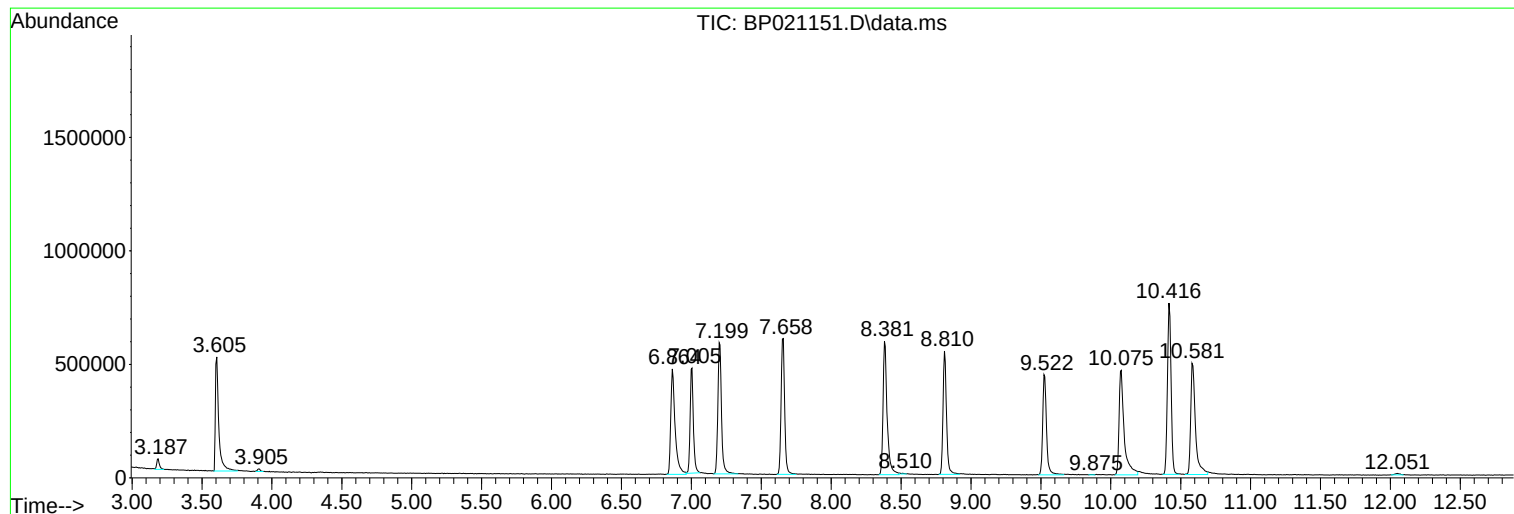

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021151.D
Acq On : 25 Jul 2024 17:22
Operator : MA/JU
Sample : PB162259BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK259

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072524\
Data File : BP021151.D
Acq On : 25 Jul 2024 17:22
Operator : MA/JU
Sample : PB162259BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK259

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc