

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006334.D
 Acq On : 26 Jul 2021 12:37
 Operator : CG/JU
 Sample : M3034-01 10X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT3

Quant Time: Jul 26 13:30:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 12:12:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	237493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.575	136	994625	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.416	164	560589	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.163	188	1109417	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	1056517	20.000	ng/ul	0.00
88) Perylene-d12	23.610	264	1065222	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	32893	5.170	ng/uL	0.00
4) Pyridine-d5	3.716	84	190321	10.076	ng/ul	0.01
7) Phenol-d5	6.957	99	255254	11.444	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	456164	32.869	ng/ul	0.00
11) 2-Chlorophenol-d4	7.322	132	520213	31.393	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113	413819	23.592	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	257099	34.715	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.657	143	257023	36.347	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	460675	33.245	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	641605	28.124	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1567559	39.289	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	1795746	36.634	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	86866	10.965	ng/ul	0.00
60) Fluorene-d10	15.410	176	1286225	38.348	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	187254	30.277	ng/ul	0.00
73) Anthracene-d10	17.263	188	2078109	41.495	ng/ul	0.00
81) Pyrene-d10	19.504	212	2296059	42.252	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.462	264	2194883	40.547	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.881	163	58585	1.496	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006334.D
Acq On : 26 Jul 2021 12:37
Operator : CG/JU
Sample : M3034-01 10X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT3


Quant Time: Jul 26 13:30:56 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 12:12:19 2021
Response via : Initial Calibration

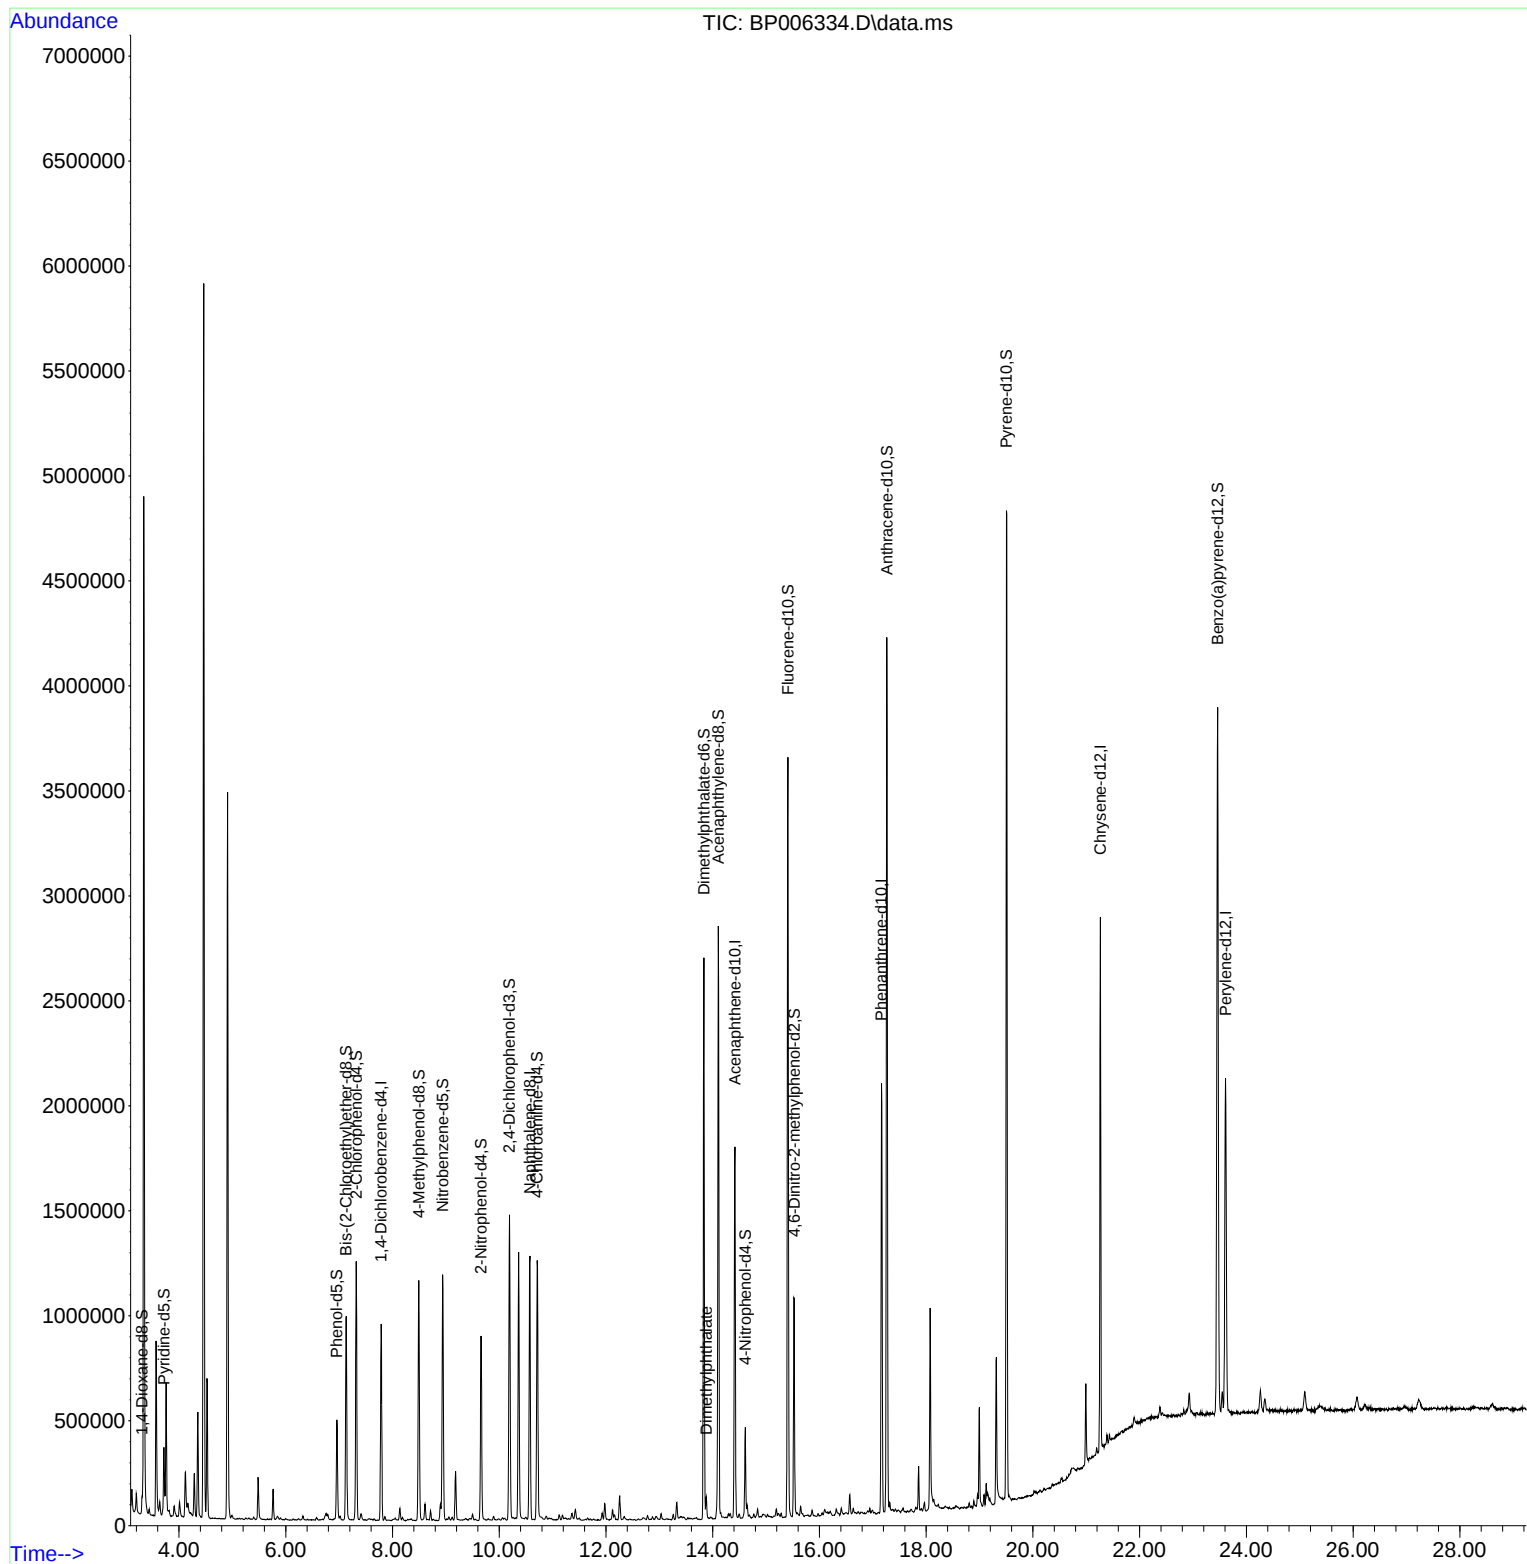

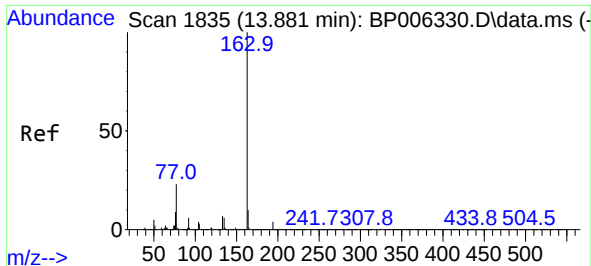

#47
 Dimethylphthalate
 Concen: 1.496 ng/ul
 RT: 13.881 min Scan# 1835
 Delta R.T. -0.006 min
 Lab File: BP006334.D
 Acq: 26 Jul 2021 12:37

Instrument :
 BNA_P
 ClientSampleId :
 C0AT3

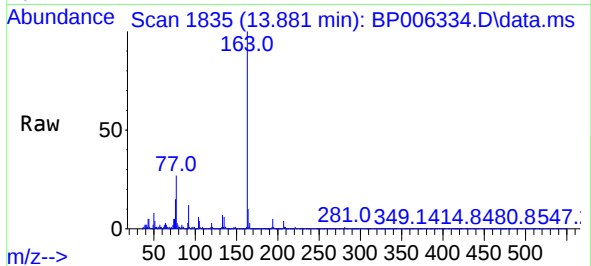

Tgt Ion:163 Resp: 58585
 Ion Ratio Lower Upper
 163 100
 194 4.5 3.0 4.6
 164 10.0 8.2 12.4

