

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006335.D
 Acq On : 26 Jul 2021 13:14
 Operator : CG/JU
 Sample : M3034-02 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT4

Quant Time: Jul 26 14:19:15 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 12:12:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	202227	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	869926	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.416	164	508949	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.169	188	1012973	20.000	ng/ul	0.00
79) Chrysene-d12	21.263	240	983499	20.000	ng/ul	0.00
88) Perylene-d12	23.615	264	985458	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	30260	5.585	ng/uL	0.00
4) Pyridine-d5	3.711	84	183341	11.400	ng/ul	0.00
7) Phenol-d5	6.957	99	207273	10.913	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	339868	28.759	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	391968	27.778	ng/ul	-0.01
15) 4-Methylphenol-d8	8.493	113	320455	21.455	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	191693	29.594	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.657	143	184466	29.826	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	340010	28.054	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	505815	25.350	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1132887	31.275	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	1319440	29.648	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	71422	9.930	ng/ul	0.00
60) Fluorene-d10	15.410	176	937990	30.803	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.528	200	137324	24.318	ng/ul	0.00
73) Anthracene-d10	17.263	188	1588633	34.742	ng/ul	0.00
81) Pyrene-d10	19.510	212	1849798	36.567	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.462	264	1768376	35.312	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.610	105	23166	1.009	ng/ul#	91
47) Dimethylphthalate	13.881	163	85284	2.399	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006335.D
Acq On : 26 Jul 2021 13:14
Operator : CG/JU
Sample : M3034-02 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT4

Quant Time: Jul 26 14:19:15 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 12:12:19 2021
Response via : Initial Calibration




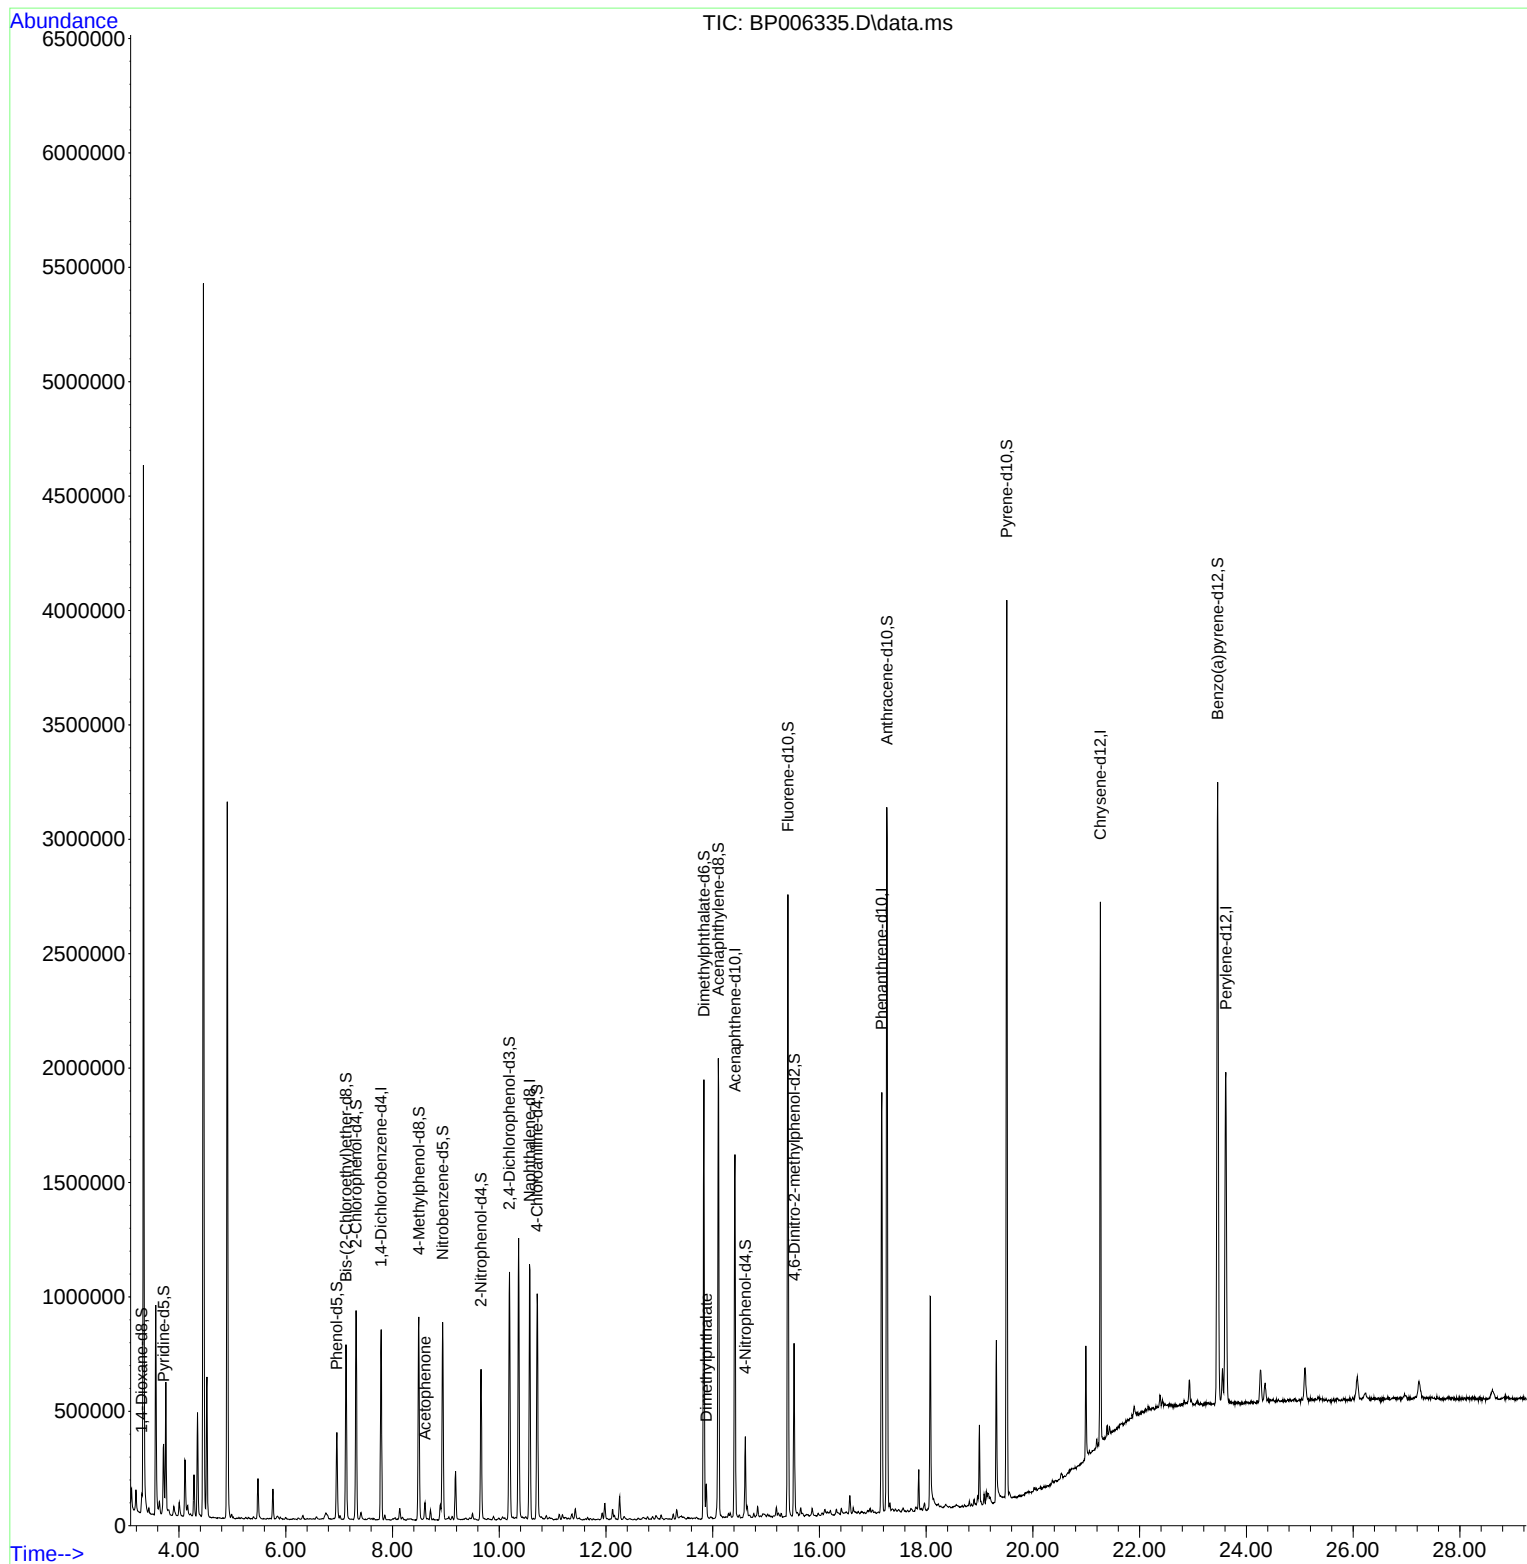


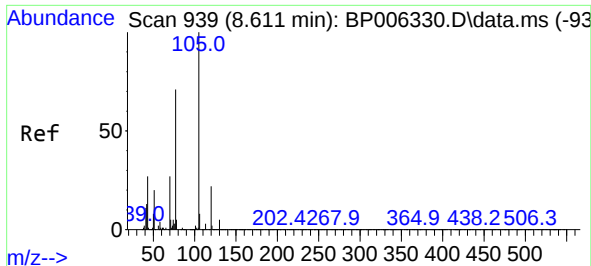

#16
Acetophenone
Concen: 1.009 ng/ul
RT: 8.610 min Scan# 939
Delta R.T. -0.006 min
Lab File: BP006335.D
Acq: 26 Jul 2021 13:14

Instrument :
BNA_P
ClientSampleId :
C0AT4

Tgt Ion:	105	Resp:	23166
Ion Ratio	Lower	Upper	
105	100		
77	88.3	65.0	97.4
51	29.4	17.9	26.9#

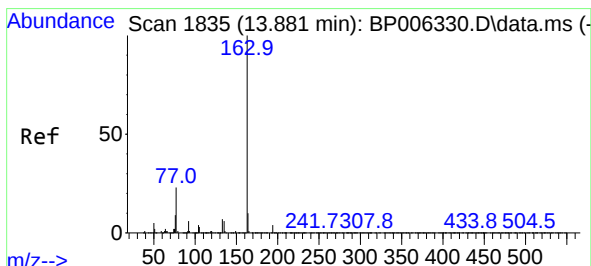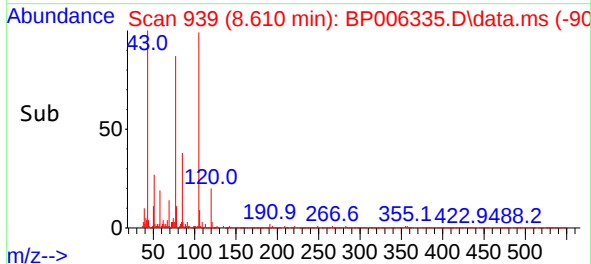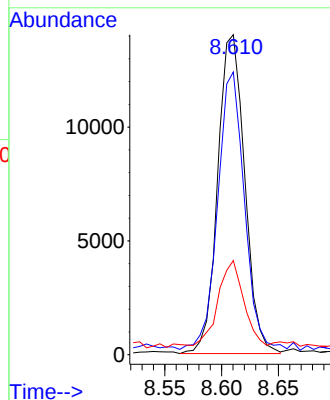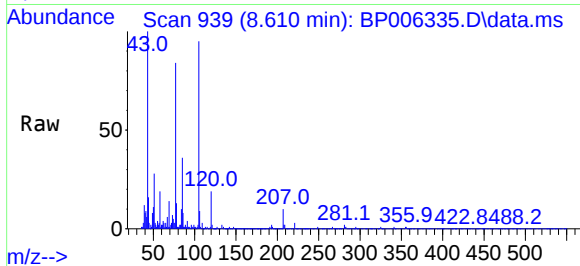

#47
Dimethylphthalate
Concen: 2.399 ng/ul
RT: 13.881 min Scan# 1835
Delta R.T. -0.006 min
Lab File: BP006335.D
Acq: 26 Jul 2021 13:14

Tgt Ion:	163	Resp:	85284
Ion Ratio	Lower	Upper	
163	100		
194	3.8	3.0	4.6
164	10.2	8.2	12.4

