

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006336.D
 Acq On : 26 Jul 2021 13:50
 Operator : CG/JU
 Sample : M3063-01DL 5X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT8DL

Quant Time: Jul 26 14:24:45 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 12:12:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	262483	20.000	ng/u1	0.00
20) Naphthalene-d8	10.569	136	1147040	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.416	164	664639	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	1303617	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1218226	20.000	ng/u1	0.00
88) Perylene-d12	23.610	264	1240614	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	13843	1.969	ng/uL	0.00
4) Pyridine-d5	3.711	84	41363	1.981	ng/u1	0.00
7) Phenol-d5	6.958	99	14338	0.582	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	82653	5.388	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	35904	1.960	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	32311	1.667	ng/u1	0.00
21) Nitrobenzene-d5	8.940	128	44449	5.204	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.658	143	18866	2.313	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	37820	2.367	ng/u1	0.00
31) 4-Chloroaniline-d4	10.710	131	105994	4.029	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	322674	6.821	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	335349	5.770	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	4189	0.446	ng/u1	0.00
60) Fluorene-d10	15.410	176	269926	6.788	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.540	200	47674	6.560	ng/u1	0.00
73) Anthracene-d10	17.263	188	426617	7.250	ng/u1	0.00
81) Pyrene-d10	19.504	212	478294	7.633	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.457	264	427996	6.789	ng/u1	0.00
Target Compounds						
58) 2,3,4,6-Tetrachlorophenol	15.040	232	18880	1.994	ng/u1	96
71) Pentachlorophenol	16.816	266	566952	64.412	ng/u1	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006336.D
Acq On : 26 Jul 2021 13:50
Operator : CG/JU
Sample : M3063-01DL 5X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT8DL

Quant Time: Jul 26 14:24:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 12:12:19 2021
Response via : Initial Calibration




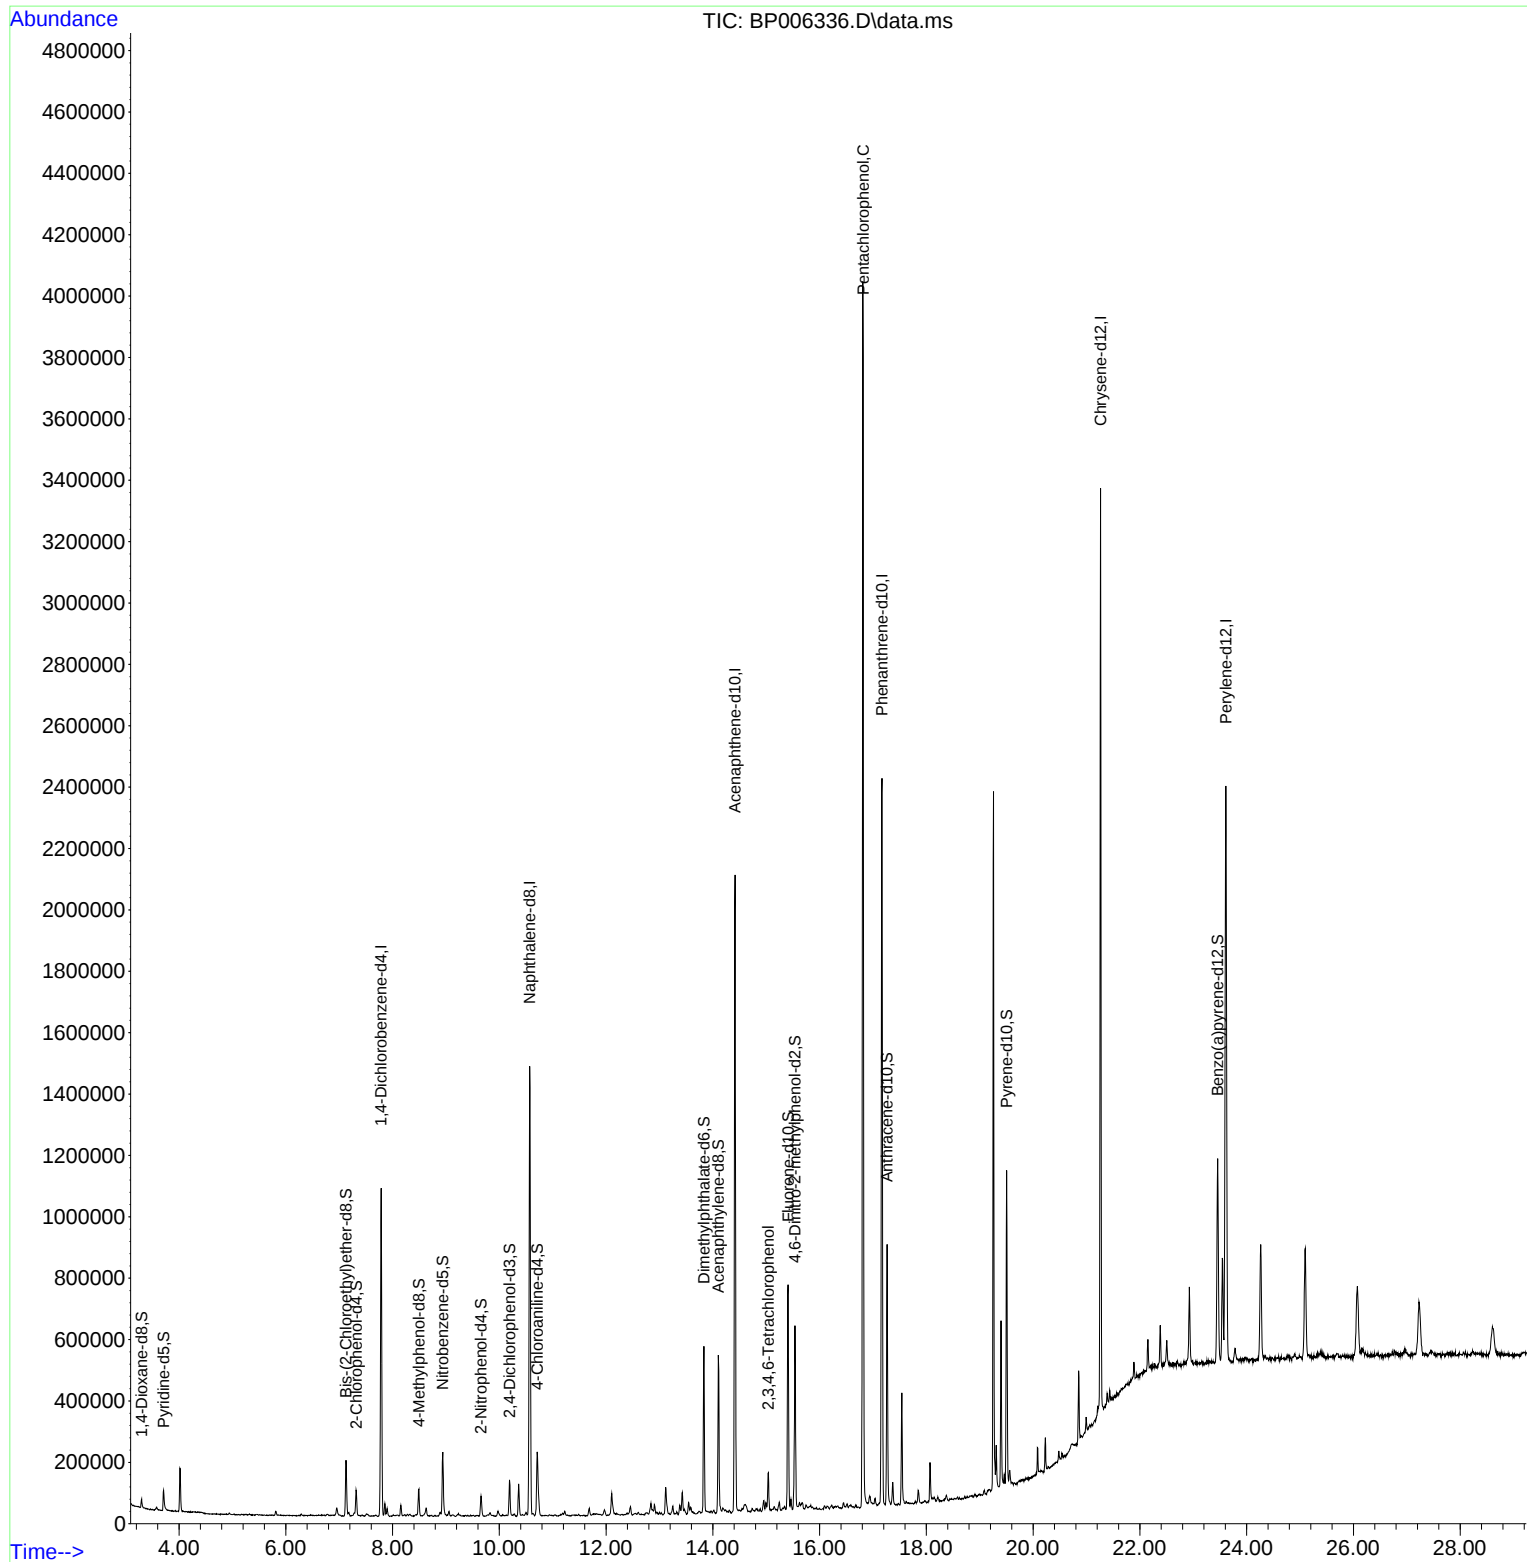


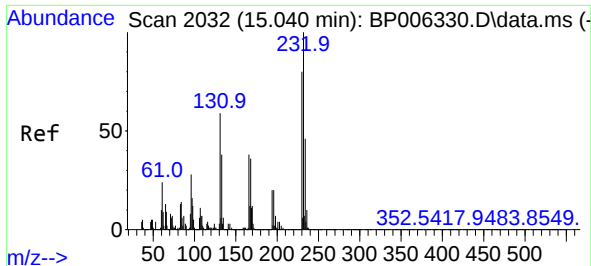

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.994 ng/ul
RT: 15.040 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BP006336.D
Acq: 26 Jul 2021 13:50

Instrument :
BNA_P
ClientSampleId :
C0AT8DL

Tgt Ion:	232	Resp:	18880
Ion Ratio	Lower	Upper	
232	100		
131	58.6	43.8	65.8
130	3.7	2.6	3.8
166	34.3	28.5	42.7

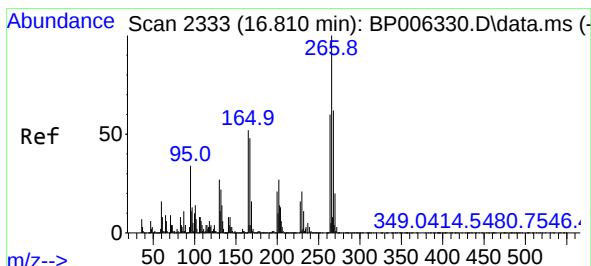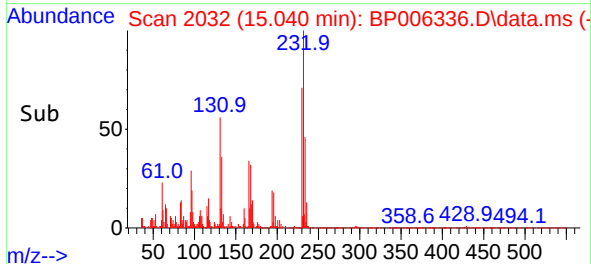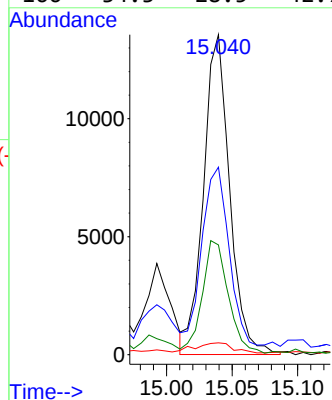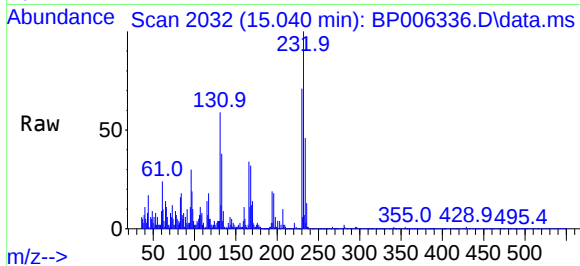

#71
Pentachlorophenol
Concen: 64.412 ng/ul
RT: 16.816 min Scan# 2334
Delta R.T. 0.000 min
Lab File: BP006336.D
Acq: 26 Jul 2021 13:50

Tgt Ion:	266	Resp:	566952
Ion Ratio	Lower	Upper	
266	100		
264	61.7	49.6	74.4
268	63.1	50.7	76.1

