

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006337.D
 Acq On : 26 Jul 2021 14:24
 Operator : CG/JU
 Sample : M3063-02DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Quant Time: Jul 26 15:11:06 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jul 26 12:12:19 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	221034	20.000	ng/u1	0.00
20) Naphthalene-d8	10.569	136	940034	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.416	164	544841	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.169	188	1093459	20.000	ng/u1	0.00
79) Chrysene-d12	21.263	240	1042199	20.000	ng/u1	0.00
88) Perylene-d12	23.610	264	1046357	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	923	0.156	ng/uL	0.00
4) Pyridine-d5	3.722	84	7958	0.453	ng/u1	0.02
7) Phenol-d5	6.958	99	6739	0.325	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	22140	1.714	ng/u1	0.00
11) 2-Chlorophenol-d4	7.322	132	17999	1.167	ng/u1	0.00
15) 4-Methylphenol-d8	8.493	113	11703	0.717	ng/u1	0.00
21) Nitrobenzene-d5	8.940	128	11043	1.578	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.657	143	9209	1.378	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	16352	1.249	ng/u1	0.00
31) 4-Chloroaniline-d4	10.716	131	31358	1.454	ng/u1	0.00
46) Dimethylphthalate-d6	13.834	166	78311	2.019	ng/u1	0.00
49) Acenaphthylene-d8	14.104	160	77741	1.632	ng/u1	0.00
54) 4-Nitrophenol-d4	14.610	143	2020	0.262	ng/u1	0.00
60) Fluorene-d10	15.410	176	66350	2.035	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.539	200	22911	3.758	ng/u1	0.00
73) Anthracene-d10	17.263	188	102339	2.073	ng/u1	0.00
81) Pyrene-d10	19.504	212	113456	2.117	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.457	264	98441	1.851	ng/u1	0.00
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.034	232	9224	1.188	ng/u1	92
71) Pentachlorophenol	16.810	266	323482	43.815	ng/u1	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006337.D
Acq On : 26 Jul 2021 14:24
Operator : CG/JU
Sample : M3063-02DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Time: Jul 26 15:11:06 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jul 26 12:12:19 2021
Response via : Initial Calibration




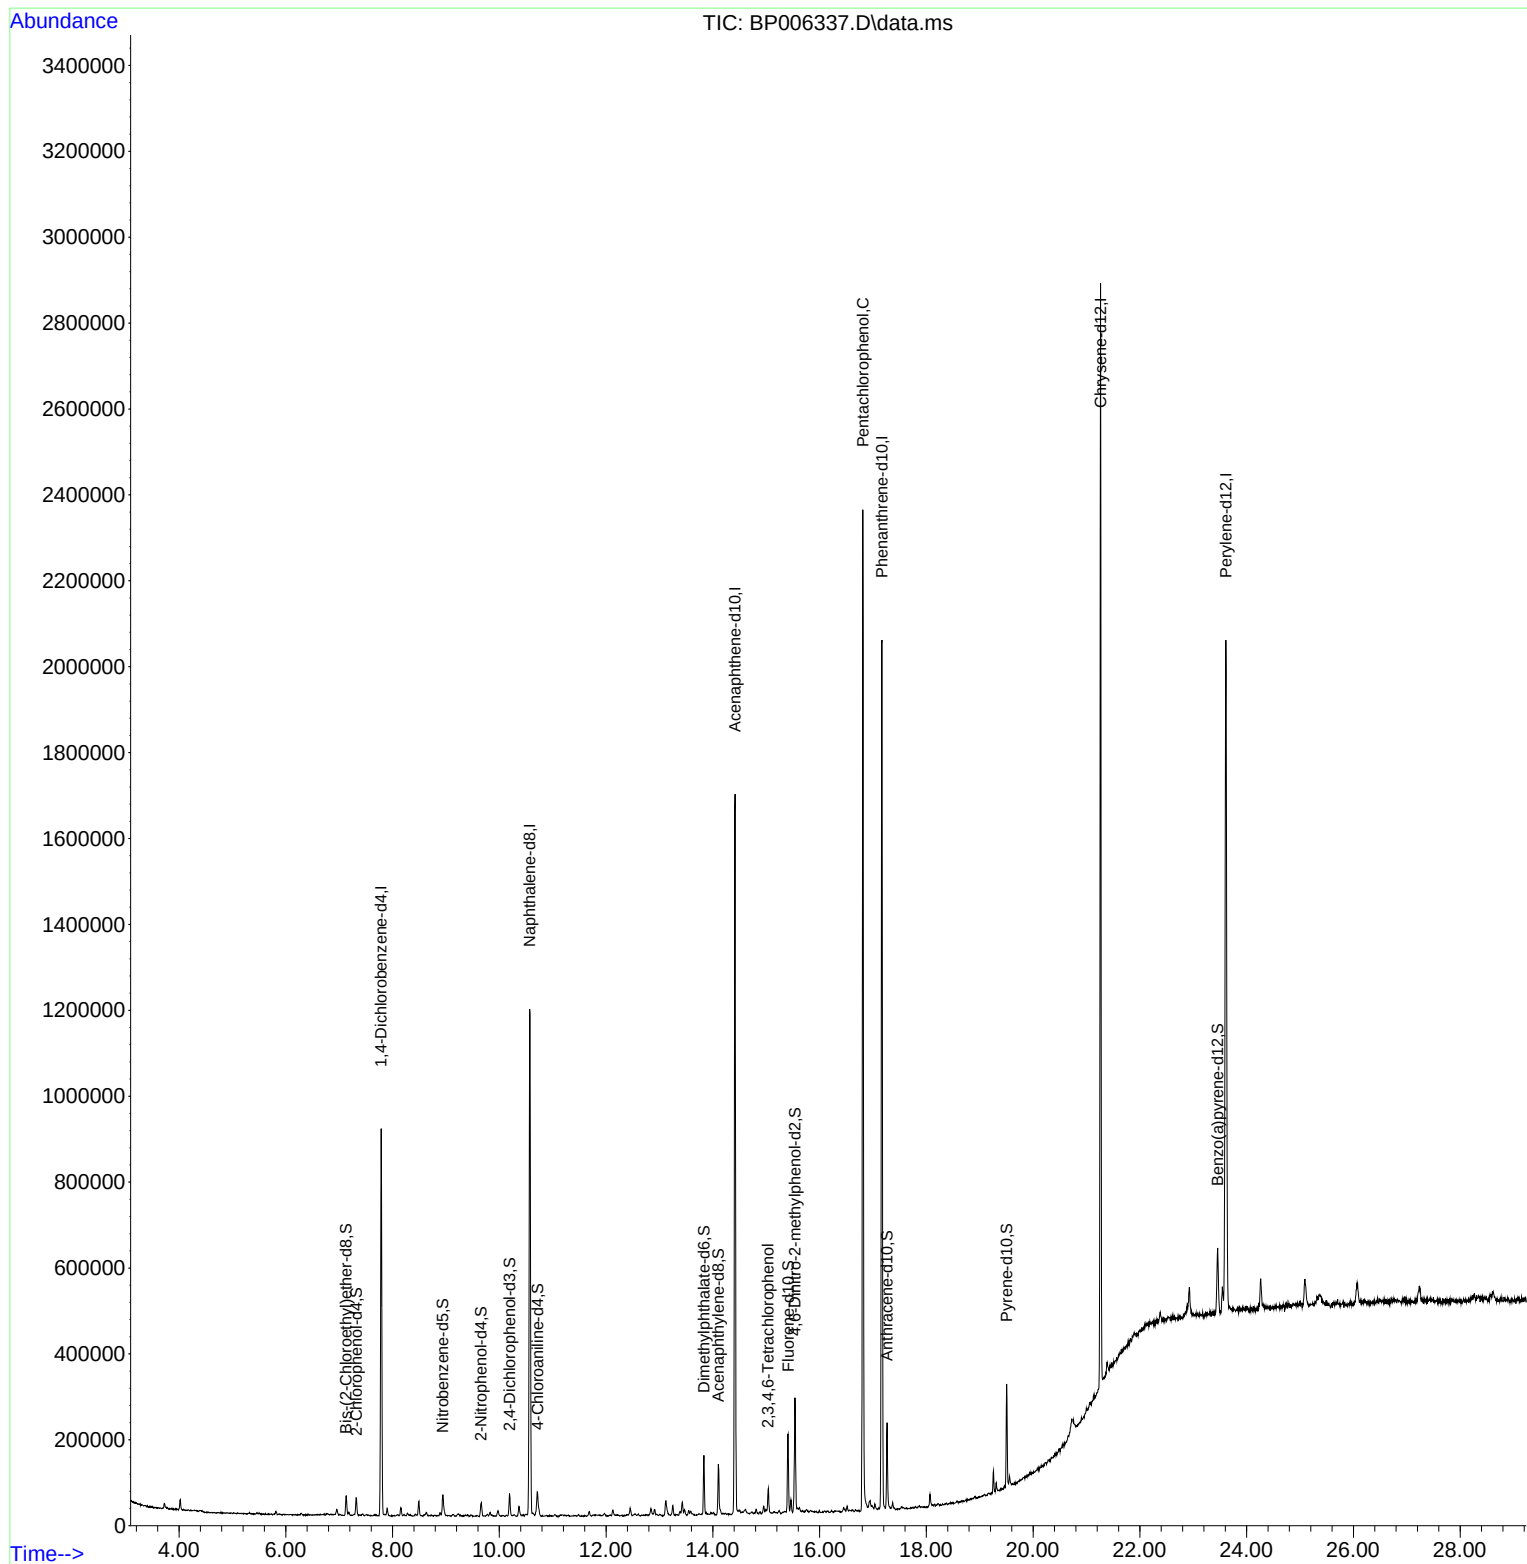


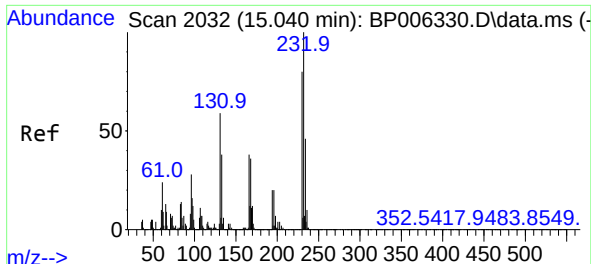

#58
2,3,4,6-Tetrachlorophenol
Concen: 1.188 ng/ul
RT: 15.034 min Scan# 2031
Delta R.T. -0.012 min
Lab File: BP006337.D
Acq: 26 Jul 2021 14:24

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Tgt Ion:	232	Resp:	9224
Ion	Ratio	Lower	Upper
232	100		
131	62.0	43.8	65.8
130	3.8	2.6	3.8
166	32.1	28.5	42.7

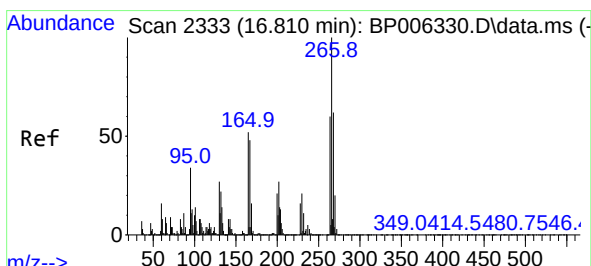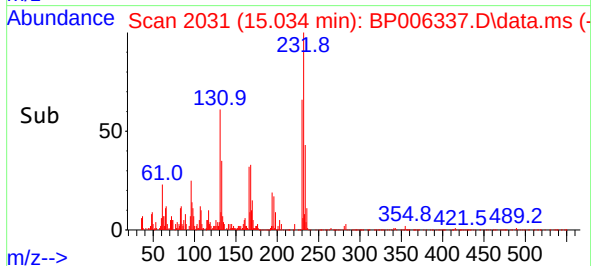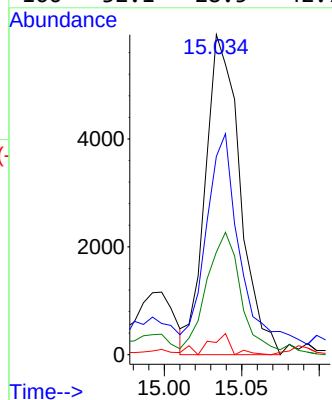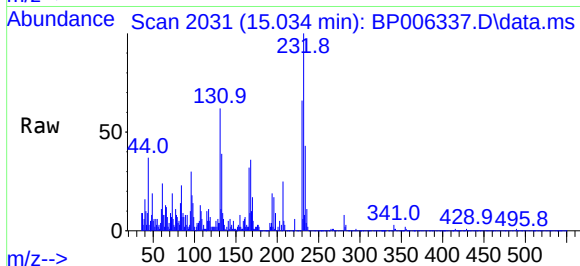

#71
Pentachlorophenol
Concen: 43.815 ng/ul
RT: 16.810 min Scan# 2333
Delta R.T. -0.006 min
Lab File: BP006337.D
Acq: 26 Jul 2021 14:24

Tgt Ion:	266	Resp:	323482
Ion	Ratio	Lower	Upper
266	100		
264	63.3	49.6	74.4
268	64.5	50.7	76.1

