

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006349.D
 Acq On : 26 Jul 2021 21:26
 Operator : CG/JU
 Sample : M3091-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0042

Quant Time: Jul 27 01:10:20 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	226958	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	959271	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.410	164	545503	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1068658	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1056673	20.000	ng/ul	-0.01
88) Perylene-d12	23.604	264	1095690	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.299	96	37662	6.194	ng/uL	0.00
4) Pyridine-d5	3.705	84	242243	13.421	ng/ul	0.00
7) Phenol-d5	6.957	99	180745	8.479	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	428505	32.309	ng/ul	0.00
11) 2-Chlorophenol-d4	7.316	132	423742	26.758	ng/ul	-0.01
15) 4-Methylphenol-d8	8.493	113	305107	18.202	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	246390	34.495	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.657	143	228661	33.528	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	397048	29.709	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	640520	29.112	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1394572	35.920	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	1660408	34.810	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	65854	8.543	ng/ul	0.00
60) Fluorene-d10	15.404	176	1178300	36.102	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	167743	28.156	ng/ul	-0.01
73) Anthracene-d10	17.263	188	1922866	39.860	ng/ul	0.00
81) Pyrene-d10	19.504	212	2144762	39.462	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	2170100	38.975	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.186	149	65318	1.463	ng/ul	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006349.D
Acq On : 26 Jul 2021 21:26
Operator : CG/JU
Sample : M3091-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0042

Quant Time: Jul 27 01:10:20 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration

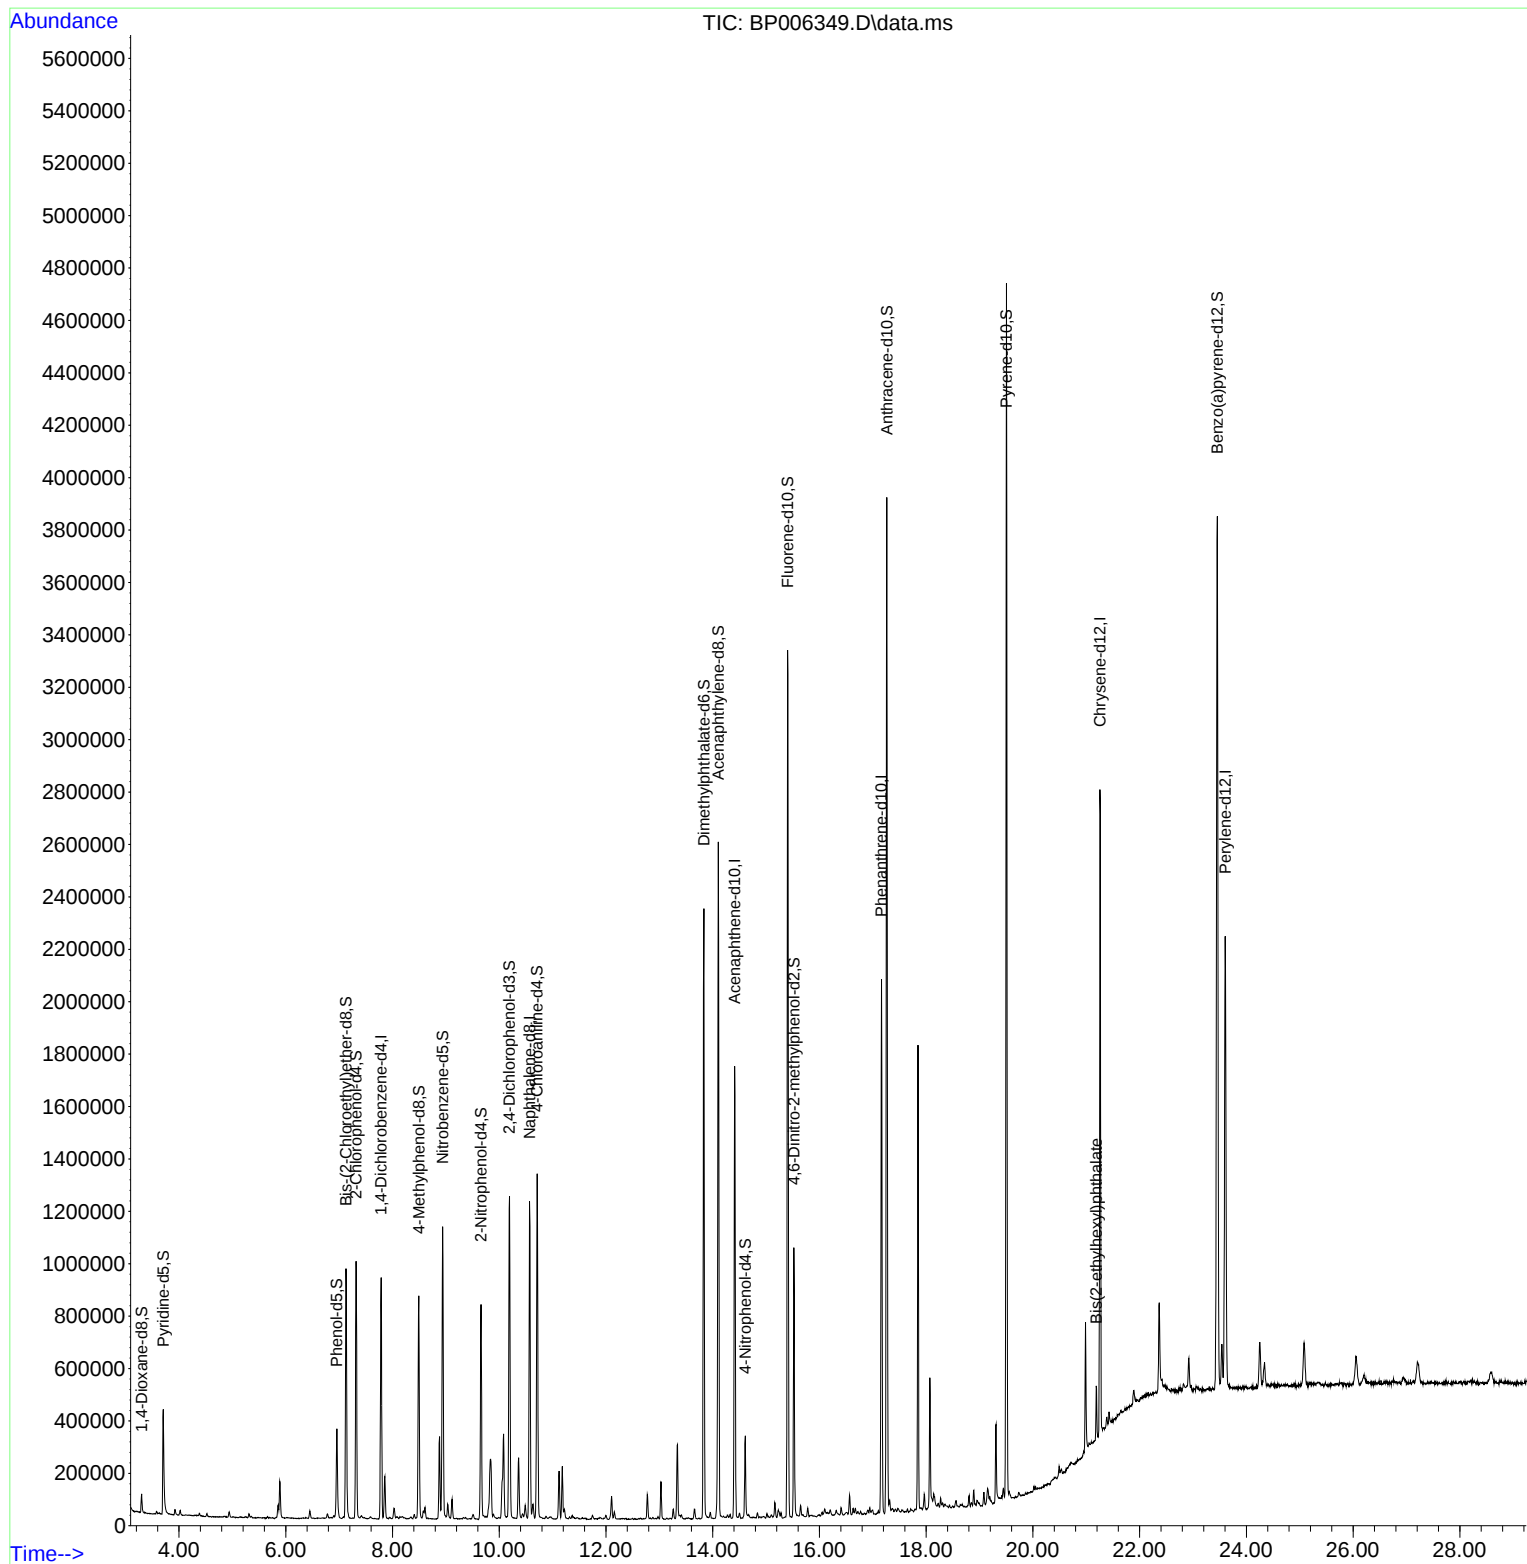

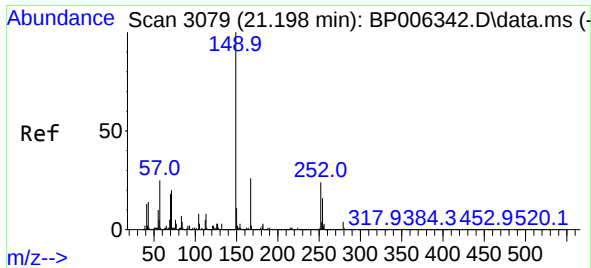

#86
Bis(2-ethylhexyl)phthalate
Concen: 1.463 ng/ul
RT: 21.186 min Scan# 3077
Delta R.T. -0.012 min
Lab File: BP006349.D
Acq: 26 Jul 2021 21:26

Instrument :
BNA_P
ClientSampleId :
C0042

Tgt Ion:149 Resp: 65318
Ion Ratio Lower Upper
149 100
167 25.3 20.3 30.5
279 3.5 2.7 4.1

