

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006352.D
 Acq On : 26 Jul 2021 23:09
 Operator : CG/JU
 Sample : M3107-05
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 BGD25

Quant Time: Jul 27 01:10:57 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	271547	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	1149363	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.410	164	655642	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1299337	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1221080	20.000	ng/ul	-0.01
88) Perylene-d12	23.604	264	1239131	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	41721	5.735	ng/uL	0.00
4) Pyridine-d5	3.717	84	246687	11.423	ng/ul	0.01
7) Phenol-d5	6.958	99	195328	7.659	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	550319	34.680	ng/ul	0.00
11) 2-Chlorophenol-d4	7.322	132	517238	27.299	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113	353419	17.622	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	316054	36.930	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.657	143	299977	36.710	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	503936	31.471	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	783599	29.724	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1923456	41.220	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	2227598	38.856	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	76912	8.301	ng/ul	0.00
60) Fluorene-d10	15.410	176	1583235	40.360	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.522	200	257982	35.616	ng/ul	-0.01
73) Anthracene-d10	17.263	188	2551132	43.495	ng/ul	0.00
81) Pyrene-d10	19.504	212	2851327	45.399	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	2715798	43.129	ng/ul	0.00
Target Compounds						
16) Acetophenone	8.610	105	42074	1.364	ng/ul	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006352.D
Acq On : 26 Jul 2021 23:09
Operator : CG/JU
Sample : M3107-05
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
BGD25


Quant Time: Jul 27 01:10:57 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration

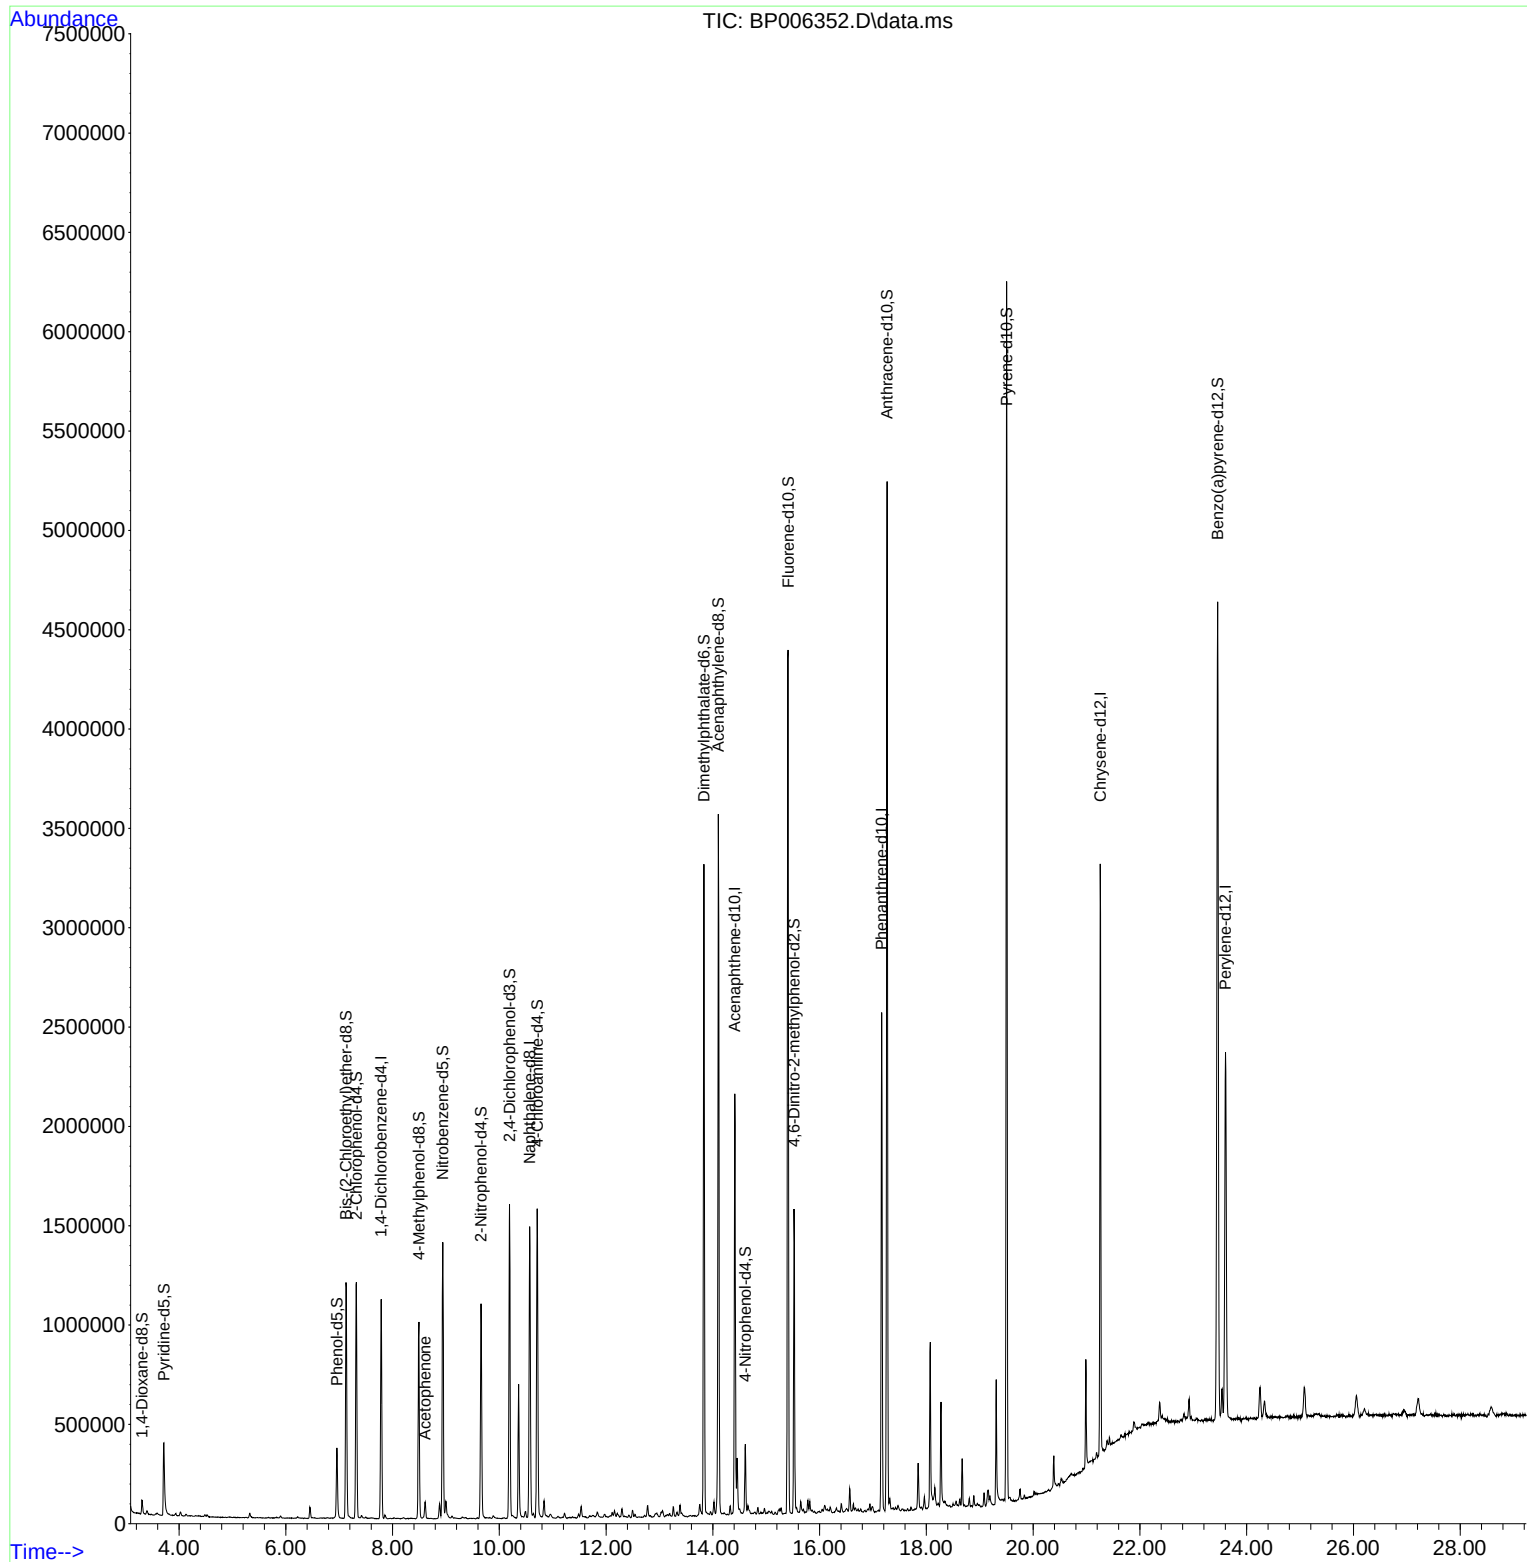

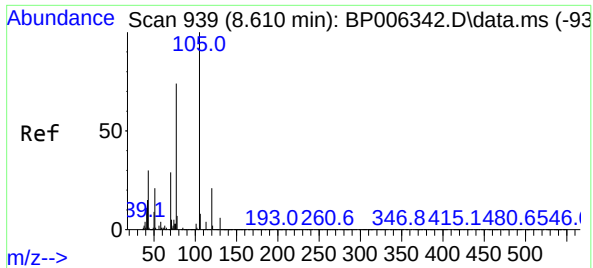

#16
Acetophenone
Concen: 1.364 ng/ul
RT: 8.610 min Scan# 939
Delta R.T. -0.006 min
Lab File: BP006352.D
Acq: 26 Jul 2021 23:09

Instrument :
BNA_P
ClientSampleId :
BGD25

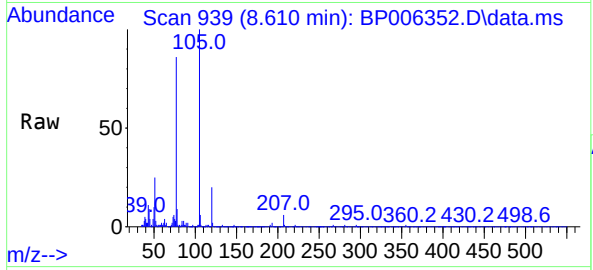

Tgt Ion:105 Resp: 42074

Ion	Ratio	Lower	Upper
105	100		
77	85.7	65.0	97.4
51	25.0	17.9	26.9

