

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006353.D
 Acq On : 26 Jul 2021 23:44
 Operator : CG/JU
 Sample : M3123-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0060

Quant Time: Jul 27 01:11:11 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Jul 24 04:29:12 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.787	152	253639	20.000	ng/ul	0.00
20) Naphthalene-d8	10.569	136	1066048	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.410	164	598871	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1170362	20.000	ng/ul	0.00
79) Chrysene-d12	21.257	240	1093565	20.000	ng/ul	-0.01
88) Perylene-d12	23.604	264	1130101	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.305	96	39107	5.755	ng/uL	0.00
4) Pyridine-d5	3.711	84	142398	7.059	ng/ul	0.00
7) Phenol-d5	6.958	99	136466	5.729	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.128	67	471542	31.814	ng/ul	0.00
11) 2-Chlorophenol-d4	7.322	132	408216	23.066	ng/ul	0.00
15) 4-Methylphenol-d8	8.493	113	265001	14.146	ng/ul	0.00
21) Nitrobenzene-d5	8.940	128	267412	33.689	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.658	143	171737	22.659	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.193	165	398038	26.800	ng/ul	0.00
31) 4-Chloroaniline-d4	10.710	131	676190	27.655	ng/ul	0.00
46) Dimethylphthalate-d6	13.834	166	1554653	36.475	ng/ul	0.00
49) Acenaphthylene-d8	14.104	160	1840357	35.144	ng/ul	0.00
54) 4-Nitrophenol-d4	14.610	143	21560	2.548	ng/ul	0.00
60) Fluorene-d10	15.404	176	1285122	35.866	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.522	200	4352	0.667	ng/ul	-0.01
73) Anthracene-d10	17.263	188	2163630	40.953	ng/ul	0.00
81) Pyrene-d10	19.504	212	2359937	41.956	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.457	264	2324152	40.470	ng/ul	0.00
Target Compounds						
					Qvalue	
6) Benzaldehyde	6.940	77	21228	1.633	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006353.D
Acq On : 26 Jul 2021 23:44
Operator : CG/JU
Sample : M3123-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0060


Quant Time: Jul 27 01:11:11 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Jul 24 04:29:12 2021
Response via : Initial Calibration

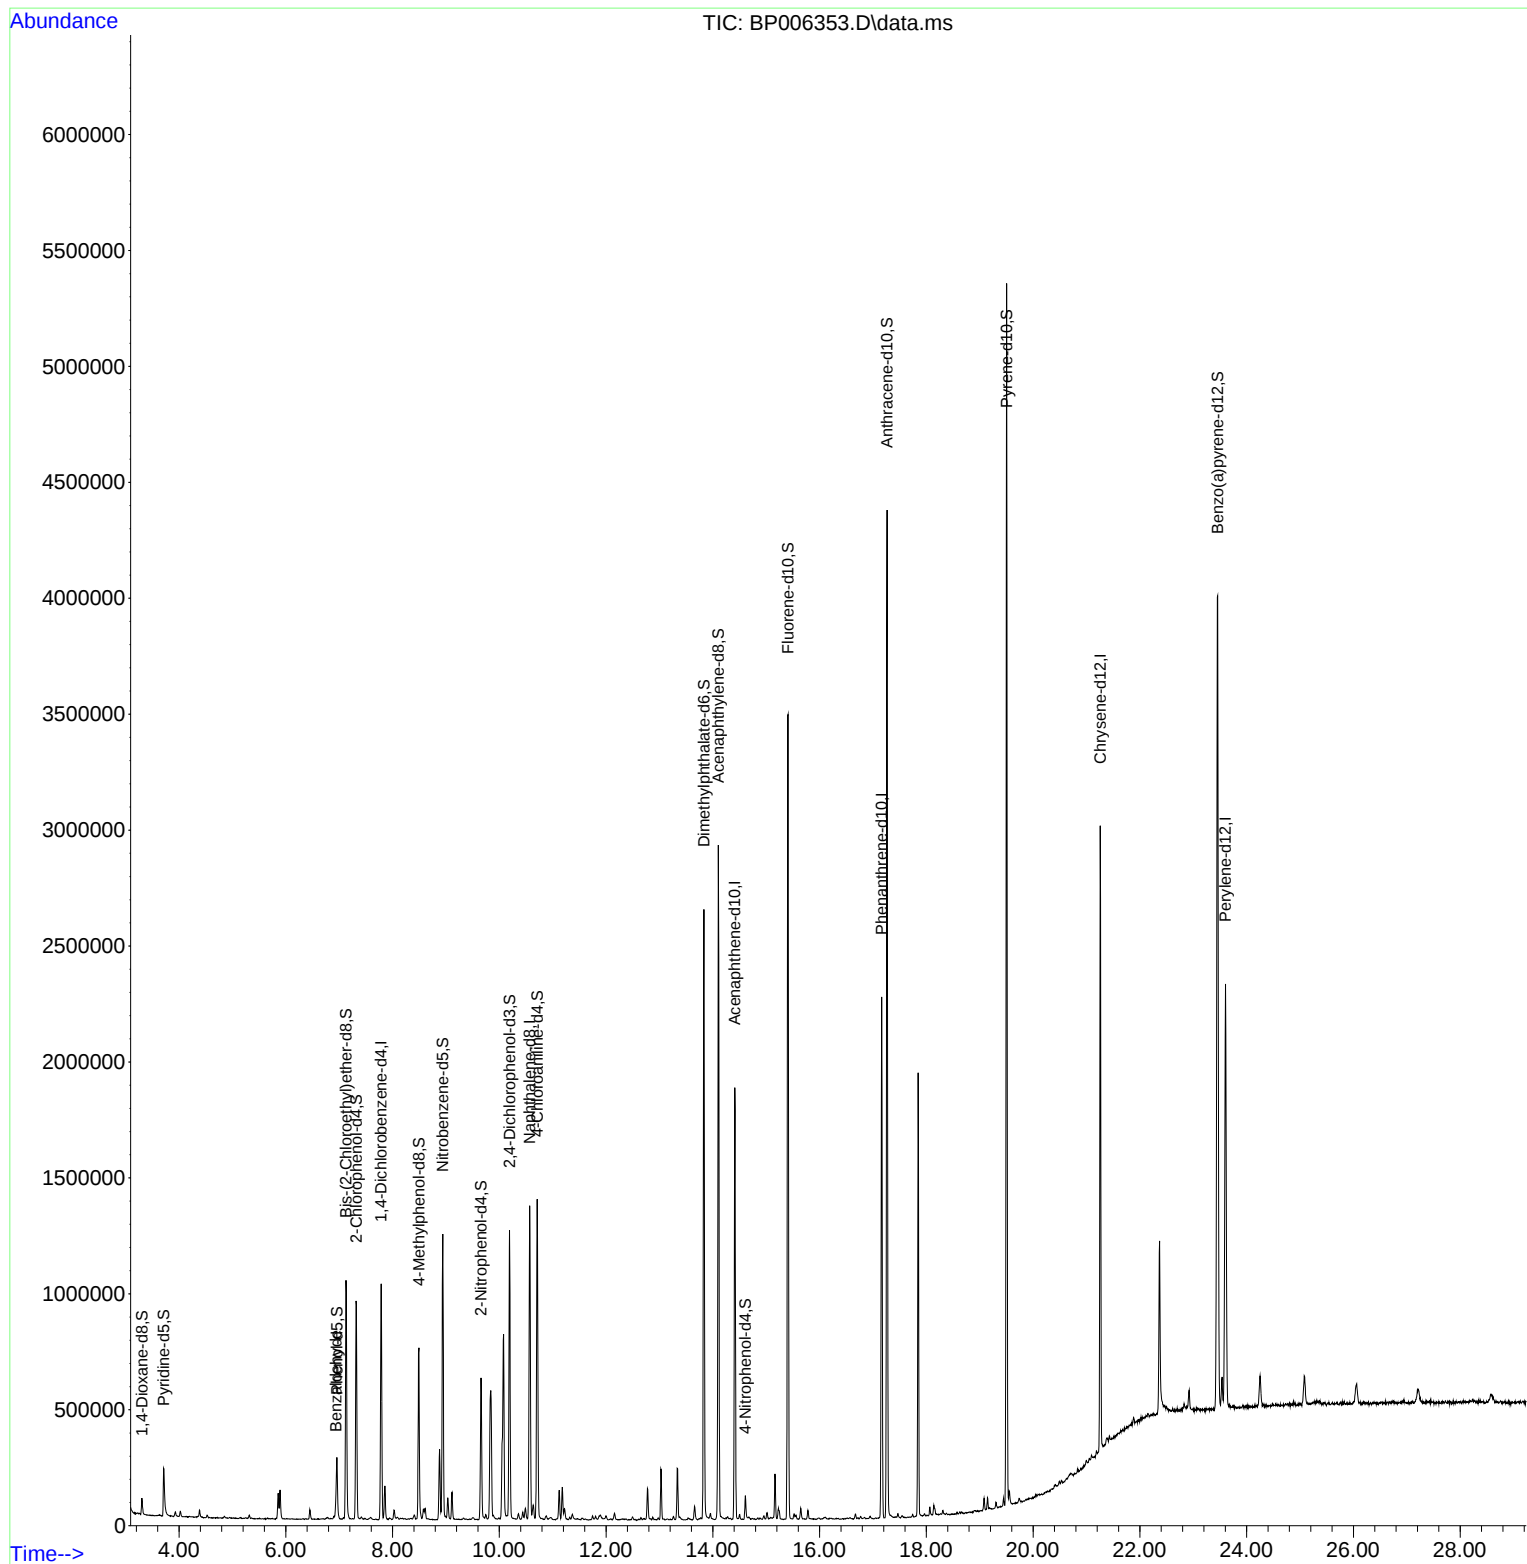

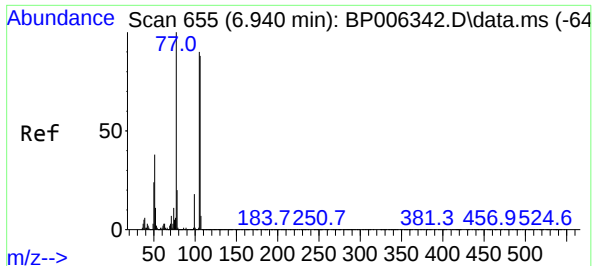

#6
Benzaldehyde
Concen: 1.633 ng/ul
RT: 6.940 min Scan# 655
Delta R.T. -0.006 min
Lab File: BP006353.D
Acq: 26 Jul 2021 23:44

Instrument :
BNA_P
ClientSampleId :
C0060

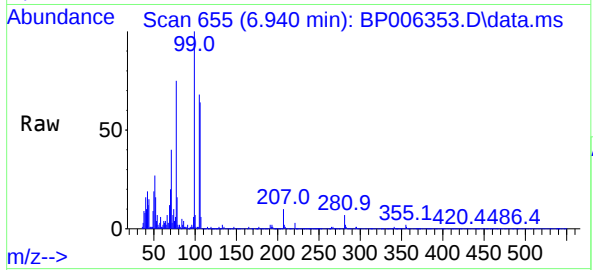

Tgt Ion: 77 Resp: 21228

Ion	Ratio	Lower	Upper
77	100		
105	90.4	74.5	111.7
106	84.4	71.0	106.4

