

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006337.D
 Acq On : 26 Jul 2021 14:24
 Operator : CG/JU
 Sample : M3063-02DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006337.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.722	105	108	113	rBV4	10883	15378	0.47%	0.070%
2	4.022	153	159	166	rBV	24832	37968	1.17%	0.172%
3	5.322	378	380	384	rVB4	4257	4445	0.14%	0.020%
4	5.816	460	464	468	rVB3	8507	12952	0.40%	0.059%
5	6.287	541	544	551	rVV6	5084	10296	0.32%	0.047%
6	6.958	653	658	663	rVB3	13290	23555	0.72%	0.107%
7	7.134	681	688	693	rBV	46119	77060	2.37%	0.349%
8	7.181	693	696	701	rVB2	8433	12383	0.38%	0.056%
9	7.281	708	713	715	rBV6	2910	4606	0.14%	0.021%
10	7.316	715	719	725	rVB	40640	65267	2.00%	0.296%
11	7.440	736	740	746	rVB6	4543	8557	0.26%	0.039%
12	7.699	780	784	786	rVB5	3064	4287	0.13%	0.019%
13	7.787	792	799	808	rBV	901509	1388759	42.64%	6.289%
14	7.899	814	818	824	rVB	16993	26151	0.80%	0.118%
15	8.087	845	850	855	rBV9	3161	5897	0.18%	0.027%
16	8.157	855	862	868	rBV2	19063	31617	0.97%	0.143%
17	8.281	879	883	886	rBV5	6118	9077	0.28%	0.041%
18	8.428	906	908	913	rBV5	3495	5069	0.16%	0.023%
19	8.493	913	919	926	rVB	33293	53702	1.65%	0.243%
20	8.581	932	934	937	rBV4	3832	5840	0.18%	0.026%
21	8.628	937	942	948	rVB7	8335	18475	0.57%	0.084%
22	8.887	983	986	990	rBV6	7692	10851	0.33%	0.049%
23	8.940	990	995	1005	rVB2	48655	99264	3.05%	0.450%
24	9.128	1022	1027	1028	rBV5	4015	5669	0.17%	0.026%
25	9.228	1038	1044	1049	rBV10	5957	14047	0.43%	0.064%
26	9.469	1082	1085	1090	rVB6	4418	6809	0.21%	0.031%
27	9.581	1100	1104	1111	rVB10	3324	7204	0.22%	0.033%
28	9.663	1111	1118	1122	rBV3	32624	61084	1.88%	0.277%
29	9.775	1132	1137	1141	rBV8	4814	7893	0.24%	0.036%
30	9.828	1141	1146	1150	rVV2	9187	14930	0.46%	0.068%
31	9.975	1165	1171	1179	rVB4	12876	24823	0.76%	0.112%
32	10.134	1194	1198	1202	rBV7	2961	5188	0.16%	0.023%
33	10.193	1202	1208	1217	rVV2	52983	91583	2.81%	0.415%
34	10.275	1219	1222	1227	rVB7	3486	5659	0.17%	0.026%
35	10.369	1232	1238	1245	rBV	23127	44259	1.36%	0.200%
36	10.499	1255	1260	1264	rVV8	5231	12643	0.39%	0.057%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006337.D
 Acq On : 26 Jul 2021 14:24
 Operator : CG/JU
 Sample : M3063-02DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

37	10.569	1264	1272	1280	rVV	1180881	2001408	61.44%	9.064%
38	10.622	1280	1281	1288	rVV7	7781	14790	0.45%	0.067%
39	10.710	1288	1296	1308	rVB2	57034	139142	4.27%	0.630%
40	11.040	1347	1352	1357	rVB8	4307	8436	0.26%	0.038%
41	11.157	1365	1372	1374	rBV8	4038	7703	0.24%	0.035%
42	11.193	1374	1378	1381	rVB6	2685	4444	0.14%	0.020%
43	11.487	1423	1428	1432	rVB7	4610	7611	0.23%	0.034%
44	11.687	1456	1462	1468	rVB6	11406	20756	0.64%	0.094%
45	11.969	1503	1510	1515	rVB10	6302	13067	0.40%	0.059%
46	12.128	1532	1537	1542	rBV	13675	24506	0.75%	0.111%
47	12.451	1587	1592	1598	rVB4	18011	31091	0.95%	0.141%
48	12.545	1601	1608	1613	rVV10	4814	11304	0.35%	0.051%
49	12.604	1613	1618	1622	rVB8	4367	5709	0.18%	0.026%
50	12.840	1653	1658	1665	rVV7	16406	34279	1.05%	0.155%
51	12.910	1665	1670	1674	rVV4	14091	25008	0.77%	0.113%
52	12.951	1674	1677	1683	rVB8	3539	6079	0.19%	0.028%
53	13.004	1683	1686	1689	rBV5	3145	5432	0.17%	0.025%
54	13.122	1697	1706	1717	rBV3	35746	86550	2.66%	0.392%
55	13.251	1720	1728	1734	rBV	23149	36290	1.11%	0.164%
56	13.387	1746	1751	1753	rBV5	8940	13584	0.42%	0.062%
57	13.428	1753	1758	1762	rVV2	29084	48931	1.50%	0.222%
58	13.469	1762	1765	1770	rVB3	12130	18854	0.58%	0.085%
59	13.545	1773	1778	1781	rBV7	11189	18125	0.56%	0.082%
60	13.587	1781	1785	1789	rVB6	6603	9446	0.29%	0.043%
61	13.834	1821	1827	1832	rBV	136232	179905	5.52%	0.815%
62	13.963	1846	1849	1853	rBV5	4905	5717	0.18%	0.026%
63	14.010	1853	1857	1859	rVV5	4358	5013	0.15%	0.023%
64	14.104	1866	1873	1885	rBV	118530	203703	6.25%	0.923%
65	14.192	1885	1888	1892	rVV6	2898	4504	0.14%	0.020%
66	14.416	1915	1926	1934	rBV	1677784	2538704	77.94%	11.497%
67	14.504	1939	1941	1944	rVV4	8430	10622	0.33%	0.048%
68	14.551	1945	1949	1951	rVV5	4309	6794	0.21%	0.031%
69	14.610	1952	1959	1965	rVB5	8800	22643	0.70%	0.103%
70	14.734	1977	1980	1984	rVB5	4564	6097	0.19%	0.028%
71	14.810	1990	1993	1997	rVB2	9463	12354	0.38%	0.056%
72	14.887	2001	2006	2010	rBV7	6357	11380	0.35%	0.052%
73	14.951	2010	2017	2021	rBV9	18820	33941	1.04%	0.154%
74	14.992	2021	2024	2026	rVV4	7713	9404	0.29%	0.043%
75	15.039	2027	2032	2043	rVB	57732	92278	2.83%	0.418%
76	15.245	2061	2067	2071	rVB9	6875	13647	0.42%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006337.D
 Acq On : 26 Jul 2021 14:24
 Operator : CG/JU
 Sample : M3063-02DL 20X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AT9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

77	15.304	2074	2077	2079	rBV4	3635	4818	0.15%	0.022%
78	15.410	2089	2095	2100	rBV	182438	272125	8.35%	1.232%
79	15.463	2100	2104	2109	rVB	30145	42810	1.31%	0.194%
80	15.539	2109	2117	2123	rBV	267378	433171	13.30%	1.962%
81	15.622	2129	2131	2135	rVB4	8851	10293	0.32%	0.047%
82	15.757	2149	2154	2161	rVB10	6243	14245	0.44%	0.065%
83	15.834	2163	2167	2171	rBV7	3432	5611	0.17%	0.025%
84	16.222	2229	2233	2234	rBV4	4784	4669	0.14%	0.021%
85	16.451	2268	2272	2274	rBV3	8461	11039	0.34%	0.050%
86	16.516	2279	2283	2288	rBV5	11965	16068	0.49%	0.073%
87	16.616	2298	2300	2305	rVB6	4997	7204	0.22%	0.033%
88	16.675	2307	2310	2313	rVV5	3831	4623	0.14%	0.021%
89	16.810	2326	2333	2347	rBV	2331691	3257302	100.00%	14.751%
90	16.945	2350	2356	2360	rVV6	15583	33815	1.04%	0.153%
91	17.033	2368	2371	2378	rVB4	12833	17643	0.54%	0.080%
92	17.169	2387	2394	2404	rVB	2021875	2921170	89.68%	13.229%
93	17.263	2404	2410	2418	rBV	199659	295930	9.09%	1.340%
94	17.369	2424	2428	2432	rVB4	12969	15454	0.47%	0.070%
95	18.069	2543	2547	2553	rVB5	25864	35399	1.09%	0.160%
96	19.257	2745	2749	2754	rBV2	52891	66813	2.05%	0.303%
97	19.310	2755	2758	2762	rVB6	19569	25259	0.78%	0.114%
98	19.504	2786	2791	2797	rBV	242540	332639	10.21%	1.506%
99	21.263	3085	3090	3097	rBV	2569116	3152871	96.79%	14.278%
100	23.610	3483	3489	3498	rVB2	1554710	3117802	95.72%	14.120%




Sum of corrected areas: 22081271

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006337.D
Acq On : 26 Jul 2021 14:24
Operator : CG/JU
Sample : M3063-02DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

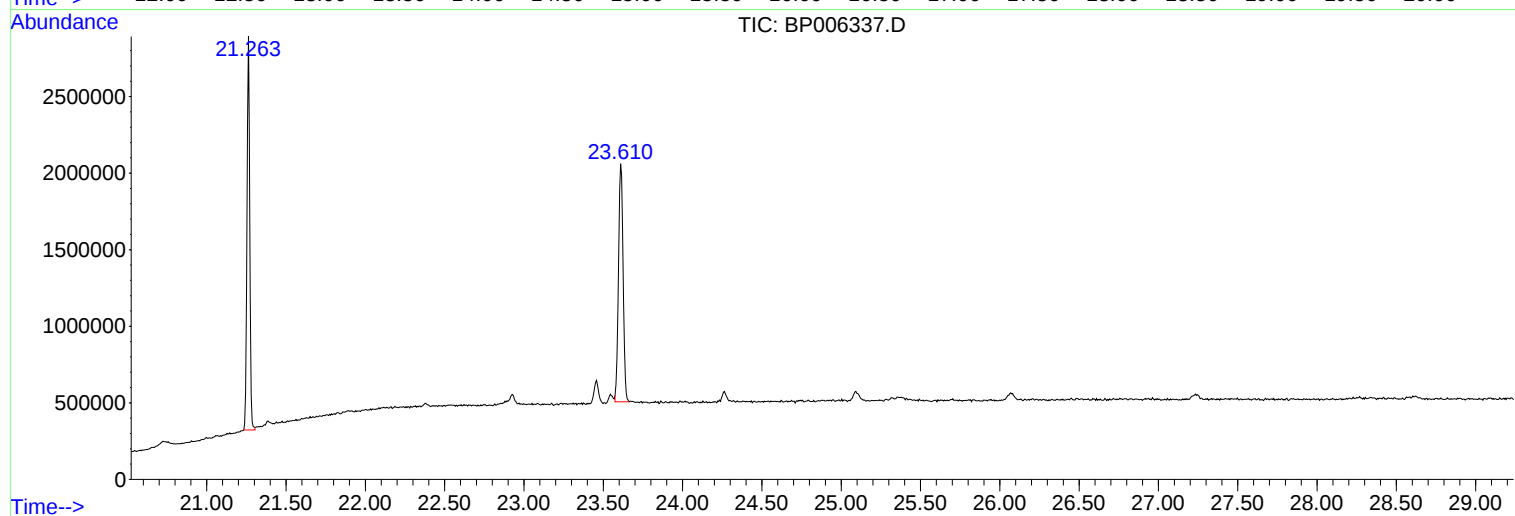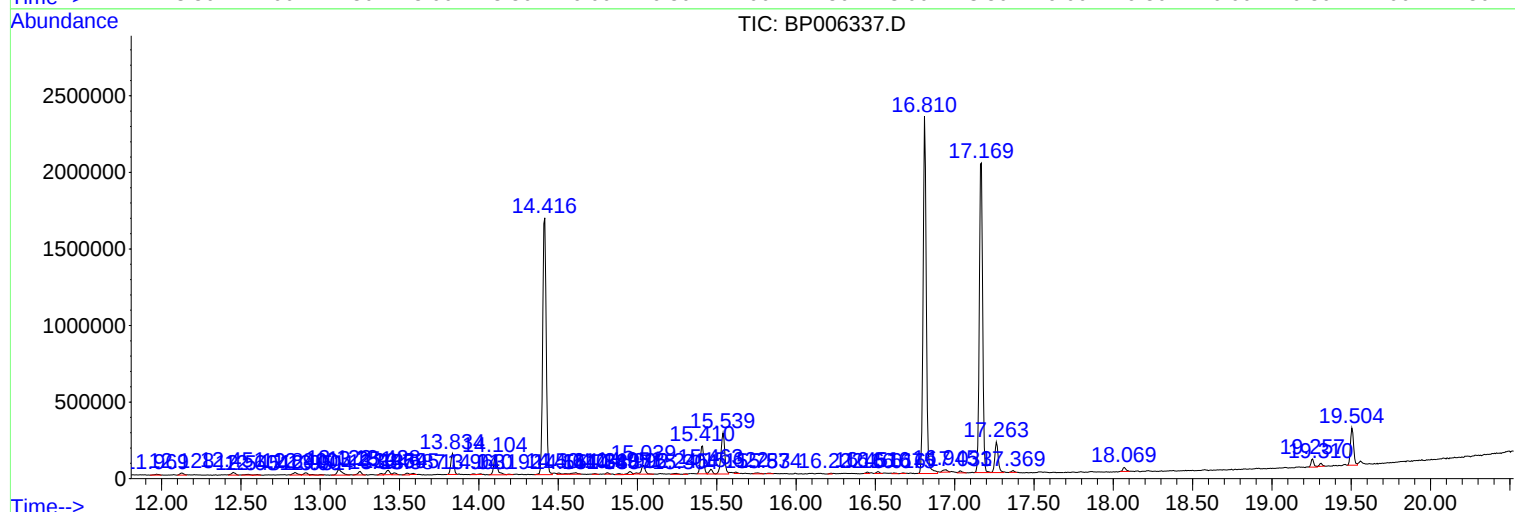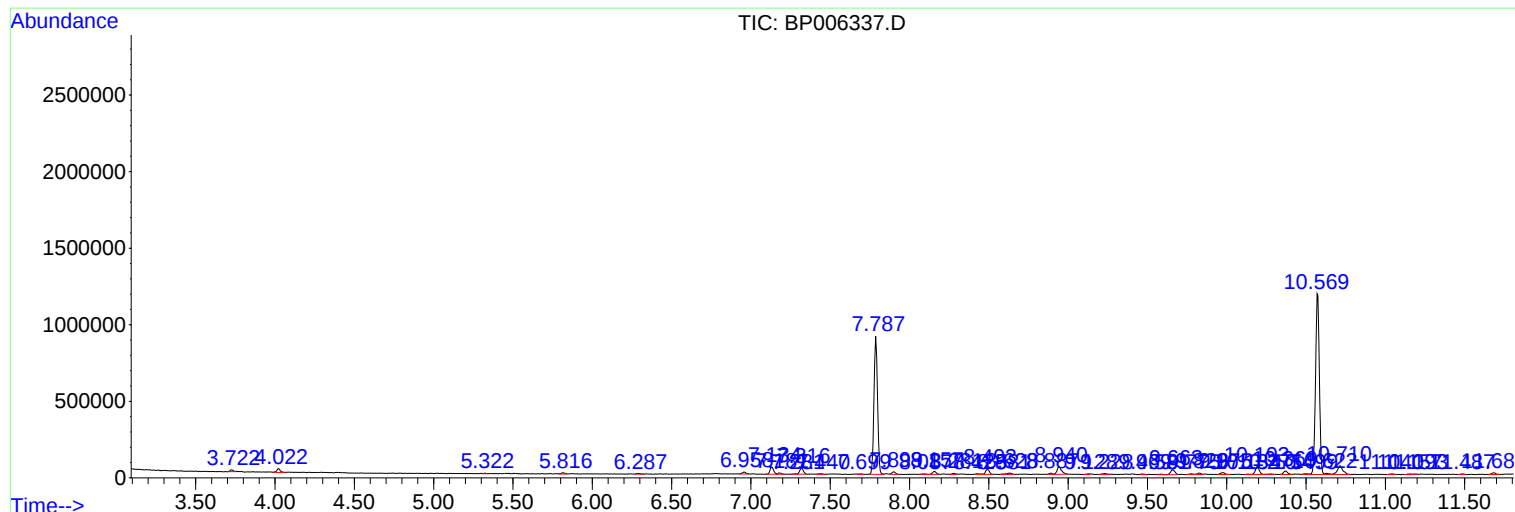

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006337.D
Acq On : 26 Jul 2021 14:24
Operator : CG/JU
Sample : M3063-02DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006337.D
Acq On : 26 Jul 2021 14:24
Operator : CG/JU
Sample : M3063-02DL 20X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AT9DL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
