

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
 Data File : BP006347.D
 Acq On : 26 Jul 2021 20:17
 Operator : CG/JU
 Sample : PB137859BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK859

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
 Title : SVOA CALIBRATION

Signal : TIC: BP006347.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	46	rVB	118974	155463	1.87%	0.168%
2	3.699	100	104	133	rBV	1427491	2267845	27.29%	2.457%
3	4.017	155	158	164	rVB	20659	30781	0.37%	0.033%
4	6.958	651	658	669	rBV	1768320	2734388	32.90%	2.963%
5	7.128	681	687	697	rBV	1374892	2202005	26.50%	2.386%
6	7.322	712	720	730	rBV	1731427	2783036	33.49%	3.016%
7	7.787	792	799	807	rVB	1127910	1748632	21.04%	1.895%
8	8.493	910	919	931	rBV	2191137	3430337	41.27%	3.717%
9	8.940	985	995	1007	rBV	1671126	2711450	32.62%	2.938%
10	9.657	1109	1117	1130	rBV	1335558	2143259	25.79%	2.322%
11	10.193	1200	1208	1221	rBV	1988241	3262390	39.25%	3.535%
12	10.569	1264	1272	1284	rVB	1562807	2612769	31.44%	2.831%
13	10.710	1286	1296	1307	rBV	2177296	3617487	43.53%	3.920%
14	12.157	1535	1542	1548	rBV	40047	66618	0.80%	0.072%
15	12.375	1576	1579	1586	rVB7	5769	9425	0.11%	0.010%
16	13.381	1746	1750	1756	rVB4	9710	15229	0.18%	0.017%
17	13.834	1820	1827	1836	rBV	3649426	5021358	60.42%	5.441%
18	14.104	1866	1873	1884	rBV	3977619	5821146	70.04%	6.308%
19	14.410	1918	1925	1932	rBV	2267195	3363714	40.47%	3.645%
20	14.610	1952	1959	1976	rBV	1949512	2759806	33.21%	2.991%
21	15.410	2087	2095	2103	rBV	4911103	7090186	85.31%	7.683%
22	15.522	2108	2114	2127	rVV	1525190	2080577	25.03%	2.255%
23	15.645	2130	2135	2142	rVB	60559	90396	1.09%	0.098%
24	15.975	2186	2191	2196	rBV8	4734	9882	0.12%	0.011%
25	16.087	2204	2210	2213	rBV7	8603	17102	0.21%	0.019%
26	16.839	2335	2338	2344	rVB7	7828	12667	0.15%	0.014%
27	16.945	2350	2356	2361	rBV3	14420	24465	0.29%	0.027%
28	17.163	2386	2393	2401	rBV	2677016	3802696	45.76%	4.121%
29	17.263	2403	2410	2430	rVV2	5587825	7684918	92.47%	8.328%
30	17.539	2452	2457	2461	rBV3	9474	14154	0.17%	0.015%
31	17.845	2506	2509	2515	rVB7	6353	9829	0.12%	0.011%
32	18.063	2543	2546	2552	rBV7	12095	19232	0.23%	0.021%
33	19.080	2714	2719	2724	rBV3	66498	95014	1.14%	0.103%
34	19.151	2726	2731	2735	rVV	66679	90574	1.09%	0.098%
35	19.504	2785	2791	2799	rBV	6416352	8310979	100.00%	9.006%
36	21.263	3084	3090	3096	rBV	3002764	3952905	47.56%	4.283%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006347.D
Acq On : 26 Jul 2021 20:17
Operator : CG/JU
Sample : PB137859BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Title : SVOA CALIBRATION

37	23.457	3456	3463	3472	rVB2	4255120	8139091	97.93%	8.820%
38	23.610	3482	3489	3503	rVB2	2011781	4081446	49.11%	4.423%


Sum of corrected areas: 92283251

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006347.D
Acq On : 26 Jul 2021 20:17
Operator : CG/JU
Sample : PB137859BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

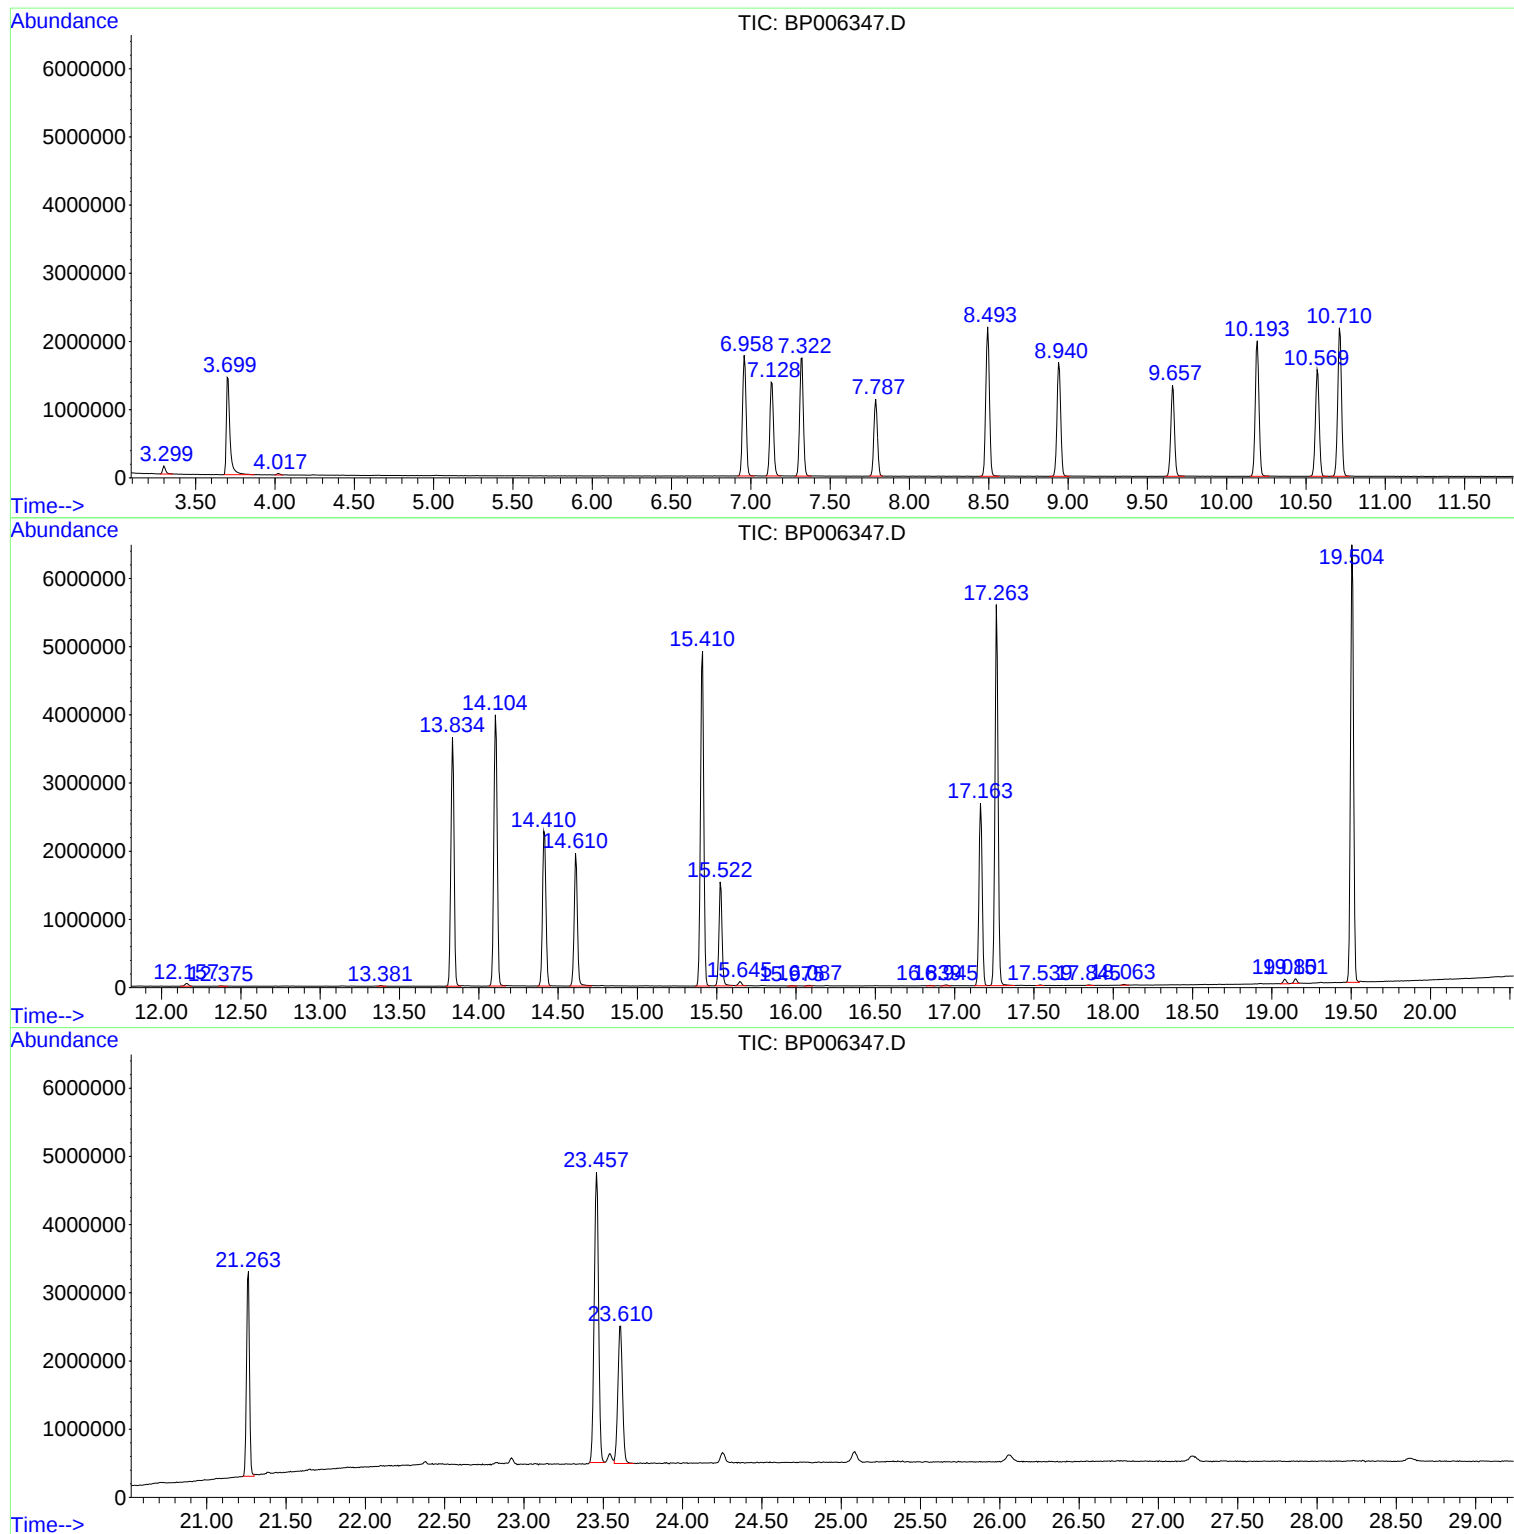

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006347.D
Acq On : 26 Jul 2021 20:17
Operator : CG/JU
Sample : PB137859BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072621\
Data File : BP006347.D
Acq On : 26 Jul 2021 20:17
Operator : CG/JU
Sample : PB137859BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK859

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SFAM-EPA-BP072421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
