

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011103.D
 Acq On : 26 Jul 2022 11:02
 Operator : CG/JU
 Sample : PB146404BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK404

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011103.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	24	rVB	186581	258027	2.48%	0.212%
2	3.569	78	82	103	rBV	2264925	3095084	29.78%	2.540%
3	3.881	132	135	140	rVB	43274	53747	0.52%	0.044%
4	6.840	631	638	653	rBV	2280634	3523000	33.89%	2.892%
5	7.005	660	666	680	rVB	1982304	3086303	29.69%	2.533%
6	7.193	692	698	711	rBV	2329017	3666415	35.27%	3.009%
7	7.663	770	778	790	rBV	1686357	2633032	25.33%	2.161%
8	8.381	893	900	918	rBV	2854657	4627015	44.51%	3.798%
9	8.828	967	976	984	rBV	2326982	3809807	36.65%	3.127%
10	9.546	1088	1098	1111	rBV	1910867	3094770	29.77%	2.540%
11	10.081	1179	1189	1202	rBV	2659565	4517031	43.46%	3.708%
12	10.457	1244	1253	1262	rBV	2461079	4116905	39.61%	3.379%
13	10.604	1270	1278	1301	rBV	2959721	4995523	48.06%	4.100%
14	12.057	1520	1525	1533	rBV2	37368	78505	0.76%	0.064%
15	13.292	1728	1735	1744	rVB8	8908	20683	0.20%	0.017%
16	13.745	1805	1812	1825	rBV	5300767	7553111	72.66%	6.200%
17	13.839	1825	1828	1833	rVB7	7235	14650	0.14%	0.012%
18	14.016	1849	1858	1873	rBV	6013946	8552043	82.27%	7.019%
19	14.328	1904	1911	1919	rBV	3772700	5426225	52.20%	4.454%
20	14.545	1941	1948	1970	rBV	1948476	3145573	30.26%	2.582%
21	15.328	2074	2081	2095	rBV	7456082	10394698	100.00%	8.532%
22	15.451	2096	2102	2117	rVV	2276349	3206508	30.85%	2.632%
23	15.569	2117	2122	2129	rVB	91546	141100	1.36%	0.116%
24	15.892	2172	2177	2182	rBV8	6385	11056	0.11%	0.009%
25	16.033	2196	2201	2206	rVB9	6225	12913	0.12%	0.011%
26	16.116	2210	2215	2221	rVB3	26681	39551	0.38%	0.032%
27	16.769	2321	2326	2332	rBV5	14196	23555	0.23%	0.019%
28	16.875	2340	2344	2351	rBV5	13023	24704	0.24%	0.020%
29	17.092	2374	2381	2391	rBV	4130239	5779300	55.60%	4.744%
30	17.192	2391	2398	2413	rVV2	7317549	10336797	99.44%	8.484%
31	17.780	2494	2498	2502	rBV7	11151	16677	0.16%	0.014%
32	19.022	2705	2709	2716	rBV2	83075	113583	1.09%	0.093%
33	19.092	2717	2721	2726	rBV	70792	104875	1.01%	0.086%
34	19.451	2776	2782	2790	rBV	7724502	10043050	96.62%	8.243%
35	21.210	3077	3081	3089	rBV	3268279	4133787	39.77%	3.393%
36	23.404	3447	3454	3462	rBV2	3832294	7401257	71.20%	6.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011103.D
Acq On : 26 Jul 2022 11:02
Operator : CG/JU
Sample : PB146404BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK404

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37 23.557 3474 3480 3488 rVB2 1849205 3782858 36.39% 3.105%




Sum of corrected areas: 121833718

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011103.D
Acq On : 26 Jul 2022 11:02
Operator : CG/JU
Sample : PB146404BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

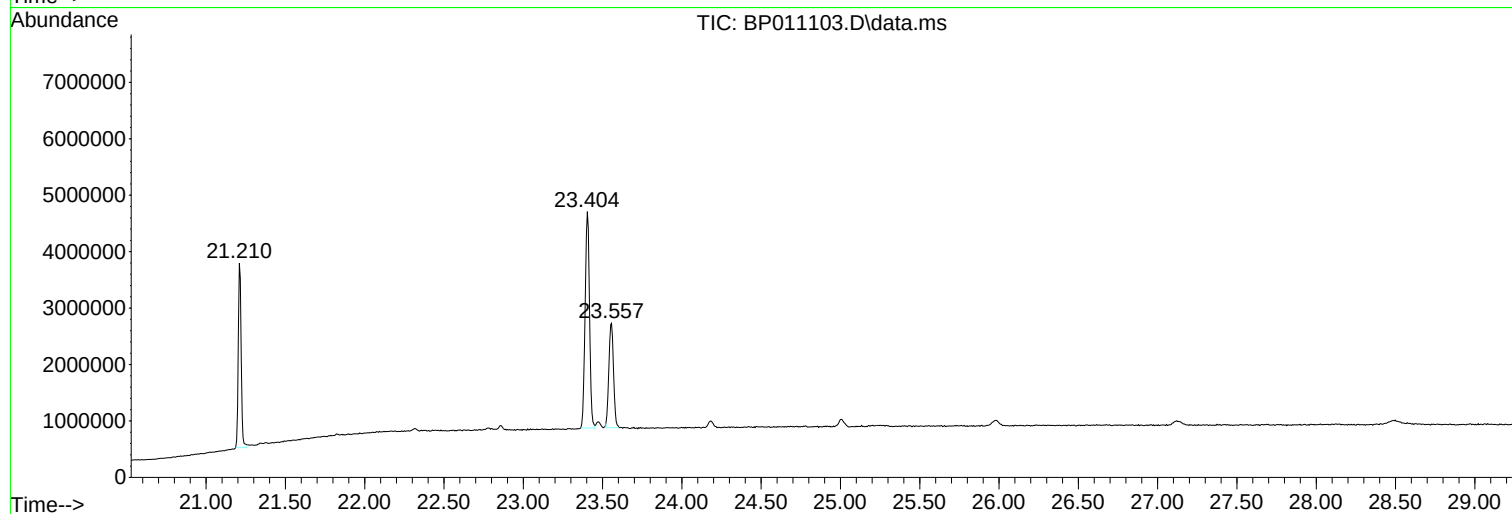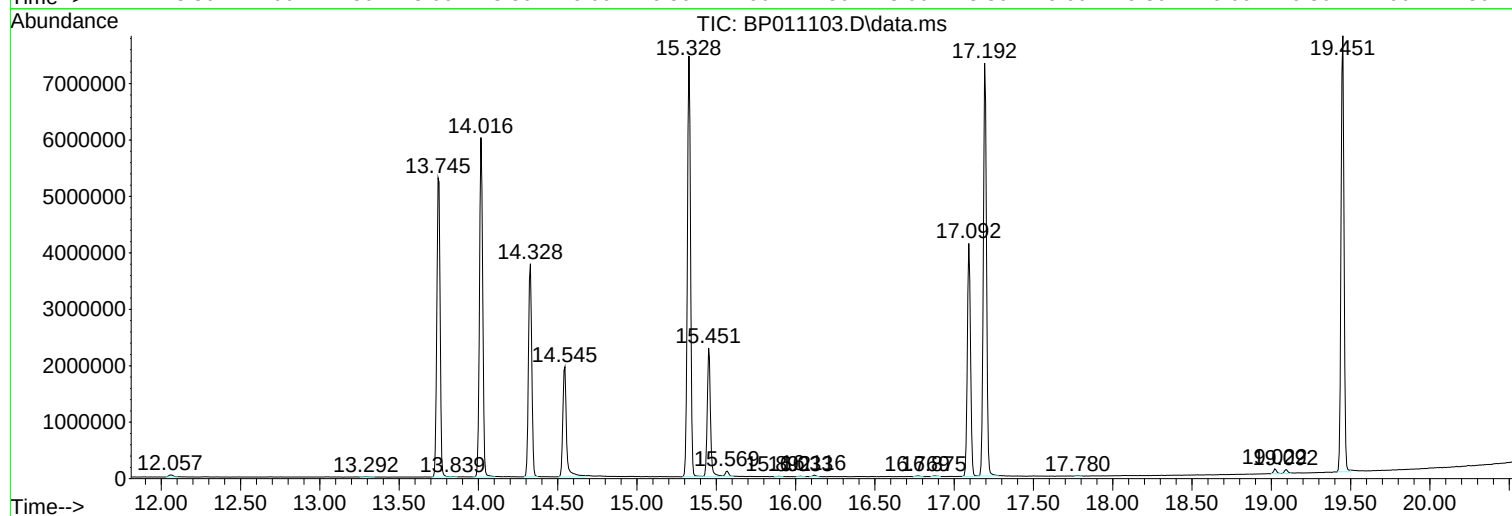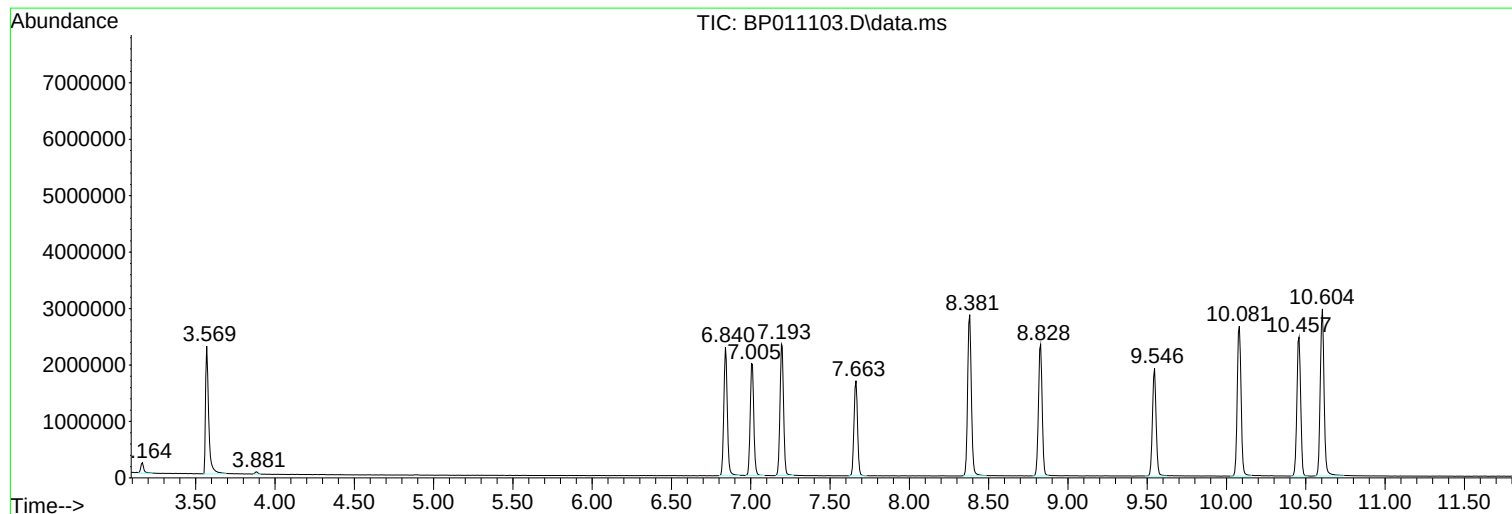

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011103.D
Acq On : 26 Jul 2022 11:02
Operator : CG/JU
Sample : PB146404BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011103.D
Acq On : 26 Jul 2022 11:02
Operator : CG/JU
Sample : PB146404BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK404

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc