

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011104.D
 Acq On : 26 Jul 2022 11:36
 Operator : CG/JU
 Sample : PB146366BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK366

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	19	rVB	179837	210084	2.19%	0.188%
2	3.570	78	82	100	rBV	2218373	3016991	31.43%	2.707%
3	3.881	131	135	140	rVB	43519	56258	0.59%	0.050%
4	6.840	632	638	655	rBV	2179559	3408573	35.51%	3.058%
5	7.011	660	667	680	rVB	1886052	2978017	31.02%	2.672%
6	7.193	691	698	710	rBV	2263490	3560948	37.10%	3.195%
7	7.663	771	778	788	rBV	1597188	2444540	25.47%	2.193%
8	8.381	892	900	913	rBV	2757937	4449150	46.35%	3.992%
9	8.828	968	976	984	rBV	2279093	3650090	38.02%	3.275%
10	9.546	1090	1098	1109	rBV	1807697	2940046	30.63%	2.638%
11	10.081	1181	1189	1208	rBV	2631139	4311558	44.92%	3.869%
12	10.457	1244	1253	1262	rBV	2312801	3800557	39.59%	3.410%
13	10.604	1269	1278	1298	rBV	2710540	4780676	49.80%	4.289%
14	12.057	1519	1525	1535	rBV2	37158	80159	0.84%	0.072%
15	13.293	1729	1735	1741	rVB5	7719	14245	0.15%	0.013%
16	13.745	1805	1812	1826	rBV	5037347	6979222	72.71%	6.262%
17	13.840	1826	1828	1835	rVB8	7960	13623	0.14%	0.012%
18	14.016	1850	1858	1870	rBV	5557986	7977563	83.11%	7.158%
19	14.328	1904	1911	1923	rBV	3370391	4855015	50.58%	4.356%
20	14.540	1941	1947	1964	rBV	1666960	2737482	28.52%	2.456%
21	15.328	2074	2081	2096	rBV	7007859	9599355	100.00%	8.613%
22	15.451	2096	2102	2117	rVV	1993383	2803439	29.20%	2.515%
23	15.569	2117	2122	2131	rVB	83380	134103	1.40%	0.120%
24	15.898	2174	2178	2182	rBV5	7222	10249	0.11%	0.009%
25	16.022	2195	2199	2209	rVB5	7647	15628	0.16%	0.014%
26	16.116	2211	2215	2220	rVB3	23456	34937	0.36%	0.031%
27	16.769	2322	2326	2332	rVB4	13963	19317	0.20%	0.017%
28	16.881	2340	2345	2349	rBV5	10193	17231	0.18%	0.015%
29	17.092	2374	2381	2391	rBV	3633577	4938769	51.45%	4.431%
30	17.192	2391	2398	2415	rVV2	6664604	9219105	96.04%	8.272%
31	19.022	2705	2709	2716	rBV	70592	100487	1.05%	0.090%
32	19.092	2717	2721	2729	rVV	62035	95307	0.99%	0.086%
33	19.451	2776	2782	2790	rBV	6290841	8580780	89.39%	7.699%
34	21.210	3077	3081	3090	rBV2	2750113	3396521	35.38%	3.048%
35	23.404	3447	3454	3461	rBV2	3592280	6812297	70.97%	6.112%
36	23.551	3473	3479	3490	rVB2	1762096	3409727	35.52%	3.059%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011104.D
Acq On : 26 Jul 2022 11:36
Operator : CG/JU
Sample : PB146366BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION




Sum of corrected areas: 111452049

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011104.D
Acq On : 26 Jul 2022 11:36
Operator : CG/JU
Sample : PB146366BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

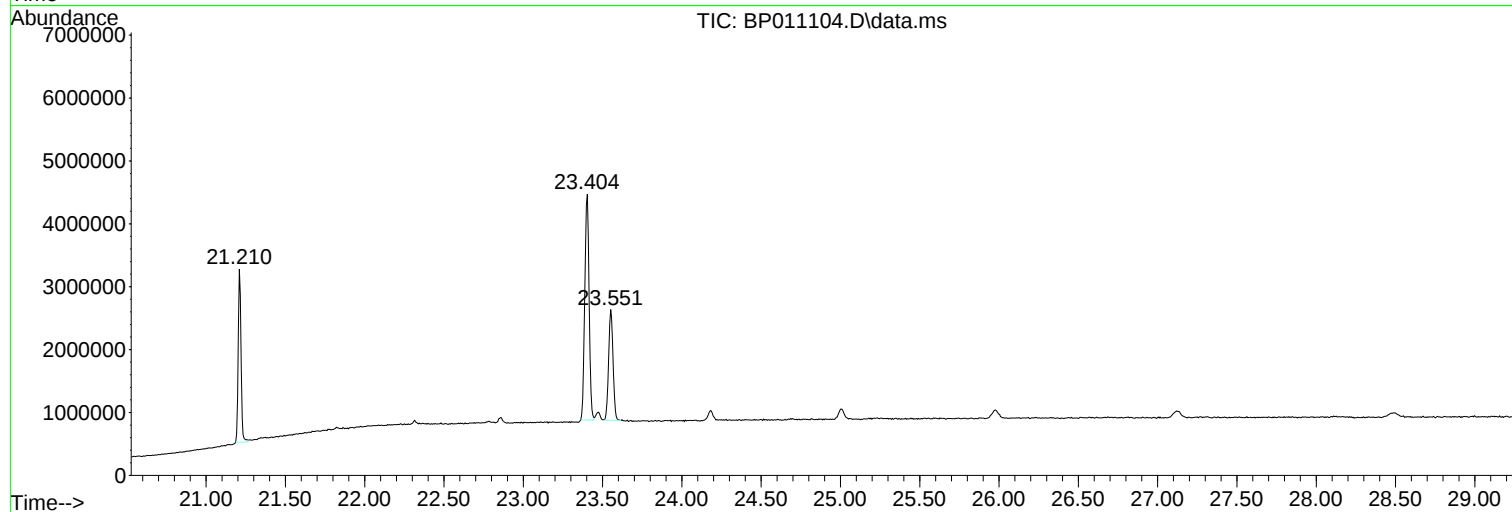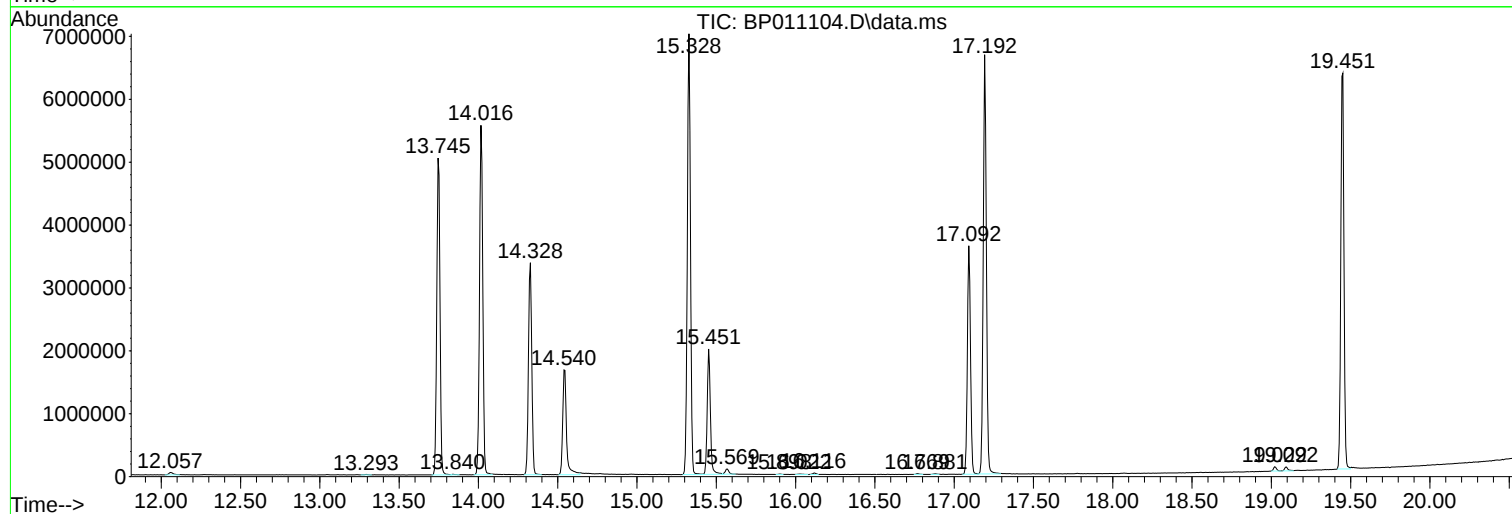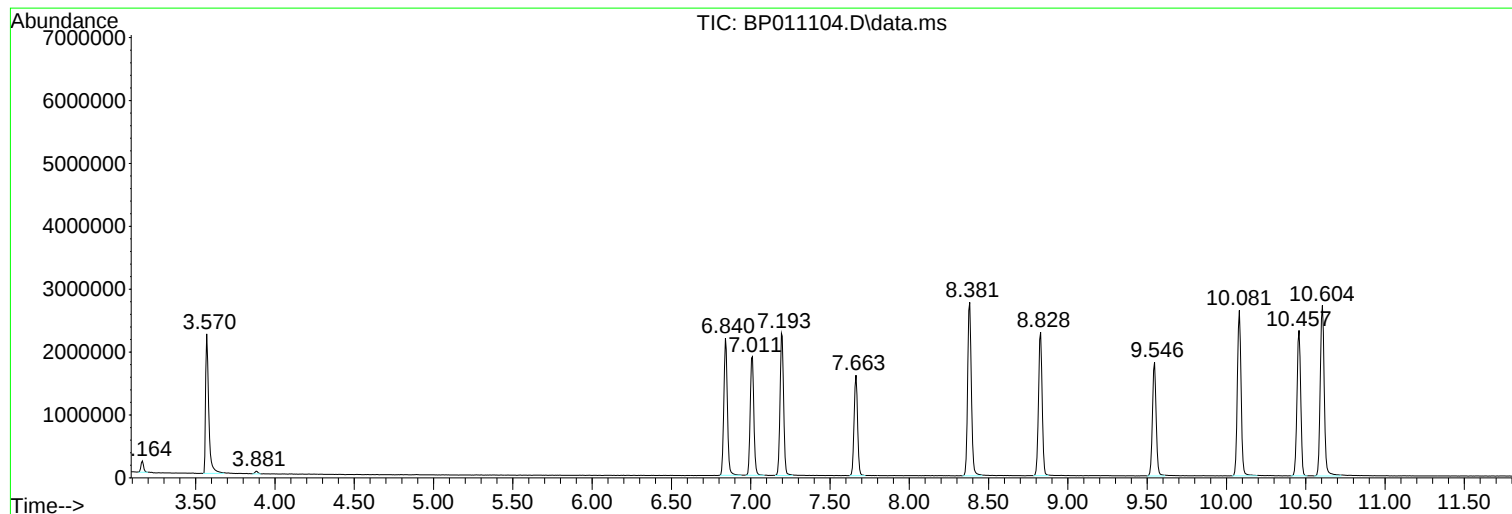

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011104.D
Acq On : 26 Jul 2022 11:36
Operator : CG/JU
Sample : PB146366BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.193	29.13 ng/ul	3560950	1,4-Dichlorobenzene-d4	7.663

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27		
2	3-(Chloromethyl)-5-isobutyl-1,2,...	174	C7H11ClN2O	189130-85-6	25		
3	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16		
4	5-Aminoindole	132	C8H8N2	005192-03-0	12		
5	1H-Indol-6-amine	132	C8H8N2	005318-27-4	12		

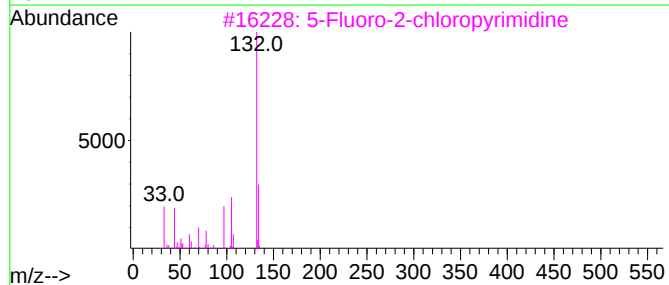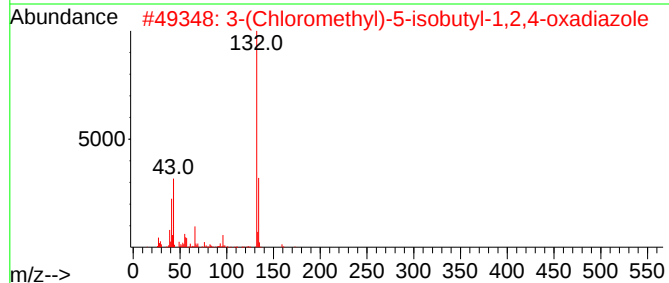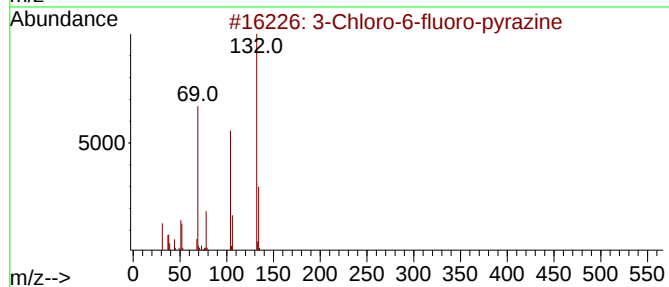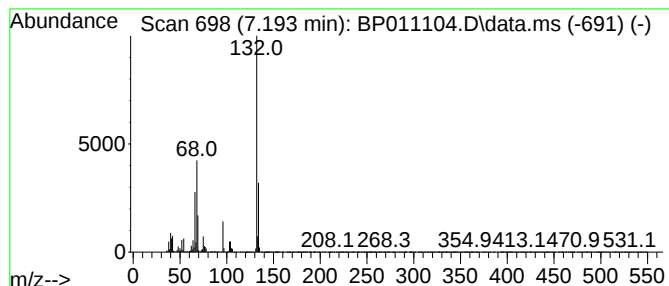

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011104.D
Acq On : 26 Jul 2022 11:36
Operator : CG/JU
Sample : PB146366BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK366

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.193	29.1	ng/ul	3560950	1	7.663	2444540	20.0