

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011105.D
 Acq On : 26 Jul 2022 12:11
 Operator : CG/JU
 Sample : N3801-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011105.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	4	7	10	rBV	36772	40684	0.33%	0.032%
2	3.164	10	13	18	rVB	156677	175534	1.43%	0.139%
3	3.575	81	83	99	rBV	598908	831933	6.79%	0.661%
4	3.793	114	120	127	rVV	73569	116366	0.95%	0.092%
5	3.881	131	135	141	rVB	55540	72085	0.59%	0.057%
6	4.399	218	223	226	rBV3	15570	25092	0.20%	0.020%
7	4.793	286	290	296	rVB2	12068	17582	0.14%	0.014%
8	4.969	315	320	324	rVB2	23032	33250	0.27%	0.026%
9	5.387	386	391	398	rVB2	16003	27908	0.23%	0.022%
10	6.840	629	638	655	rVB	556341	887075	7.24%	0.704%
11	7.005	659	666	679	rBV	2334497	3628180	29.62%	2.881%
12	7.193	691	698	710	rBV	2111722	3316122	27.07%	2.633%
13	7.287	710	714	719	rVB6	13381	24491	0.20%	0.019%
14	7.663	771	778	790	rBV	1962373	3037364	24.79%	2.412%
15	8.381	893	900	914	rBV	1617525	2670425	21.80%	2.121%
16	8.828	968	976	985	rBV	2787259	4494346	36.69%	3.569%
17	9.240	1041	1046	1050	rBV2	32561	47981	0.39%	0.038%
18	9.546	1090	1098	1109	rBV	2202047	3505656	28.62%	2.784%
19	10.081	1180	1189	1210	rBV	2958592	4887289	39.89%	3.881%
20	10.457	1242	1253	1263	rBV	2865474	4674485	38.16%	3.712%
21	10.604	1269	1278	1303	rBV	2801169	4805413	39.22%	3.816%
22	11.740	1466	1471	1477	rBV	38552	60547	0.49%	0.048%
23	12.057	1518	1525	1533	rBV2	51717	96654	0.79%	0.077%
24	12.146	1535	1540	1542	rBV4	12136	23428	0.19%	0.019%
25	12.940	1669	1675	1678	rBV7	8075	14535	0.12%	0.012%
26	13.234	1719	1725	1731	rBV5	11170	20450	0.17%	0.016%
27	13.751	1806	1813	1823	rBV	6234971	8737955	71.32%	6.939%
28	13.840	1826	1828	1834	rVB6	8160	14551	0.12%	0.012%
29	14.016	1851	1858	1878	rBV	6772425	10088278	82.35%	8.011%
30	14.328	1903	1911	1920	rBV	4177254	5931589	48.42%	4.710%
31	14.545	1942	1948	1967	rBV	262188	526846	4.30%	0.418%
32	14.692	1971	1973	1979	rVV6	12095	23723	0.19%	0.019%
33	14.769	1981	1986	1993	rVB9	19710	35430	0.29%	0.028%
34	15.139	2046	2049	2052	rBV2	11251	15327	0.13%	0.012%
35	15.192	2056	2058	2063	rVB3	10469	12744	0.10%	0.010%
36	15.328	2074	2081	2091	rBV	8778487	12250983	100.00%	9.728%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011105.D
 Acq On : 26 Jul 2022 12:11
 Operator : CG/JU
 Sample : N3801-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.451	2096	2102	2117	rVV	2734147	3732666	30.47%	2.964%
38	15.569	2117	2122	2132	rVB	108112	175077	1.43%	0.139%
39	16.016	2191	2198	2200	rBV7	11111	18521	0.15%	0.015%
40	16.063	2202	2206	2211	rVV5	19567	36489	0.30%	0.029%
41	16.116	2211	2215	2221	rVB2	31407	46520	0.38%	0.037%
42	16.769	2322	2326	2333	rVB8	16026	25846	0.21%	0.021%
43	16.869	2339	2343	2350	rBV3	19918	34294	0.28%	0.027%
44	17.092	2374	2381	2391	rBV	4190110	5939830	48.48%	4.717%
45	17.192	2392	2398	2413	rVV2	8309725	11771811	96.09%	9.348%
46	17.398	2429	2433	2437	rVB2	11447	17026	0.14%	0.014%
47	17.610	2466	2469	2475	rBV7	9088	14876	0.12%	0.012%
48	17.775	2494	2497	2502	rVB7	11188	16431	0.13%	0.013%
49	18.075	2545	2548	2552	rVB	14079	17518	0.14%	0.014%
50	18.463	2612	2614	2619	rBV5	9180	12886	0.11%	0.010%
51	19.022	2705	2709	2714	rBV2	97229	123312	1.01%	0.098%
52	19.092	2717	2721	2727	rVV	89561	121407	0.99%	0.096%
53	19.157	2730	2732	2737	rVV6	15492	18796	0.15%	0.015%
54	19.392	2770	2772	2775	rVB2	21447	19428	0.16%	0.015%
55	19.445	2776	2781	2789	rBV	8403607	11107627	90.67%	8.820%
56	21.210	3076	3081	3089	rBV	3315134	4202373	34.30%	3.337%
57	23.404	3447	3454	3461	rBV2	4885259	9048933	73.86%	7.186%
58	23.551	3473	3479	3491	rVB2	2135487	4257558	34.75%	3.381%




Sum of corrected areas: 125931526

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011105.D
Acq On : 26 Jul 2022 12:11
Operator : CG/JU
Sample : N3801-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

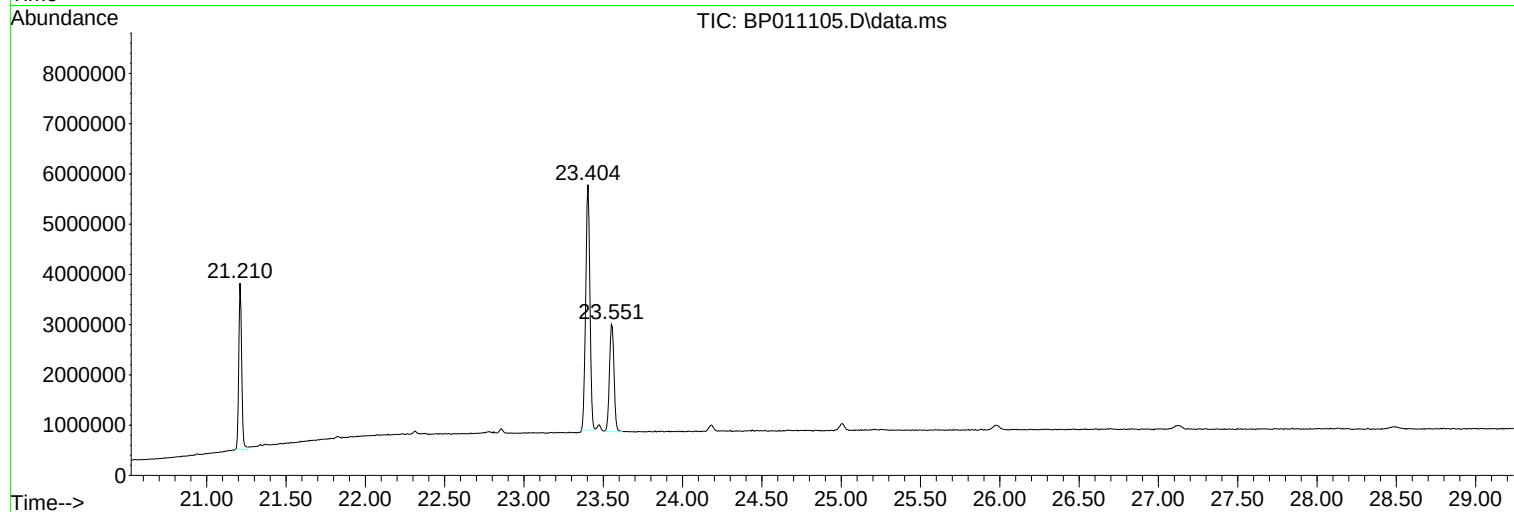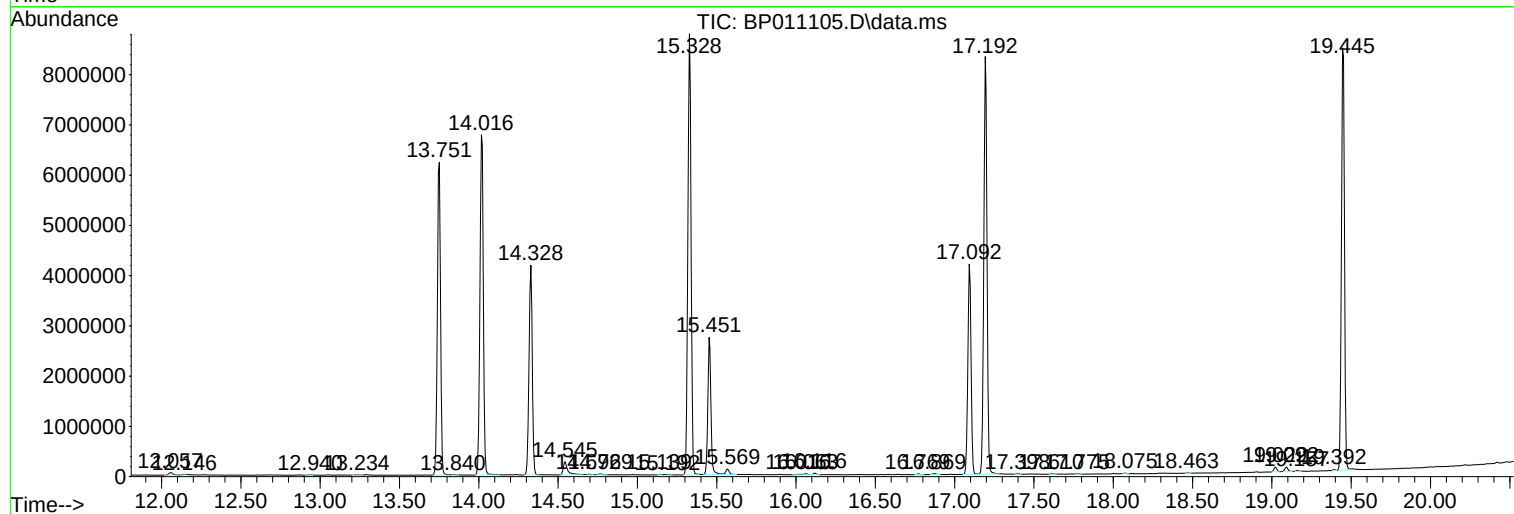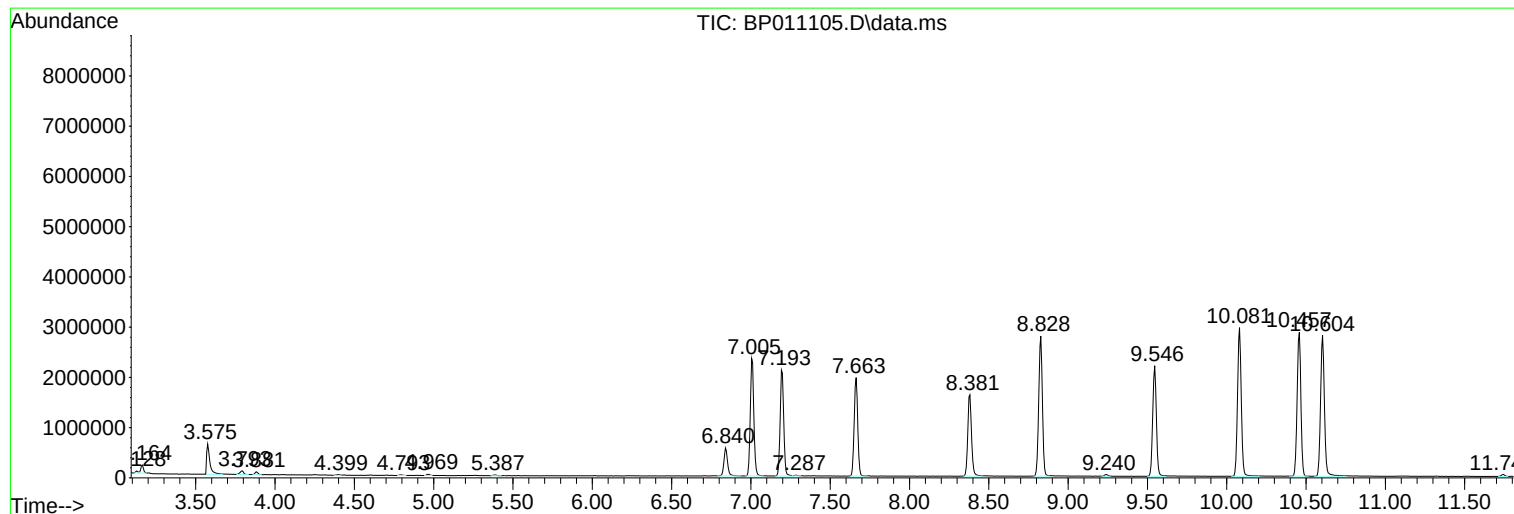

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011105.D
Acq On : 26 Jul 2022 12:11
Operator : CG/JU
Sample : N3801-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011105.D
Acq On : 26 Jul 2022 12:11
Operator : CG/JU
Sample : N3801-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc