

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011106.D
 Acq On : 26 Jul 2022 12:45
 Operator : CG/JU
 Sample : N3801-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011106.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	23	rVB	147560	200254	1.85%	0.172%
2	3.576	81	83	102	rVB	596172	837170	7.74%	0.720%
3	3.793	115	120	124	rVB	65357	92403	0.85%	0.080%
4	3.881	132	135	141	rVB	44165	61361	0.57%	0.053%
5	4.705	272	275	280	rVB5	7190	10941	0.10%	0.009%
6	4.787	286	289	298	rVB5	10243	18659	0.17%	0.016%
7	5.270	367	371	376	rVB	8558	15337	0.14%	0.013%
8	5.387	387	391	398	rVB	15209	23386	0.22%	0.020%
9	6.840	632	638	651	rVB	520458	841870	7.78%	0.724%
10	7.005	660	666	678	rBV	2088301	3256822	30.11%	2.803%
11	7.105	679	683	688	rVV	11299	17992	0.17%	0.015%
12	7.193	692	698	709	rVV	1962028	3060048	28.29%	2.633%
13	7.287	711	714	724	rVB9	12823	25002	0.23%	0.022%
14	7.664	770	778	786	rBV	1982653	3094433	28.61%	2.663%
15	7.734	786	790	795	rVB3	11606	19502	0.18%	0.017%
16	8.375	892	899	912	rBV	1549200	2561441	23.68%	2.204%
17	8.828	968	976	984	rBV	2507406	4054118	37.48%	3.489%
18	9.240	1039	1046	1053	rBV	64966	106458	0.98%	0.092%
19	9.546	1090	1098	1111	rBV	1959696	3166752	29.28%	2.725%
20	10.081	1180	1189	1201	rBV	2759007	4621814	42.73%	3.977%
21	10.246	1212	1217	1236	rVB5	40665	118423	1.09%	0.102%
22	10.458	1244	1253	1262	rBV	2899253	4815981	44.52%	4.144%
23	10.605	1268	1278	1294	rBV	1680050	2972908	27.49%	2.558%
24	11.116	1361	1365	1372	rVB4	11328	21740	0.20%	0.019%
25	11.252	1381	1388	1402	rBV3	27444	69628	0.64%	0.060%
26	11.740	1464	1471	1477	rVB	38495	66714	0.62%	0.057%
27	11.846	1483	1489	1493	rBV9	6795	13651	0.13%	0.012%
28	12.057	1517	1525	1531	rBV	50260	82414	0.76%	0.071%
29	12.269	1557	1561	1567	rVB8	5777	10917	0.10%	0.009%
30	12.681	1625	1631	1635	rBV3	19382	35569	0.33%	0.031%
31	12.769	1641	1646	1649	rBV3	10643	21471	0.20%	0.018%
32	12.934	1667	1674	1683	rVB5	29286	53529	0.49%	0.046%
33	13.151	1706	1711	1717	rVB3	20165	28030	0.26%	0.024%
34	13.228	1717	1724	1730	rBV3	15226	31271	0.29%	0.027%
35	13.287	1730	1734	1739	rVB3	9009	14844	0.14%	0.013%
36	13.640	1788	1794	1800	rBV10	7331	18699	0.17%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011106.D
 Acq On : 26 Jul 2022 12:45
 Operator : CG/JU
 Sample : N3801-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHY2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	13.746	1805	1812	1822	rBV	5449078	7760454	71.75%	6.678%
38	13.857	1828	1831	1839	rVB9	13461	24527	0.23%	0.021%
39	14.016	1850	1858	1872	rBV	6166353	8885656	82.15%	7.647%
40	14.128	1872	1877	1885	rVB	61914	117472	1.09%	0.101%
41	14.234	1892	1895	1899	rVB2	18074	23987	0.22%	0.021%
42	14.328	1904	1911	1922	rBV	4258480	6166122	57.01%	5.306%
43	14.546	1942	1948	1964	rBV	231586	464303	4.29%	0.400%
44	14.698	1969	1974	1982	rVV	152830	269560	2.49%	0.232%
45	14.763	1982	1985	1992	rVB8	22355	32234	0.30%	0.028%
46	15.146	2043	2050	2056	rBV	144322	208349	1.93%	0.179%
47	15.198	2056	2059	2064	rVB2	14532	19397	0.18%	0.017%
48	15.328	2074	2081	2088	rBV	7686326	10816393	100.00%	9.308%
49	15.451	2096	2102	2117	rBV	2488003	3246079	30.01%	2.793%
50	15.569	2117	2122	2128	rVV	96064	150770	1.39%	0.130%
51	15.622	2128	2131	2136	rVB6	10792	13541	0.13%	0.012%
52	15.710	2143	2146	2152	rVB8	8847	10868	0.10%	0.009%
53	15.816	2161	2164	2169	rVB7	7809	12555	0.12%	0.011%
54	15.898	2174	2178	2184	rBV8	10175	19437	0.18%	0.017%
55	16.028	2194	2200	2204	rBV8	18252	38901	0.36%	0.033%
56	16.122	2211	2216	2220	rVV4	22561	35063	0.32%	0.030%
57	16.345	2247	2254	2257	rBV8	16075	25276	0.23%	0.022%
58	16.563	2286	2291	2300	rVB8	12168	27768	0.26%	0.024%
59	16.769	2318	2326	2333	rBV8	18821	42896	0.40%	0.037%
60	16.869	2339	2343	2348	rBV3	17663	38153	0.35%	0.033%
61	16.975	2358	2361	2365	rVB4	12356	15272	0.14%	0.013%
62	17.092	2374	2381	2391	rBV	4556020	6292186	58.17%	5.415%
63	17.192	2391	2398	2413	rBV2	7235812	10412843	96.27%	8.961%
64	17.398	2429	2433	2440	rVB2	22139	36599	0.34%	0.031%
65	17.492	2444	2449	2453	rBV7	11530	22990	0.21%	0.020%
66	17.722	2485	2488	2493	rBV5	13241	17827	0.16%	0.015%
67	17.781	2495	2498	2505	rVV9	12506	18286	0.17%	0.016%
68	18.004	2531	2536	2543	rBV	65537	119027	1.10%	0.102%
69	18.075	2545	2548	2554	rVB	52360	67953	0.63%	0.058%
70	18.239	2570	2576	2580	rBV9	17004	33394	0.31%	0.029%
71	18.287	2582	2584	2587	rVV4	13630	13779	0.13%	0.012%
72	19.022	2705	2709	2714	rBV2	82321	108611	1.00%	0.093%
73	19.092	2717	2721	2725	rVV	72902	100996	0.93%	0.087%
74	19.398	2770	2773	2776	rVB5	41729	43055	0.40%	0.037%
75	19.451	2776	2782	2789	rBV	7589839	9861065	91.17%	8.486%
76	20.945	3033	3036	3043	rBV4	132143	208210	1.92%	0.179%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011106.D
Acq On : 26 Jul 2022 12:45
Operator : CG/JU
Sample : N3801-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

77	21.210	3077	3081	3088	rBV	3427656	4203946	38.87%	3.618%
78	23.404	3447	3454	3462	rBV2	4010405	7404385	68.46%	6.372%
79	23.551	3473	3479	3494	rVB2	2185145	4312365	39.87%	3.711%



Sum of corrected areas: 116204102

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011106.D
Acq On : 26 Jul 2022 12:45
Operator : CG/JU
Sample : N3801-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

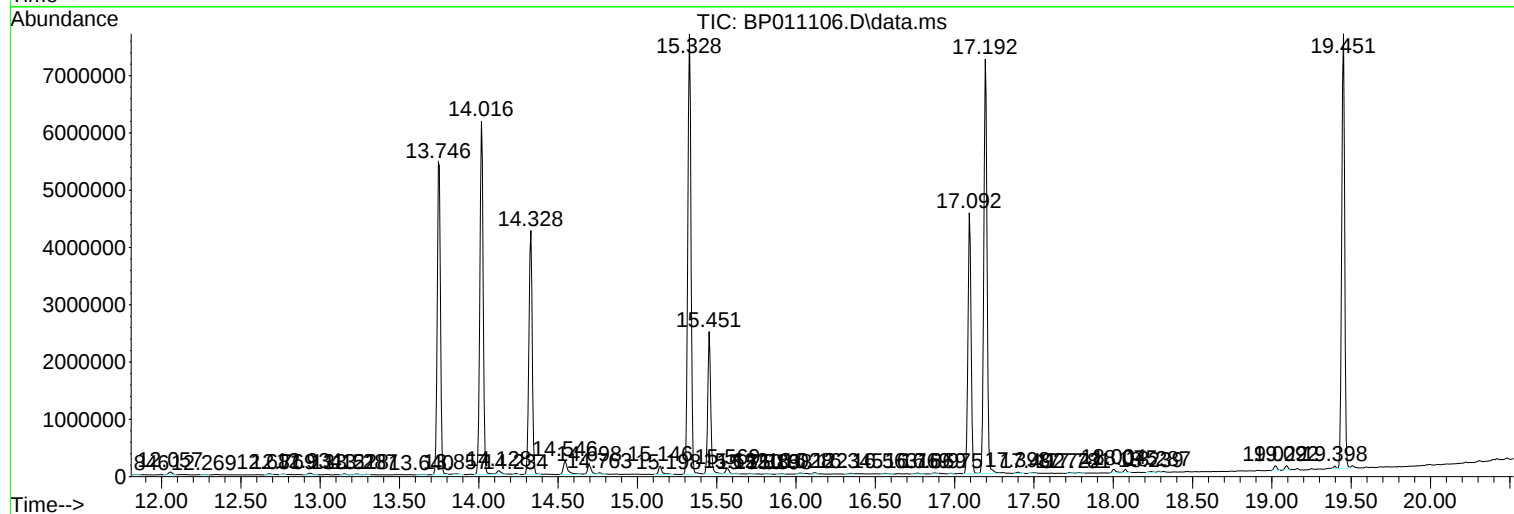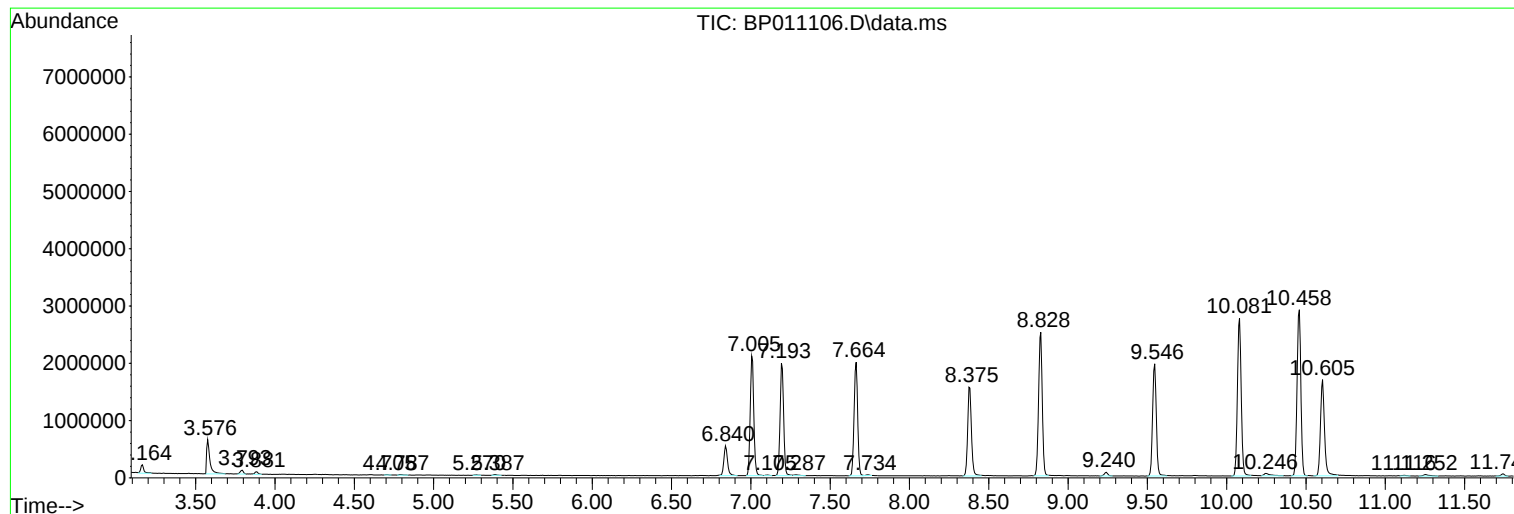

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011106.D
Acq On : 26 Jul 2022 12:45
Operator : CG/JU
Sample : N3801-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011106.D
Acq On : 26 Jul 2022 12:45
Operator : CG/JU
Sample : N3801-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHY2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------