

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011107.D
 Acq On : 26 Jul 2022 13:20
 Operator : CG/JU
 Sample : N3801-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011107.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.164	9	13	24	rVB	143790	192969	2.02%	0.179%
2	3.575	80	83	104	rVB	632323	890283	9.30%	0.824%
3	3.793	115	120	127	rVB	72384	102181	1.07%	0.095%
4	3.881	132	135	141	rVB	44049	51567	0.54%	0.048%
5	4.393	220	222	227	rVB2	19534	23467	0.25%	0.022%
6	4.793	286	290	295	rBV5	10016	18682	0.20%	0.017%
7	5.263	367	370	374	rVB4	8921	12905	0.13%	0.012%
8	5.387	384	391	394	rBV	14618	22909	0.24%	0.021%
9	6.840	632	638	650	rVB	443009	698508	7.30%	0.647%
10	7.005	660	666	679	rBV	1974806	3130427	32.70%	2.898%
11	7.193	692	698	709	rBV	1802944	2851281	29.79%	2.640%
12	7.287	711	714	721	rVB4	13858	22775	0.24%	0.021%
13	7.663	771	778	787	rBV	1947577	2985632	31.19%	2.764%
14	7.740	787	791	798	rVB3	9386	17973	0.19%	0.017%
15	8.381	892	900	915	rBV	1345678	2219102	23.18%	2.055%
16	8.828	968	976	992	rVV	2365779	3839891	40.12%	3.555%
17	9.240	1041	1046	1052	rVB	30749	46378	0.48%	0.043%
18	9.546	1089	1098	1117	rBV	1788306	2939394	30.71%	2.721%
19	10.081	1181	1189	1213	rBV	2466758	4083355	42.66%	3.781%
20	10.457	1242	1253	1266	rVB	2801100	4495381	46.96%	4.162%
21	10.604	1268	1278	1295	rBV	2365222	4060535	42.42%	3.759%
22	11.122	1355	1366	1373	rBV3	14938	36672	0.38%	0.034%
23	11.745	1464	1472	1476	rBV	24420	40891	0.43%	0.038%
24	12.057	1519	1525	1533	rBV2	43163	75666	0.79%	0.070%
25	12.275	1557	1562	1568	rVB10	4598	9758	0.10%	0.009%
26	12.687	1627	1632	1634	rBV6	6426	9744	0.10%	0.009%
27	12.934	1669	1674	1679	rBV5	13162	20923	0.22%	0.019%
28	13.234	1717	1725	1728	rBV6	13117	22410	0.23%	0.021%
29	13.292	1728	1735	1743	rVB5	7364	19456	0.20%	0.018%
30	13.751	1806	1813	1825	rBV	4743795	6740734	70.42%	6.241%
31	14.016	1851	1858	1871	rBV	5487788	7911721	82.66%	7.325%
32	14.328	1902	1911	1923	rBV	3786444	5386925	56.28%	4.987%
33	14.545	1942	1948	1963	rBV2	159189	364972	3.81%	0.338%
34	14.769	1982	1986	1989	rVB6	7762	11400	0.12%	0.011%
35	15.145	2044	2050	2052	rBV	28678	41111	0.43%	0.038%
36	15.169	2052	2054	2063	rVB	19578	28404	0.30%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011107.D
 Acq On : 26 Jul 2022 13:20
 Operator : CG/JU
 Sample : N3801-10
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.328	2074	2081	2096	rBV	6974246	9571952	100.00%	8.862%
38	15.451	2096	2102	2115	rVV	1981629	2682324	28.02%	2.483%
39	15.569	2117	2122	2130	rVB	82392	132449	1.38%	0.123%
40	15.816	2159	2164	2170	rBV10	7618	13852	0.14%	0.013%
41	15.945	2182	2186	2193	rVB2	57201	80160	0.84%	0.074%
42	16.033	2196	2201	2202	rBV4	7360	10699	0.11%	0.010%
43	16.110	2209	2214	2221	rVB3	61745	96932	1.01%	0.090%
44	16.569	2287	2292	2297	rBV2	56586	84019	0.88%	0.078%
45	16.775	2323	2327	2331	rVB6	15898	22525	0.24%	0.021%
46	16.875	2339	2344	2353	rVB8	14252	29020	0.30%	0.027%
47	16.980	2356	2362	2365	rBV8	7545	16186	0.17%	0.015%
48	17.092	2374	2381	2391	rBV	3773709	5259325	54.95%	4.869%
49	17.192	2391	2398	2414	rBV2	6455761	9104729	95.12%	8.429%
50	17.398	2430	2433	2437	rVB	11191	13034	0.14%	0.012%
51	17.727	2485	2489	2493	rBV2	38724	45168	0.47%	0.042%
52	17.780	2495	2498	2501	rVB4	14014	15589	0.16%	0.014%
53	18.075	2544	2548	2553	rBV	21455	34360	0.36%	0.032%
54	18.263	2576	2580	2583	rBV	24447	31816	0.33%	0.029%
55	19.022	2705	2709	2715	rBV3	74278	98094	1.02%	0.091%
56	19.092	2717	2721	2727	rVV2	67344	92921	0.97%	0.086%
57	19.451	2776	2782	2790	rBV	6900873	9143950	95.53%	8.466%
58	21.216	3076	3082	3089	rBV	3415292	4547179	47.51%	4.210%
59	23.404	3447	3454	3462	rBV2	4489070	8740159	91.31%	8.092%
60	23.557	3474	3480	3489	rVB2	2375790	4717883	49.29%	4.368%




Sum of corrected areas: 108010707

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011107.D
Acq On : 26 Jul 2022 13:20
Operator : CG/JU
Sample : N3801-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

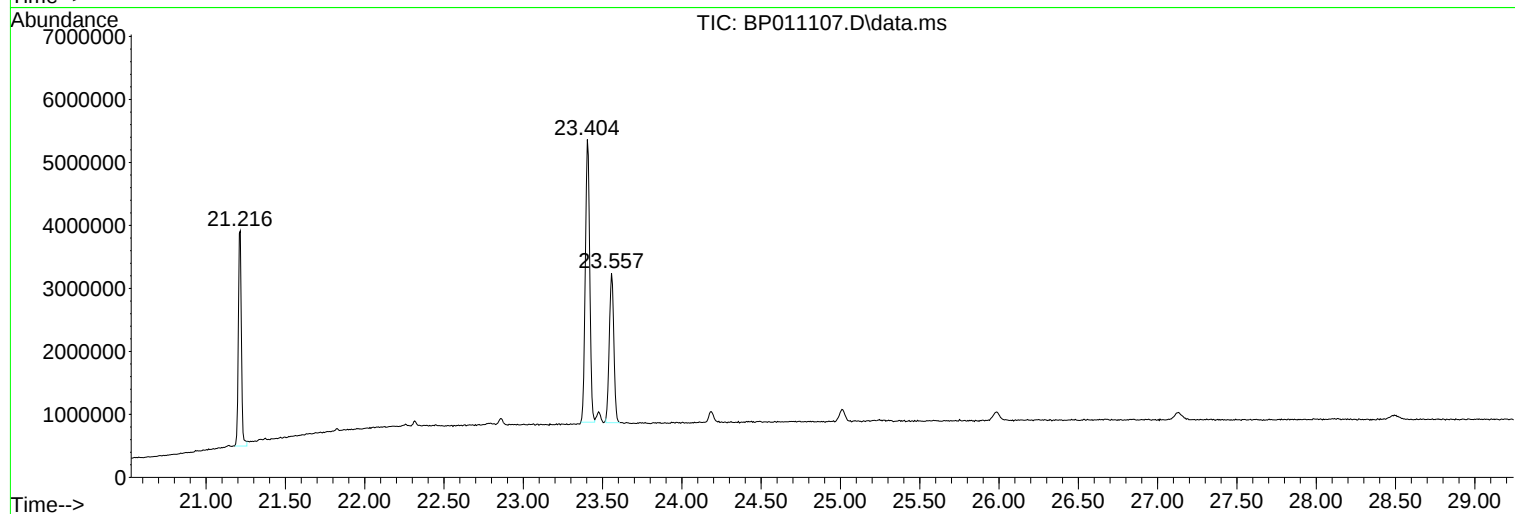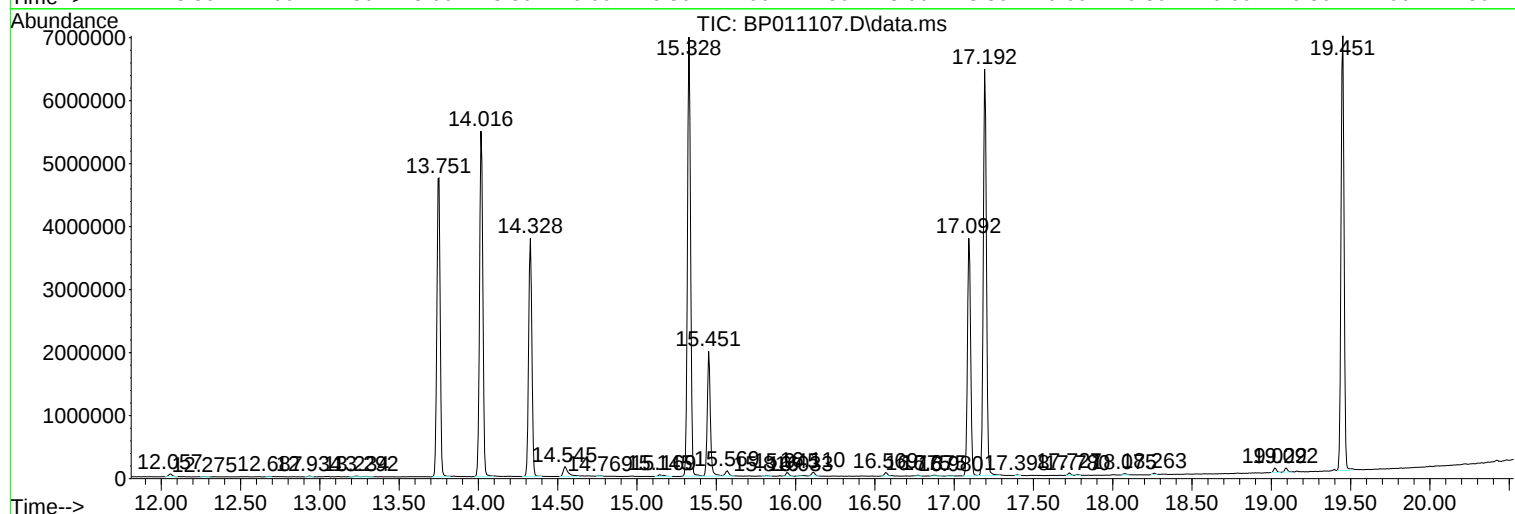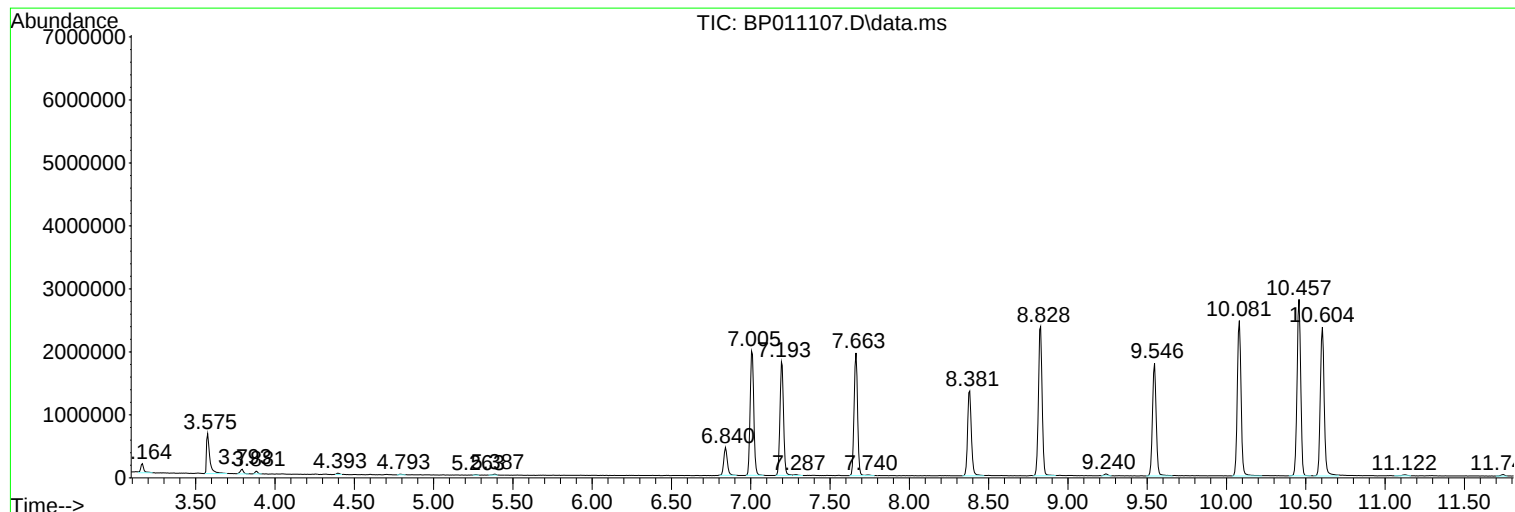

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011107.D
Acq On : 26 Jul 2022 13:20
Operator : CG/JU
Sample : N3801-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011107.D
Acq On : 26 Jul 2022 13:20
Operator : CG/JU
Sample : N3801-10
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc