

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011108.D
 Acq On : 26 Jul 2022 13:54
 Operator : CG/JU
 Sample : N3801-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011108.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.128	3	7	10	rBV	321174	380141	4.15%	0.378%
2	3.164	10	13	28	rVB	137140	215725	2.35%	0.214%
3	3.575	80	83	100	rBV	590074	830657	9.06%	0.826%
4	3.793	113	120	127	rVB2	55162	104120	1.14%	0.104%
5	3.881	132	135	140	rVB	38841	47265	0.52%	0.047%
6	4.399	220	223	227	rVB4	17451	22809	0.25%	0.023%
7	5.381	387	390	399	rVB2	12863	19949	0.22%	0.020%
8	6.840	633	638	649	rVB	342323	548965	5.99%	0.546%
9	7.005	660	666	683	rVB	1704942	2630260	28.70%	2.615%
10	7.193	691	698	709	rBV	1487713	2340233	25.54%	2.326%
11	7.287	711	714	719	rVB5	10682	15583	0.17%	0.015%
12	7.663	769	778	788	rBV	1851848	2829788	30.88%	2.813%
13	8.381	893	900	916	rBV	1080363	1816261	19.82%	1.806%
14	8.828	967	976	985	rBV	2008736	3249498	35.46%	3.230%
15	9.240	1041	1046	1054	rVB	25500	42961	0.47%	0.043%
16	9.546	1090	1098	1113	rBV	1551561	2475948	27.02%	2.461%
17	10.081	1180	1189	1201	rBV	2093459	3445522	37.60%	3.425%
18	10.457	1244	1253	1266	rBV	2631282	4335295	47.31%	4.310%
19	10.604	1270	1278	1298	rBV	2095555	3660056	39.94%	3.638%
20	11.746	1463	1472	1476	rBV	31580	51105	0.56%	0.051%
21	12.063	1519	1526	1532	rBV2	36025	70794	0.77%	0.070%
22	12.134	1532	1538	1544	rVB2	4782	13173	0.14%	0.013%
23	12.675	1623	1630	1640	rBV5	11316	28646	0.31%	0.028%
24	12.934	1670	1674	1680	rBV2	17723	24559	0.27%	0.024%
25	13.151	1707	1711	1717	rVB4	8379	13152	0.14%	0.013%
26	13.234	1721	1725	1729	rBV4	10162	16568	0.18%	0.016%
27	13.745	1805	1812	1823	rBV	4343712	6298364	68.73%	6.261%
28	14.016	1850	1858	1872	rBV	4939236	7118166	77.67%	7.076%
29	14.234	1891	1895	1902	rVB	17079	24780	0.27%	0.025%
30	14.328	1904	1911	1924	rVV	3854747	5388127	58.80%	5.356%
31	14.545	1942	1948	1962	rBV	135674	303568	3.31%	0.302%
32	14.769	1982	1986	1991	rVB7	10375	15808	0.17%	0.016%
33	14.969	2016	2020	2024	rVB7	7833	11900	0.13%	0.012%
34	15.145	2045	2050	2053	rBV	74771	112197	1.22%	0.112%
35	15.192	2056	2058	2062	rVB2	21430	26781	0.29%	0.027%
36	15.328	2074	2081	2096	rBV	6543359	8959606	97.77%	8.907%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
 Data File : BP011108.D
 Acq On : 26 Jul 2022 13:54
 Operator : CG/JU
 Sample : N3801-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHX9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.451	2096	2102	2117	rBV	1976541	2713670	29.61%	2.698%
38	15.569	2117	2122	2126	rVV2	73425	99642	1.09%	0.099%
39	15.716	2143	2147	2150	rVB6	6642	9243	0.10%	0.009%
40	16.063	2203	2206	2211	rBV2	16081	23514	0.26%	0.023%
41	16.116	2212	2215	2222	rVB5	21472	34520	0.38%	0.034%
42	16.575	2290	2293	2298	rVB7	10920	15789	0.17%	0.016%
43	16.775	2322	2327	2332	rVB9	10451	14759	0.16%	0.015%
44	16.869	2338	2343	2348	rBV4	28133	48007	0.52%	0.048%
45	17.092	2375	2381	2390	rBV	3771391	5348240	58.36%	5.317%
46	17.192	2392	2398	2413	rVV2	6462692	9164192	100.00%	9.110%
47	17.398	2430	2433	2438	rBV	12241	17484	0.19%	0.017%
48	17.616	2466	2470	2474	rBV5	13642	20329	0.22%	0.020%
49	17.781	2494	2498	2503	rVB8	17682	25741	0.28%	0.026%
50	18.010	2533	2537	2542	rBV7	6650	11955	0.13%	0.012%
51	18.075	2545	2548	2553	rVB	28046	33371	0.36%	0.033%
52	18.298	2582	2586	2587	rBV3	13789	17469	0.19%	0.017%
53	19.028	2706	2710	2714	rVB2	68574	88264	0.96%	0.088%
54	19.092	2717	2721	2730	rVV	70088	100802	1.10%	0.100%
55	19.398	2770	2773	2776	rBV3	24308	28522	0.31%	0.028%
56	19.451	2776	2782	2789	rBV	6981665	8942166	97.58%	8.889%
57	21.216	3077	3082	3092	rBV	3229768	4154391	45.33%	4.130%
58	23.404	3447	3454	3463	rBV2	4144118	7923070	86.46%	7.876%
59	23.557	3474	3480	3493	rVB2	2171674	4270833	46.60%	4.246%




Sum of corrected areas: 100594303

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011108.D
Acq On : 26 Jul 2022 13:54
Operator : CG/JU
Sample : N3801-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

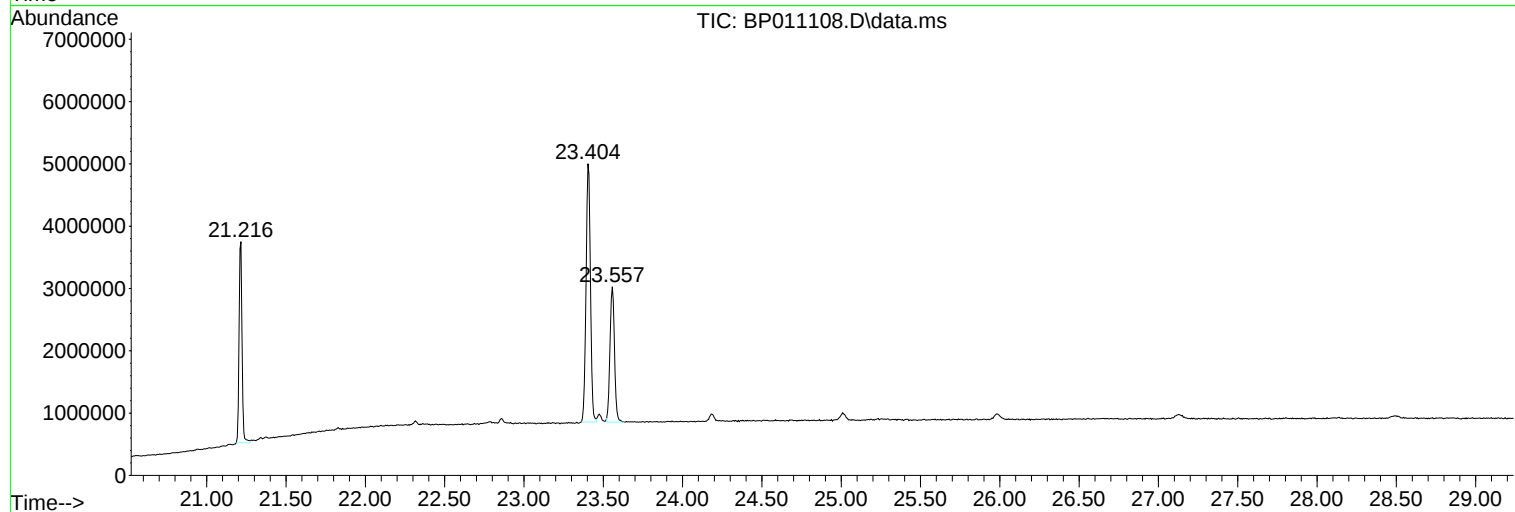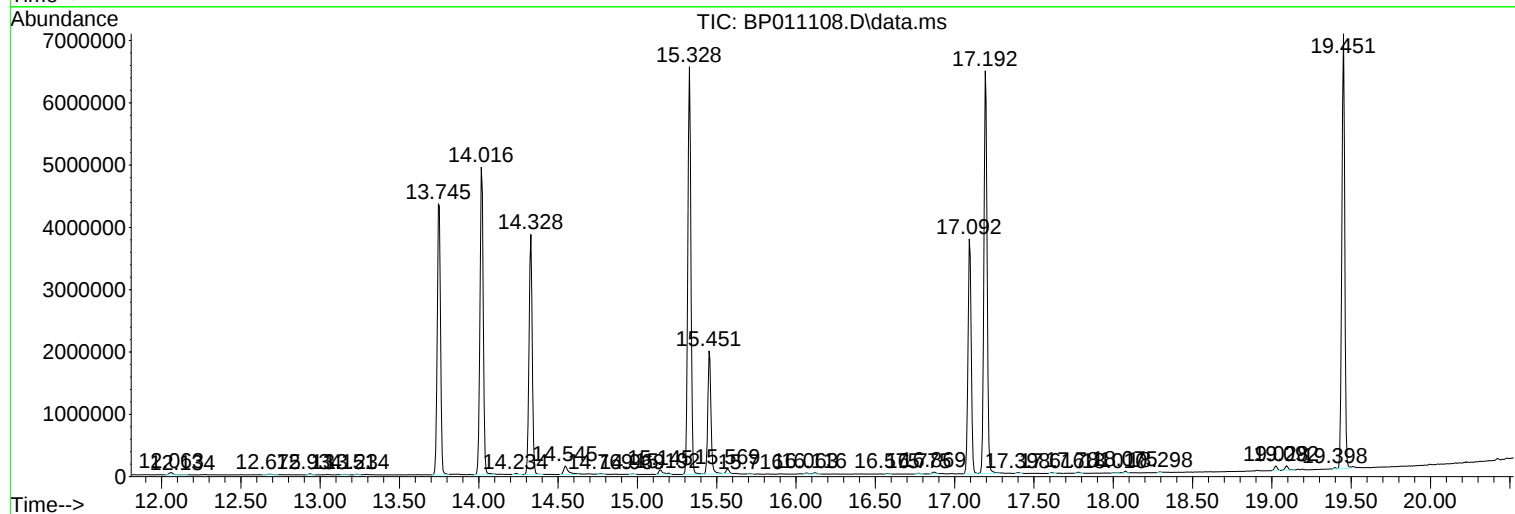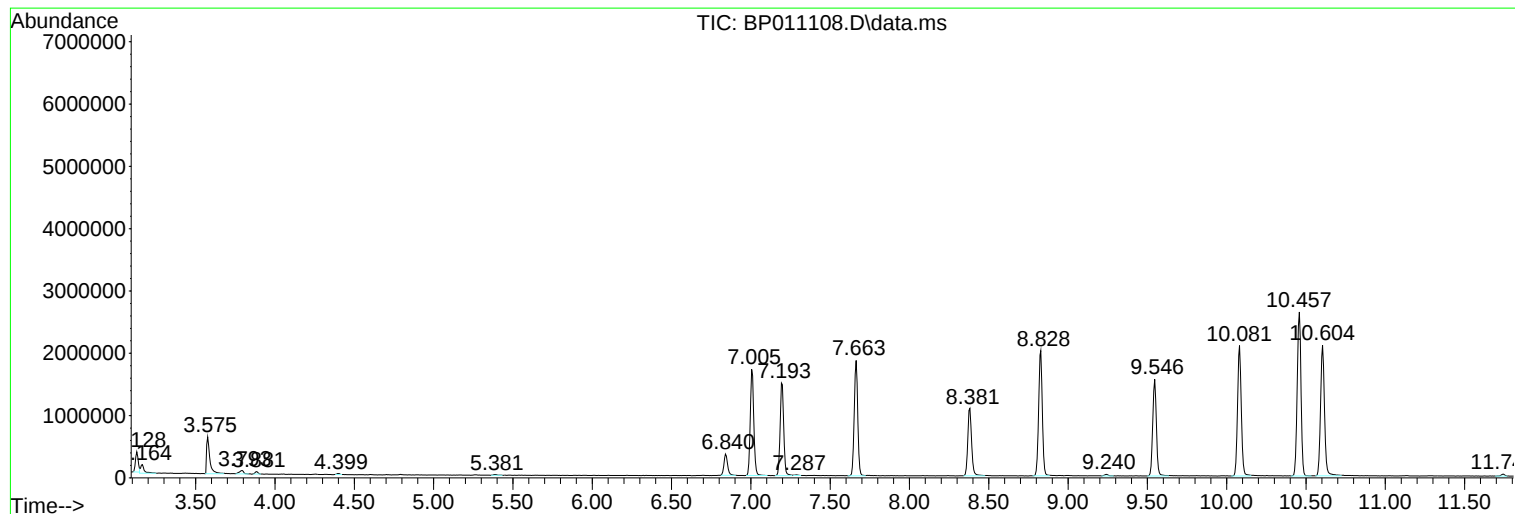

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011108.D
Acq On : 26 Jul 2022 13:54
Operator : CG/JU
Sample : N3801-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072622\
Data File : BP011108.D
Acq On : 26 Jul 2022 13:54
Operator : CG/JU
Sample : N3801-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHX9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------